

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047702.D
 Acq On : 28 Sep 2024 21:57
 Operator : RC/JU
 Sample : P3927-04DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC82DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	115	118	127	rBV	53428	89096	2.67%	0.336%
2	4.004	170	173	180	rVB2	14990	20825	0.62%	0.079%
3	4.934	327	331	337	rBV3	13140	24022	0.72%	0.091%
4	5.840	480	485	495	rBV4	18824	33987	1.02%	0.128%
5	6.128	529	534	541	rVV3	39957	67461	2.02%	0.255%
6	6.816	647	651	656	rVB4	14279	24626	0.74%	0.093%
7	6.875	656	661	664	rBV2	17640	26571	0.80%	0.100%
8	6.975	672	678	685	rBV2	116210	202227	6.06%	0.764%
9	7.140	700	706	714	rBV	83774	142152	4.26%	0.537%
10	7.245	720	724	730	rVV2	15662	22370	0.67%	0.084%
11	7.345	734	741	751	rVV	99234	160201	4.80%	0.605%
12	7.451	753	759	767	rVB2	87562	151780	4.55%	0.573%
13	7.722	801	805	813	rBV8	11270	29669	0.89%	0.112%
14	7.816	813	821	828	rVV	841732	1363749	40.88%	5.150%
15	7.887	828	833	838	rVV4	18347	35544	1.07%	0.134%
16	8.045	855	860	864	rVV4	16491	33981	1.02%	0.128%
17	8.245	888	894	899	rVV	68934	113057	3.39%	0.427%
18	8.292	899	902	907	rVV4	15453	25839	0.77%	0.098%
19	8.357	907	913	918	rVV4	18222	34757	1.04%	0.131%
20	8.416	918	923	926	rVV2	19291	30867	0.93%	0.117%
21	8.451	926	929	932	rVV5	16282	26537	0.80%	0.100%
22	8.516	935	940	948	rVV	116216	204966	6.14%	0.774%
23	8.586	948	952	955	rVV2	20815	33843	1.01%	0.128%
24	8.622	955	958	964	rVV4	15027	25571	0.77%	0.097%
25	8.692	964	970	976	rVV7	10566	20961	0.63%	0.079%
26	8.810	986	990	1000	rVB7	19812	36838	1.10%	0.139%
27	8.963	1011	1016	1023	rVB2	83021	144778	4.34%	0.547%
28	9.051	1025	1031	1034	rVV	87014	125430	3.76%	0.474%
29	9.104	1034	1040	1049	rVV	148495	273386	8.19%	1.032%
30	9.398	1085	1090	1096	rBV5	22948	37013	1.11%	0.140%
31	9.533	1110	1113	1118	rVB4	15409	25791	0.77%	0.097%
32	9.686	1132	1139	1147	rBV4	74545	149970	4.50%	0.566%
33	9.763	1147	1152	1156	rBV7	13291	21986	0.66%	0.083%
34	10.104	1204	1210	1215	rVV	39897	65362	1.96%	0.247%
35	10.228	1223	1231	1240	rVB	107345	195117	5.85%	0.737%
36	10.304	1240	1244	1248	rBV5	14749	22610	0.68%	0.085%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047702.D
 Acq On : 28 Sep 2024 21:57
 Operator : RC/JU
 Sample : P3927-04DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC82DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	10.486	1269	1275	1281	rBV5	14346	32353	0.97%	0.122%
38	10.604	1286	1295	1303	rBV	1243086	2178387	65.30%	8.226%
39	10.739	1312	1318	1324	rBV2	138126	263427	7.90%	0.995%
40	10.810	1326	1330	1335	rVV3	24306	42285	1.27%	0.160%
41	10.898	1338	1345	1354	rVV5	28746	64853	1.94%	0.245%
42	10.992	1356	1361	1369	rVB	39625	68671	2.06%	0.259%
43	11.122	1377	1383	1391	rVB6	18233	42958	1.29%	0.162%
44	11.504	1442	1448	1451	rBV8	17830	30550	0.92%	0.115%
45	11.645	1467	1472	1476	rBV3	16613	24127	0.72%	0.091%
46	11.710	1477	1483	1489	rVV3	14681	27163	0.81%	0.103%
47	11.880	1501	1512	1518	rBV5	28352	65439	1.96%	0.247%
48	12.039	1533	1539	1542	rBV3	31985	55575	1.67%	0.210%
49	12.075	1542	1545	1550	rVV2	21817	26799	0.80%	0.101%
50	12.157	1550	1559	1566	rVV2	11532	24729	0.74%	0.093%
51	12.286	1573	1581	1587	rVB4	35995	78674	2.36%	0.297%
52	12.445	1602	1608	1612	rVV4	34609	58514	1.75%	0.221%
53	12.492	1612	1616	1619	rVV3	12886	21804	0.65%	0.082%
54	12.692	1643	1650	1657	rVV3	11294	30556	0.92%	0.115%
55	13.027	1703	1707	1710	rVB	19121	27828	0.83%	0.105%
56	13.204	1733	1737	1743	rVV4	14282	24349	0.73%	0.092%
57	13.280	1743	1750	1754	rVV3	40594	60869	1.82%	0.230%
58	13.498	1780	1787	1796	rVB3	19196	50018	1.50%	0.189%
59	13.633	1801	1810	1816	rBV10	21916	55444	1.66%	0.209%
60	13.716	1819	1824	1829	rBV4	22099	40032	1.20%	0.151%
61	13.769	1829	1833	1837	rVV4	17815	29438	0.88%	0.111%
62	13.851	1842	1847	1855	rVB	215600	313067	9.38%	1.182%
63	13.998	1867	1872	1877	rBV5	22219	36251	1.09%	0.137%
64	14.139	1890	1896	1901	rVV	218316	312300	9.36%	1.179%
65	14.357	1928	1933	1938	rBV	129526	159494	4.78%	0.602%
66	14.445	1942	1948	1956	rVB	1620102	2353110	70.54%	8.886%
67	14.527	1956	1962	1969	rBV9	13277	24081	0.72%	0.091%
68	14.592	1969	1973	1976	rBV	18825	23542	0.71%	0.089%
69	14.633	1976	1980	1987	rBV3	49975	103732	3.11%	0.392%
70	14.851	2012	2017	2022	rVB8	11334	22418	0.67%	0.085%
71	14.921	2022	2029	2034	rVB4	13729	27082	0.81%	0.102%
72	14.980	2034	2039	2044	rBV9	17500	35573	1.07%	0.134%
73	15.068	2049	2054	2059	rVV2	177405	260848	7.82%	0.985%
74	15.204	2073	2077	2080	rVV3	22098	32009	0.96%	0.121%
75	15.304	2087	2094	2099	rVB2	55652	92444	2.77%	0.349%
76	15.433	2108	2116	2122	rBV	293395	444603	13.33%	1.679%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047702.D
 Acq On : 28 Sep 2024 21:57
 Operator : RC/JU
 Sample : P3927-04DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC82DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

77	15.545	2129	2135	2145	rBV3	75565	139225	4.17%	0.526%
78	15.710	2154	2163	2168	rBV3	22090	40142	1.20%	0.152%
79	15.798	2173	2178	2185	rVV	145442	211141	6.33%	0.797%
80	16.162	2236	2240	2243	rBV	58602	74718	2.24%	0.282%
81	16.362	2270	2274	2283	rVB5	24423	42624	1.28%	0.161%
82	16.515	2292	2300	2308	rBV	43777	93741	2.81%	0.354%
83	16.833	2348	2354	2368	rBV	2206077	3059754	91.72%	11.554%
84	16.951	2371	2374	2379	rVV	62433	97200	2.91%	0.367%
85	17.009	2379	2384	2393	rVB5	28632	55554	1.67%	0.210%
86	17.180	2407	2413	2424	rVV	1835339	2757884	82.67%	10.414%
87	17.280	2424	2430	2436	rBV	311967	457481	13.71%	1.728%
88	17.486	2460	2465	2469	rBV7	12860	25052	0.75%	0.095%
89	17.692	2495	2500	2504	rVB	44784	58740	1.76%	0.222%
90	17.798	2515	2518	2524	rVB8	16740	24364	0.73%	0.092%
91	17.862	2524	2529	2533	rBV	69610	90091	2.70%	0.340%
92	18.074	2560	2565	2573	rVB6	45108	69650	2.09%	0.263%
93	18.380	2613	2617	2622	rBV	40197	54246	1.63%	0.205%
94	18.521	2637	2641	2646	rBV4	18262	33726	1.01%	0.127%
95	19.027	2721	2727	2733	rVB3	47030	85422	2.56%	0.323%
96	19.162	2747	2750	2753	rBV2	22024	22362	0.67%	0.084%
97	19.568	2814	2819	2826	rBV	387842	545622	16.36%	2.060%
98	21.409	3126	3132	3145	rBV	1946653	2917391	87.45%	11.017%
99	24.203	3602	3607	3618	rVB2	201799	480992	14.42%	1.816%
100	24.415	3635	3643	3659	rVB	1244400	3336070	100.00%	12.598%




Sum of corrected areas: 26481528

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047702.D
Acq On : 28 Sep 2024 21:57
Operator : RC/JU
Sample : P3927-04DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC82DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

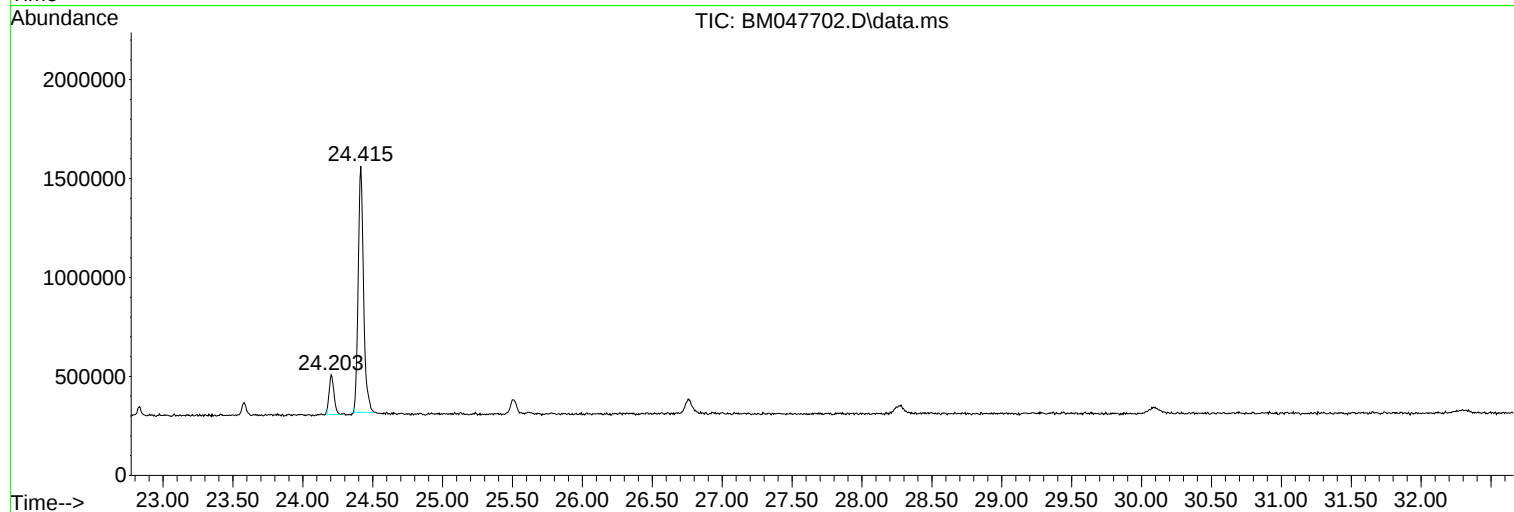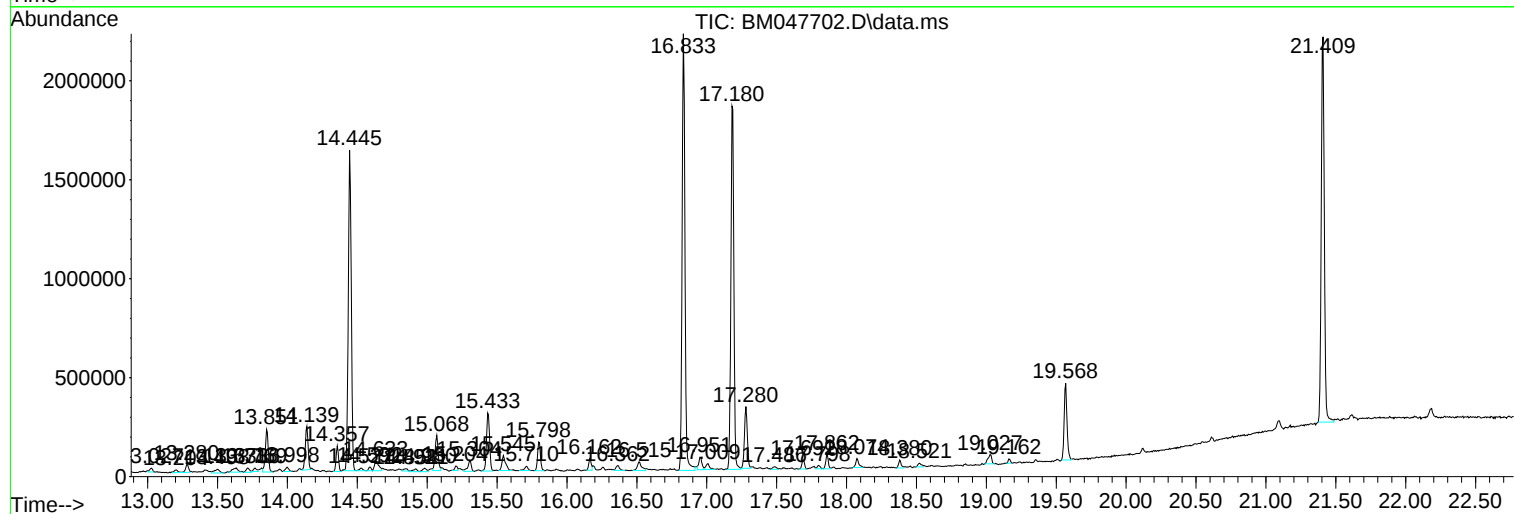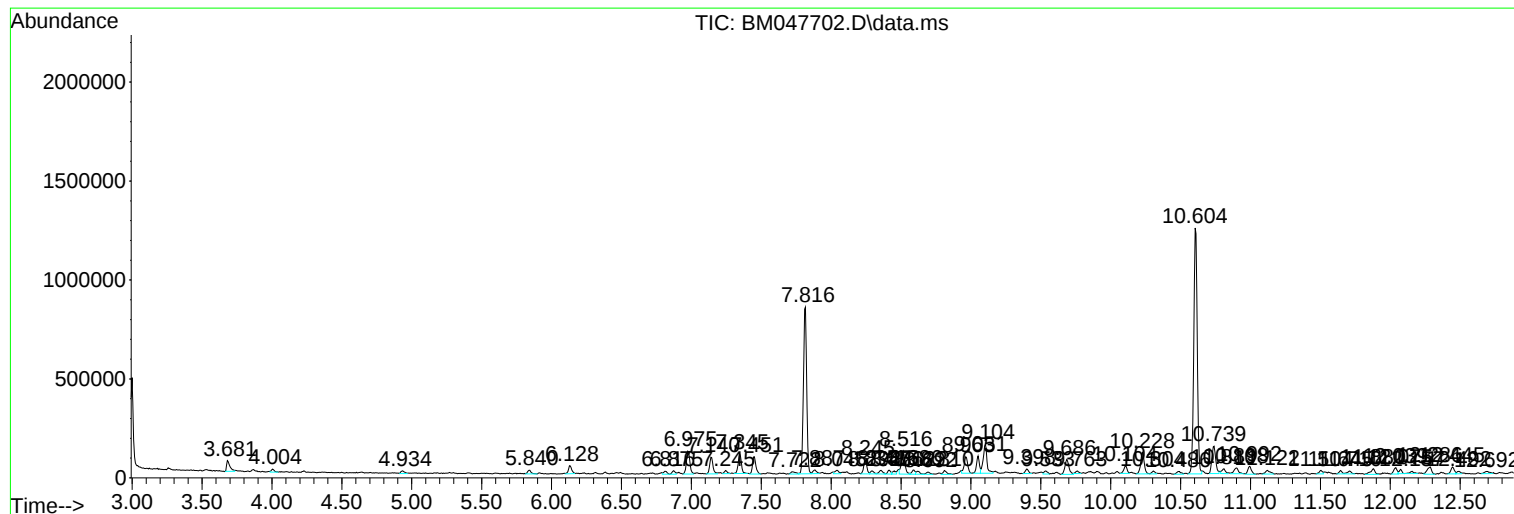

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047702.D
Acq On : 28 Sep 2024 21:57
Operator : RC/JU
Sample : P3927-04DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC82DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.451	2.23 ng/ul	151780	1,4-Dichlorobenzene-d4	7.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Decane	142	C10H22	000124-18-5	90
2			Tetradecane	198	C14H30	000629-59-4	78
3			Octane, 2,4,6-trimethyl-	156	C11H24	062016-37-9	78
4			Tetradecane	198	C14H30	000629-59-4	78
5			Carbonic acid, prop-1-en-2-yl tr...	284	C17H32O3	1000382-90-8	78

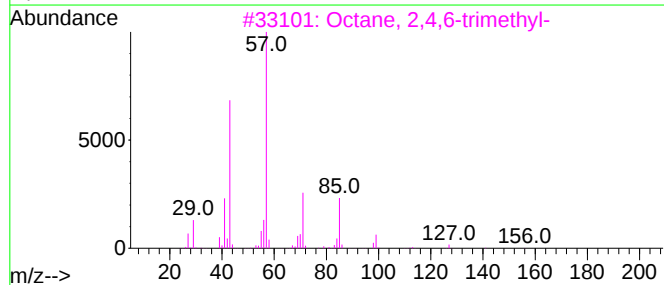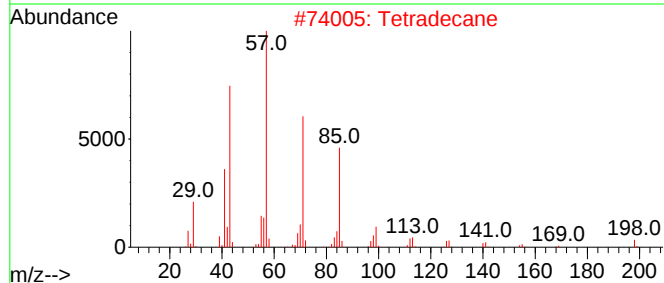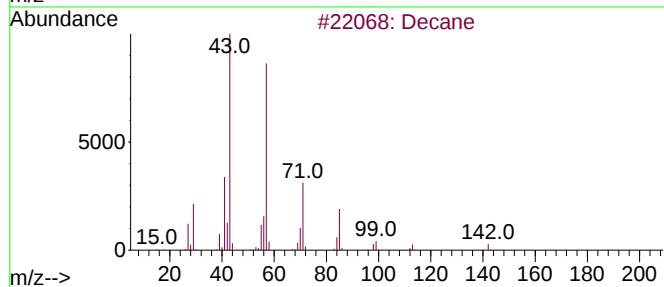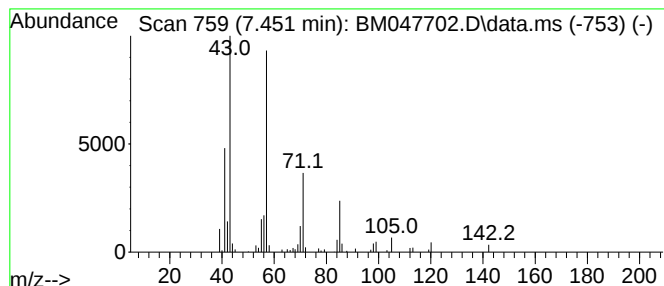

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047702.D
Acq On : 28 Sep 2024 21:57
Operator : RC/JU
Sample : P3927-04DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC82DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Hexanoic acid, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.104	4.01 ng/ul	273386	1,4-Dichlorobenzene-d4	7.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
2			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
3			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	83
4			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	78
5			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	59

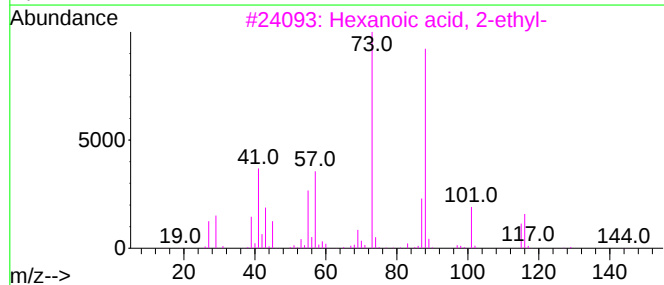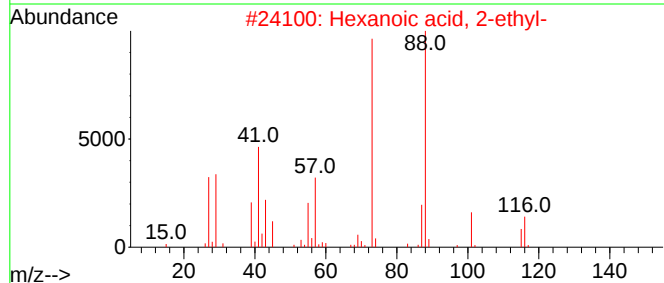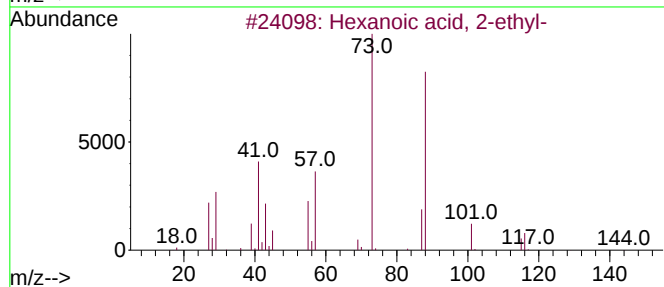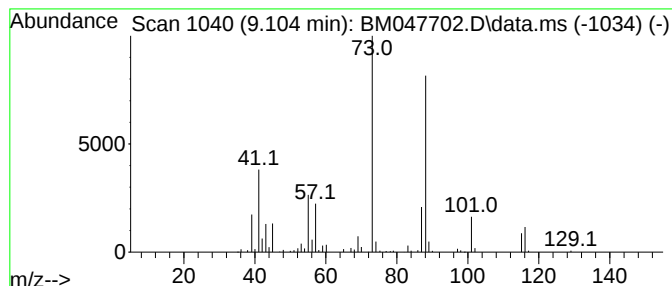

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047702.D
Acq On : 28 Sep 2024 21:57
Operator : RC/JU
Sample : P3927-04DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC82DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	7.451	2.2	ng/ul	151780	1	7.816	1363750	20.0
Hexanoic acid, ...	9.104	4.0	ng/ul	273386	1	7.816	1363750	20.0