

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047703.D
 Acq On : 28 Sep 2024 22:36
 Operator : RC/JU
 Sample : P3927-02DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047703.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	115	119	125	rBV2	39337	65329	1.83%	0.346%
2	3.857	146	148	152	rVB5	3746	3983	0.11%	0.021%
3	4.004	169	173	180	rVB2	22952	30425	0.85%	0.161%
4	4.228	208	211	217	rVB6	8333	11409	0.32%	0.060%
5	4.563	267	268	270	rBV	5478	3986	0.11%	0.021%
6	4.940	328	332	336	rBV6	3022	5570	0.16%	0.029%
7	5.028	344	347	350	rBV5	2946	3918	0.11%	0.021%
8	5.257	382	386	389	rBV5	3267	5096	0.14%	0.027%
9	5.416	411	413	416	rVB4	4416	4598	0.13%	0.024%
10	6.545	602	605	611	rBV7	2696	5892	0.16%	0.031%
11	6.822	647	652	654	rBV5	3099	4511	0.13%	0.024%
12	6.875	658	661	664	rBV5	2668	4222	0.12%	0.022%
13	6.975	673	678	685	rBV2	47426	77574	2.17%	0.410%
14	7.145	701	707	714	rBV	41578	70199	1.96%	0.371%
15	7.345	736	741	749	rVB2	44157	72535	2.03%	0.384%
16	7.451	754	759	763	rBV7	9937	20351	0.57%	0.108%
17	7.728	805	806	811	rVB5	3070	3945	0.11%	0.021%
18	7.816	813	821	830	rBV	728744	1166757	32.61%	6.174%
19	7.886	830	833	836	rVB5	4968	6724	0.19%	0.036%
20	8.016	852	855	858	rVB4	3182	4506	0.13%	0.024%
21	8.410	919	922	927	rVB4	5559	7101	0.20%	0.038%
22	8.516	927	940	947	rBV	50593	96246	2.69%	0.509%
23	8.586	947	952	957	rVV6	3120	6639	0.19%	0.035%
24	8.963	1012	1016	1026	rVV	37926	64752	1.81%	0.343%
25	9.051	1026	1031	1036	rVB3	14928	24969	0.70%	0.132%
26	9.539	1111	1114	1119	rBV5	2952	5964	0.17%	0.032%
27	9.598	1122	1124	1132	rVB7	2424	4140	0.12%	0.022%
28	9.692	1134	1140	1146	rBV3	26435	48987	1.37%	0.259%
29	10.227	1226	1231	1237	rBV2	42219	73890	2.07%	0.391%
30	10.610	1288	1296	1310	rBV	924344	1596710	44.62%	8.449%
31	10.739	1310	1318	1333	rVB3	53632	118981	3.33%	0.630%
32	10.992	1356	1361	1370	rVB7	6717	16263	0.45%	0.086%
33	11.122	1378	1383	1387	rBV3	20254	34377	0.96%	0.182%
34	11.451	1434	1439	1443	rBV6	3238	5526	0.15%	0.029%
35	11.498	1443	1447	1448	rVV3	3941	4392	0.12%	0.023%
36	11.522	1449	1451	1457	rVB3	3905	6730	0.19%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047703.D
 Acq On : 28 Sep 2024 22:36
 Operator : RC/JU
 Sample : P3927-02DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	11.645	1469	1472	1475	rBV4	3920	4033	0.11%	0.021%
38	11.851	1501	1507	1508	rBV4	3508	4794	0.13%	0.025%
39	11.880	1508	1512	1516	rVV3	8713	13554	0.38%	0.072%
40	11.951	1522	1524	1530	rVB4	3346	5014	0.14%	0.027%
41	12.039	1530	1539	1543	rBV6	8864	20289	0.57%	0.107%
42	12.074	1543	1545	1551	rVB5	8005	8248	0.23%	0.044%
43	12.445	1602	1608	1615	rBV7	13893	28213	0.79%	0.149%
44	12.692	1645	1650	1654	rBV4	4628	9034	0.25%	0.048%
45	12.863	1674	1679	1682	rVB4	3035	5544	0.15%	0.029%
46	12.992	1699	1701	1704	rBV4	4127	5601	0.16%	0.030%
47	13.021	1704	1706	1712	rVB6	3951	4882	0.14%	0.026%
48	13.280	1743	1750	1757	rBV5	12312	23757	0.66%	0.126%
49	13.498	1783	1787	1794	rVB4	8185	14530	0.41%	0.077%
50	13.639	1807	1811	1814	rBV6	3624	6200	0.17%	0.033%
51	13.774	1828	1834	1836	rBV7	3691	6042	0.17%	0.032%
52	13.857	1843	1848	1856	rVB	104003	150070	4.19%	0.794%
53	13.939	1856	1862	1867	rVB6	4830	10314	0.29%	0.055%
54	13.992	1867	1871	1872	rBV4	3414	4073	0.11%	0.022%
55	14.086	1883	1887	1888	rBV3	5389	5708	0.16%	0.030%
56	14.139	1891	1896	1905	rVB	108469	168253	4.70%	0.890%
57	14.357	1928	1933	1938	rBV	91621	117608	3.29%	0.622%
58	14.445	1942	1948	1956	rVV	1372120	1975466	55.21%	10.453%
59	14.527	1958	1962	1966	rVB3	7803	9237	0.26%	0.049%
60	14.633	1975	1980	1986	rBV10	13370	33575	0.94%	0.178%
61	14.992	2036	2041	2044	rVB5	8259	10804	0.30%	0.057%
62	15.021	2044	2046	2049	rBV4	6017	8091	0.23%	0.043%
63	15.068	2049	2054	2060	rVB2	49176	73365	2.05%	0.388%
64	15.180	2070	2073	2079	rVB7	7146	11031	0.31%	0.058%
65	15.233	2079	2082	2084	rVV3	6001	7635	0.21%	0.040%
66	15.257	2084	2086	2088	rVV3	7712	10218	0.29%	0.054%
67	15.280	2088	2090	2091	rVV2	11158	10319	0.29%	0.055%
68	15.304	2091	2094	2099	rVB2	23195	31228	0.87%	0.165%
69	15.433	2111	2116	2123	rVB	149141	220723	6.17%	1.168%
70	15.545	2130	2135	2147	rVB7	34543	59003	1.65%	0.312%
71	15.639	2147	2151	2154	rBV4	2609	4271	0.12%	0.023%
72	15.709	2159	2163	2167	rVB7	10669	16034	0.45%	0.085%
73	15.798	2174	2178	2185	rBV2	48539	70332	1.97%	0.372%
74	15.927	2197	2200	2203	rVB4	3996	5152	0.14%	0.027%
75	16.162	2237	2240	2243	rBV2	22865	30368	0.85%	0.161%
76	16.192	2243	2245	2251	rVB5	9460	10817	0.30%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047703.D
 Acq On : 28 Sep 2024 22:36
 Operator : RC/JU
 Sample : P3927-02DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

77	16.362	2270	2274	2278	rBV7	9181	13784	0.39%	0.073%
78	16.674	2323	2327	2334	rBV7	7391	13212	0.37%	0.070%
79	16.727	2334	2336	2340	rBV5	3692	4468	0.12%	0.024%
80	16.833	2348	2354	2369	rBV	2638703	3578063	100.00%	18.932%
81	16.951	2371	2374	2379	rVV4	31894	50917	1.42%	0.269%
82	17.004	2381	2383	2392	rVB6	13863	22103	0.62%	0.117%
83	17.186	2407	2414	2423	rBV	1614503	2350980	65.71%	12.440%
84	17.280	2425	2430	2436	rVV2	163809	238936	6.68%	1.264%
85	17.321	2436	2437	2444	rVB6	11837	13528	0.38%	0.072%
86	17.374	2444	2446	2450	rVB5	5318	5851	0.16%	0.031%
87	17.468	2459	2462	2463	rBV3	4190	4288	0.12%	0.023%
88	17.692	2496	2500	2504	rVB2	18721	23966	0.67%	0.127%
89	17.762	2509	2512	2515	rBV4	6682	8610	0.24%	0.046%
90	17.803	2515	2519	2523	rVV4	12654	16583	0.46%	0.088%
91	17.851	2526	2527	2532	rVB5	4602	5384	0.15%	0.028%
92	18.045	2558	2560	2562	rBV3	3949	4214	0.12%	0.022%
93	18.074	2562	2565	2573	rVV7	18274	30111	0.84%	0.159%
94	18.386	2613	2618	2620	rBV3	15553	21211	0.59%	0.112%
95	18.962	2714	2716	2718	rBV2	5878	4004	0.11%	0.021%
96	19.015	2722	2725	2728	rVV5	14354	17758	0.50%	0.094%
97	19.356	2780	2783	2786	rBV5	11777	14055	0.39%	0.074%
98	19.568	2814	2819	2825	rBV	184411	278444	7.78%	1.473%
99	21.409	3126	3132	3139	rBV	1652891	2476769	69.22%	13.105%
100	24.409	3635	3642	3664	rVB	1046084	2801394	78.29%	14.823%




Sum of corrected areas: 18899260

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047703.D
Acq On : 28 Sep 2024 22:36
Operator : RC/JU
Sample : P3927-02DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC80DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

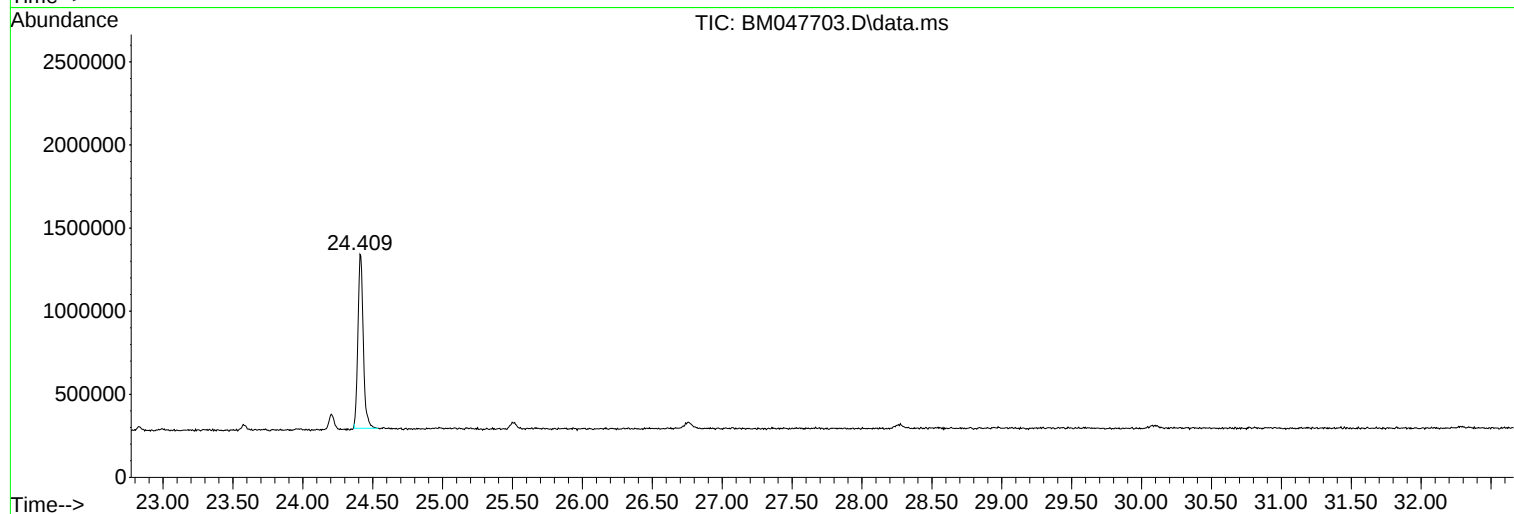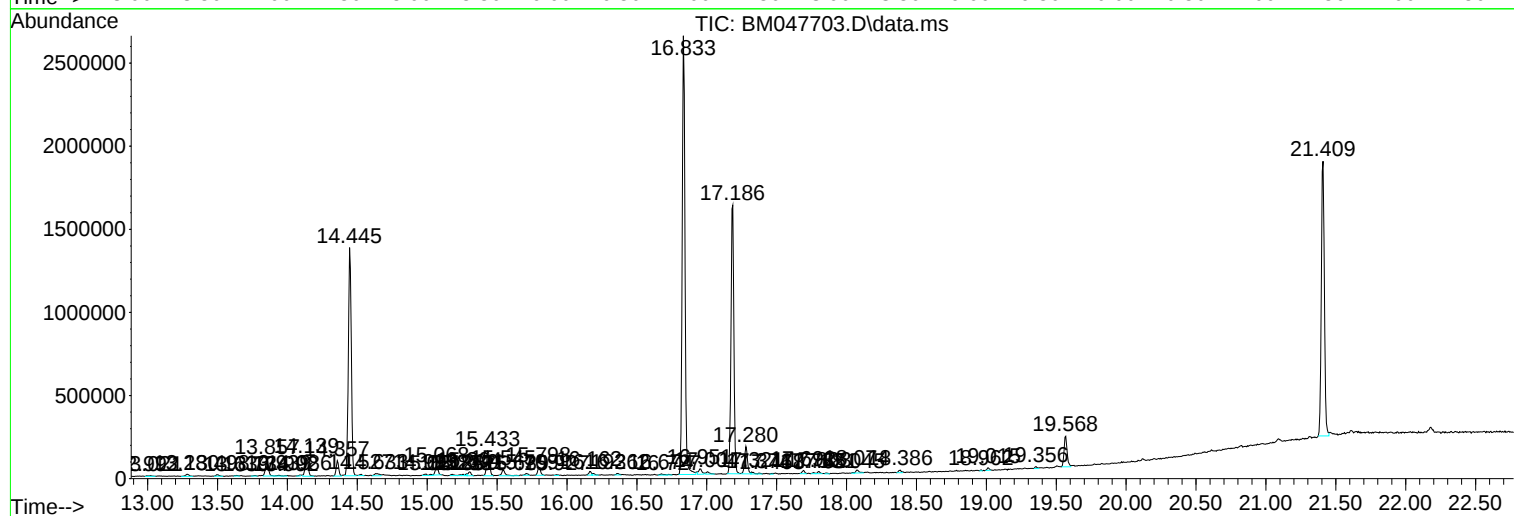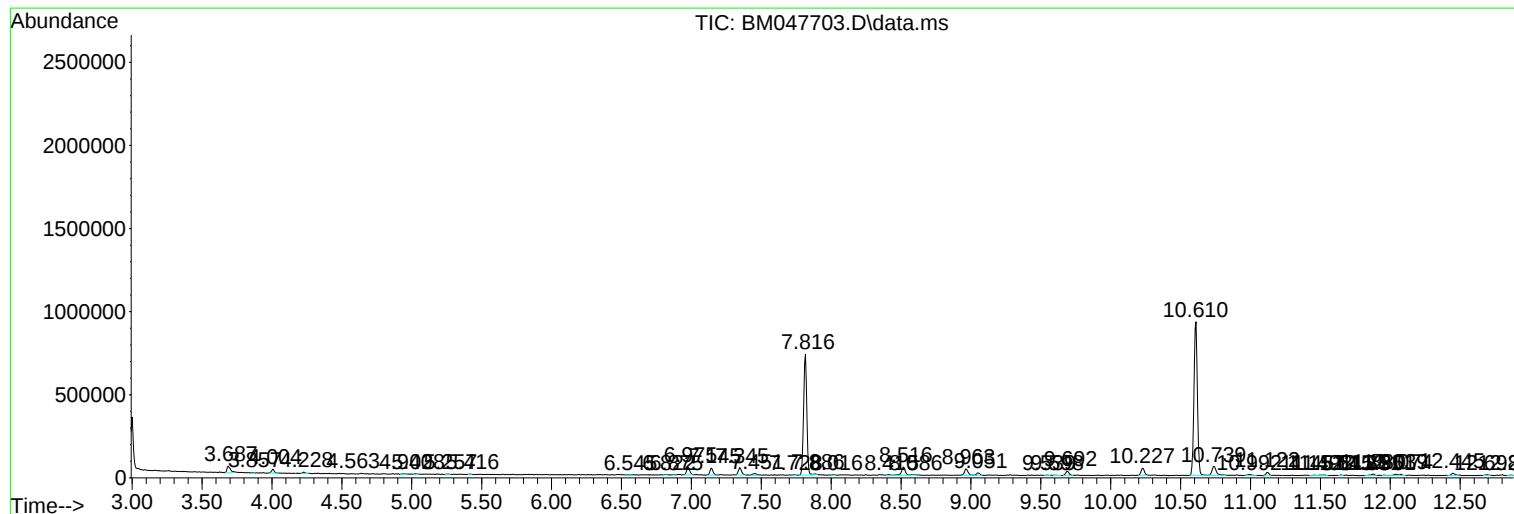

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047703.D
Acq On : 28 Sep 2024 22:36
Operator : RC/JU
Sample : P3927-02DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC80DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047703.D
Acq On : 28 Sep 2024 22:36
Operator : RC/JU
Sample : P3927-02DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC80DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc