

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092922\
 Data File : BM036802.D
 Acq On : 29 Sep 2022 15:30
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SICV032

Quant Time: Sep 30 01:56:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 30 01:50:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.986	152	262140	20.000	ng/u1	0.00
20) Naphthalene-d8	10.798	136	1226095	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.615	164	808080	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.351	188	1673728	20.000	ng/u1	0.00
79) Chrysene-d12	21.515	240	1713499	20.000	ng/u1	0.00
88) Perylene-d12	23.938	264	1721397	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	50924	7.096	ng/uL	0.00
4) Pyridine-d5	3.798	84	382470	17.053	ng/u1	0.00
7) Phenol-d5	7.145	99	432152	16.187	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	329882	19.788	ng/u1	0.00
11) 2-Chlorophenol-d4	7.516	132	347448	19.287	ng/u1	0.00
15) 4-Methylphenol-d8	8.692	113	373904	18.354	ng/u1	0.00
21) Nitrobenzene-d5	9.151	128	183708	19.559	ng/u1	0.00
24) 2-Nitrophenol-d4	9.875	143	179089	19.727	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	344892	19.473	ng/u1	0.00
31) 4-Chloroaniline-d4	10.933	131	568360	18.579	ng/u1	0.00
46) Dimethylphthalate-d6	14.027	166	1156369	20.309	ng/u1	0.00
49) Acenaphthylene-d8	14.310	160	1359196	20.943	ng/u1	0.00
54) 4-Nitrophenol-d4	14.804	143	221576	18.093	ng/u1	0.00
60) Fluorene-d10	15.598	176	955994	19.178	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.715	200	157276	17.081	ng/u1	0.00
73) Anthracene-d10	17.445	188	1463913	18.850	ng/u1	0.00
81) Pyrene-d10	19.733	212	1686986	19.484	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.780	264	1630418	18.885	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.404	88	54070	7.018	ng/uL	98
5) Pyridine	3.816	79	348724	15.420	ng/u1	99
6) Benzaldehyde	7.122	77	313199	25.471	ng/u1	98
8) Phenol	7.169	94	472165	16.605	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.410	93	391724	17.626	ng/u1	97
12) 2-Chlorophenol	7.545	128	362889	18.385	ng/u1	100
13) 2-Methylphenol	8.428	108	365028	17.436	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.522	45	518113	17.628	ng/u1	99
16) Acetophenone	8.816	105	650886	19.099	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.798	70	334424	19.106	ng/u1	97
18) 4-Methylphenol	8.757	108	408900	17.690	ng/u1	98
19) Hexachloroethane	9.069	117	143696	18.139	ng/u1	97
22) Nitrobenzene	9.192	77	455826	18.050	ng/u1	98
23) Isophorone	9.728	82	917343	18.676	ng/u1	97
25) 2-Nitrophenol	9.910	139	204343	19.222	ng/u1	96
26) 2,4-Dimethylphenol	9.963	107	441946	18.304	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.204	93	568020	18.956	ng/u1	99
29) 2,4-Dichlorophenol	10.439	162	353771	19.011	ng/u1	99
30) Naphthalene	10.845	128	1278266	18.443	ng/u1	100
32) 4-Chloroaniline	10.957	127	575357	18.169	ng/u1	99
33) Hexachlorobutadiene	11.127	225	197324	18.968	ng/u1	99
34) Caprolactam	11.739	113	130902	19.420	ng/u1	92
35) 4-Chloro-3-methylphenol	12.074	107	415235	18.963	ng/u1	97
36) 2-Methylnaphthalene	12.451	142	885411	19.047	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092922\
 Data File : BM036802.D
 Acq On : 29 Sep 2022 15:30
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SICV032


Quant Time: Sep 30 01:56:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 30 01:50:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.669	142	852843	18.268	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.810	216	415467	18.658	ng/ul	99
40) Hexachlorocyclopentadiene	12.792	237	239141	18.672	ng/ul	98
41) 2,4,6-Trichlorophenol	13.051	196	271122	19.002	ng/ul	99
42) 2,4,5-Trichlorophenol	13.121	196	289695	18.482	ng/ul	98
43) 1,1'-Biphenyl	13.451	154	1205890	19.411	ng/ul	100
44) 2-Chloronaphthalene	13.492	162	874492	18.272	ng/ul	99
45) 2-Nitroaniline	13.698	65	278929	18.510	ng/ul	98
47) Dimethylphthalate	14.074	163	1136461	18.768	ng/ul	99
48) 2,6-Dinitrotoluene	14.192	165	232391	21.382	ng/ul	96
50) Acenaphthylene	14.333	152	1452180	19.308	ng/ul	99
51) 3-Nitroaniline	14.515	138	268988	20.505	ng/ul	98
52) Acenaphthene	14.674	153	977724	18.112	ng/ul	99
53) 2,4-Dinitrophenol	14.721	184	105239	15.655	ng/ul	93
55) 4-Nitrophenol	14.815	109	176194	17.345	ng/ul	96
56) Dibenzofuran	15.010	168	1371720	19.104	ng/ul	97
57) 2,4-Dinitrotoluene	14.968	165	307884	19.273	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.233	232	251240	19.534	ng/ul	93
59) Diethylphthalate	15.427	149	1143365	18.532	ng/ul	99
61) Fluorene	15.657	166	1135171	18.613	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.651	204	521030	18.567	ng/ul	97
63) 4-Nitroaniline	15.674	138	285910	23.163	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.727	198	163105	16.448	ng/ul	99
67) N-Nitrosodiphenylamine	15.862	169	954966	18.657	ng/ul	99
68) 4-Bromophenyl-phenylether	16.539	248	289948	18.488	ng/ul	99
69) Hexachlorobenzene	16.651	284	333196	18.360	ng/ul	99
70) Atrazine	16.809	200	324916	18.235	ng/ul	99
71) Pentachlorophenol	16.998	266	194576	16.846	ng/ul	97
72) Phenanthrene	17.392	178	1738442	17.984	ng/ul	100
74) Anthracene	17.480	178	1776809	18.397	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.416	216	407745	18.094	ng/ul	100
76) Pentachlorobenzene	14.927	250	410272	17.292	ng/ul	98
77) Carbazole	17.751	167	1679966	18.620	ng/ul	99
78) Di-n-butylphthalate	18.315	149	1940546	18.536	ng/ul	100
80) Fluoranthene	19.397	202	1948789	18.372	ng/ul	99
82) Pyrene	19.762	202	2101651	18.470	ng/ul	96
83) Butylbenzylphthalate	20.656	149	836593	18.005	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.433	252	788534	20.617	ng/ul	98
85) Benzo(a)anthracene	21.497	228	2026208	18.148	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.427	149	1317877	18.597	ng/ul	99
87) Chrysene	21.556	228	1906002	18.097	ng/ul	100
89) Di-n-octyl phthalate	22.362	149	2077295	17.022	ng/ul	100
90) Benzo(b)fluoranthene	23.197	252	2045812	17.920	ng/ul	99
91) Benzo(k)fluoranthene	23.244	252	2019361	18.313	ng/ul	99
93) Benzo(a)pyrene	23.827	252	1815449	18.266	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.450	276	2223968	18.883	ng/ul	98
95) Dibenzo(a,h)anthracene	26.473	278	1952215	18.226	ng/ul	99
96) Benzo(g,h,i)perylene	27.226	276	1884068	18.308	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 30 01:56:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 30 01:50:26 2022
Response via : Initial Calibration




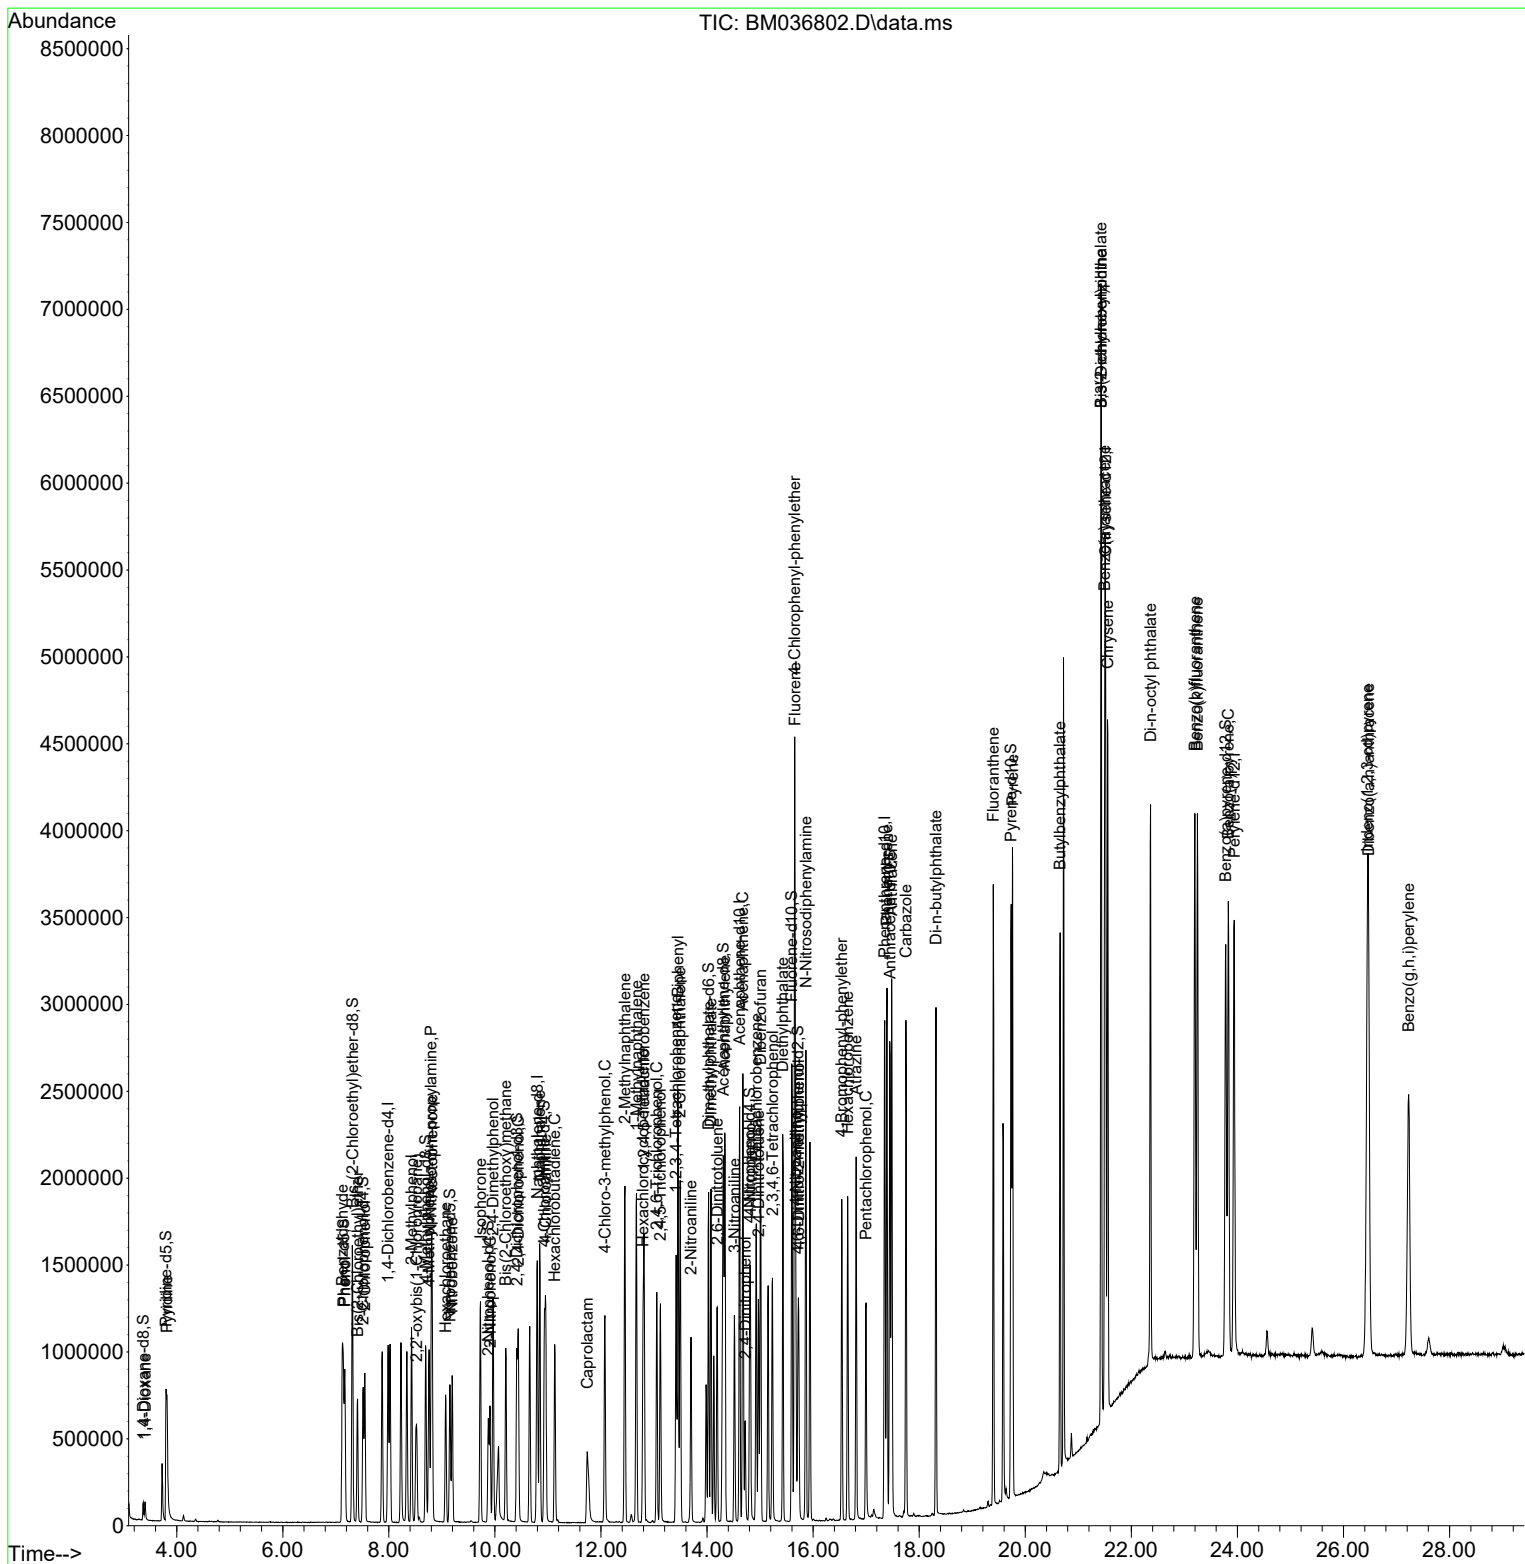




#2
1,4-Dioxane
Concen: 7.018 ng/uL
RT: 3.404 min Scan# 54
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion: 88 Resp: 54070
Ion Ratio Lower Upper
88 100
43 25.5 21.5 32.3
58 71.2 55.5 83.3

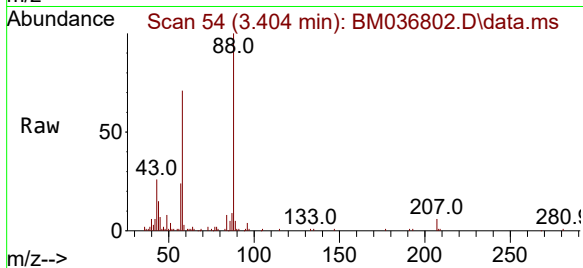

#5
Pyridine
Concen: 15.420 ng/uL
RT: 3.816 min Scan# 124
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion: 79 Resp: 348724
Ion Ratio Lower Upper
79 100
52 73.1 57.6 86.4
51 33.4 26.9 40.3




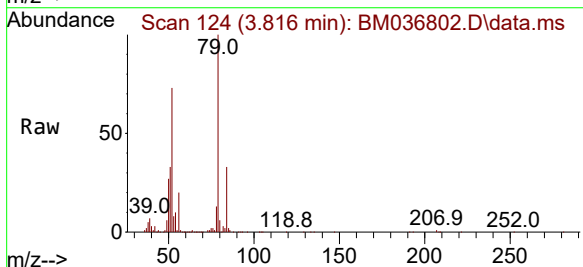


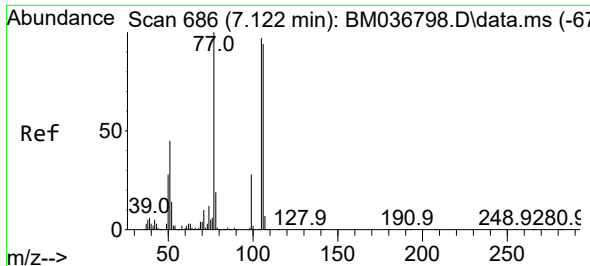

#6
Benzaldehyde
Concen: 25.471 ng/ul
RT: 7.122 min Scan# 686
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion: 77 Resp: 313199
Ion Ratio Lower Upper
77 100
105 99.3 77.2 115.8
106 94.9 74.7 112.1

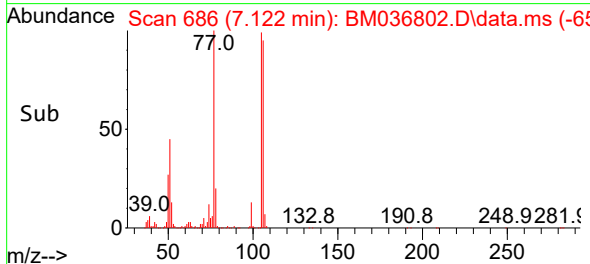

#8
Phenol
Concen: 16.605 ng/ul
RT: 7.169 min Scan# 694
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion: 94 Resp: 472165
Ion Ratio Lower Upper
94 100
65 27.8 23.0 34.4
66 35.2 29.1 43.7


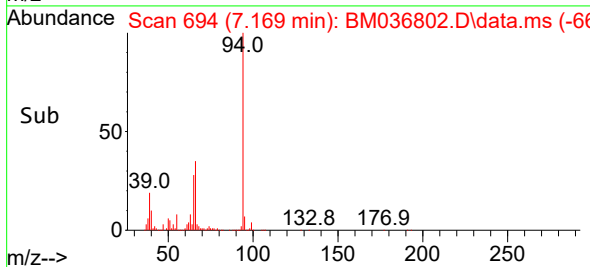

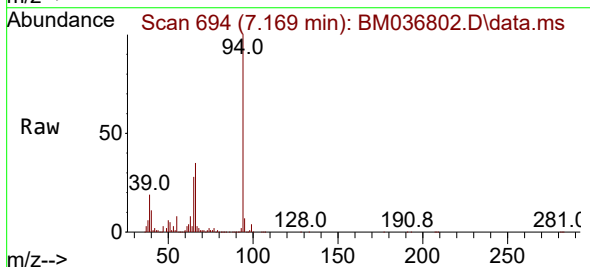




#10
Bis(2-Chloroethyl)ether
Concen: 17.626 ng/ul
RT: 7.410 min Scan# 735
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion: 93 Resp: 391724
Ion Ratio Lower Upper
93 100
63 74.9 62.7 94.1
95 31.9 25.4 38.2



#12
2-Chlorophenol
Concen: 18.385 ng/ul
RT: 7.545 min Scan# 758
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:128 Resp: 362889
Ion Ratio Lower Upper
128 100
64 49.0 39.1 58.7
130 32.3 25.6 38.4





#13

2-Methylphenol

Concen: 17.436 ng/ul

RT: 8.428 min Scan# 908

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :





SICV032

Tgt Ion:108 Resp: 365028

Ion Ratio Lower Upper

108 100

107 85.7 69.2 103.8



#14

2,2'-oxybis(1-Chloropropane)

Concen: 17.628 ng/ul

RT: 8.522 min Scan# 924

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30




Tgt Ion: 45 Resp: 518113


Ion Ratio Lower Upper

45 100

77 15.6 12.4 18.6

79 12.3 9.3 13.9









#16
Acetophenone
Concen: 19.099 ng/ul
RT: 8.816 min Scan# 974
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:105 Resp: 650886
Ion Ratio Lower Upper
105 100
77 77.6 62.7 94.1
51 26.0 21.2 31.8

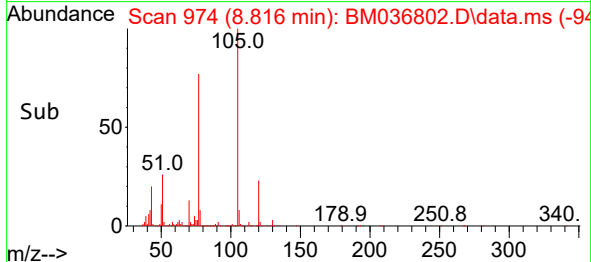

#17
N-Nitroso-di-n-propylamine
Concen: 19.106 ng/ul
RT: 8.798 min Scan# 971
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion: 70 Resp: 334424
Ion Ratio Lower Upper
70 100
42 52.1 44.2 66.2
101 9.3 7.3 10.9
130 19.6 15.0 22.6

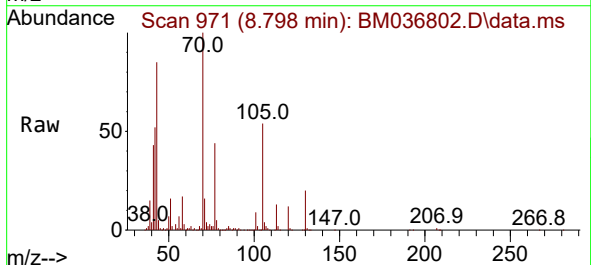



#18

4-Methylphenol

Concen: 17.690 ng/ul

RT: 8.757 min Scan# 964

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :





SICV032

Tgt Ion:108 Resp: 408900

Ion Ratio Lower Upper

108 100

107 108.9 88.5 132.7

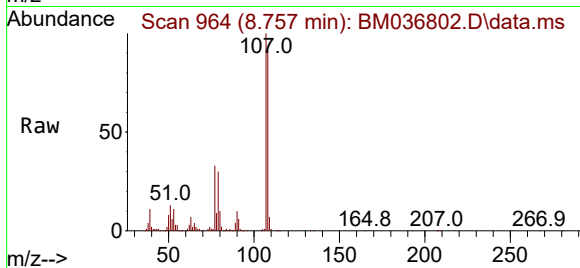

#19

Hexachloroethane

Concen: 18.139 ng/ul

RT: 9.069 min Scan# 1017

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30




Tgt Ion:117 Resp: 143696


Ion Ratio Lower Upper

117 100

201 89.7 68.3 102.5

199 54.9 43.8 65.6




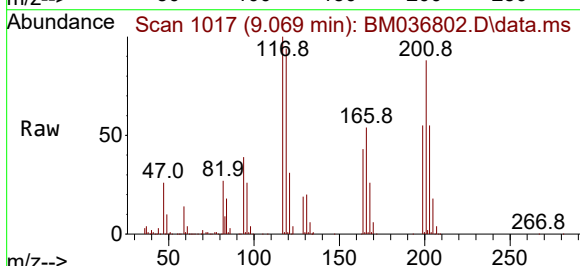




#22
 Nitrobenzene
 Concen: 18.050 ng/ul
 RT: 9.192 min Scan# 1038
 Delta R.T. 0.000 min
 Lab File: BM036802.D
 Acq: 29 Sep 2022 15:30




Instrument :
 BNA_M
 ClientSampleId :
 SICV032


Tgt Ion: 77 Resp: 455826
 Ion Ratio Lower Upper
 77 100
 123 43.9 34.3 51.5
 65 12.8 10.9 16.3

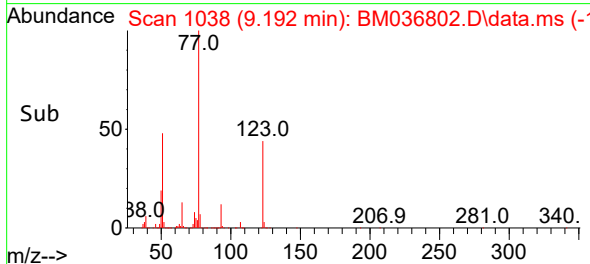

#23
 Isophorone
 Concen: 18.676 ng/ul
 RT: 9.728 min Scan# 1129
 Delta R.T. 0.006 min
 Lab File: BM036802.D
 Acq: 29 Sep 2022 15:30

Tgt Ion: 82 Resp: 917343
 Ion Ratio Lower Upper
 82 100
 95 6.9 5.0 7.4
 138 17.4 12.9 19.3


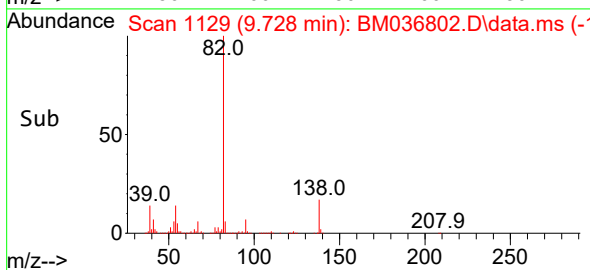

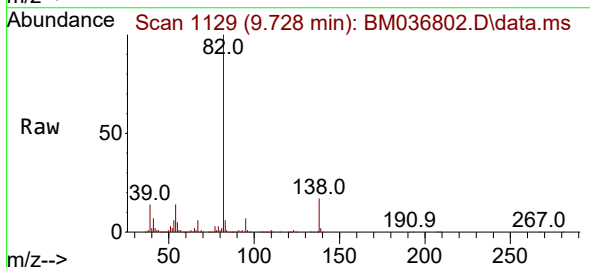


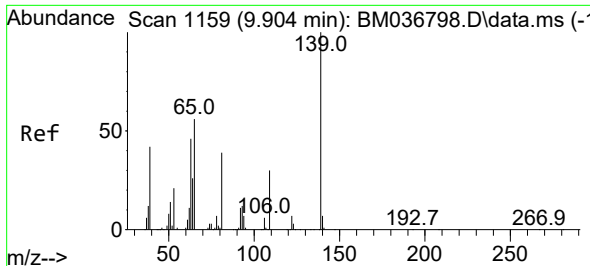

#25
2-Nitrophenol
Concen: 19.222 ng/ul
RT: 9.910 min Scan# 1160
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:139 Resp: 204343
Ion Ratio Lower Upper
139 100
65 52.9 46.0 69.0
109 30.0 24.2 36.2

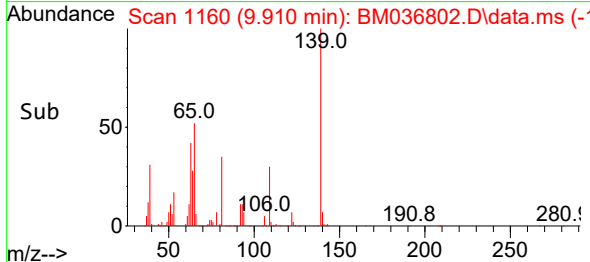

#26
2,4-Dimethylphenol
Concen: 18.304 ng/ul
RT: 9.963 min Scan# 1169
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:107 Resp: 441946
Ion Ratio Lower Upper
107 100
121 49.5 41.4 62.0
122 85.8 71.1 106.7


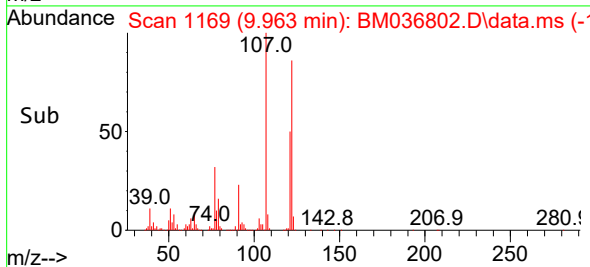

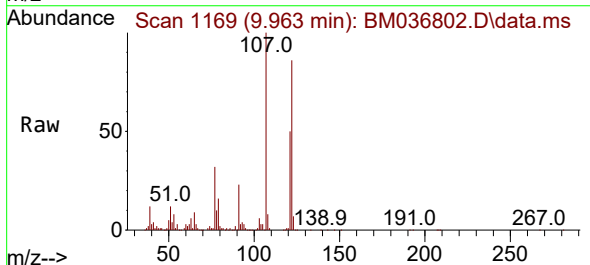


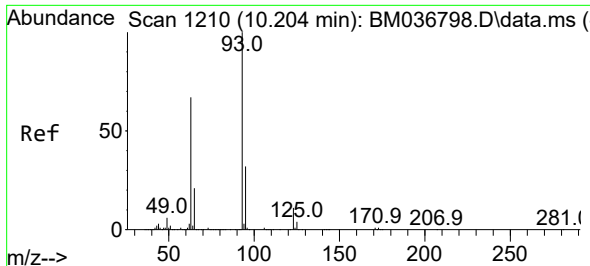

#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.956 ng/ul
 RT: 10.204 min Scan# 1210
 Delta R.T. 0.000 min
 Lab File: BM036802.D
 Acq: 29 Sep 2022 15:30




Instrument :
 BNA_M
 ClientSampleId :
 SICV032


Tgt Ion: 93 Resp: 568020
 Ion Ratio Lower Upper
 93 100
 95 32.5 25.6 38.4
 123 11.1 8.6 12.8

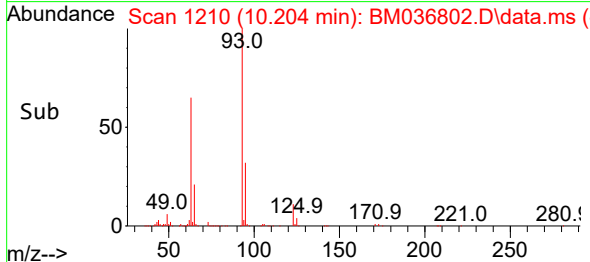

#29
 2,4-Dichlorophenol
 Concen: 19.011 ng/ul
 RT: 10.439 min Scan# 1250
 Delta R.T. 0.000 min
 Lab File: BM036802.D
 Acq: 29 Sep 2022 15:30

Tgt Ion: 162 Resp: 353771
 Ion Ratio Lower Upper
 162 100
 164 65.3 51.8 77.6
 98 37.6 30.9 46.3


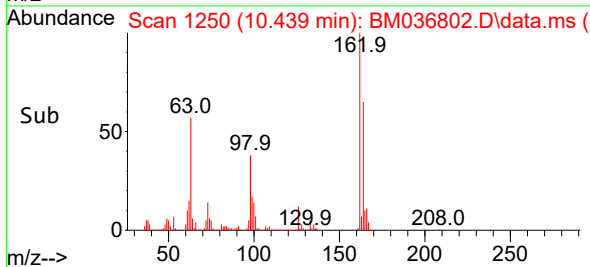

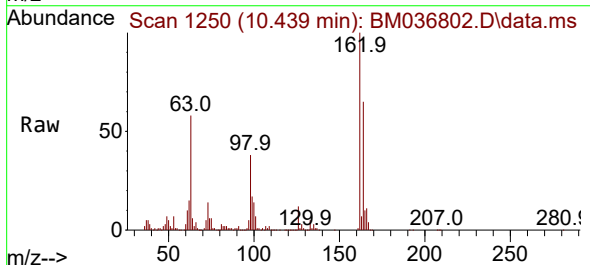


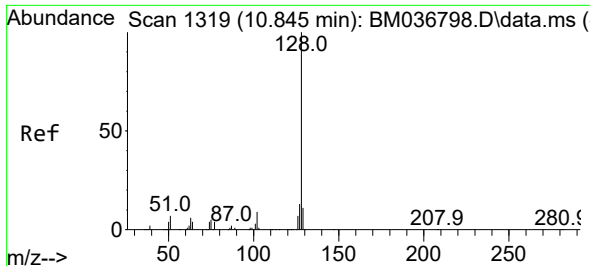

#30
Naphthalene
Concen: 18.443 ng/ul
RT: 10.845 min Scan# 1319
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:128 Resp: 1278266
Ion Ratio Lower Upper
128 100
129 10.9 8.6 12.8
127 12.8 10.4 15.6

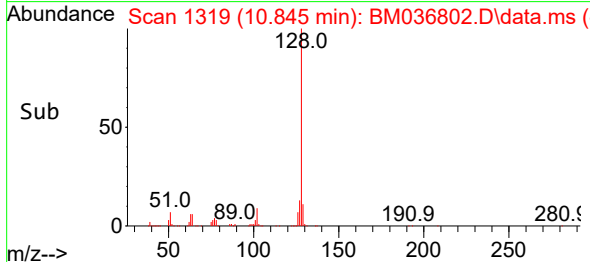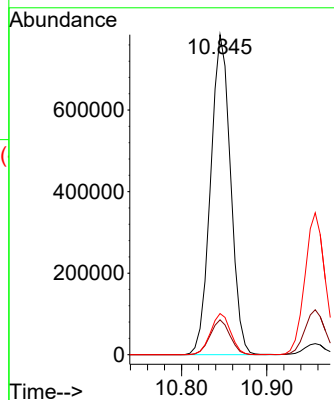

#32
4-Chloroaniline
Concen: 18.169 ng/ul
RT: 10.957 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:127 Resp: 575357
Ion Ratio Lower Upper
127 100
129 31.6 25.7 38.5


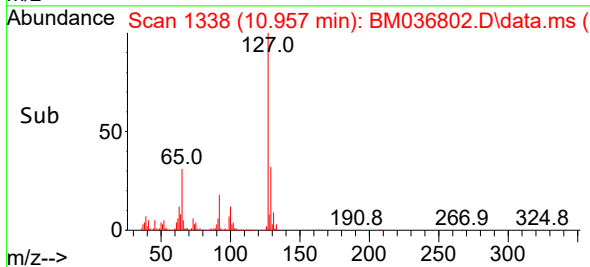
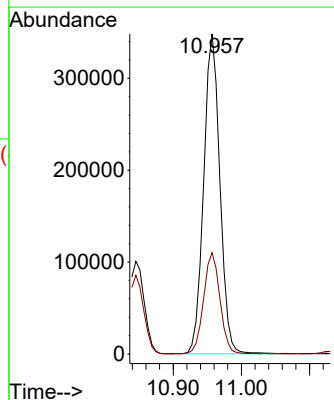
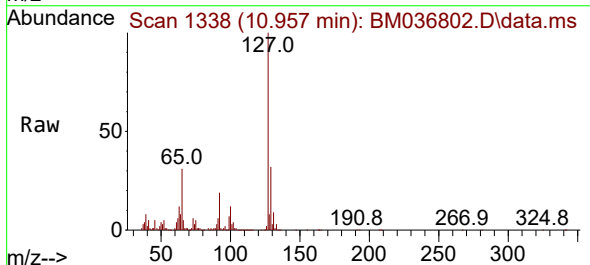




#33
Hexachlorobutadiene
Concen: 18.968 ng/ul
RT: 11.127 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:225 Resp: 197324
Ion Ratio Lower Upper
225 100
223 61.8 50.0 75.0
227 61.7 50.4 75.6



#34
Caprolactam
Concen: 19.420 ng/ul
RT: 11.739 min Scan# 1471
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:113 Resp: 130902
Ion Ratio Lower Upper
113 100
55 164.5 138.6 208.0
56 119.7 105.9 158.9




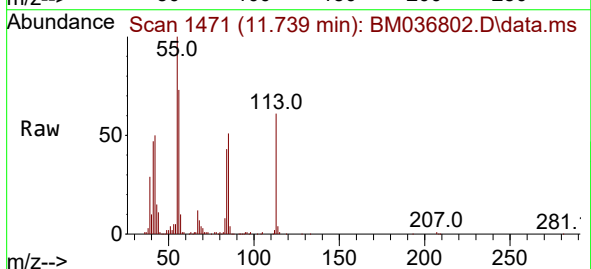




#35
4-Chloro-3-methylphenol
Concen: 18.963 ng/ul
RT: 12.074 min Scan# 1528
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:107 Resp: 415235
Ion Ratio Lower Upper
107 100
144 26.6 20.2 30.4
142 79.0 61.3 91.9

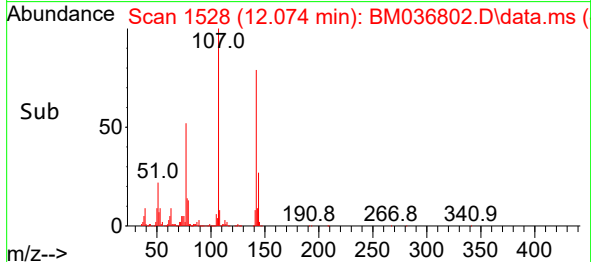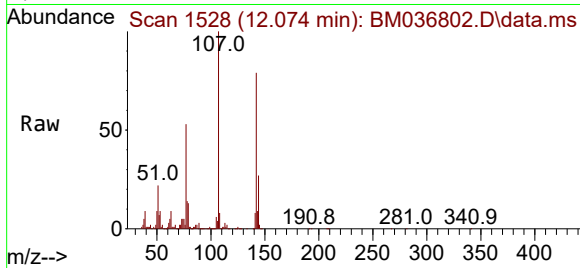

#36
2-Methylnaphthalene
Concen: 19.047 ng/ul
RT: 12.451 min Scan# 1592
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:142 Resp: 885411
Ion Ratio Lower Upper
142 100
141 89.8 71.4 107.2

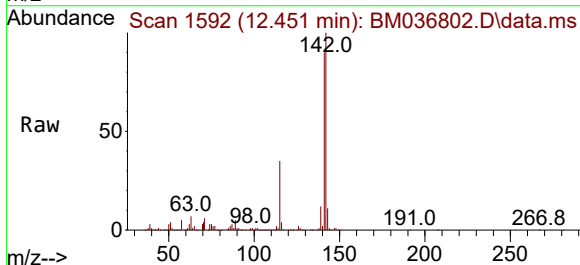



#37

1-Methylnaphthalene

Concen: 18.268 ng/ul

RT: 12.669 min Scan# 1629

Delta R.T. 0.006 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:142 Resp: 852843

Ion Ratio Lower Upper

142 100

141 92.1 73.4 110.2

116 3.7 3.1 4.7

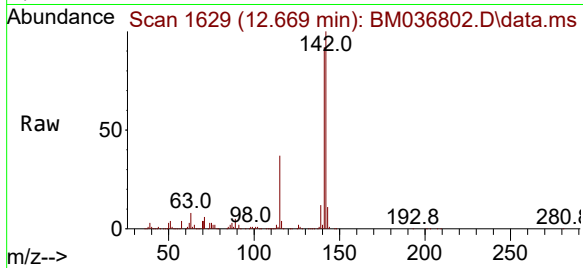

#39

1,2,4,5-Tetrachlorobenzene

Concen: 18.658 ng/ul

RT: 12.810 min Scan# 1653

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Tgt Ion:216 Resp: 415467




Ion Ratio Lower Upper


216 100

214 79.3 63.4 95.0

179 21.4 17.5 26.3

108 20.4 17.3 25.9



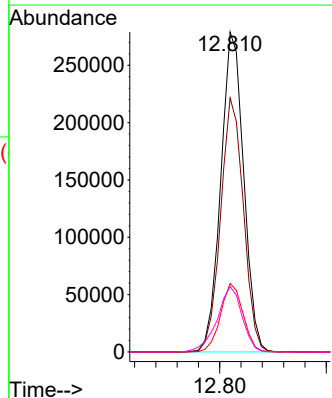
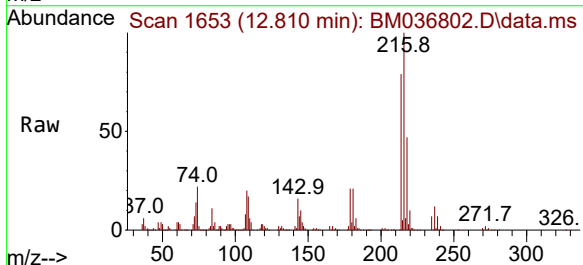




#40
Hexachlorocyclopentadiene
Concen: 18.672 ng/ul
RT: 12.792 min Scan# 1650
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:237 Resp: 239141
Ion Ratio Lower Upper
237 100
235 64.2 49.8 74.6
272 13.5 10.3 15.5

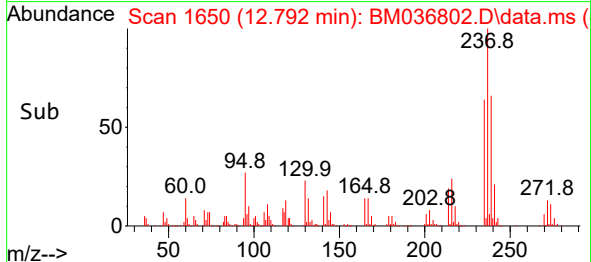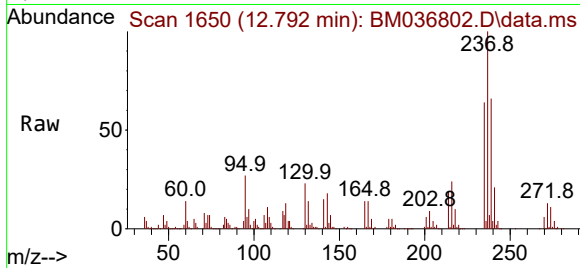

#41
2,4,6-Trichlorophenol
Concen: 19.002 ng/ul
RT: 13.051 min Scan# 1694
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:196 Resp: 271122
Ion Ratio Lower Upper
196 100
198 95.3 77.0 115.4
200 30.8 24.6 37.0




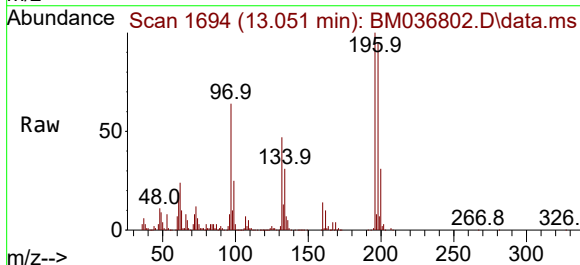




#42
2,4,5-Trichlorophenol
Concen: 18.482 ng/ul
RT: 13.121 min Scan# 1705
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:196 Resp: 289695
Ion Ratio Lower Upper
196 100
198 97.9 76.4 114.6
200 31.5 24.2 36.2

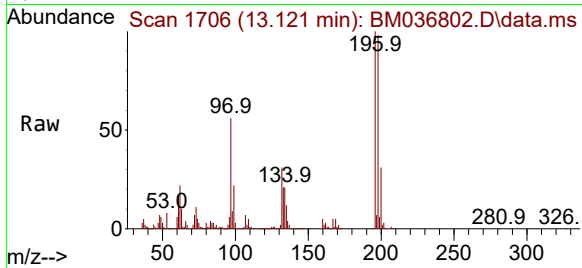

#43
1,1'-Biphenyl
Concen: 19.411 ng/ul
RT: 13.451 min Scan# 1762
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:154 Resp: 1205890
Ion Ratio Lower Upper
154 100
153 40.1 31.9 47.9
76 14.1 11.4 17.2




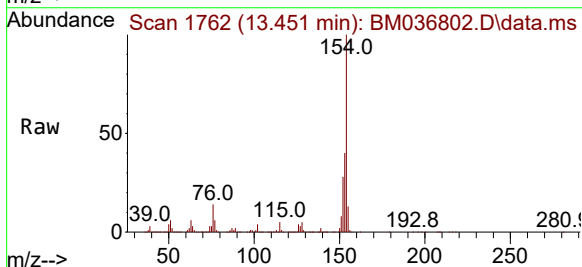




#44
2-Chloronaphthalene
Concen: 18.272 ng/ul
RT: 13.492 min Scan# 1769
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:162 Resp: 874492
Ion Ratio Lower Upper
162 100
164 33.0 25.7 38.5
127 41.1 32.5 48.7

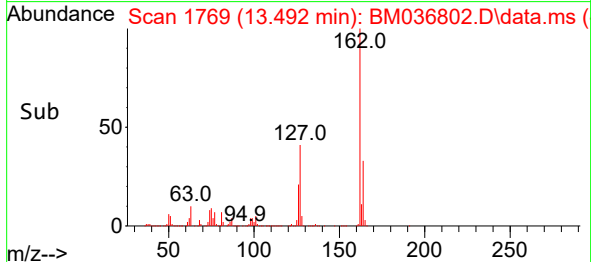

#45
2-Nitroaniline
Concen: 18.510 ng/ul
RT: 13.698 min Scan# 1804
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion: 65 Resp: 278929
Ion Ratio Lower Upper
65 100
92 69.8 53.5 80.3
138 101.8 81.4 122.0

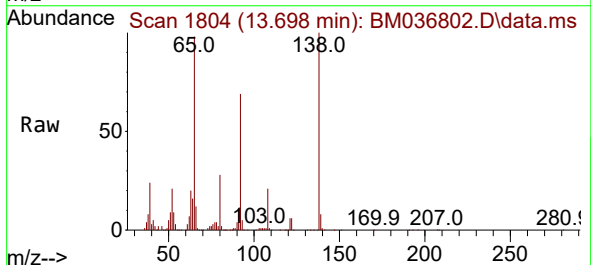



#47

Dimethylphthalate

Concen: 18.768 ng/ul

RT: 14.074 min Scan# 1868

Delta R.T. 0.006 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:163 Resp: 1136461

Ion Ratio Lower Upper

163 100

194 4.0 3.0 4.6

164 9.8 8.2 12.4

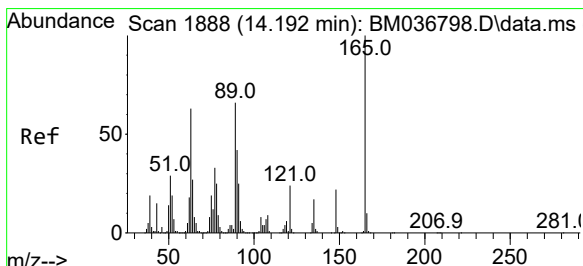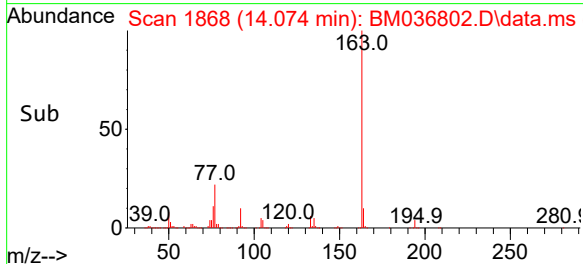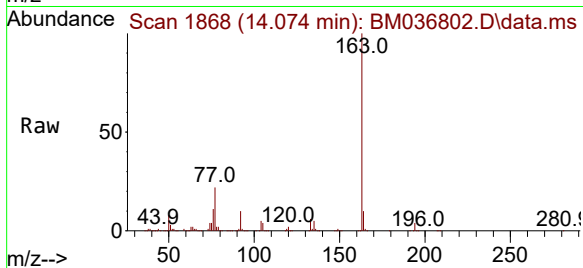

#48

2,6-Dinitrotoluene

Concen: 21.382 ng/ul

RT: 14.192 min Scan# 1888

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30




Tgt Ion:165 Resp: 232391


Ion Ratio Lower Upper

165 100

89 63.2 53.0 79.4

121 22.2 19.0 28.4


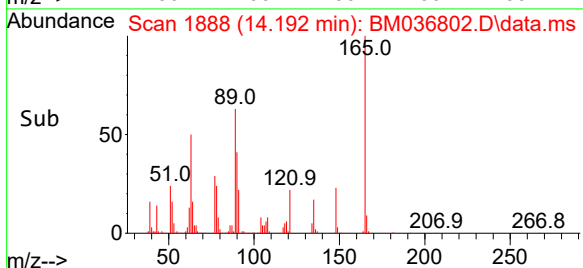
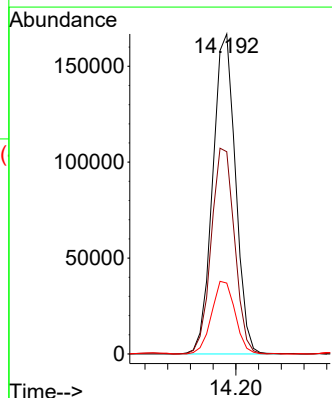
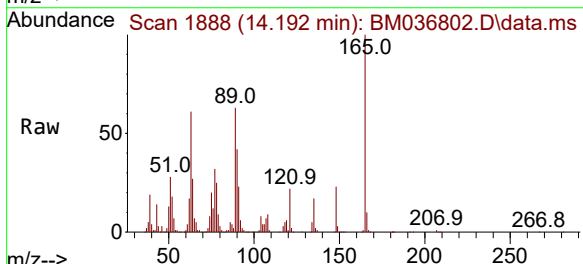




#50
Acenaphthylene
Concen: 19.308 ng/ul
RT: 14.333 min Scan# 1912
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:152 Resp: 1452180
Ion Ratio Lower Upper
152 100
151 19.6 16.0 24.0
153 13.2 10.4 15.6

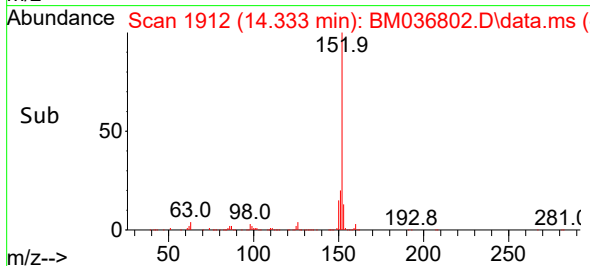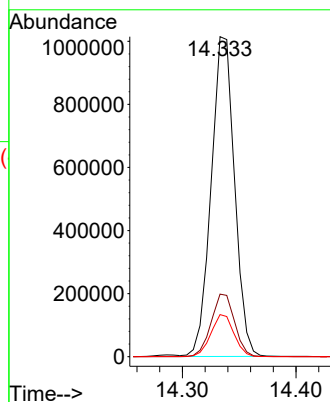

#51
3-Nitroaniline
Concen: 20.505 ng/ul
RT: 14.515 min Scan# 1943
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:138 Resp: 268988
Ion Ratio Lower Upper
138 100
108 10.6 8.6 12.8
92 119.6 97.7 146.5


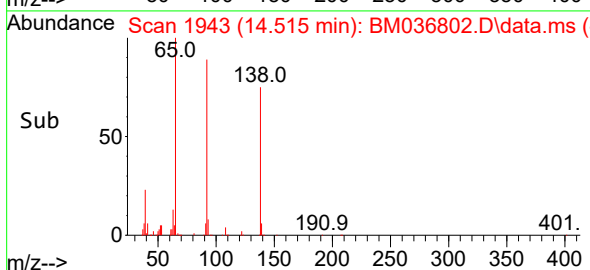

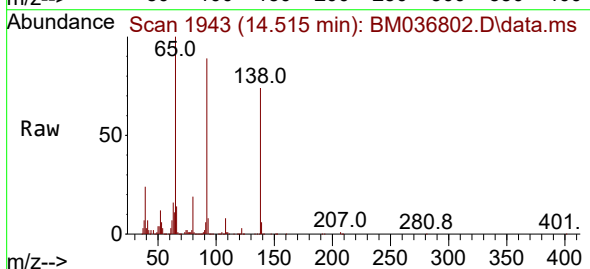




#52
Acenaphthene
Concen: 18.112 ng/ul
RT: 14.674 min Scan# 1970
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:153 Resp: 977724
Ion Ratio Lower Upper
153 100
152 47.9 38.6 58.0
154 89.0 70.6 105.8

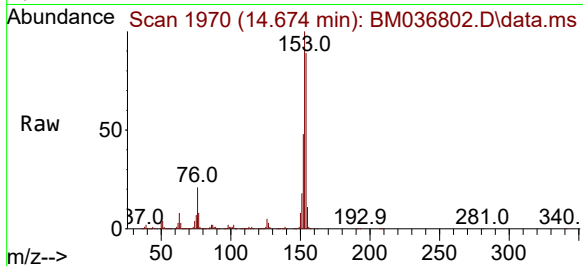

#53
2,4-Dinitrophenol
Concen: 15.655 ng/ul
RT: 14.721 min Scan# 1978
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:184 Resp: 105239
Ion Ratio Lower Upper
184 100
63 76.1 69.2 103.8
154 64.1 51.9 77.9




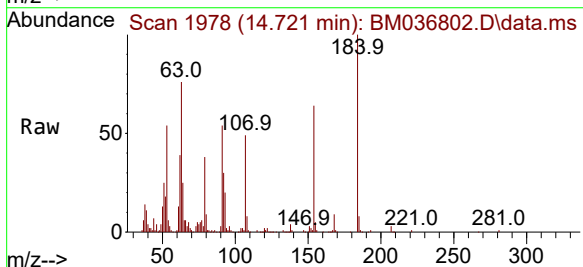




#55
4-Nitrophenol
Concen: 17.345 ng/ul
RT: 14.815 min Scan# 1994
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:109 Resp: 176194
Ion Ratio Lower Upper
109 100
139 137.4 104.7 157.1
65 145.5 113.8 170.6



#56
Dibenzofuran
Concen: 19.104 ng/ul
RT: 15.010 min Scan# 2027
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:168 Resp: 1371720
Ion Ratio Lower Upper
168 100
139 37.8 31.6 47.4





#57

2,4-Dinitrotoluene

Concen: 19.273 ng/ul

RT: 14.968 min Scan# 20

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:165 Resp: 307884

Ion Ratio Lower Upper

165 100

63 50.3 42.2 63.4

182 2.5 2.2 3.4

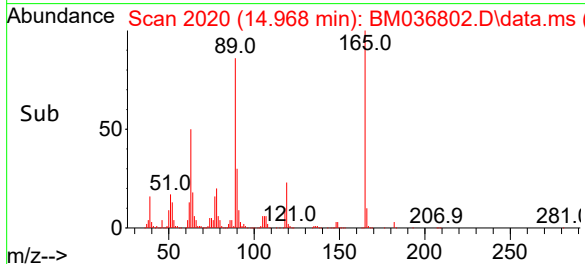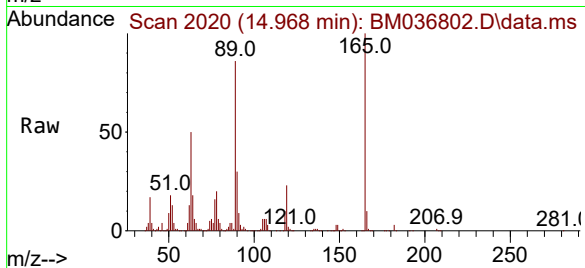

#58

2,3,4,6-Tetrachlorophenol

Concen: 19.534 ng/ul

RT: 15.233 min Scan# 2065

Delta R.T. 0.006 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Tgt Ion:232 Resp: 251240




Ion Ratio Lower Upper


232 100

131 50.8 46.2 69.2

130 2.5 2.2 3.4

166 32.5 27.8 41.8


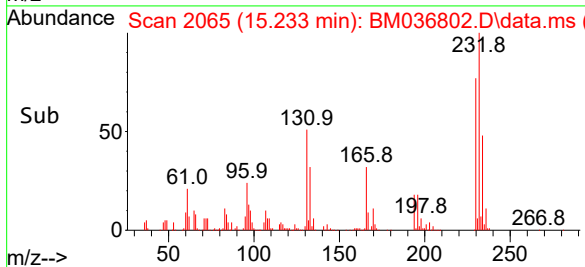

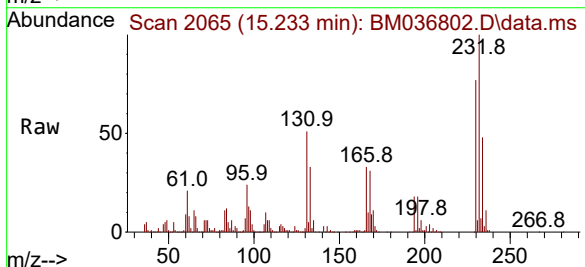




#59
Diethylphthalate
Concen: 18.532 ng/ul
RT: 15.427 min Scan# 2098
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:149 Resp: 1143365
Ion Ratio Lower Upper
149 100
177 20.6 16.9 25.3
150 12.2 10.0 15.0

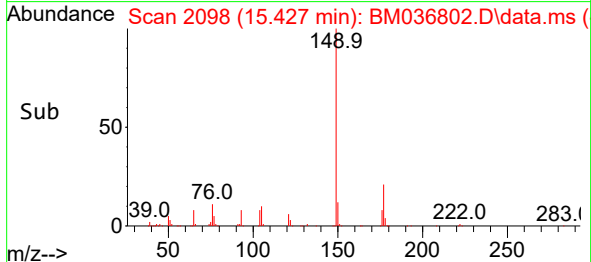

#61
Fluorene
Concen: 18.613 ng/ul
RT: 15.657 min Scan# 2137
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:166 Resp: 1135171
Ion Ratio Lower Upper
166 100
165 97.5 77.7 116.5
167 13.2 10.6 16.0





#62

4-Chlorophenyl-phenylether

Concen: 18.567 ng/ul

RT: 15.651 min Scan# 2135

Delta R.T. 0.006 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:204 Resp: 521030

Ion Ratio Lower Upper

204 100

206 32.9 25.8 38.6

141 62.4 52.4 78.6

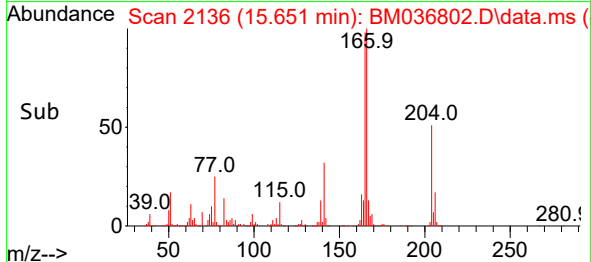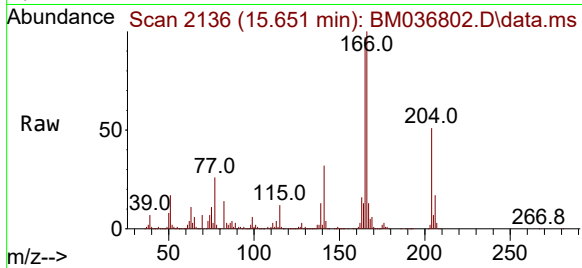

#63

4-Nitroaniline

Concen: 23.163 ng/ul

RT: 15.674 min Scan# 2140

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30




Tgt Ion:138 Resp: 285910


Ion Ratio Lower Upper

138 100

92 51.7 44.3 66.5

108 75.9 64.2 96.4


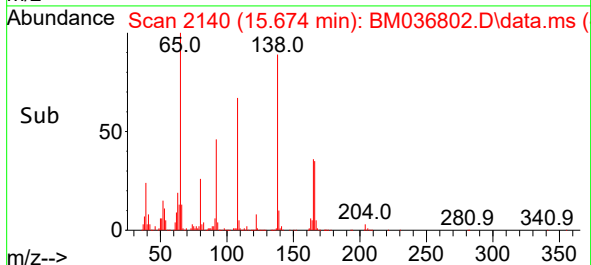
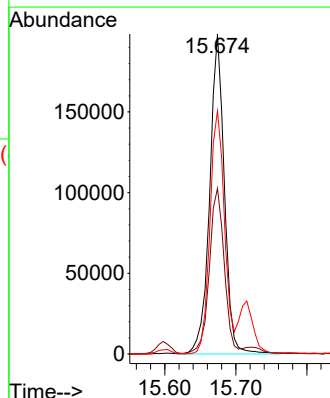
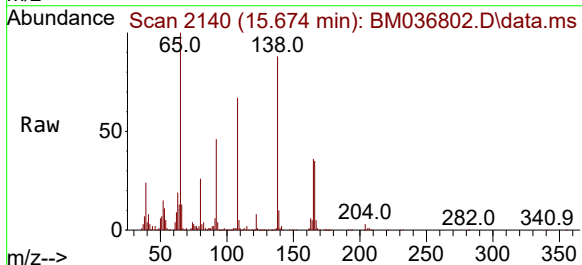




#66
 4,6-Dinitro-2-methylphenol
 Concen: 16.448 ng/ul
 RT: 15.727 min Scan# 2149
 Delta R.T. 0.000 min
 Lab File: BM036802.D
 Acq: 29 Sep 2022 15:30




Instrument :
 BNA_M
 ClientSampleId :
 SICV032


Tgt Ion:198 Resp: 163105
 Ion Ratio Lower Upper
 198 100
 182 5.8 4.6 7.0
 77 31.4 25.7 38.5

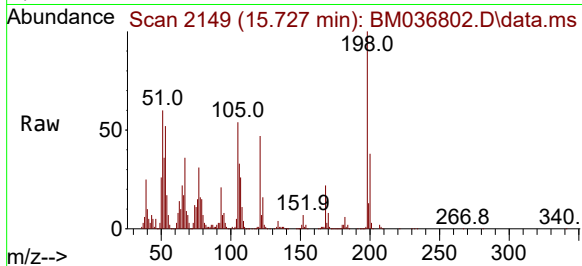

#67
 N-Nitrosodiphenylamine
 Concen: 18.657 ng/ul
 RT: 15.862 min Scan# 2172
 Delta R.T. 0.000 min
 Lab File: BM036802.D
 Acq: 29 Sep 2022 15:30

Tgt Ion:169 Resp: 954966
 Ion Ratio Lower Upper
 169 100
 168 66.9 54.3 81.5
 167 36.6 29.7 44.5




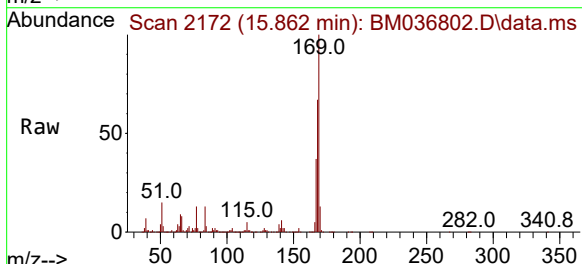




#68
4-Bromophenyl-phenylether
Concen: 18.488 ng/ul
RT: 16.539 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:248 Resp: 289948
Ion Ratio Lower Upper
248 100
250 97.3 77.1 115.7
141 86.9 69.9 104.9



#69
Hexachlorobenzene
Concen: 18.360 ng/ul
RT: 16.651 min Scan# 2306
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:284 Resp: 333196
Ion Ratio Lower Upper
284 100
142 39.8 32.5 48.7
249 30.6 23.8 35.8





#70

Atrazine

Concen: 18.235 ng/ul

RT: 16.809 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:200 Resp: 324916

Ion Ratio Lower Upper

200 100

173 27.7 22.5 33.7

215 47.4 38.5 57.7

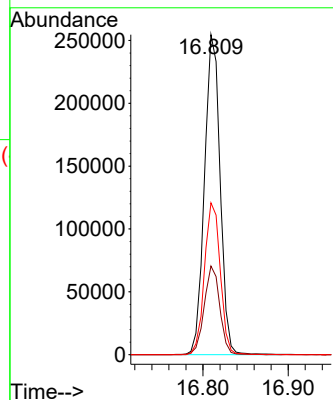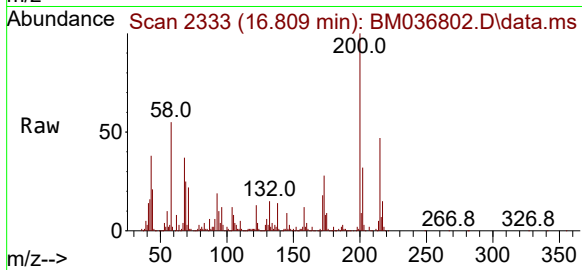

#71

Pentachlorophenol

Concen: 16.846 ng/ul

RT: 16.998 min Scan# 2365

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30




Tgt Ion:266 Resp: 194576


Ion Ratio Lower Upper

266 100

264 64.1 48.7 73.1

268 64.1 50.5 75.7



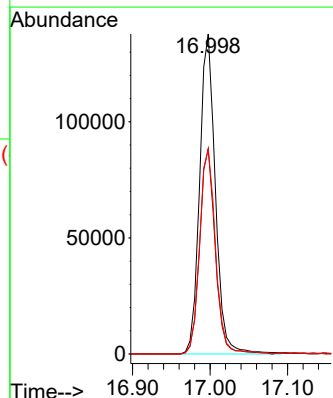
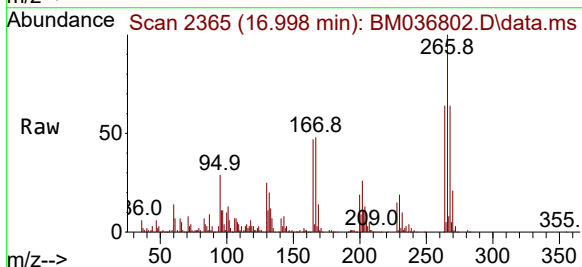




#72
Phenanthrene
Concen: 17.984 ng/ul
RT: 17.392 min Scan# 2432
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:178 Resp: 1738442
Ion Ratio Lower Upper
178 100
179 14.9 12.1 18.1
176 19.4 15.5 23.3

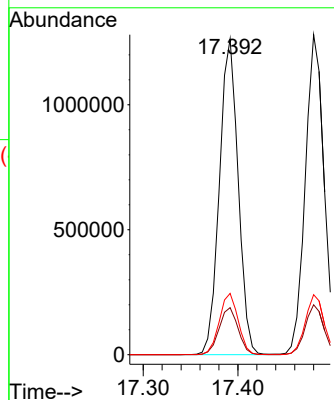

#74
Anthracene
Concen: 18.397 ng/ul
RT: 17.480 min Scan# 2447
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:178 Resp: 1776809
Ion Ratio Lower Upper
178 100
179 15.6 12.6 18.8
176 18.8 15.1 22.7



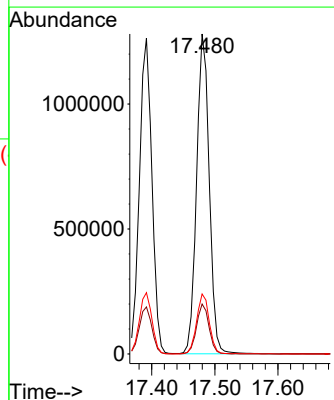





#75
1,2,3,4-Tetrachlorobenzene
Concen: 18.094 ng/uL
RT: 13.416 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:216 Resp: 407745
Ion Ratio Lower Upper
216 100
214 78.6 62.6 93.8
218 47.7 38.2 57.4

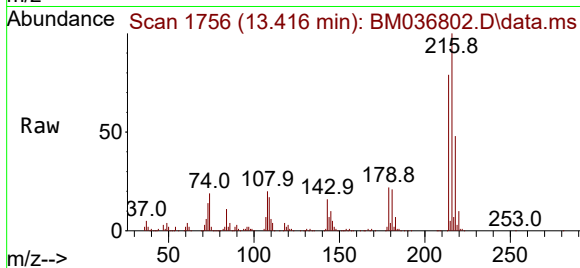

#76
Pentachlorobenzene
Concen: 17.292 ng/uL
RT: 14.927 min Scan# 2013
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:250 Resp: 410272
Ion Ratio Lower Upper
250 100
248 62.7 51.8 77.6
252 64.6 52.1 78.1

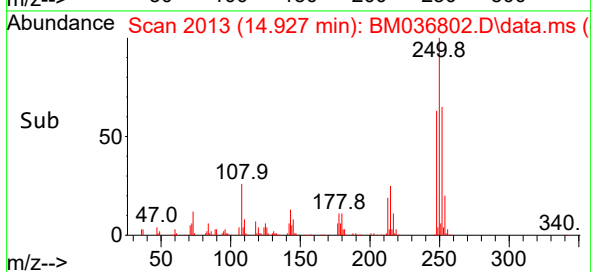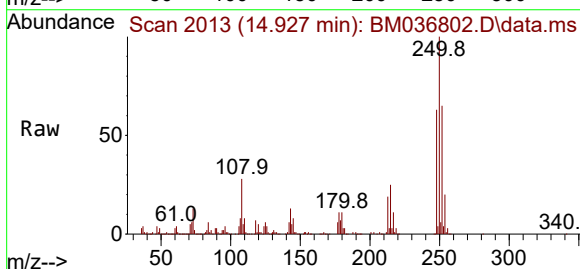



#77

Carbazole

Concen: 18.620 ng/ul

RT: 17.751 min Scan# 2493

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :





BNA_M

ClientSampleId :

SICV032

Tgt Ion:167 Resp: 1679966

Ion	Ratio	Lower	Upper
167	100		
166	21.2	17.4	26.0
139	13.3	10.8	16.2

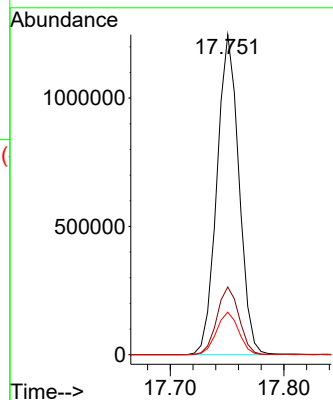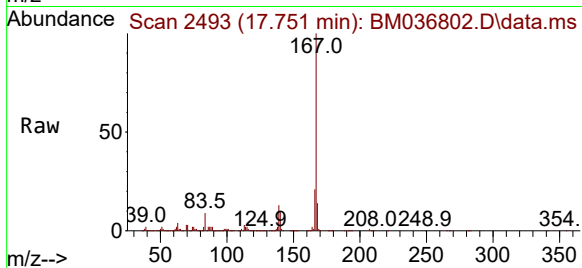

#78

Di-n-butylphthalate

Concen: 18.536 ng/ul

RT: 18.315 min Scan# 2589




Delta R.T. 0.000 min


Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Tgt Ion:149 Resp: 1940546

Ion	Ratio	Lower	Upper
149	100		
150	9.1	7.3	10.9
104	5.3	4.5	6.7


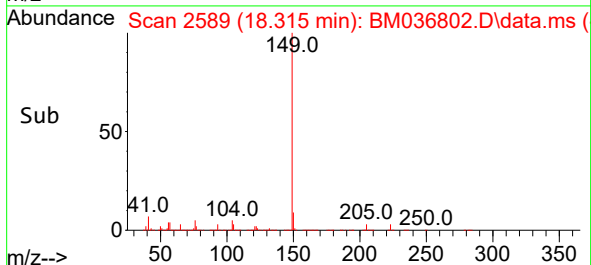
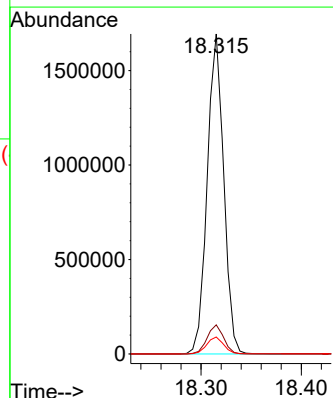
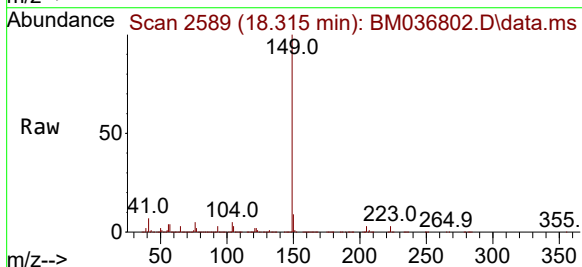


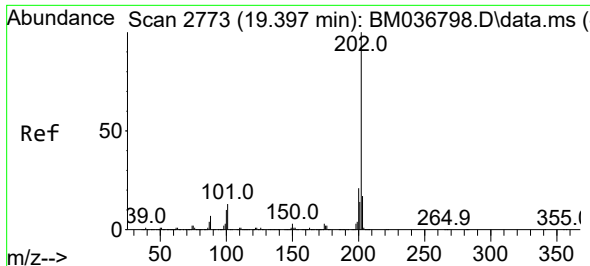

#80
Fluoranthene
Concen: 18.372 ng/ul
RT: 19.397 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:202 Resp: 1948789
Ion Ratio Lower Upper
202 100
101 12.9 10.5 15.7
100 9.6 8.2 12.2

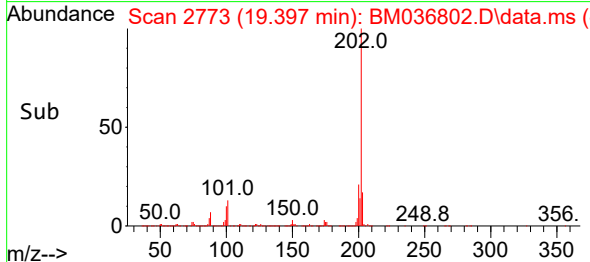

#82
Pyrene
Concen: 18.470 ng/ul
RT: 19.762 min Scan# 2835
Delta R.T. 0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:202 Resp: 2101651
Ion Ratio Lower Upper
202 100
101 14.1 12.6 19.0
100 11.8 10.5 15.7

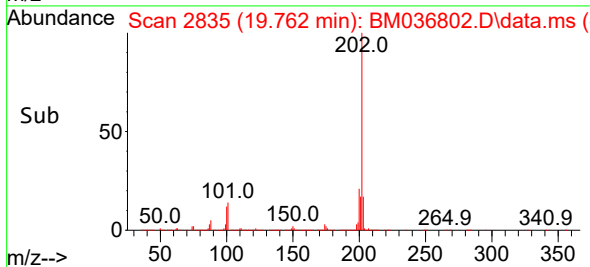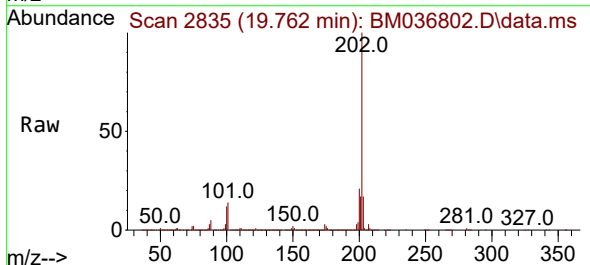



#83

Butylbenzylphthalate

Concen: 18.005 ng/ul

RT: 20.656 min Scan# 2987

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:149 Resp: 836593

Ion Ratio Lower Upper

149 100

91 76.8 61.8 92.8

206 19.3 15.0 22.6

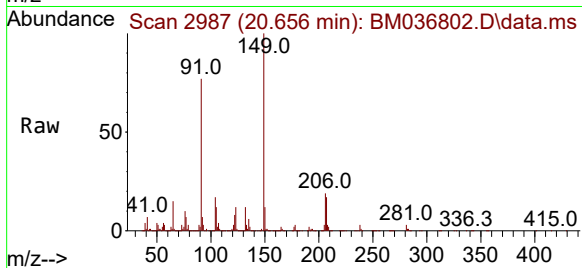

#84

3,3'-Dichlorobenzidine

Concen: 20.617 ng/ul

RT: 21.433 min Scan# 3119

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30




Tgt Ion:252 Resp: 788534


Ion Ratio Lower Upper

252 100

254 63.6 51.8 77.8

126 13.4 11.5 17.3

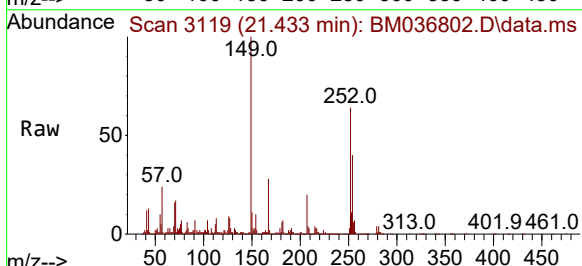



#85

Benzo(a)anthracene

Concen: 18.148 ng/ul

RT: 21.497 min Scan# 31

Delta R.T. -0.006 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:228 Resp: 2026208

Ion Ratio Lower Upper

228 100

229 19.8 15.8 23.8

226 27.4 22.1 33.1



#86

Bis(2-ethylhexyl)phthalate

Concen: 18.597 ng/ul

RT: 21.427 min Scan# 3118

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30




Tgt Ion:149 Resp: 1317877


Ion Ratio Lower Upper

149 100

167 27.2 21.4 32.2

279 3.4 2.5 3.7





#87

Chrysene

Concen: 18.097 ng/ul

RT: 21.556 min Scan# 3140

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:228 Resp: 1906002

Ion Ratio Lower Upper

228 100

226 30.4 24.3 36.5

229 19.8 15.8 23.6



#89

Di-n-octyl phthalate

Concen: 17.022 ng/ul




RT: 22.362 min Scan# 3277


Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Tgt Ion:149 Resp: 2077295









#90
Benzo(b)fluoranthene
Concen: 17.920 ng/ul
RT: 23.197 min Scan# 3419
Delta R.T. 0.000 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30




Instrument :
BNA_M
ClientSampleId :
SICV032


Tgt Ion:252 Resp: 2045812
Ion Ratio Lower Upper
252 100
253 21.7 17.7 26.5
125 11.8 9.9 14.9



#91
Benzo(k)fluoranthene
Concen: 18.313 ng/ul
RT: 23.244 min Scan# 3427
Delta R.T. -0.006 min
Lab File: BM036802.D
Acq: 29 Sep 2022 15:30

Tgt Ion:252 Resp: 2019361
Ion Ratio Lower Upper
252 100
253 22.0 17.9 26.9
125 11.8 9.7 14.5





#93

Benzo(a)pyrene

Concen: 18.266 ng/ul

RT: 23.827 min Scan# 3

Delta R.T. -0.006 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:252 Resp: 1815449

Ion Ratio Lower Upper

252 100

253 22.1 17.3 25.9

125 13.0 10.5 15.7

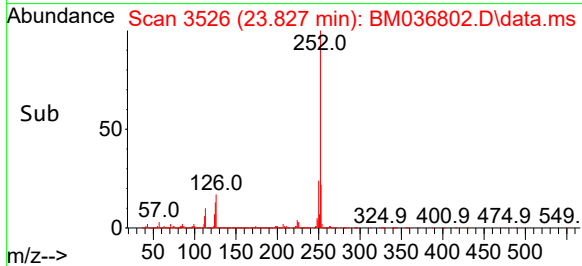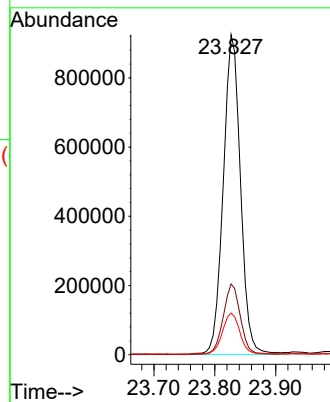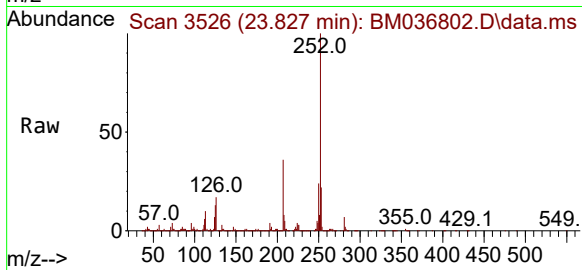

#94

Indeno(1,2,3-cd)pyrene

Concen: 18.883 ng/ul

RT: 26.450 min Scan# 3972

Delta R.T. -0.006 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30




Tgt Ion:276 Resp: 2223968


Ion Ratio Lower Upper

276 100

138 28.1 24.0 36.0

277 24.9 19.7 29.5

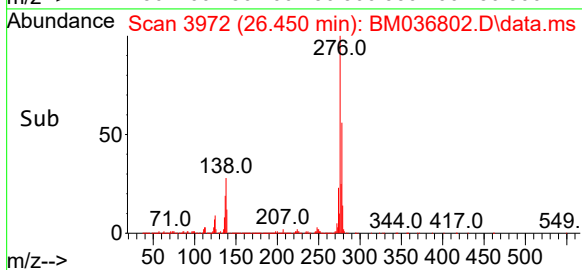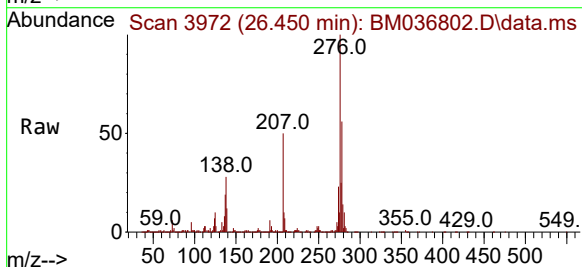



#95

Dibenzo(a,h)anthracene

Concen: 18.226 ng/ul

RT: 26.473 min Scan# 3976

Delta R.T. 0.000 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Instrument :

BNA_M

ClientSampleId :

SICV032





Tgt Ion:278 Resp: 1952215

Ion Ratio Lower Upper

278 100

139 19.2 16.1 24.1

279 23.8 19.4 29.2



#96

Benzo(g,h,i)perylene

Concen: 18.308 ng/ul

RT: 27.226 min Scan# 4104

Delta R.T. -0.006 min

Lab File: BM036802.D

Acq: 29 Sep 2022 15:30

Tgt Ion:276 Resp: 1884068

Ion Ratio Lower Upper

276 100

138 25.7 21.0 31.4

277 23.1 19.1 28.7

