
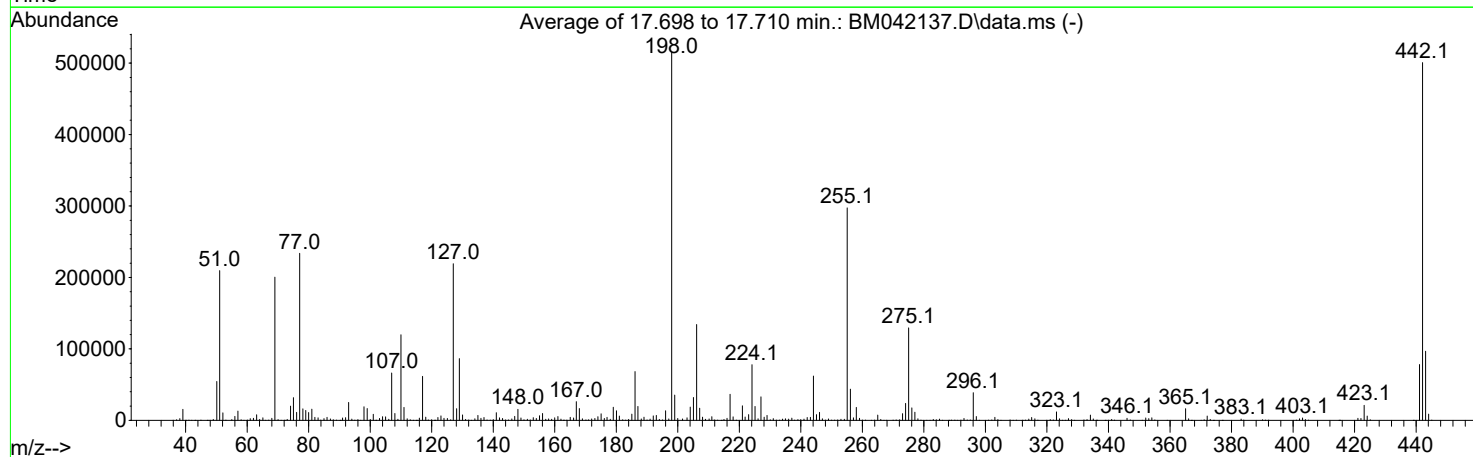


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092923\
Data File : BM042137.D
Acq On : 29 Sep 2023 09:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 19 04:49:34 2023

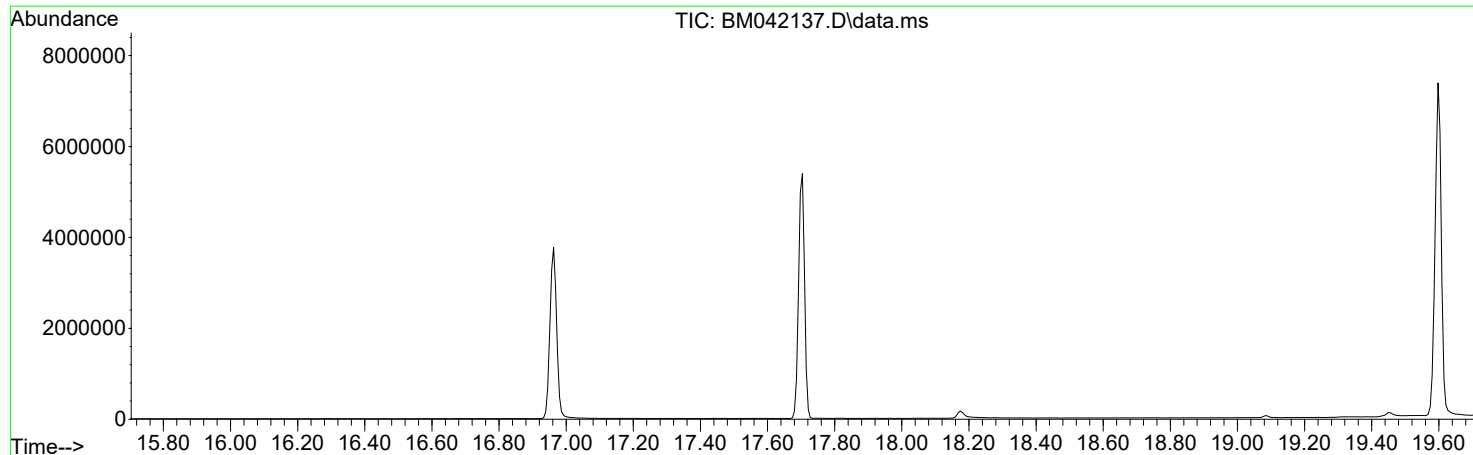

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	209693	PASS
68	69	0.00	2	1.5	3005	PASS
69	198	0.00	100	38.9	200403	PASS
70	69	0.00	2	0.6	1133	PASS
127	198	10	80	42.6	219307	PASS
197	198	0.00	2	0.4	2094	PASS
198	198	100	100	100.0	514859	PASS
199	198	5	9	6.9	35387	PASS
275	198	10	60	25.2	129499	PASS
365	198	1	100	3.2	16364	PASS
441	198	0.01	100	15.2	78171	PASS
442	442	50	100	100.0	500779	PASS
443	442	15	24	19.3	96701	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/29/2023	BNA_M	<u>BM042137.D</u>
Compound Name	Response	Retention Time
DDT	1875796	20.786
DDD	22214	20.398
DDE	1000	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23214	1899010	1.22

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092923\
 Data File : BM042137.D
 Acq On : 29 Sep 2023 09:23
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 02:08:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 19 04:49:34 2023
 Response via : Initial Calibration

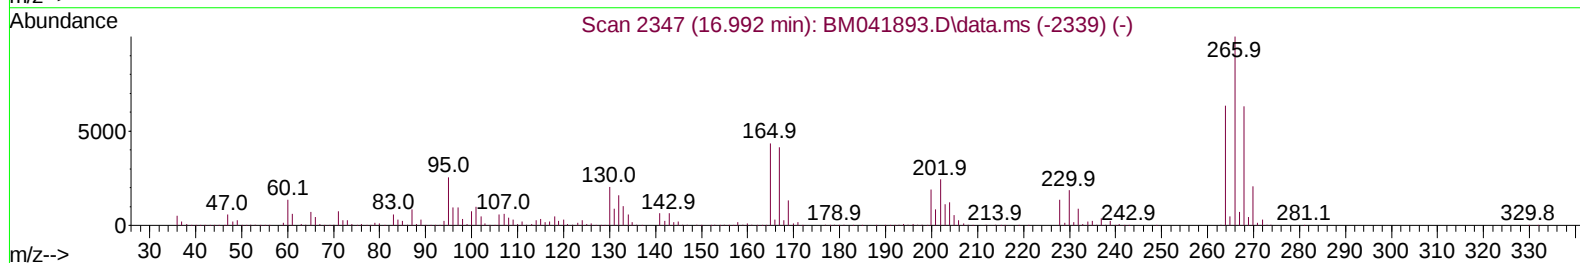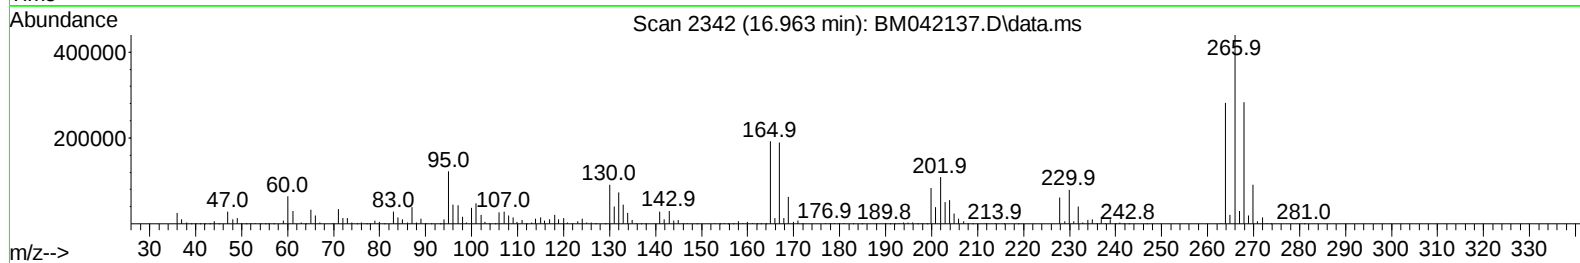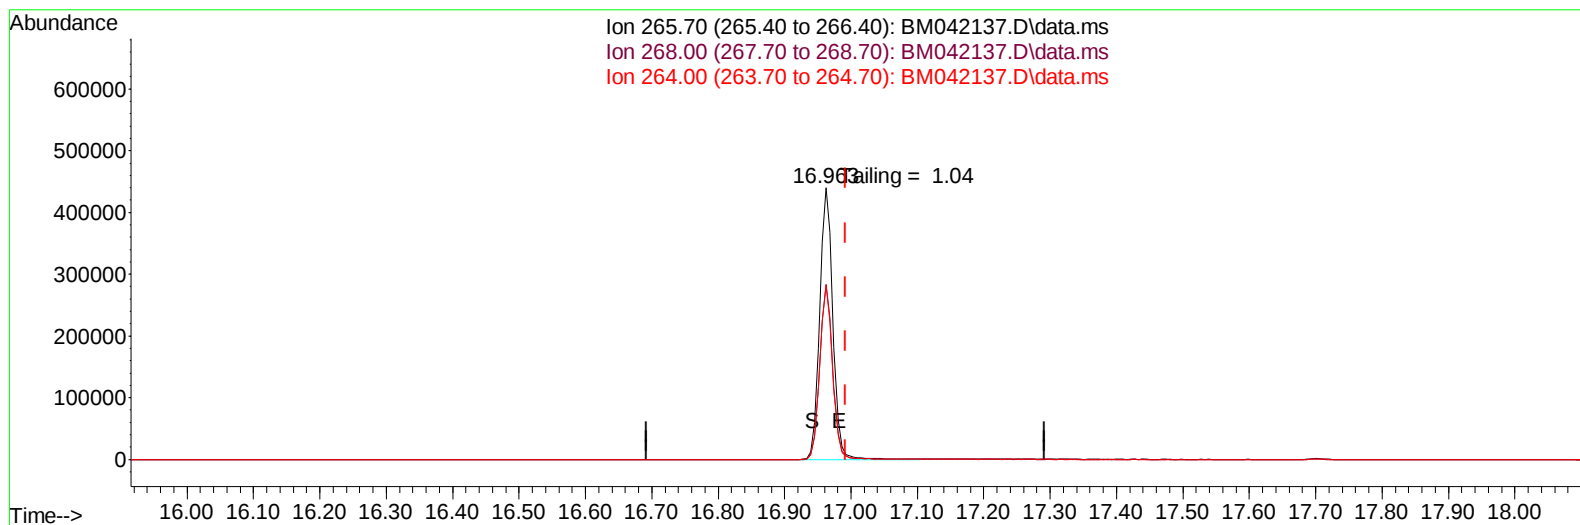

TIC: BM042137.D\data.ms



(70) Pentachlorophenol (C)

16.963min (-0.029) 0.00 ng

response 606106

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.43
264.00	63.30	64.21
0.00	0.00	0.00

Instrument :
BNA_M
ClientSampleId :
DFTPP

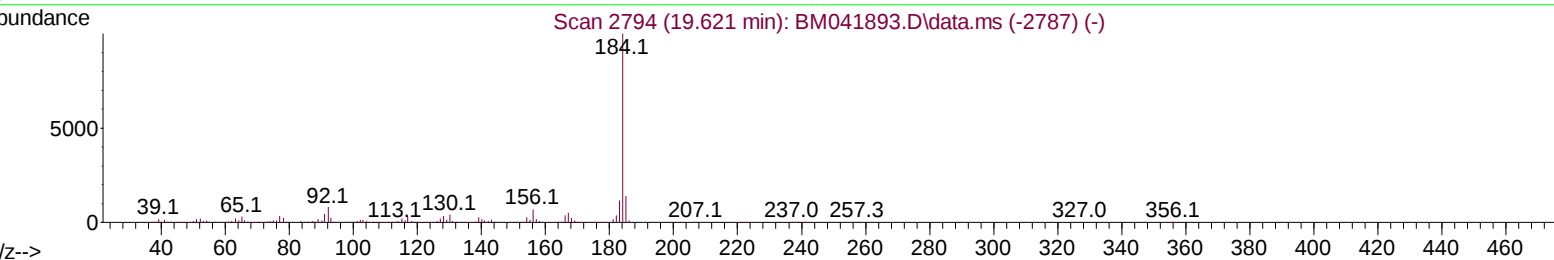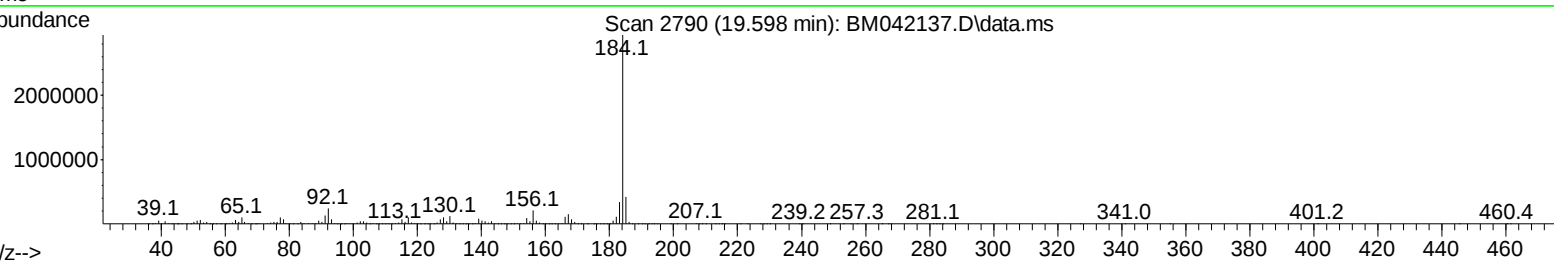

TIC: BM042137.D\data.ms

(77) Benzidine

19.598min (-0.024) 301411.22 ng

response **3869852**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.14
183.00	11.40	11.54
0.00	0.00	0.00