

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM093019\
 Data File : BM022847.D
 Acq On : 01 Oct 2019 05:37
 Operator : JU
 Sample : K5027-04
 Misc : GCMS CONFIRMATION
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 01 06:34:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 27 18:03:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	255840	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1091293	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.44	164	705165	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.18	188	1407445	20.00	ng/ul	0.00
78) Chrysene-d12	21.36	240	1009470	20.00	ng/ul	-0.01
86) Perylene-d12	23.62	264	934907	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	7.28	67	243	0.02	ng/ul	0.14
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.60	131	1332	0.06	ng/ul	-0.13
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.43	176	1297	0.03	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.36	188	8498	0.12	ng/ul	0.07
79) Pyrene-d10	19.57	212	560	0.01	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.62	264	926623	19.16	ng/ul	0.12

Target Compounds


				Ovalue
69) Pentachlorophenol	16.83	266	15839	1.290 ng/ul 98
84) Bis(2-ethylhexyl)phthalate	21.27	149	45729	1.094 ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM093019\
Data File : BM022847.D
Acq On : 01 Oct 2019 05:37
Operator : JU
Sample : K5027-04
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 01 06:34:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 27 18:03:27 2019
Response via : Initial Calibration

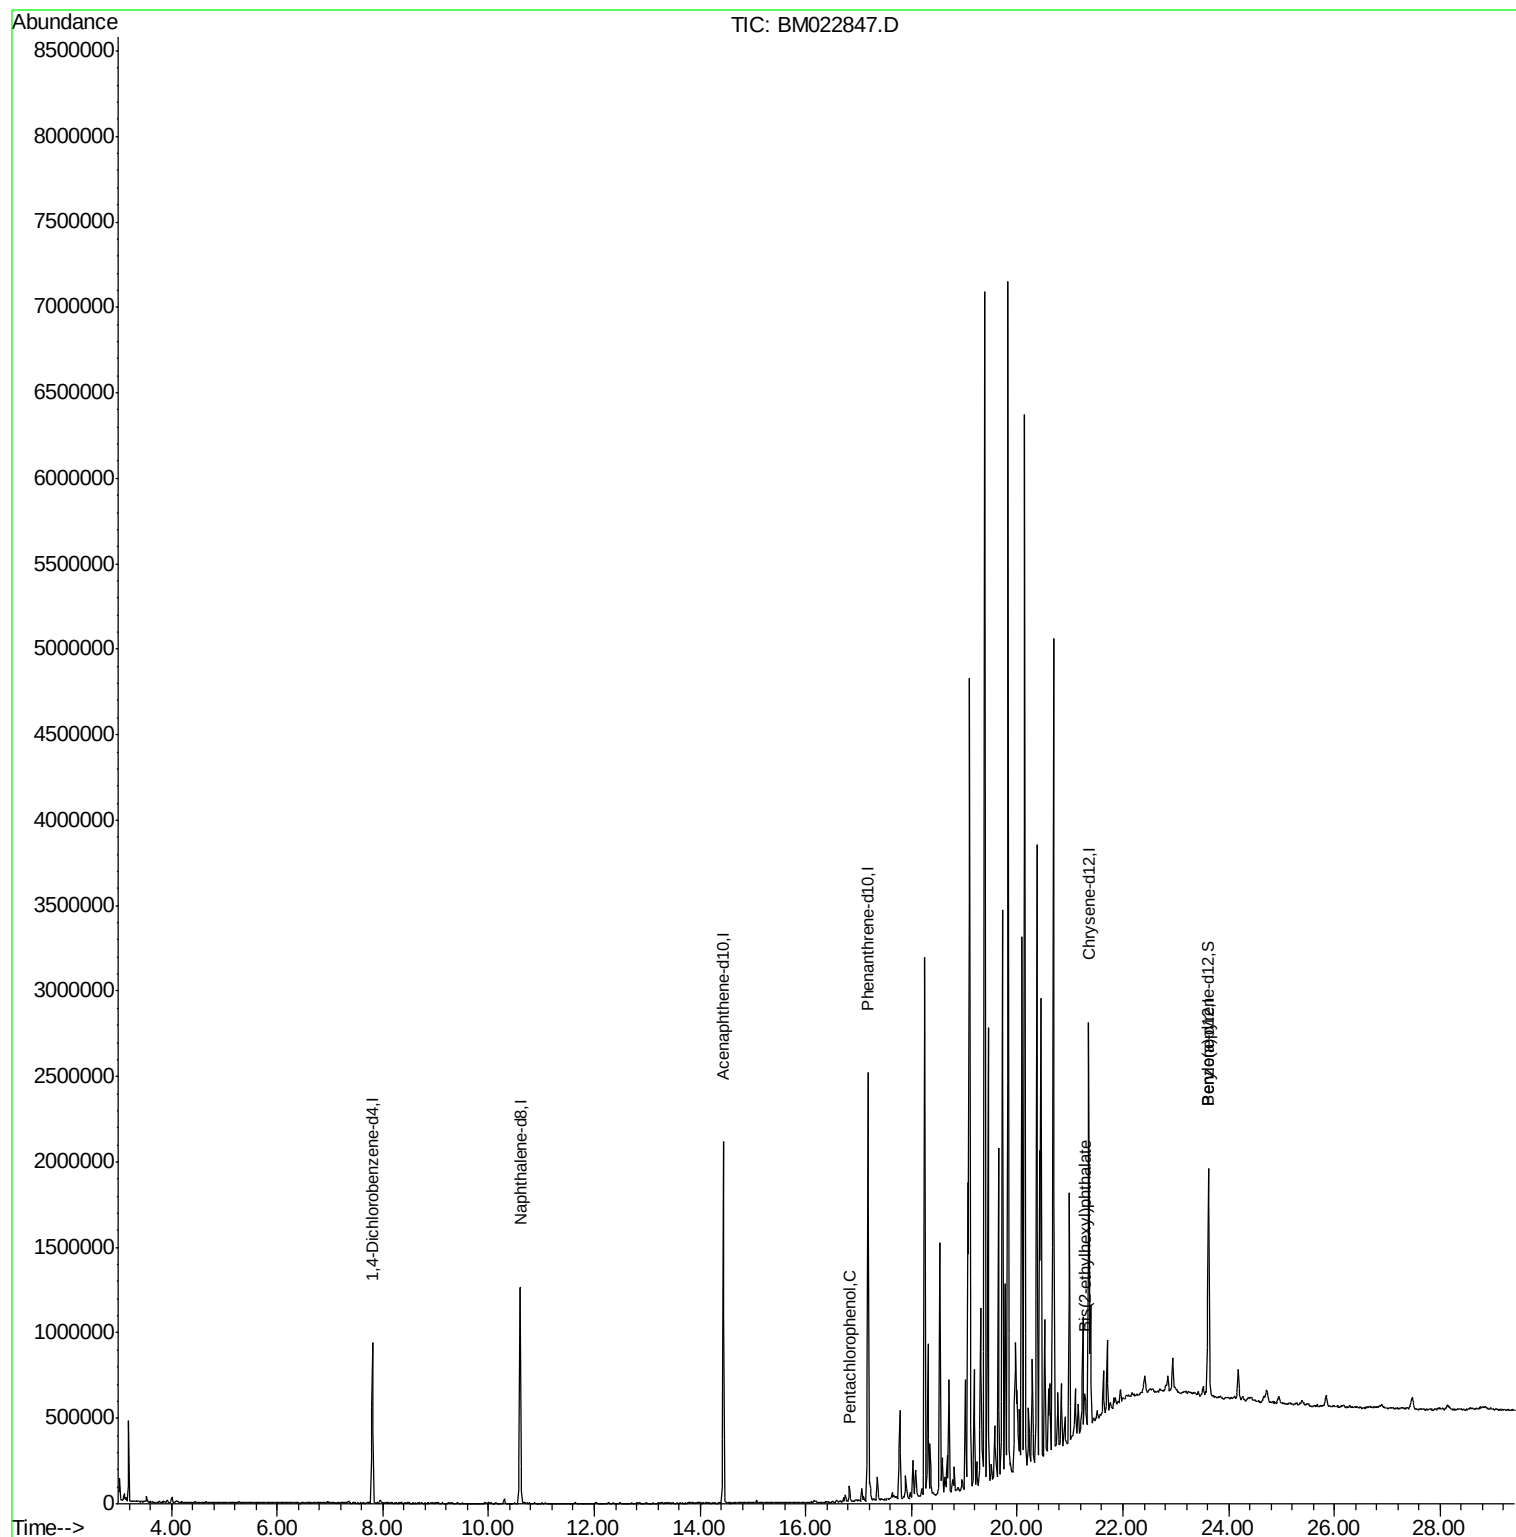

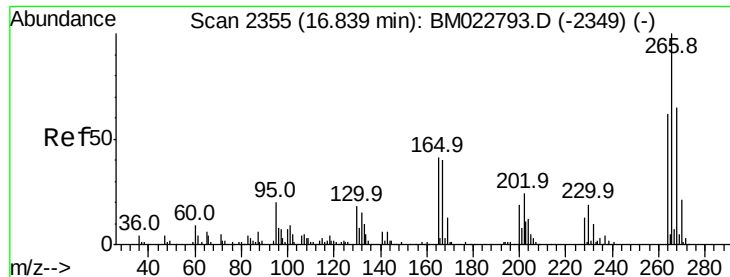

#69

Pentachlorophenol

Concen: 1.290 ng/ul

RT: 16.83 min Scan# 2353

Delta R.T. -0.01 min

Lab File: BM022847.D

Acq: 01 Oct 2019 05:37

Instrument :

BNA_M

ClientSampled :


Tot Ion:266 Resp: 15839

Ion Ratio Lower Upper

266 100

264 65.3 50.8 76.2




268 63.5 51.4 77.0

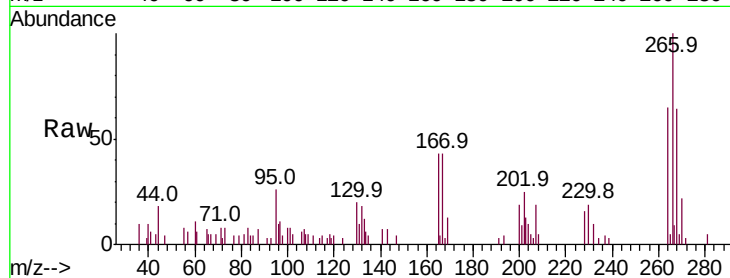

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

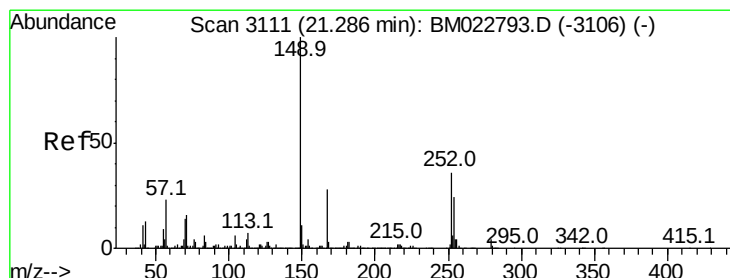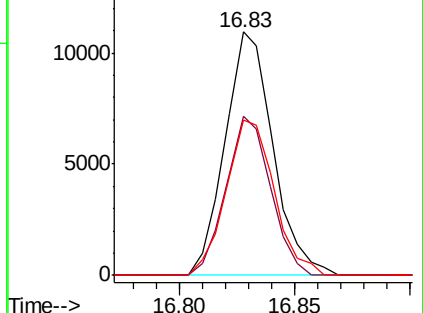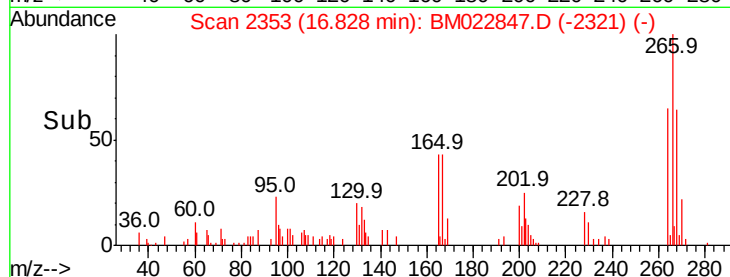

#84

Bis(2-ethylhexyl)phthalate

Concen: 1.094 ng/ul

RT: 21.27 min Scan# 3109

Delta R.T. -0.01 min

Lab File: BM022847.D

Acq: 01 Oct 2019 05:37


Tgt Ion:149 Resp: 45729

Ion Ratio Lower Upper

149 100

167 27.2 22.1 33.1

279 4.5 3.3 4.9

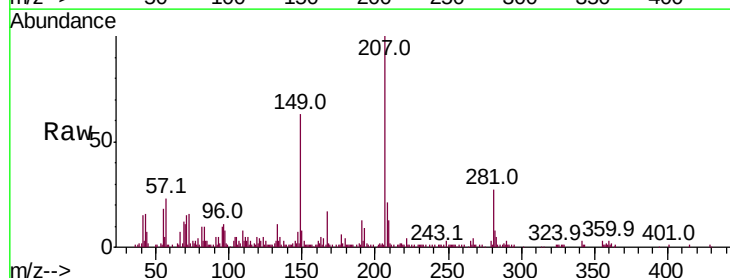

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

