

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
 Data File : BM022834.D
 Acq On : 30 Sep 2019 20:32
 Operator : JU
 Sample : K5006-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETJW0

Quant Time: Sep 30 23:38:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 27 18:03:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	266071	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1181882	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.44	164	758159	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.18	188	1570638	20.00	ng/ul	0.00
78) Chrysene-d12	21.36	240	1532112	20.00	ng/ul	0.00
86) Perylene-d12	23.63	264	1383940	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	33144	5.39	ng/uL	0.00
5) Phenol-d5	6.97	99	153574	6.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	310074	24.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	384233	20.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	265377	13.79	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	222141	24.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	243363	24.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	439328	22.15	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.73	131	67566	2.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.85	166	1498957	25.47	ng/ul	0.00
47) Acenaphthylene-d8	14.13	160	1702196	25.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	67308	5.79	ng/ul	-0.01
58) Fluorene-d10	15.43	176	1305714	26.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.54	200	210644	20.61	ng/ul	-0.01
71) Anthracene-d10	17.28	188	2147629	28.00	ng/ul	0.00
79) Pyrene-d10	19.57	212	2443781	29.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.49	264	2063575	28.82	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.90	163	157594	2.607	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
Data File : BM022834.D
Acq On : 30 Sep 2019 20:32
Operator : JU
Sample : K5006-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETJW0

Quant Time: Sep 30 23:38:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 27 18:03:27 2019
Response via : Initial Calibration

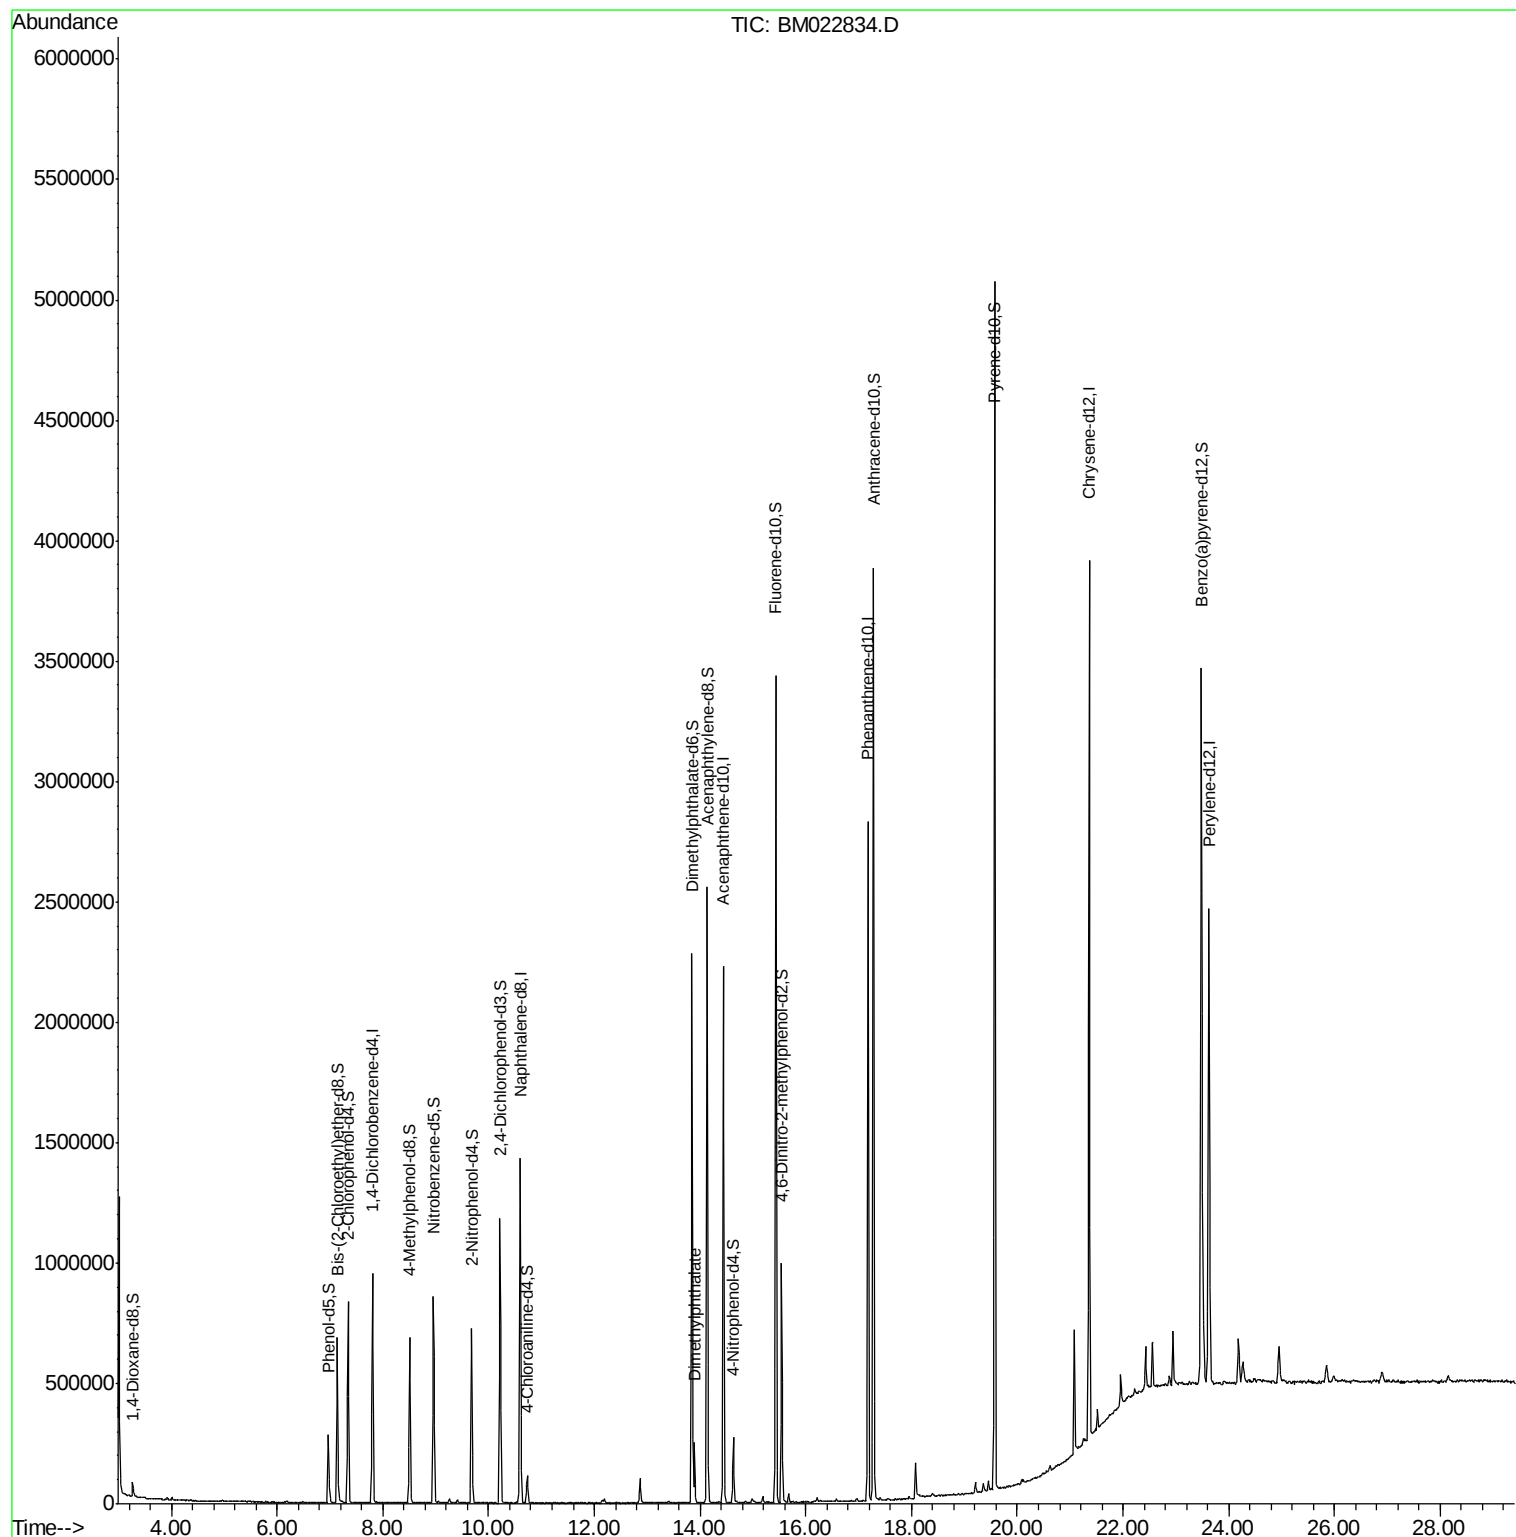

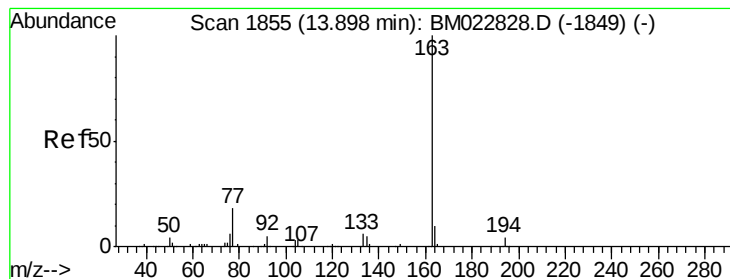

#45

Dimethylphthalate

Concen: 2.607 ng/ul

RT: 13.90 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BM022834.D

Acq: 30 Sep 2019 20:32

Instrument :

BNA_M

ClientSampleId :

ETJW0


Tgt Ion:163 Resp: 157594

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.1 8.1 12.1

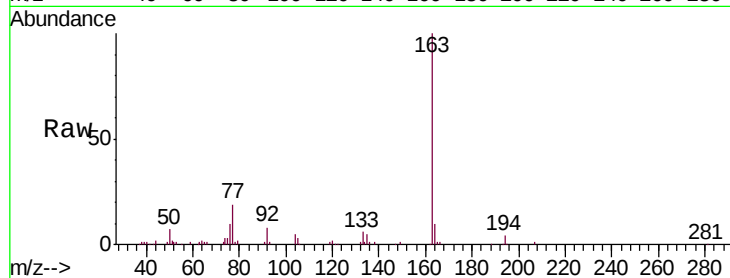

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

