

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
 Data File : BM022837.D
 Acq On : 30 Sep 2019 22:21
 Operator : JU
 Sample : K5006-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETJW3

Quant Time: Sep 30 23:39:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 27 18:03:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	259846	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1187784	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.44	164	787202	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.18	188	1656499	20.00	ng/ul	0.00
78) Chrysene-d12	21.36	240	1557566	20.00	ng/ul	-0.01
86) Perylene-d12	23.63	264	1382963	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	29415	4.90	ng/uL	0.00
5) Phenol-d5	6.97	99	132740	5.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	312453	24.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	377289	20.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	251110	13.36	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	225204	24.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	245384	24.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	448999	22.53	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.73	131	48944	2.02	ng/ul	0.00
44) Dimethylphthalate-d6	13.85	166	1605626	26.28	ng/ul	0.00
47) Acenaphthylene-d8	14.13	160	1807057	25.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	62250	5.16	ng/ul	-0.01
58) Fluorene-d10	15.43	176	1455655	27.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.54	200	251914	23.37	ng/ul	-0.01
71) Anthracene-d10	17.28	188	2462145	30.44	ng/ul	0.00
79) Pyrene-d10	19.57	212	2802131	33.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.48	264	2248514	31.43	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.90	163	170651	2.719	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
Data File : BM022837.D
Acq On : 30 Sep 2019 22:21
Operator : JU
Sample : K5006-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETJW3

Quant Time: Sep 30 23:39:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 27 18:03:27 2019
Response via : Initial Calibration

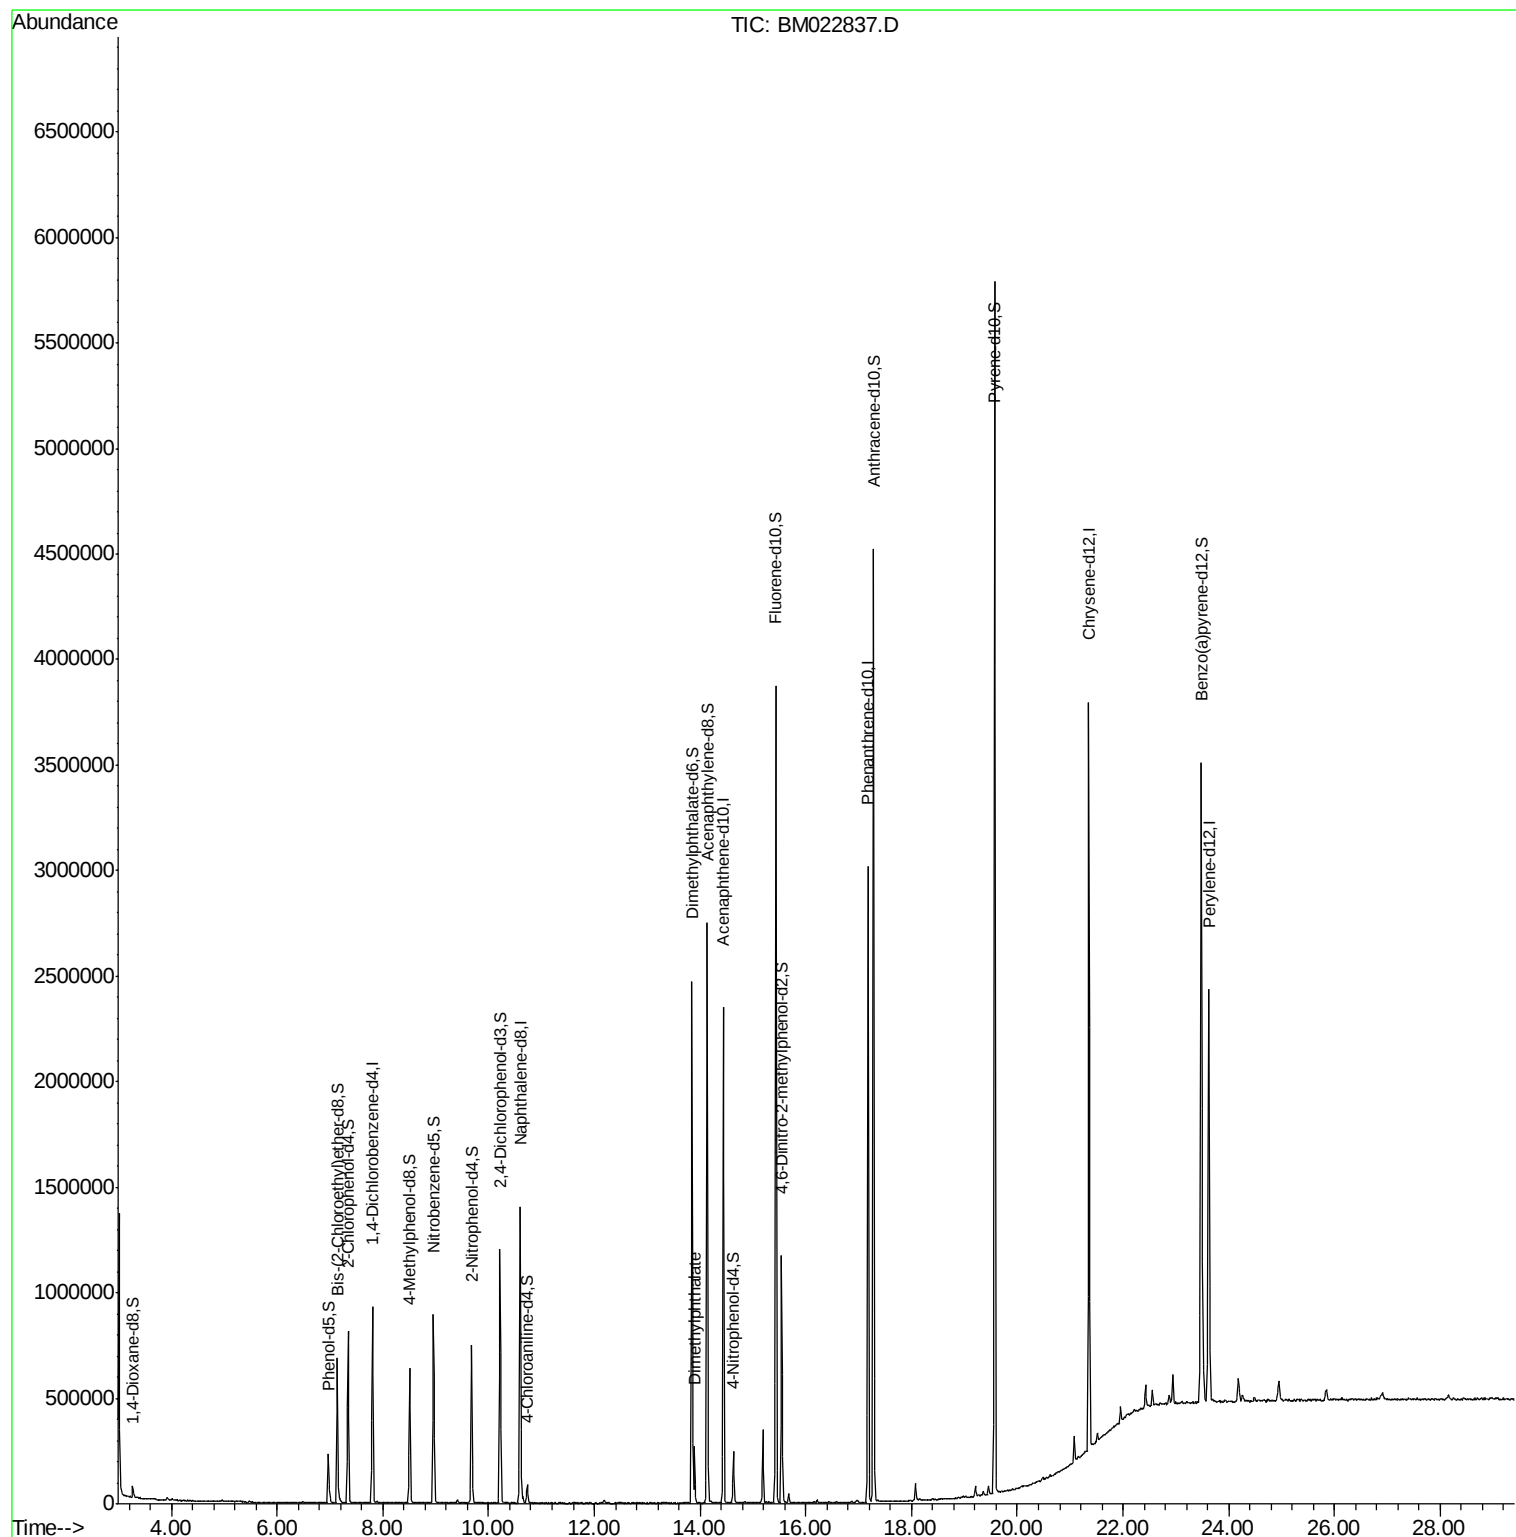

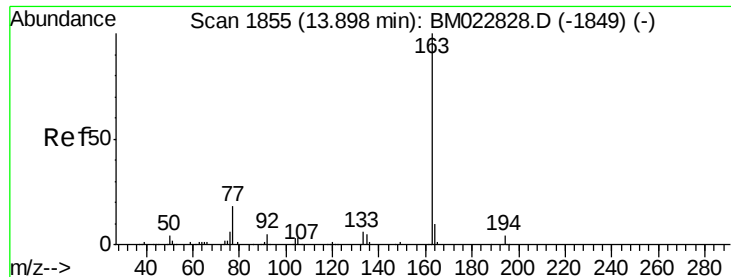

#45

Dimethylphthalate

Concen: 2.719 ng/ul

RT: 13.90 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BM022837.D

Acq: 30 Sep 2019 22:21

Instrument :

BNA_M

ClientSampleId :

ETJW3


Tgt Ion:163 Resp: 170651

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 9.8 8.1 12.1

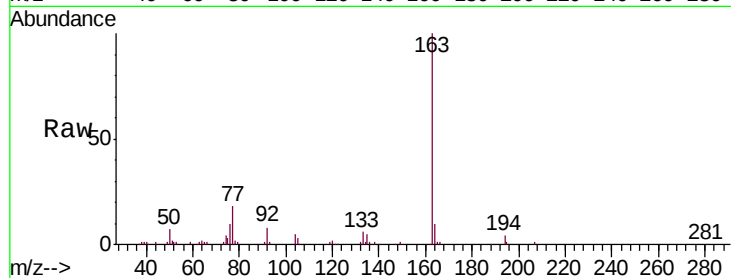

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

