

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
 Data File : BM022825.D
 Acq On : 30 Sep 2019 15:04
 Operator : JU
 Sample : K4958-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNZ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	45	48	60	rVB	25428	47257	1.17%	0.108%
2	3.922	153	159	170	rVV	53815	92729	2.29%	0.212%
3	4.010	170	174	179	rVB	10594	14442	0.36%	0.033%
4	4.104	185	190	197	rVB	18613	28281	0.70%	0.065%
5	4.457	247	250	256	rVB	10218	13774	0.34%	0.032%
6	4.928	326	330	343	rVB	47905	81361	2.01%	0.186%
7	6.198	542	546	551	rVB	18252	25447	0.63%	0.058%
8	6.969	671	677	691	rBV2	487034	882370	21.79%	2.020%
9	7.140	699	706	724	rBV	372179	613201	15.14%	1.404%
10	7.340	733	740	748	rBV	518041	818949	20.22%	1.875%
11	7.810	813	820	827	rBV	799051	1269457	31.35%	2.907%
12	7.881	829	832	840	rVB3	5338	8842	0.22%	0.020%
13	8.510	932	939	952	rBV	593302	948826	23.43%	2.173%
14	8.634	956	960	966	rVB	17688	29872	0.74%	0.068%
15	8.963	1008	1016	1025	rBV	463492	776236	19.17%	1.777%
16	9.410	1087	1092	1098	rVB	15432	22954	0.57%	0.053%
17	9.681	1132	1138	1147	rBV	378077	619792	15.31%	1.419%
18	10.222	1223	1230	1242	rBV	626237	1060580	26.19%	2.428%
19	10.598	1287	1294	1301	rBV	1172127	1956220	48.31%	4.479%
20	10.651	1301	1303	1309	rVB	9672	11855	0.29%	0.027%
21	10.733	1309	1317	1327	rBV	595813	1041154	25.71%	2.384%
22	11.398	1424	1430	1435	rBV6	4681	8883	0.22%	0.020%
23	12.192	1560	1565	1571	rVB2	9110	14208	0.35%	0.033%
24	12.810	1664	1670	1674	rBV2	5170	9411	0.23%	0.022%
25	13.057	1708	1712	1716	rVB4	8074	10935	0.27%	0.025%
26	13.280	1746	1750	1756	rVB	6180	8322	0.21%	0.019%
27	13.851	1841	1847	1851	rBV	1261147	1682959	41.56%	3.854%
28	13.898	1851	1855	1861	rVB	310055	418100	10.33%	0.957%
29	14.133	1886	1895	1905	rBV	1412890	2068305	51.08%	4.736%
30	14.445	1941	1948	1956	rBV	1953430	2832589	69.95%	6.486%
31	14.627	1973	1979	1993	rBV	467465	677554	16.73%	1.551%
32	14.798	2001	2008	2012	rVB3	5477	11035	0.27%	0.025%
33	14.857	2013	2018	2024	rBV2	55809	76730	1.89%	0.176%
34	15.257	2079	2086	2089	rBV2	8540	13656	0.34%	0.031%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
 Data File : BM022825.D
 Acq On : 30 Sep 2019 15:04
 Operator : JU
 Sample : K4958-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNZ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

35	15.304	2090	2094	2097	rVB2	6585	8260	0.20%	0.019%
36	15.433	2110	2116	2123	rBV	1897026	2629552	64.94%	6.021%
37	15.545	2129	2135	2145	rBV	371763	535171	13.22%	1.225%
38	15.674	2152	2157	2162	rBV	18880	25893	0.64%	0.059%
39	16.215	2246	2249	2256	rVB5	7782	13036	0.32%	0.030%
40	16.439	2281	2287	2292	rBV5	5288	10526	0.26%	0.024%
41	16.727	2332	2336	2341	rVB2	10646	13235	0.33%	0.030%
42	16.968	2371	2377	2380	rBV3	8574	18090	0.45%	0.041%
43	17.180	2407	2413	2418	rBV2	2386949	3391256	83.75%	7.765%
44	17.221	2418	2420	2424	rVV	79067	91950	2.27%	0.211%
45	17.280	2424	2430	2440	rVV	2089446	2887979	71.32%	6.613%
46	17.368	2443	2445	2450	rVB5	8850	10721	0.26%	0.025%
47	17.427	2450	2455	2460	rBV6	5946	14337	0.35%	0.033%
48	17.568	2474	2479	2487	rBV3	34079	52012	1.28%	0.119%
49	17.686	2493	2499	2503	rBV6	5766	10208	0.25%	0.023%
50	18.074	2557	2565	2574	rBV2	83080	154444	3.81%	0.354%
51	18.145	2574	2577	2581	rVB	17006	22679	0.56%	0.052%
52	18.251	2591	2595	2606	rVB3	16038	36595	0.90%	0.084%
53	18.509	2636	2639	2643	rVB	44010	51106	1.26%	0.117%
54	18.556	2643	2647	2651	rBV2	10069	16820	0.42%	0.039%
55	18.968	2715	2717	2723	rVB7	13201	15191	0.38%	0.035%
56	19.203	2754	2757	2758	rBV	24282	26420	0.65%	0.060%
57	19.239	2758	2763	2769	rVB	257585	350319	8.65%	0.802%
58	19.356	2781	2783	2788	rVB4	14170	13871	0.34%	0.032%
59	19.456	2798	2800	2804	rBV	19974	22781	0.56%	0.052%
60	19.574	2814	2820	2834	rBV	2762414	4049221	100.00%	9.272%
61	20.092	2906	2908	2912	rVB	33074	36344	0.90%	0.083%
62	20.198	2923	2926	2930	rBV	30825	40234	0.99%	0.092%
63	21.080	3072	3076	3081	rBV3	290689	380329	9.39%	0.871%
64	21.362	3118	3124	3128	rBV	3130726	4004533	98.90%	9.169%
65	22.944	3390	3393	3406	rVB	317754	599857	14.81%	1.374%
66	23.486	3479	3485	3490	rBV	1488663	2767757	68.35%	6.338%
67	23.627	3503	3509	3523	rVB	1671869	3175517	78.42%	7.271%


Sum of corrected areas: 43672530

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
Data File : BM022825.D
Acq On : 30 Sep 2019 15:04
Operator : JU
Sample : K4958-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNZ2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

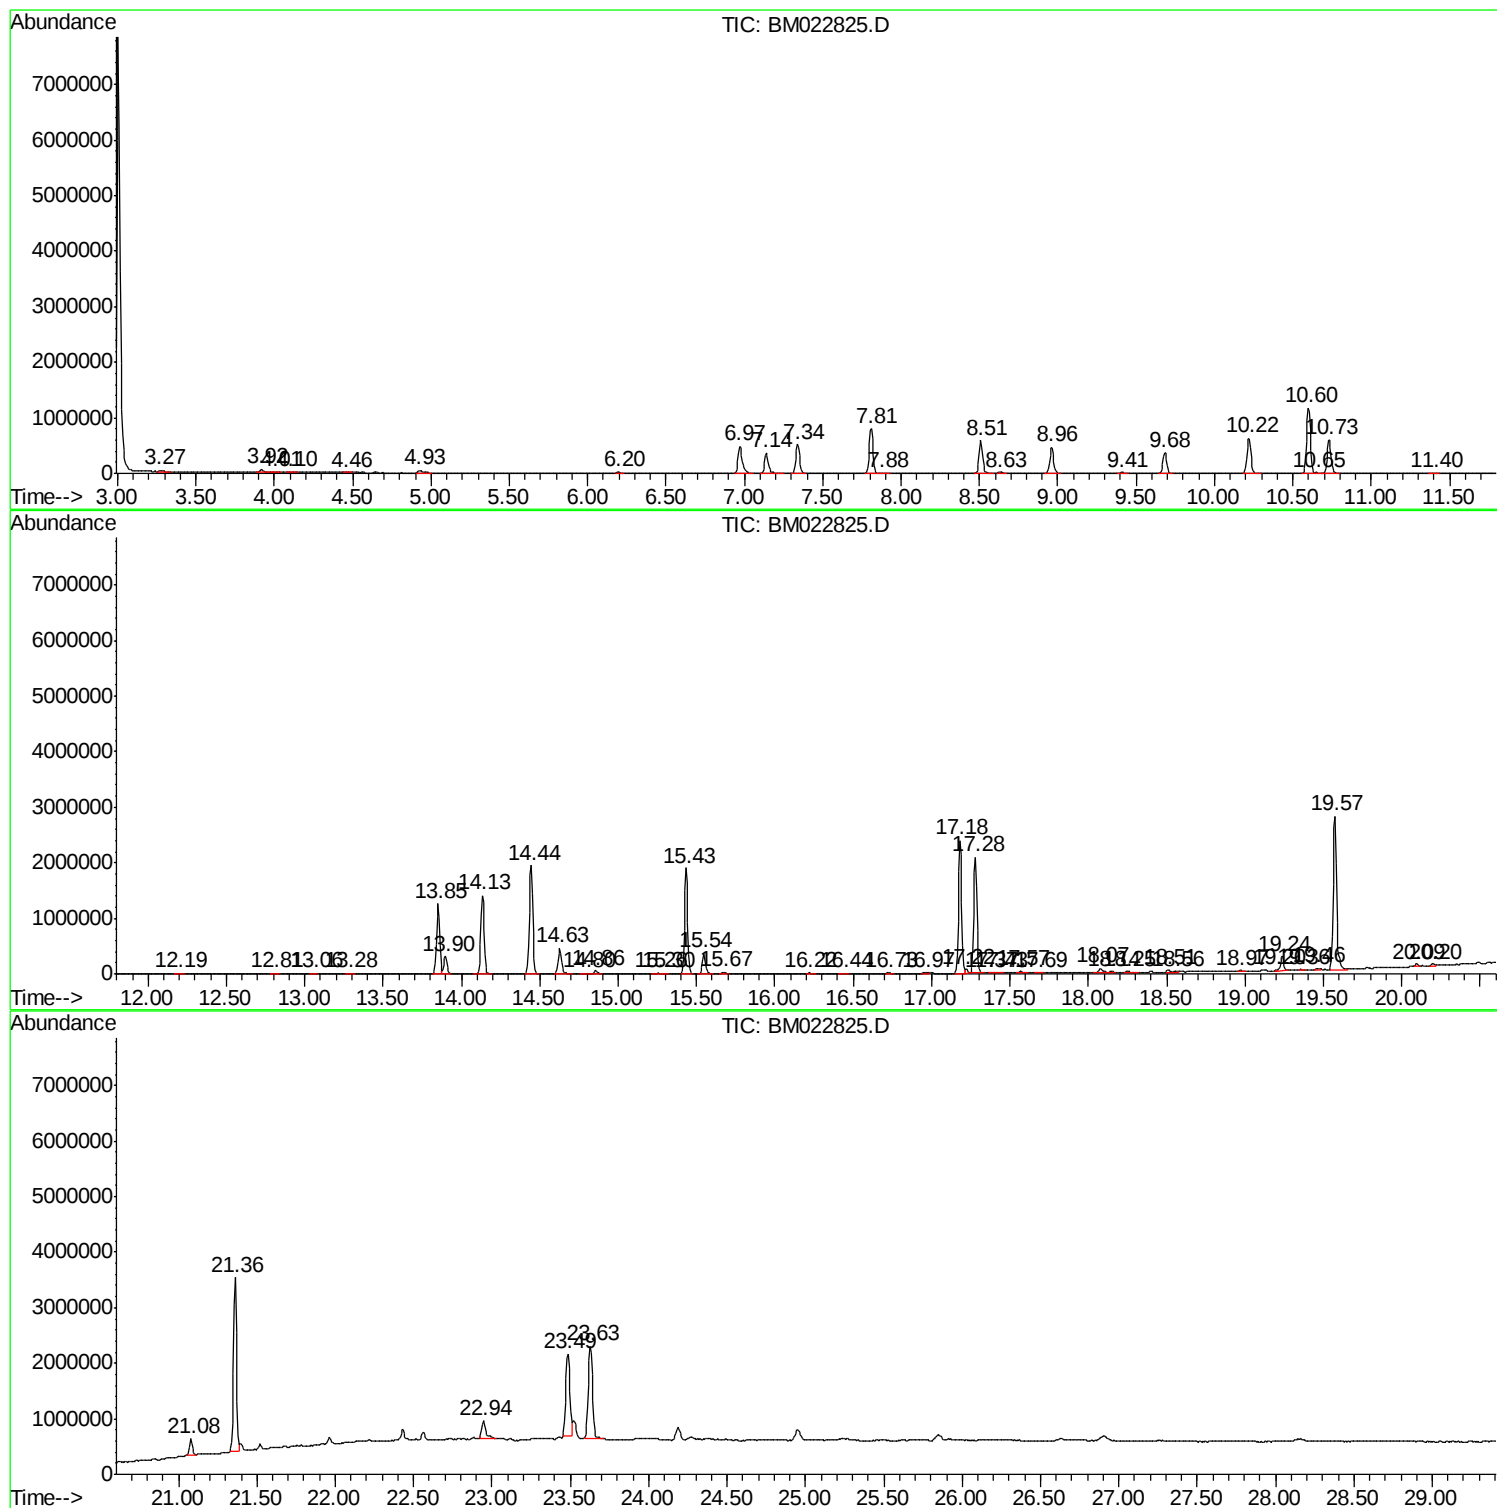

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
Data File : BM022825.D
Acq On : 30 Sep 2019 15:04
Operator : JU
Sample : K4958-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNZ2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM093019\
Data File : BM022825.D
Acq On : 30 Sep 2019 15:04
Operator : JU
Sample : K4958-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNZ2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc