

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100118\
 Data File : BM016918.D
 Acq On : 01 Oct 2018 12:14
 Operator : MJ/SJ
 Sample : J5127-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B65

Quant Time: Oct 02 08:03:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 27 02:42:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	341476	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1400918	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	653650	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1208893	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	1174446	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1323511	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul	
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul	
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul	
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul	
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
77) Fluoranthene	19.17	202	89315	1.160	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100118\
Data File : BM016918.D
Acq On : 01 Oct 2018 12:14
Operator : MJ/SJ
Sample : J5127-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B65

Quant Time: Oct 02 08:03:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 27 02:42:56 2018
Response via : Initial Calibration

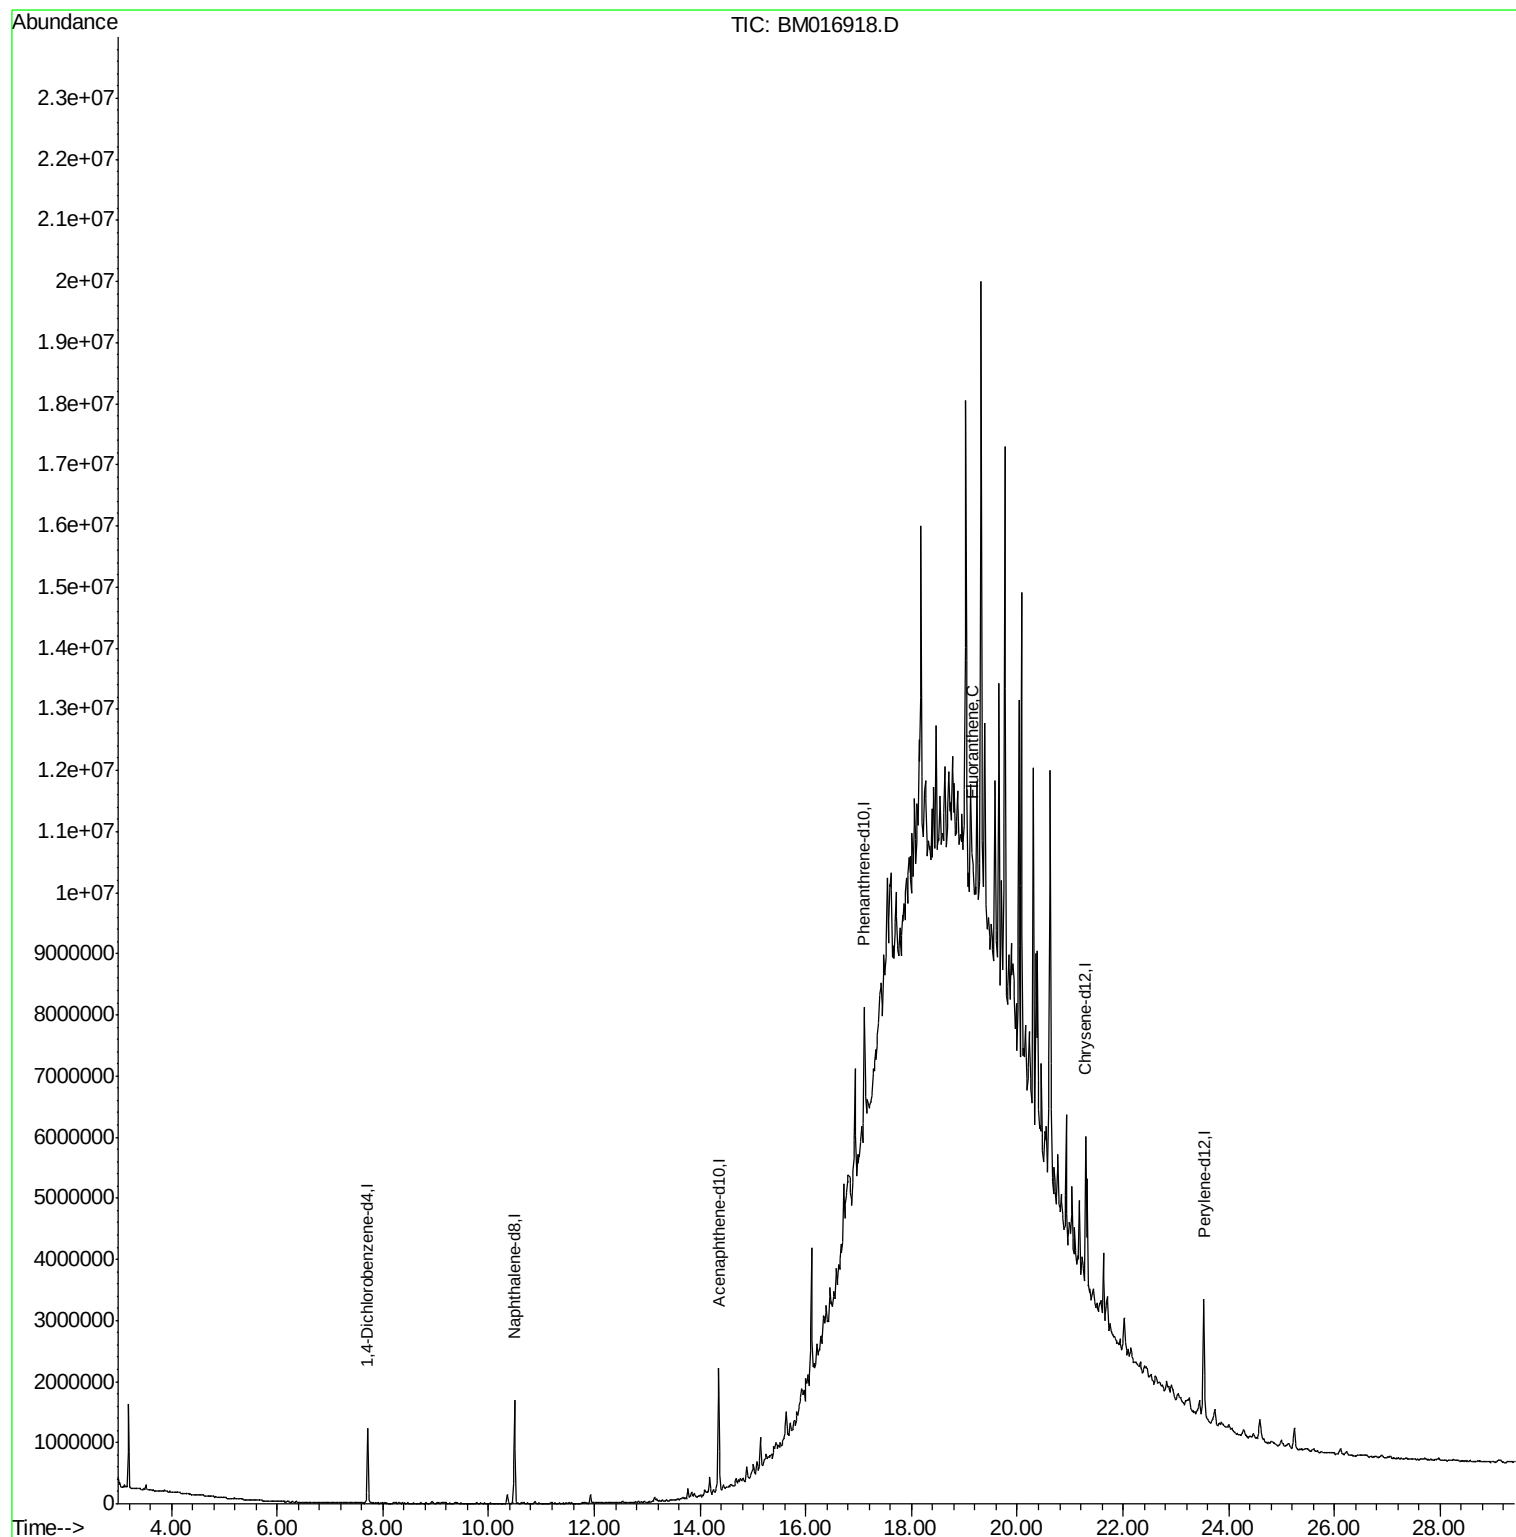


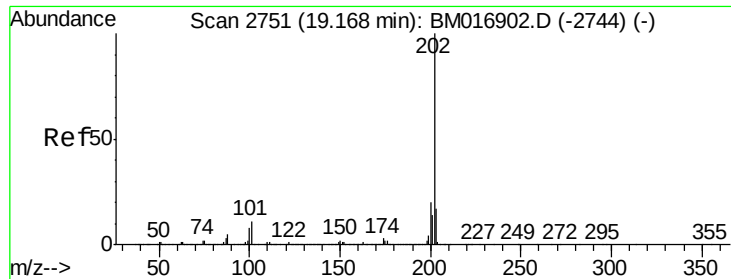

#77
 Fluoranthene
 Concen: 1.160 ng/ul
 RT: 19.17 min Scan# 2751
 Delta R.T. 0.00 min
 Lab File: BM016918.D
 Acq: 01 Oct 2018 12:14

Instrument :
 BNA_M
 ClientSampleId :
 C0B65

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.4	6.1	9.1#
100	13.2	4.6	7.0#

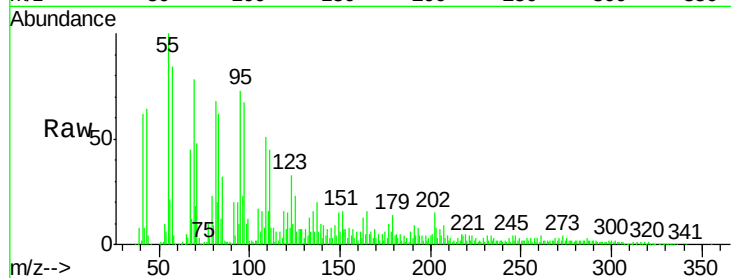

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

