

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
 Data File : BM016938.D
 Acq On : 02 Oct 2018 01:15
 Operator : MJ/SJ
 Sample : J5125-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B71

Quant Time: Oct 02 09:23:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 27 02:42:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	369969	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1551732	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.35	164	780677	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1404412	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1349404	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	1510285	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds				Ovalue
73) 1,2,3,4-Tetrachlorobenzene	13.14	216	32061	1.379 ng/uL 97
77) Fluoranthene	19.17	202	103518	1.158 ng/ul# 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
Data File : BM016938.D
Acq On : 02 Oct 2018 01:15
Operator : MJ/SJ
Sample : J5125-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B71

Quant Time: Oct 02 09:23:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 27 02:42:56 2018
Response via : Initial Calibration

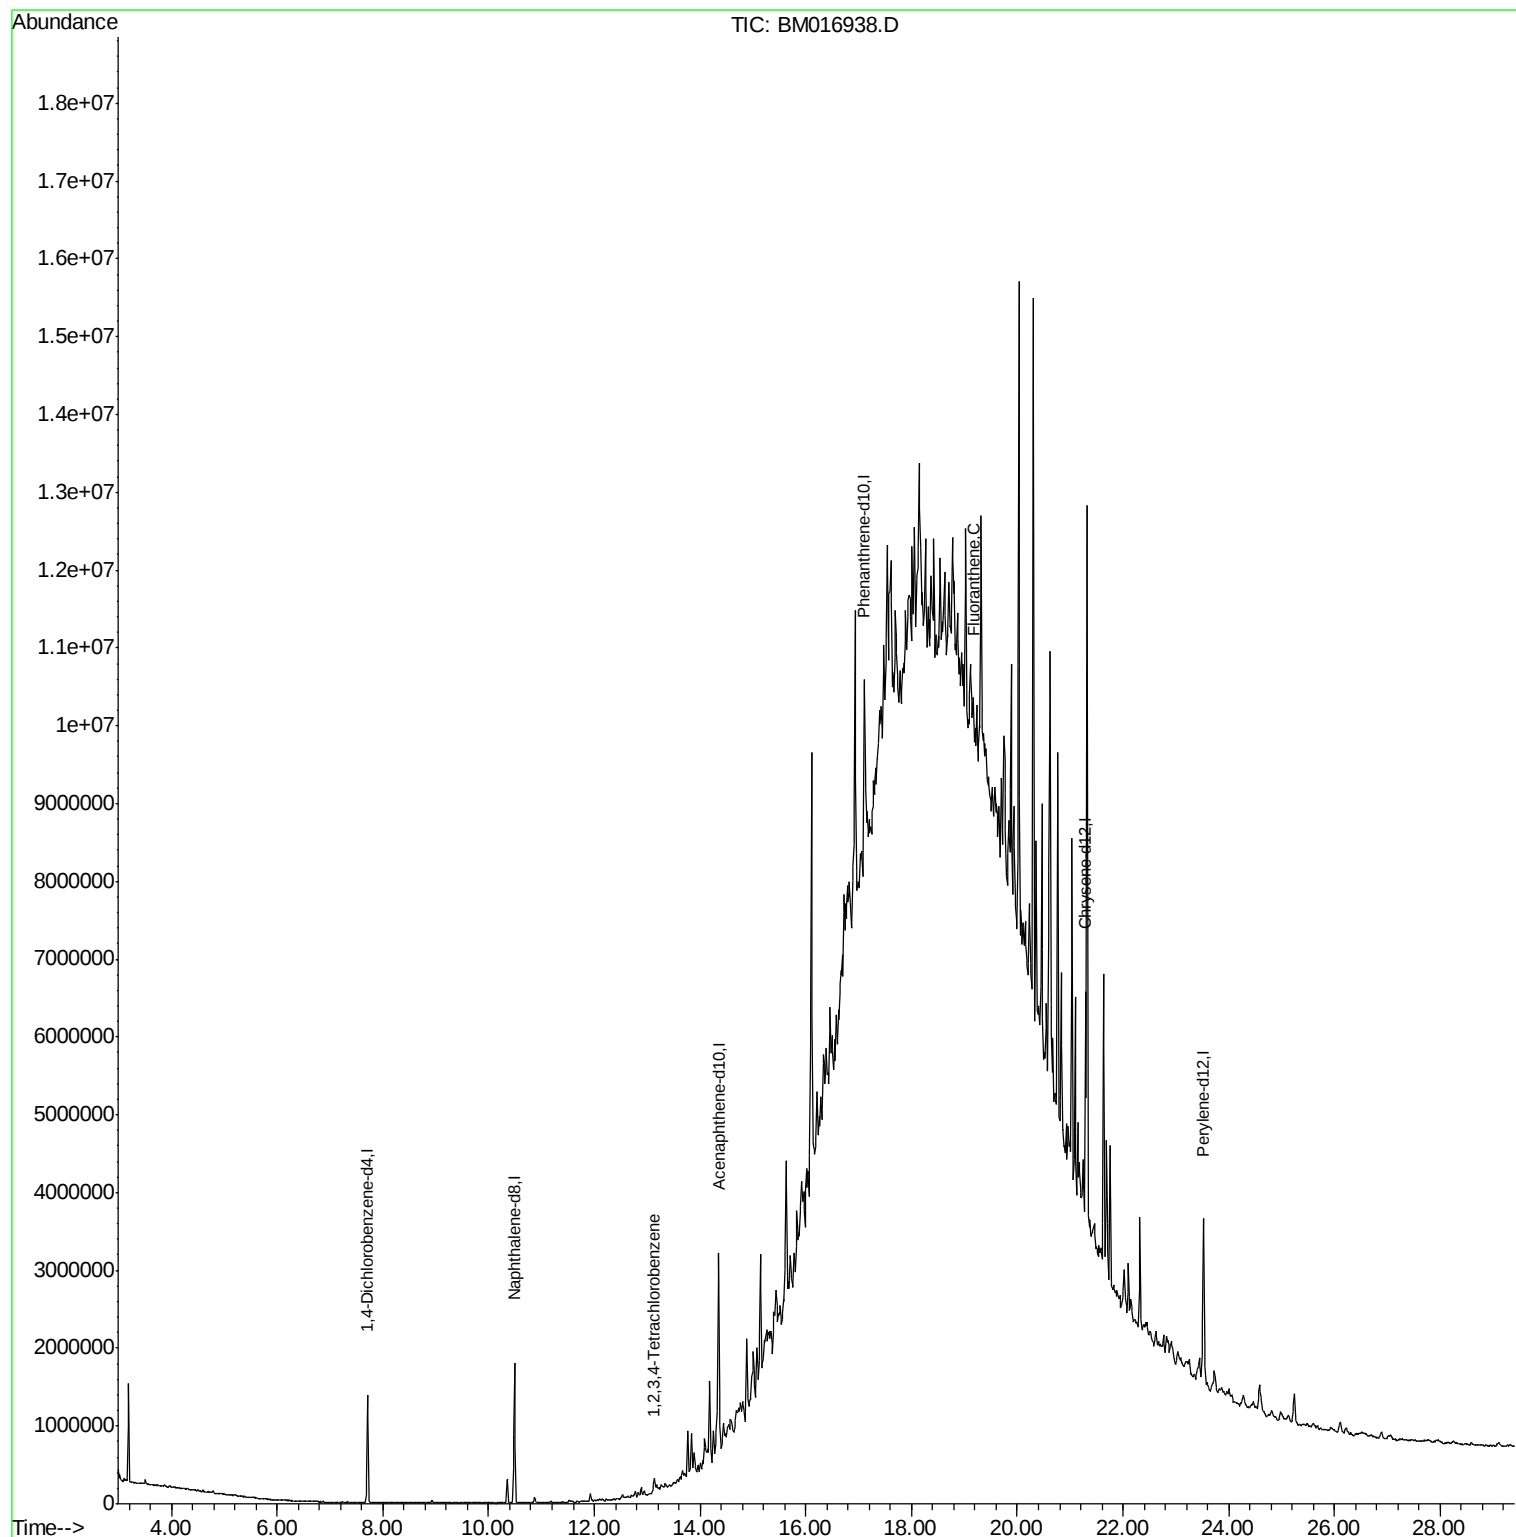

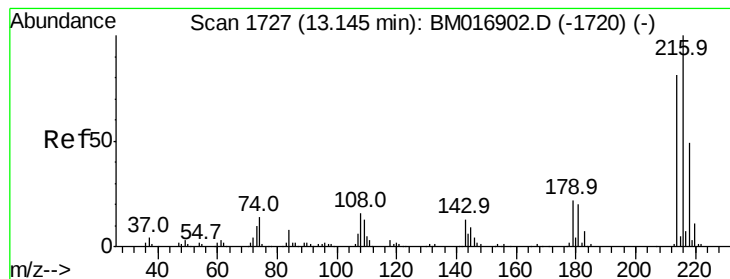

#73

1,2,3,4-Tetrachlorobenzene

Concen: 1.379 ng/uL

RT: 13.14 min Scan# 1726

Delta R.T. -0.01 min

Lab File: BM016938.D

Acq: 02 Oct 2018 01:15

Instrument :

BNA_M

ClientSampleId :

C0B71


Tot Ion:216 Resp: 32061

Ion Ratio Lower Upper

216 100

214 77.3 64.1 96.1




218 47.0 39.4 59.0

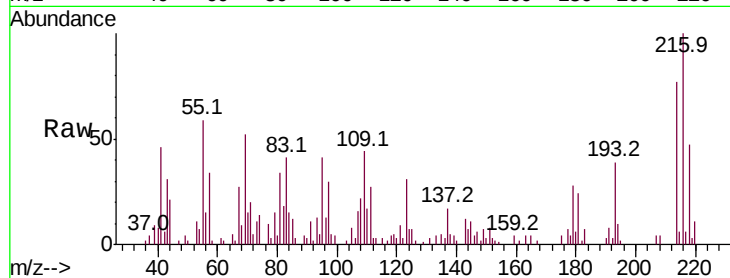

Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

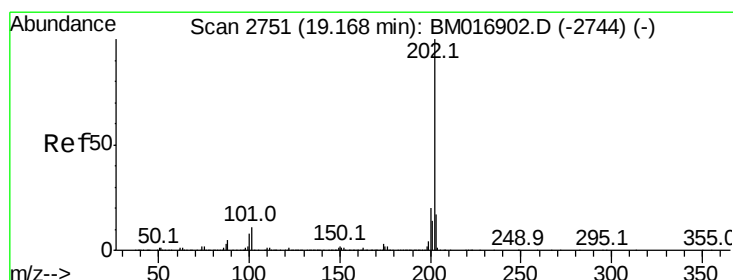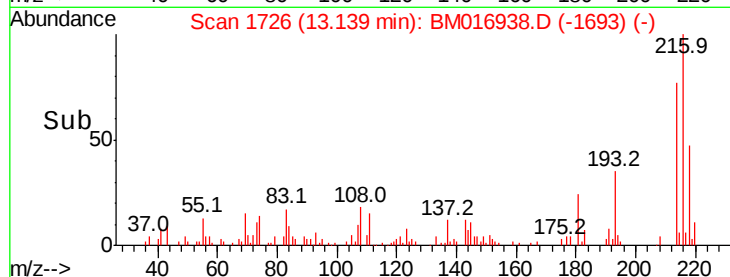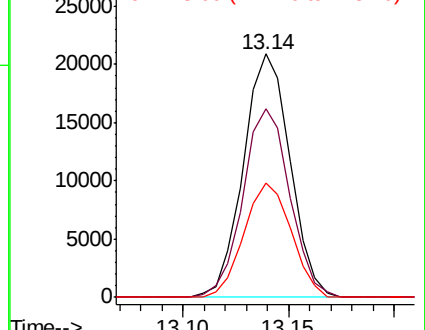

#77

Fluoranthene

Concen: 1.158 ng/uL

RT: 19.17 min Scan# 2751

Delta R.T. -0.00 min

Lab File: BM016938.D

Acq: 02 Oct 2018 01:15


Tgt Ion:202 Resp: 103518

Ion Ratio Lower Upper

202 100

101 13.8 6.1 9.1#

100 12.7 4.6 7.0#

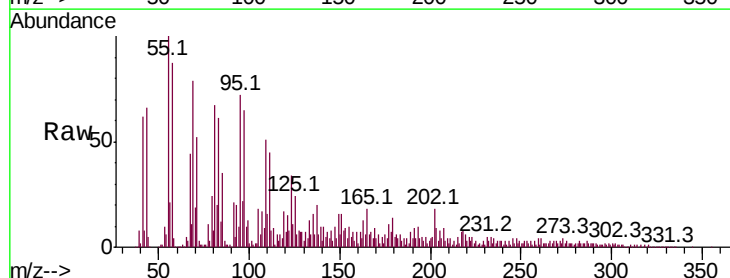

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

