

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100118\
 Data File : BM016941.D
 Acq On : 02 Oct 2018 03:04
 Operator : MJ/SJ
 Sample : J5125-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B74

Quant Time: Oct 02 09:17:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 27 02:42:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	418449	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1762881	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.35	164	864576	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1523205	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	1484099	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	1597993	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul

Target Compounds


					Qvalue
37) 1,2,4,5-Tetrachlorobenzene	12.53	216	31232	1.052 ng/ul#	95
73) 1,2,3,4-Tetrachlorobenzene	13.14	216	63971	2.538 ng/uL	96
74) Pentachlorobenzene	14.67	250	44559	1.959 ng/uL	100
85) Chrysene	21.34	228	125296	1.462 ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100118\
Data File : BM016941.D
Acq On : 02 Oct 2018 03:04
Operator : MJ/SJ
Sample : J5125-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B74

Quant Time: Oct 02 09:17:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 27 02:42:56 2018
Response via : Initial Calibration

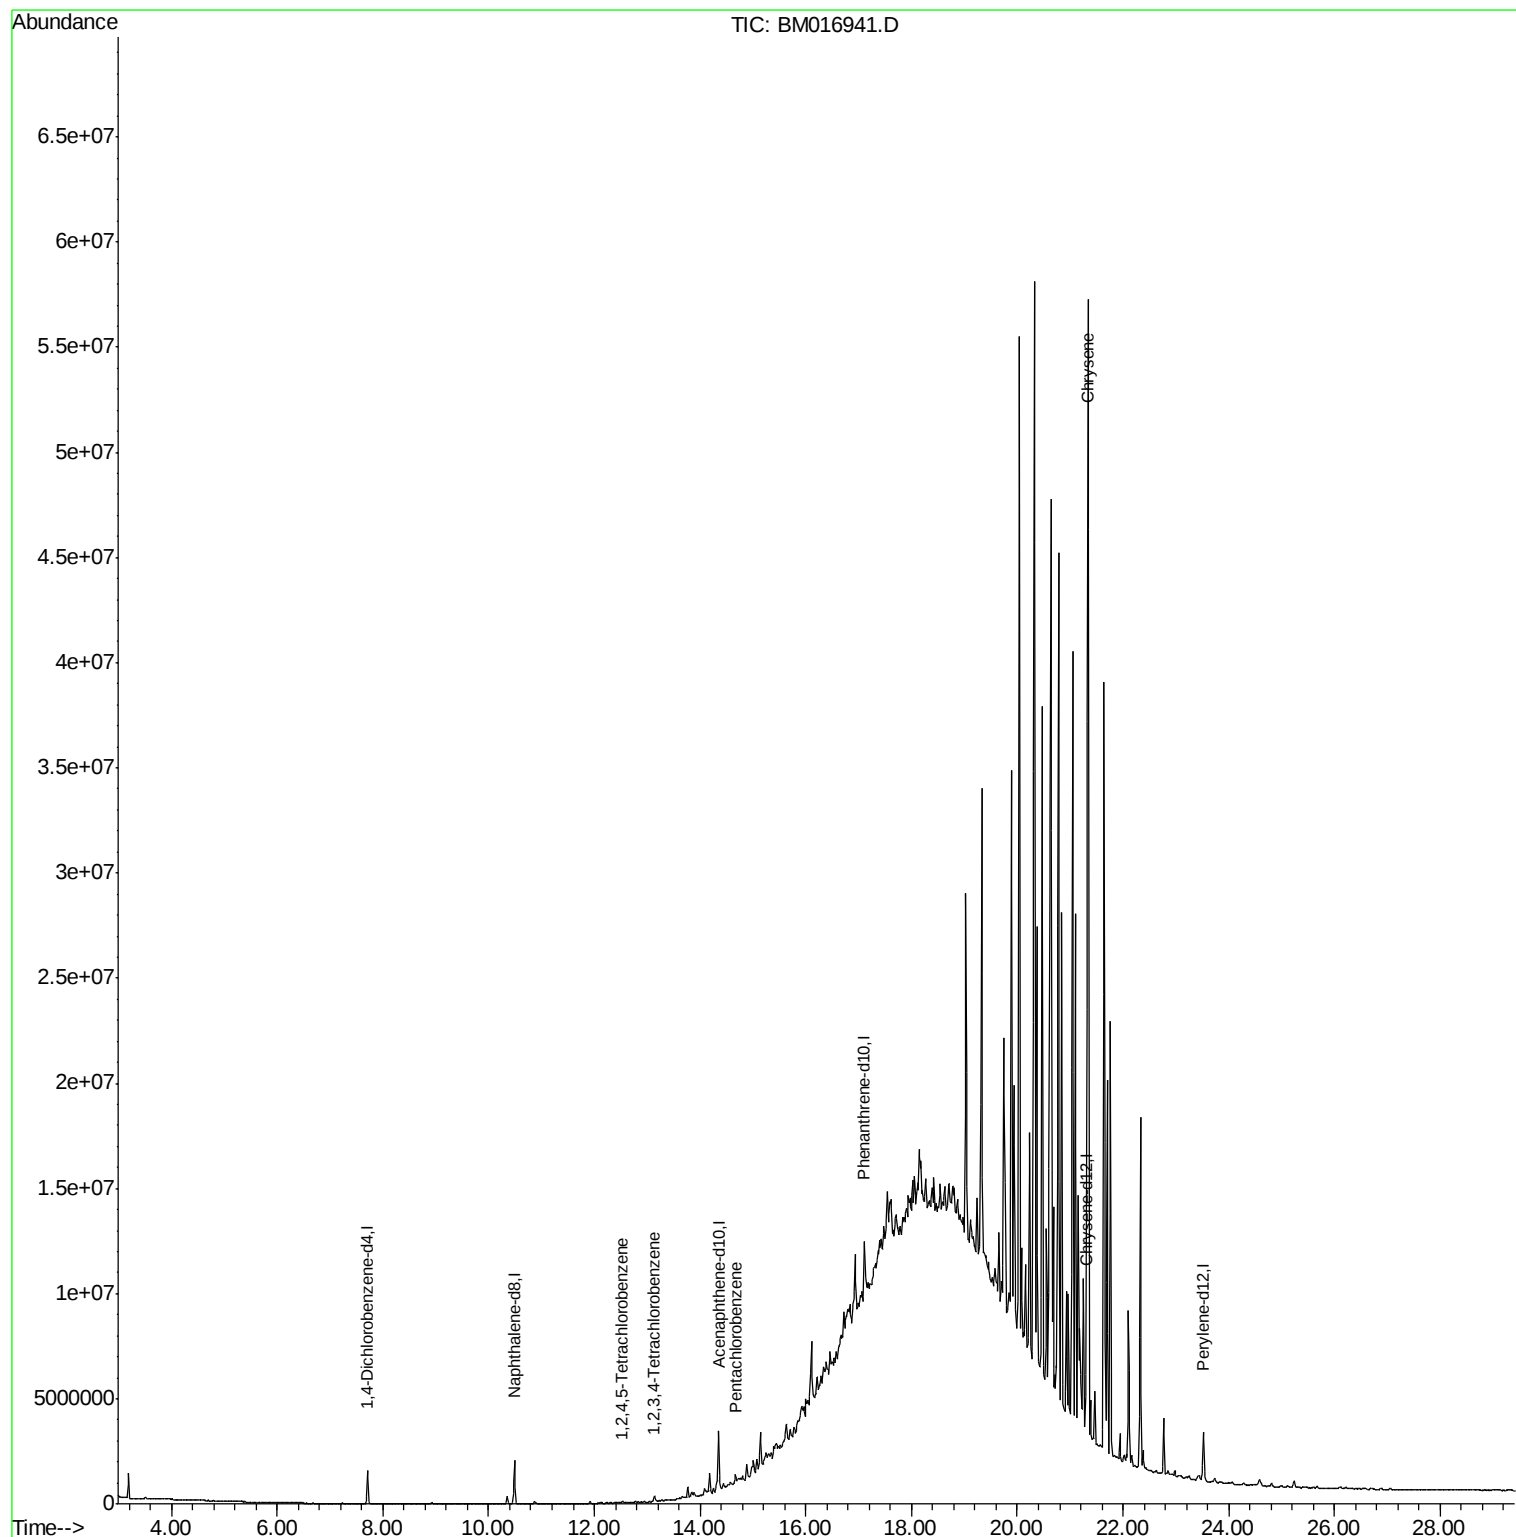


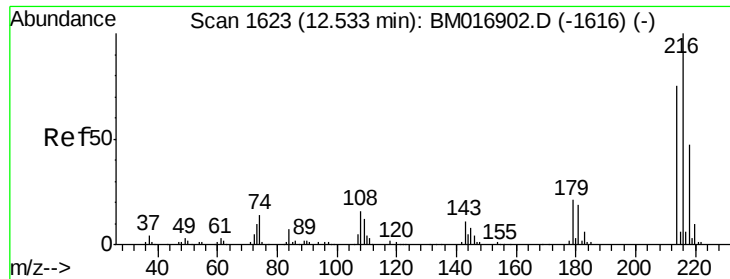




#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 1.052 ng/uL
 RT: 12.53 min Scan# 1622
 Delta R.T. -0.01 min
 Lab File: BM016941.D
 Acq: 02 Oct 2018 03:04

Instrument :
 BNA_M
 ClientSampleId :
 C0B74

Tgt Ion:	216	Resp:	31232
Ion	Ratio	Lower	Upper
216	100		
214	77.8	64.1	96.1
179	23.3	14.5	21.7#
108	16.6	10.4	15.6#

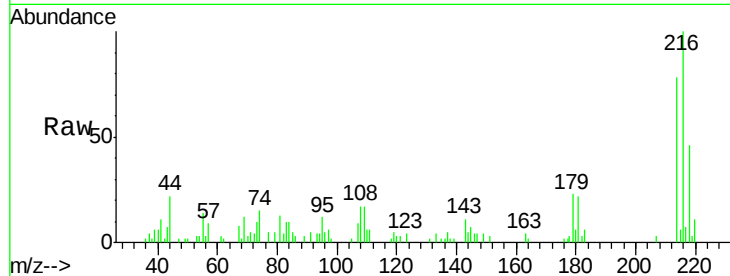


Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 108.00 (107.70 to 108.70): E

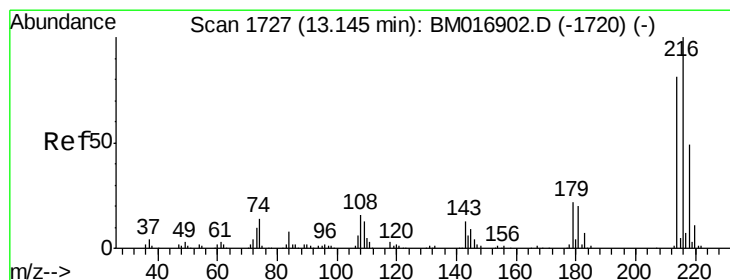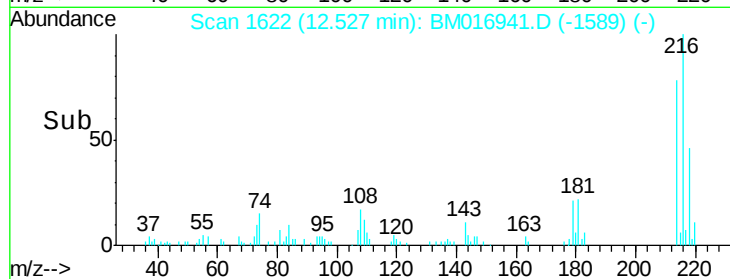
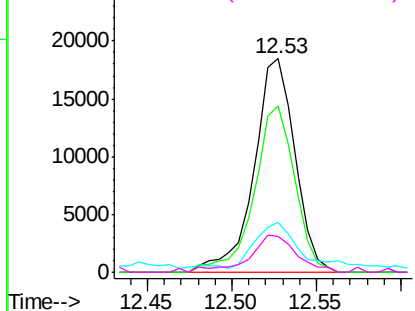



#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 2.538 ng/uL
 RT: 13.14 min Scan# 1726
 Delta R.T. -0.01 min
 Lab File: BM016941.D
 Acq: 02 Oct 2018 03:04

Tgt Ion:	216	Resp:	63971
Ion	Ratio	Lower	Upper
216	100		
214	75.8	64.1	96.1
218	47.6	39.4	59.0

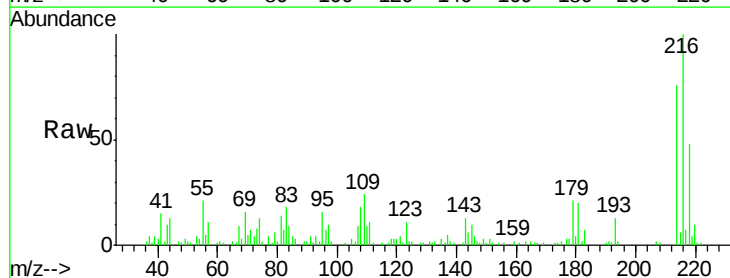

Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 218.00 (217.70 to 218.70): E



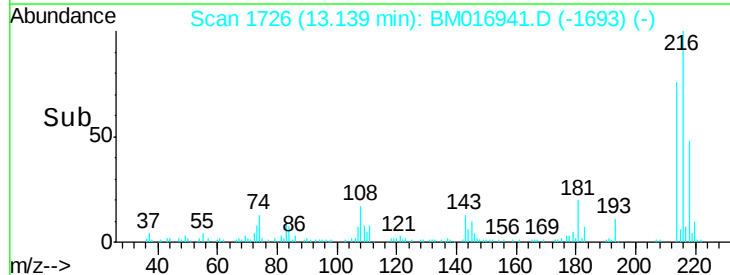
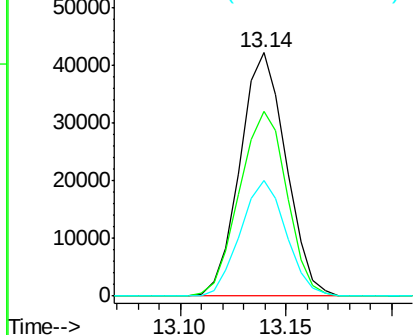


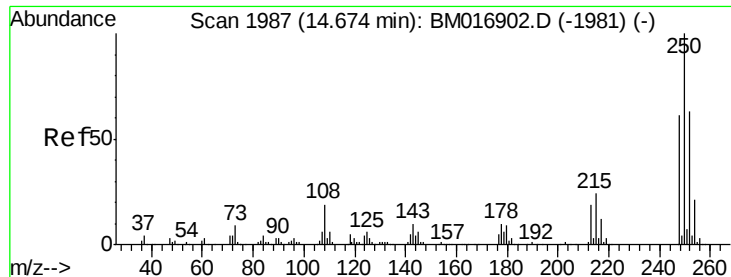

#74
 Pentachlorobenzene
 Concen: 1.959 ng/uL
 RT: 14.67 min Scan# 1986
 Delta R.T. -0.01 min
 Lab File: BM016941.D
 Acq: 02 Oct 2018 03:04

Instrument :
 BNA_M
 ClientSampleId :
 C0B74

Tgt Ion	Ratio	Lower	Upper
250	100		
248	64.5	51.4	77.2
252	61.9	49.8	74.6

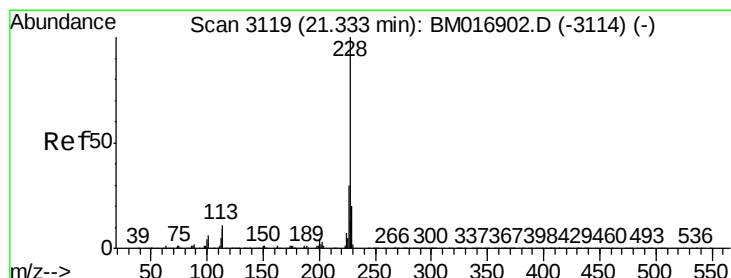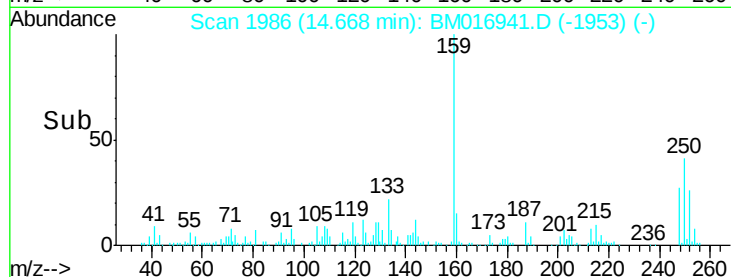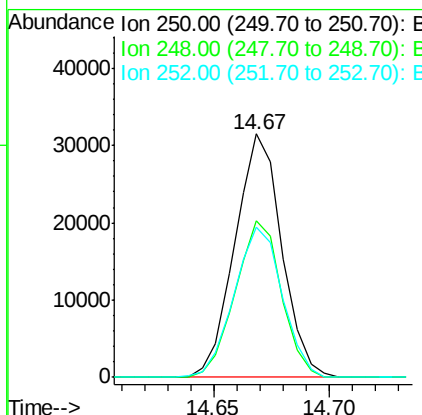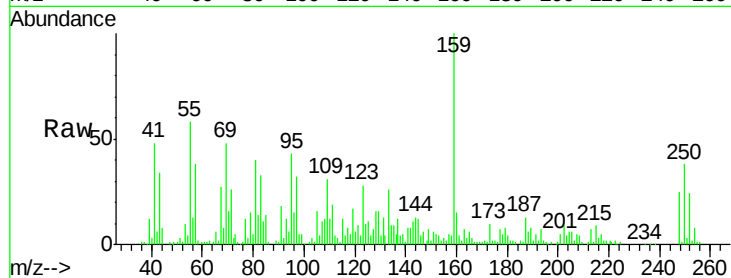

#85
 Chrysene
 Concen: 1.462 ng/uL
 RT: 21.34 min Scan# 3120
 Delta R.T. 0.01 min
 Lab File: BM016941.D
 Acq: 02 Oct 2018 03:04

Tgt Ion	Ratio	Lower	Upper
228	100		
226	40.8	24.1	36.1#
229	61.7	16.0	24.0#

