

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
 Data File : BM016933.D
 Acq On : 01 Oct 2018 22:15
 Operator : MJ/SJ
 Sample : J5124-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	40	rVB	1643251	1653724	44.77%	6.920%
2	3.516	87	90	94	rVB	73169	80476	2.18%	0.337%
3	4.593	271	273	283	rVB	56085	75418	2.04%	0.316%
4	4.787	303	306	312	rVB	133256	172746	4.68%	0.723%
5	5.104	357	360	365	rVB2	32806	41010	1.11%	0.172%
6	6.804	647	649	653	rVB4	6627	8624	0.23%	0.036%
7	7.339	734	740	742	rBV3	13153	20012	0.54%	0.084%
8	7.710	795	803	811	rBV	1175938	1830288	49.55%	7.659%
9	7.839	822	825	831	rVB5	5937	9161	0.25%	0.038%
10	7.992	845	851	854	rVB4	5096	7445	0.20%	0.031%
11	8.033	854	858	863	rBV4	4560	7186	0.19%	0.030%
12	8.216	885	889	893	rBV4	6958	12513	0.34%	0.052%
13	8.298	900	903	907	rVB4	4934	7010	0.19%	0.029%
14	8.745	976	979	983	rVB5	4744	7254	0.20%	0.030%
15	8.933	1005	1011	1016	rVB4	14150	23927	0.65%	0.100%
16	9.016	1020	1025	1028	rBV6	6083	10885	0.29%	0.046%
17	10.357	1248	1253	1256	rBV2	9307	14862	0.40%	0.062%
18	10.492	1266	1276	1282	rBV	1603026	2762590	74.79%	11.561%
19	10.539	1282	1284	1288	rVB	25964	31380	0.85%	0.131%
20	10.657	1300	1304	1309	rVB4	3624	5703	0.15%	0.024%
21	11.327	1413	1418	1425	rVB7	4940	9250	0.25%	0.039%
22	11.410	1430	1432	1437	rVB4	6030	8538	0.23%	0.036%
23	11.516	1443	1450	1454	rBV4	7925	13226	0.36%	0.055%
24	11.921	1512	1519	1525	rVB	66137	95370	2.58%	0.399%
25	12.157	1554	1559	1564	rBV2	17260	26895	0.73%	0.113%
26	12.374	1593	1596	1602	rBV3	8112	11261	0.30%	0.047%
27	12.610	1631	1636	1640	rBV6	3239	6357	0.17%	0.027%
28	12.827	1669	1673	1680	rBV6	3848	7021	0.19%	0.029%
29	13.180	1728	1733	1740	rVB2	24486	35577	0.96%	0.149%
30	13.510	1783	1789	1791	rBV4	5430	7471	0.20%	0.031%
31	13.674	1811	1817	1819	rBV4	6314	10514	0.28%	0.044%
32	13.768	1830	1833	1837	rVB5	4631	6662	0.18%	0.028%
33	13.839	1840	1845	1849	rVB6	7319	11146	0.30%	0.047%
34	13.898	1849	1855	1859	rBV4	6251	14332	0.39%	0.060%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
Data File : BM016933.D
Acq On : 01 Oct 2018 22:15
Operator : MJ/SJ
Sample : J5124-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B61

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Title : SVOA CALIBRATION

35	14.004	1869	1873	1877	rBV7	6991	11996	0.32%	0.050%
36	14.080	1880	1886	1889	rBV2	14788	27751	0.75%	0.116%
37	14.180	1899	1903	1911	rVB7	14322	24833	0.67%	0.104%
38	14.262	1911	1917	1921	rBV7	13427	26462	0.72%	0.111%
39	14.351	1921	1932	1940	rBV2	2348717	3591343	97.23%	15.029%
40	14.880	2019	2022	2029	rBV3	60714	94140	2.55%	0.394%
41	15.139	2062	2066	2070	rBV2	117199	198118	5.36%	0.829%
42	15.427	2107	2115	2117	rBV6	101787	289764	7.84%	1.213%
43	17.103	2396	2400	2404	rBV2	2595499	3693737	100.00%	15.457%
44	19.162	2747	2750	2754	rVB	1454396	1723202	46.65%	7.211%
45	21.286	3107	3111	3115	rBV2	2575911	3563695	96.48%	14.913%
46	23.521	3486	3491	3499	rVB2	1847662	3605501	97.61%	15.088%


Sum of corrected areas: 23896376

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
Data File : BM016933.D
Acq On : 01 Oct 2018 22:15
Operator : MJ/SJ
Sample : J5124-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B61

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

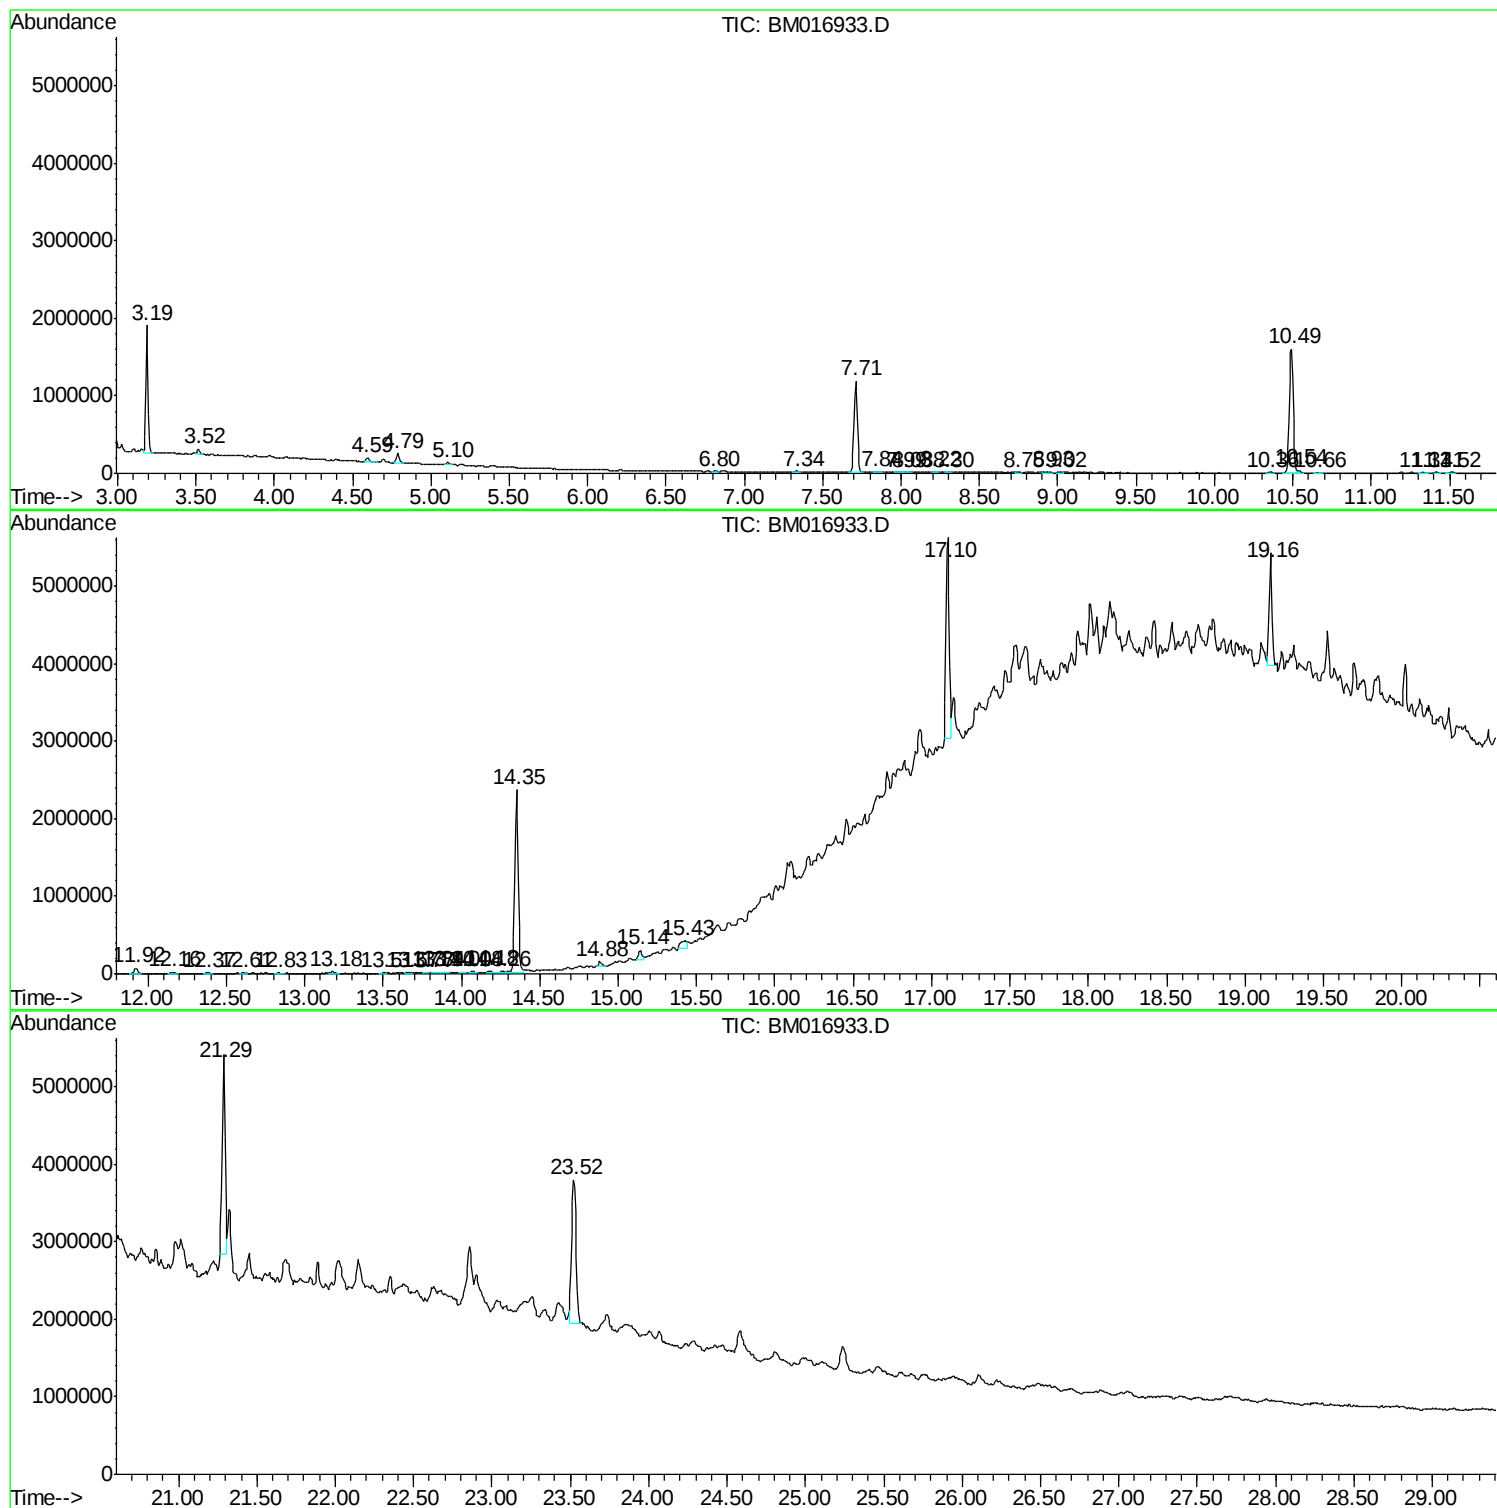

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
Data File : BM016933.D
Acq On : 01 Oct 2018 22:15
Operator : MJ/SJ
Sample : J5124-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B61










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.19	18.07 ng/ul	1653720	1,4-Dichlorobenzene-d4	7.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	91
2		Heptane	100	C7H16	000142-82-5	90
3		Heptane	100	C7H16	000142-82-5	90
4		Heptane	100	C7H16	000142-82-5	87
5		Pentane, 3,3-dimethyl-	100	C7H16	000562-49-2	40

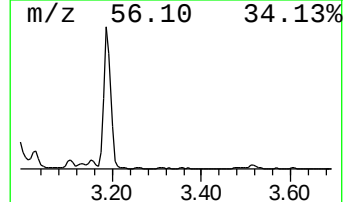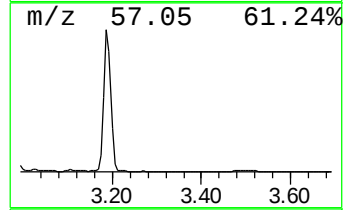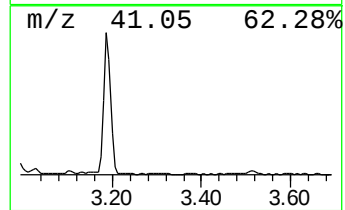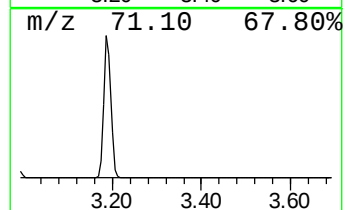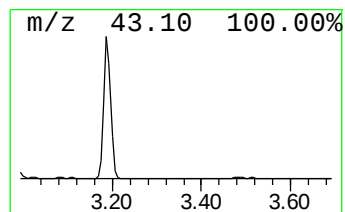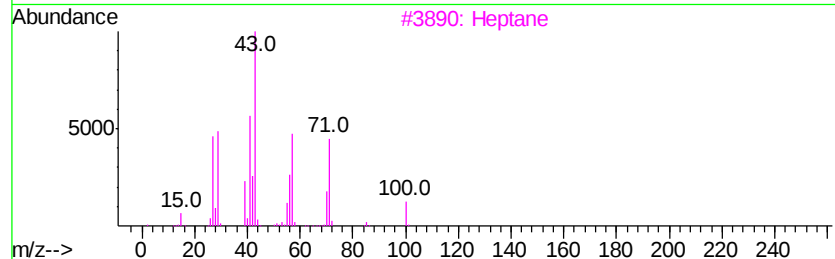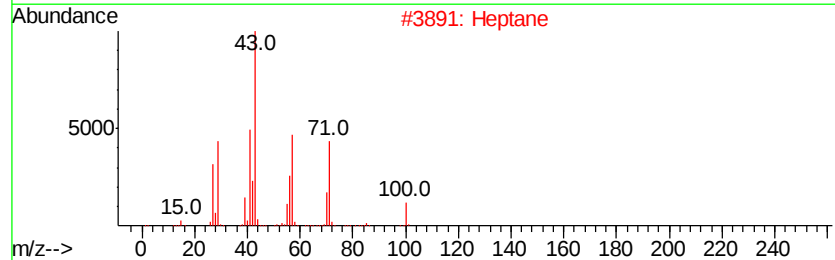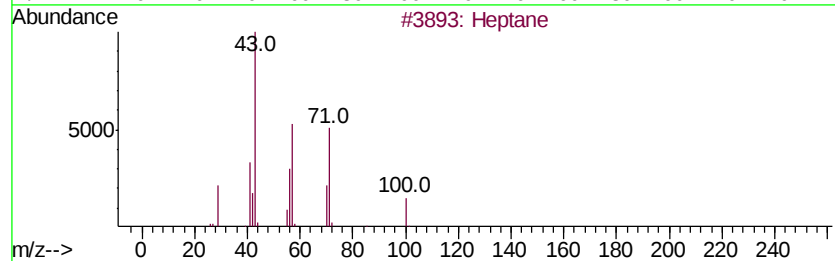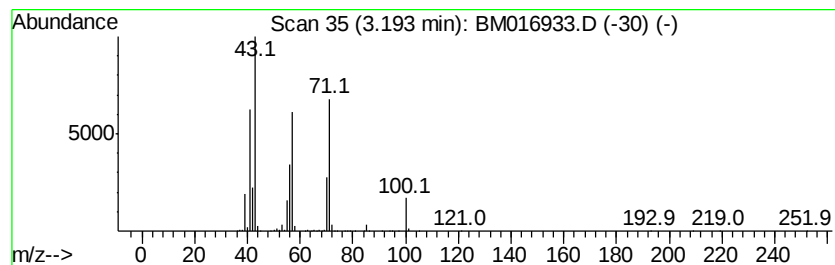

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100118\
Data File : BM016933.D
Acq On : 01 Oct 2018 22:15
Operator : MJ/SJ
Sample : J5124-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B61

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.19	18.1	ng/ul	1653720	1	7.71	1830290	20.0