

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
 Data File : BM016942.D
 Acq On : 02 Oct 2018 03:40
 Operator : MJ/SJ
 Sample : J5125-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	39	rVB	1310617	1346522	28.51%	5.483%
2	7.563	776	778	782	rVB5	3835	5701	0.12%	0.023%
3	7.710	795	803	813	rBV	1381468	2132218	45.15%	8.683%
4	8.028	852	857	864	rVB4	5634	10225	0.22%	0.042%
5	8.928	1003	1010	1015	rBV5	4917	10523	0.22%	0.043%
6	10.351	1245	1252	1257	rBV5	5524	9493	0.20%	0.039%
7	10.486	1263	1275	1284	rBV	1839483	3144891	66.59%	12.806%
8	10.628	1293	1299	1302	rBV6	4411	8087	0.17%	0.033%
9	10.745	1314	1319	1327	rVB5	7075	12099	0.26%	0.049%
10	10.951	1351	1354	1359	rVB4	6245	10109	0.21%	0.041%
11	11.922	1513	1519	1525	rBV3	12539	22020	0.47%	0.090%
12	13.174	1729	1732	1737	rVB3	4523	6655	0.14%	0.027%
13	13.669	1811	1816	1818	rBV5	4591	6318	0.13%	0.026%
14	13.769	1827	1833	1837	rBV4	19627	31890	0.68%	0.130%
15	13.839	1841	1845	1848	rVB5	9415	14629	0.31%	0.060%
16	13.957	1862	1865	1869	rVB4	5731	6450	0.14%	0.026%
17	13.992	1869	1871	1877	rBV6	5018	9374	0.20%	0.038%
18	14.092	1883	1888	1891	rBV7	9175	16170	0.34%	0.066%
19	14.145	1894	1897	1899	rVV4	5365	6621	0.14%	0.027%
20	14.180	1899	1903	1910	rVB5	36272	57372	1.21%	0.234%
21	14.257	1911	1916	1919	rBV6	10771	18700	0.40%	0.076%
22	14.351	1921	1932	1941	rBV2	2719122	4248353	89.95%	17.300%
23	14.445	1943	1948	1952	rVB8	8890	18528	0.39%	0.075%
24	14.516	1957	1960	1963	rBV5	6594	10840	0.23%	0.044%
25	14.686	1984	1989	1991	rBV5	8161	16250	0.34%	0.066%
26	14.886	2018	2023	2030	rBV6	28930	56642	1.20%	0.231%
27	14.974	2035	2038	2040	rBV4	11178	15418	0.33%	0.063%
28	15.074	2049	2055	2060	rBV9	23070	55512	1.18%	0.226%
29	15.139	2062	2066	2070	rVV4	48702	75598	1.60%	0.308%
30	15.621	2145	2148	2154	rVB2	38646	65559	1.39%	0.267%
31	16.004	2211	2213	2215	rBV2	29777	25957	0.55%	0.106%
32	16.098	2226	2229	2234	rVB	157736	216005	4.57%	0.880%
33	16.921	2366	2369	2376	rVB	255324	356889	7.56%	1.453%
34	17.098	2394	2399	2408	rBV2	3004530	4723029	100.00%	19.233%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
Data File : BM016942.D
Acq On : 02 Oct 2018 03:40
Operator : MJ/SJ
Sample : J5125-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B75

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Title : SVOA CALIBRATION

35	21.286	3107	3111	3115	rBV	3010373	3965901	83.97%	16.150%
36	23.521	3485	3491	3500	rVB	1968809	3820594	80.89%	15.558%


Sum of corrected areas: 24557142

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
Data File : BM016942.D
Acq On : 02 Oct 2018 03:40
Operator : MJ/SJ
Sample : J5125-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B75

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

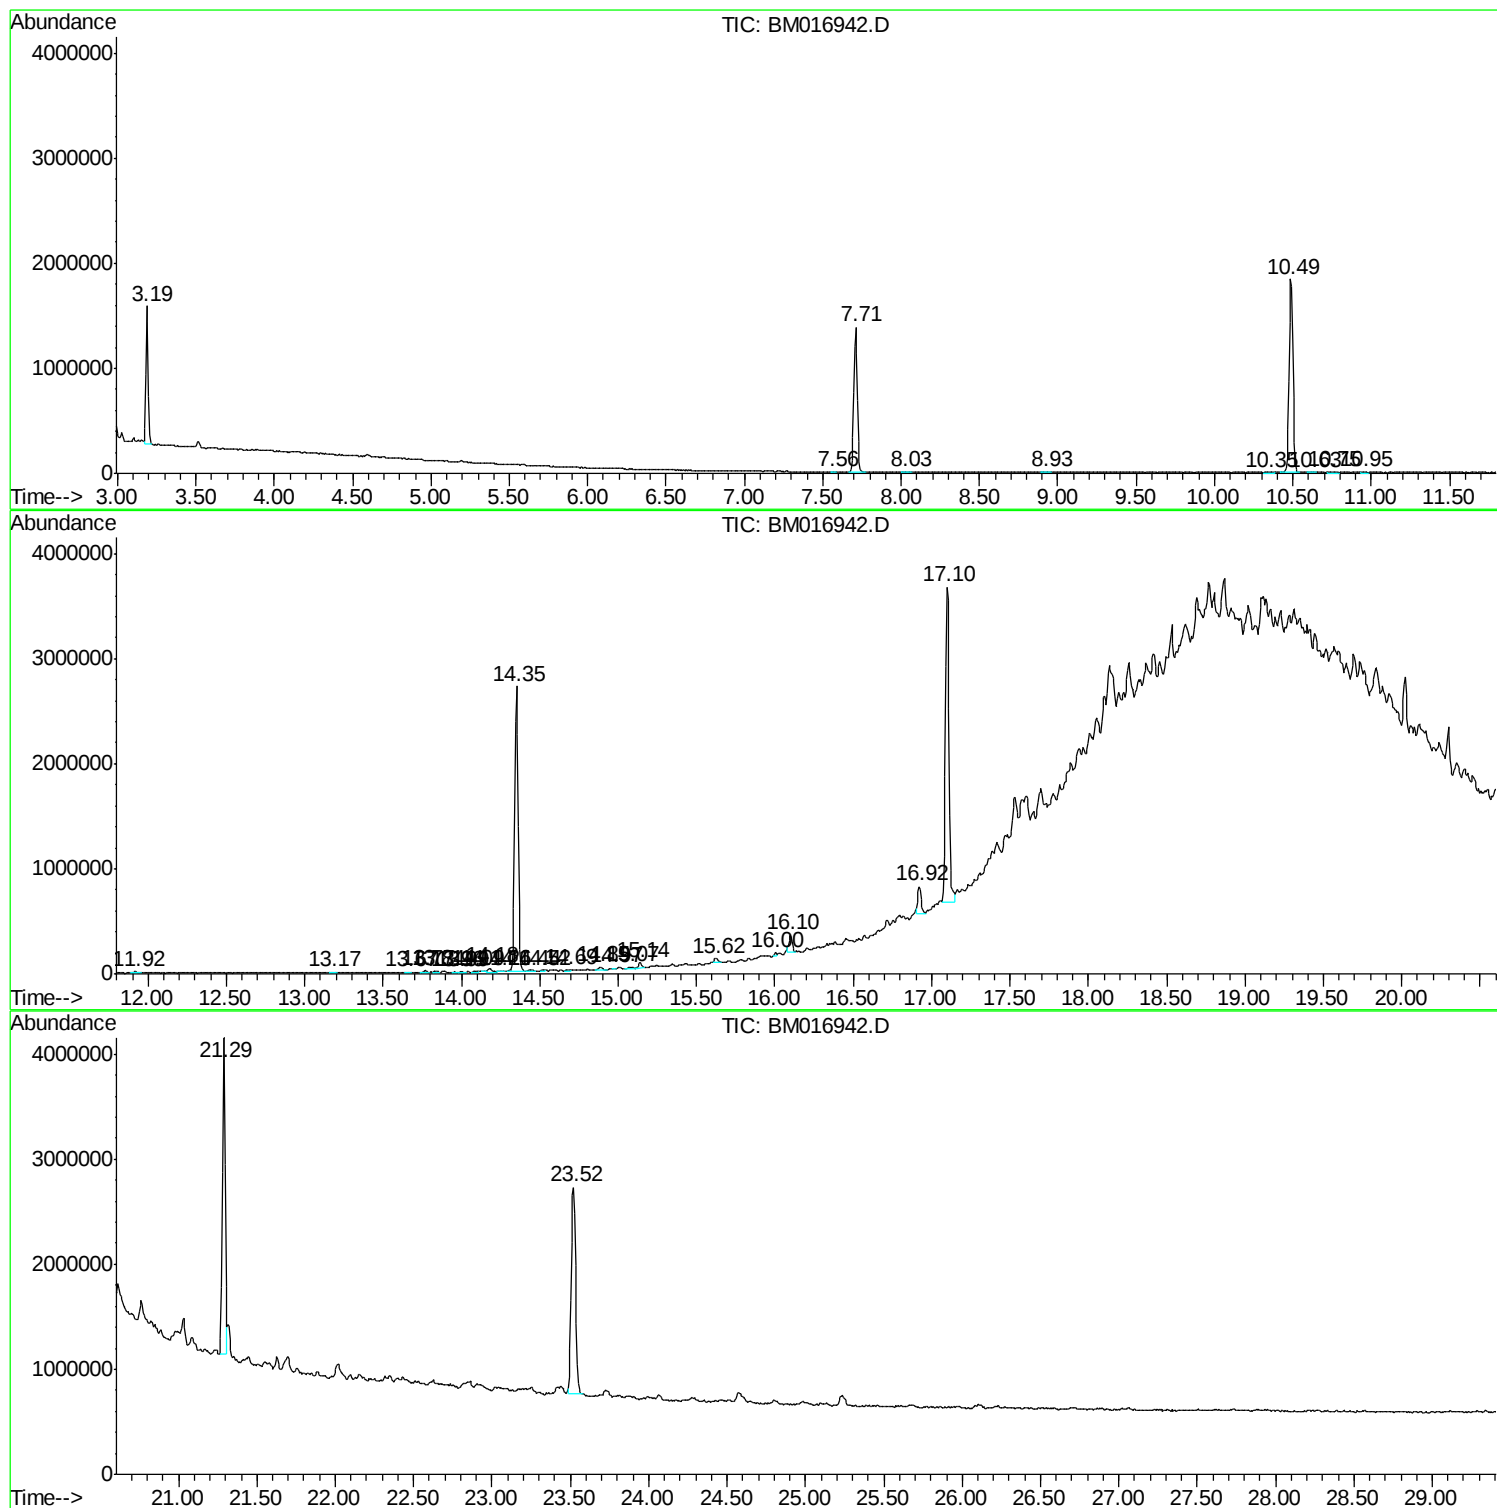

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100118\
Data File : BM016942.D
Acq On : 02 Oct 2018 03:40
Operator : MJ/SJ
Sample : J5125-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B75










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.19	12.63 ng/ul	1346520	1,4-Dichlorobenzene-d4	7.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	91
2		Heptane	100	C7H16	000142-82-5	91
3		Heptane	100	C7H16	000142-82-5	91
4		Heptane	100	C7H16	000142-82-5	87
5		Butane, 2,2-dimethyl-	86	C6H14	000075-83-2	38

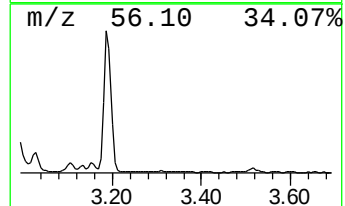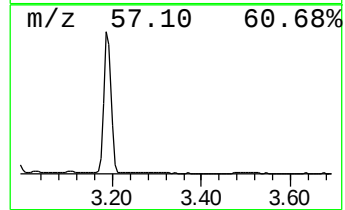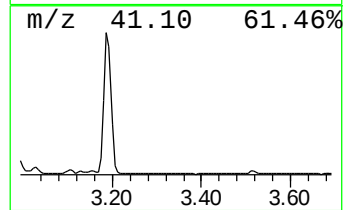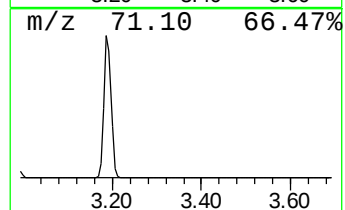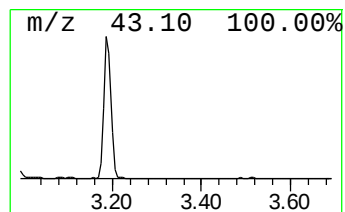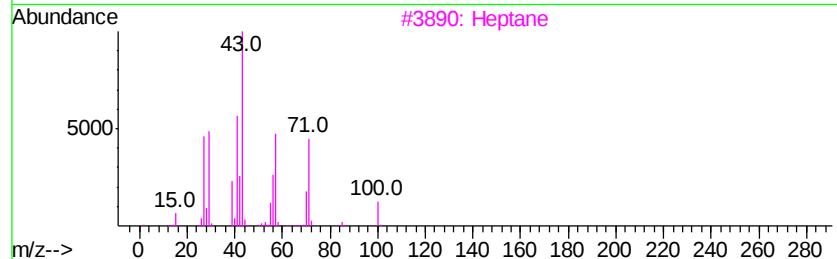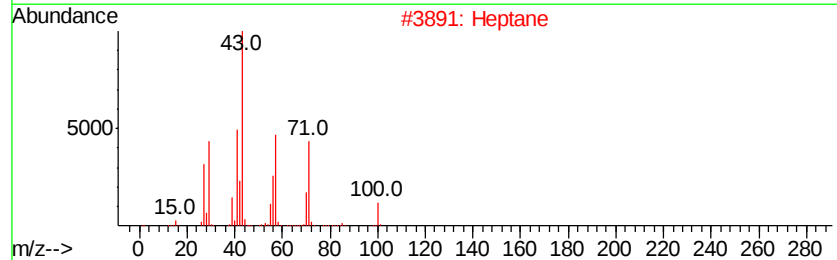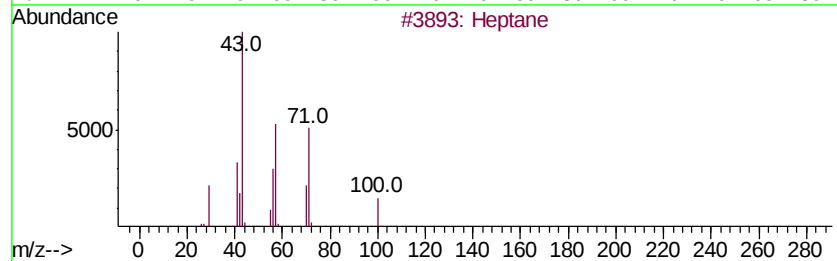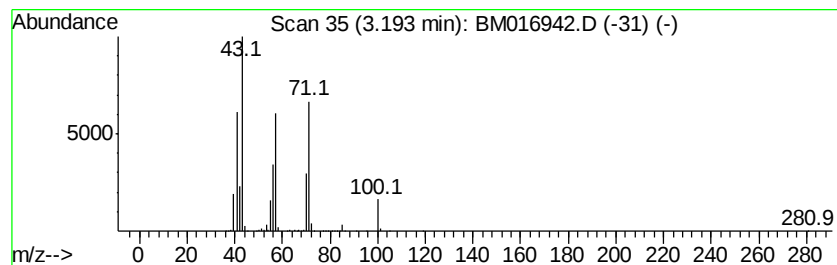

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100118\
Data File : BM016942.D
Acq On : 02 Oct 2018 03:40
Operator : MJ/SJ
Sample : J5125-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B75

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.19	12.6	ng/ul	1346520	1	7.71	2132220	20.0