

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100119\
 Data File : BM022862.D
 Acq On : 01 Oct 2019 19:52
 Operator : JU
 Sample : K4983-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 02 01:09:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 27 18:03:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	216772	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	980978	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.44	164	632294	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.18	188	1310521	20.00	ng/ul	0.00
78) Chrysene-d12	21.36	240	1258354	20.00	ng/ul	-0.01
86) Perylene-d12	23.62	264	1136647	20.00	ng/ul	-0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.27	96	24458	4.88	ng/uL	0.00
5) Phenol-d5	6.97	99	124651	6.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	268820	25.64	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.33	132	321239	20.83	ng/ul	-0.01
13) 4-Methylphenol-d8	8.50	113	232089	14.80	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	195939	25.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	216947	26.24	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.22	165	397287	24.14	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.73	131	518922	25.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.85	166	1409304	28.72	ng/ul	0.00
47) Acenaphthylene-d8	14.13	160	1537224	27.13	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	73019	7.53	ng/ul	0.00
58) Fluorene-d10	15.43	176	1166965	27.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.54	200	224561	26.33	ng/ul	-0.01
71) Anthracene-d10	17.27	188	2031848	31.75	ng/ul	-0.01
79) Pyrene-d10	19.57	212	2357177	34.80	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.48	264	1987402	33.80	ng/ul	-0.02


Target Compounds				Ovalue		
4) Benzaldehyde	6.96	77	11327	1.305	ng/ul#	1
6) Phenol	6.99	94	33617	1.674	ng/ul	98
11) 2-Methylphenol	8.25	108	87200	5.635	ng/ul	99
14) Acetophenone	8.61	105	40927	1.707	ng/ul#	42
16) 4-Methylphenol	8.57	108	150618	8.802	ng/ul	94
17) Hexachloroethane	8.91	117	28010	4.455	ng/ul#	6
24) 2,4-Dimethylphenol	9.77	107	231061	12.551	ng/ul	100
28) Naphthalene	10.65	128	332002	6.267	ng/ul	99
34) 2-Methylnaphthalene	12.26	142	223430	5.625	ng/ul	99
35) 1-Methylnaphthalene	12.47	142	165426	4.361	ng/ul	99
45) Dimethylphthalate	13.89	163	70256	1.394	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100119\
Data File : BM022862.D
Acq On : 01 Oct 2019 19:52
Operator : JU
Sample : K4983-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 02 01:09:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 27 18:03:27 2019
Response via : Initial Calibration

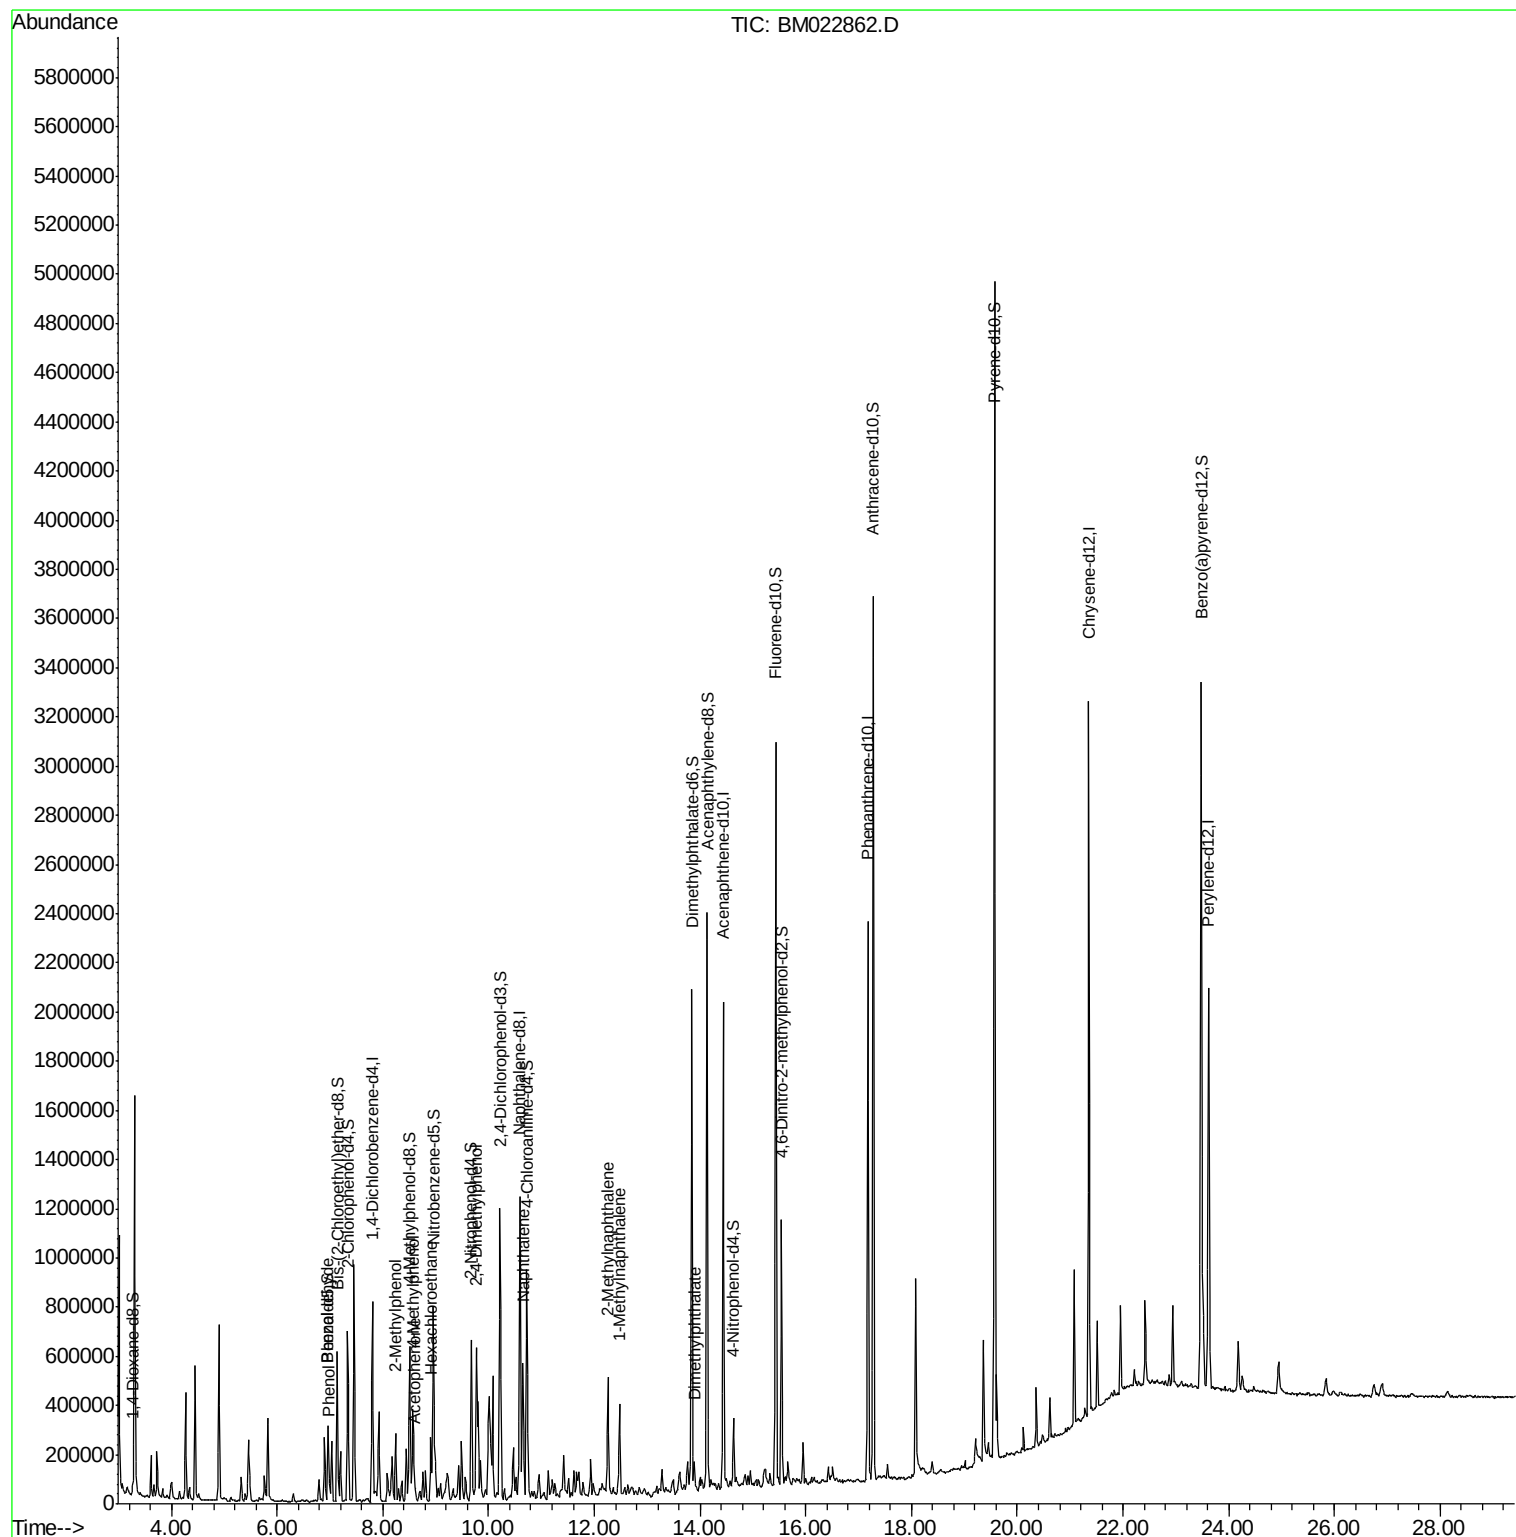

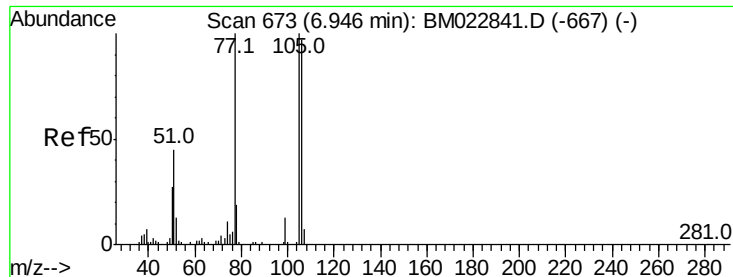

#4

Benzaldehyde

Concen: 1.305 ng/ul

RT: 6.96 min Scan# 675

Delta R.T. 0.01 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 77 Resp: 11327

Ion Ratio Lower Upper

77 100

105 754.2 80.6 120.8#




106 80.6 77.0 115.6

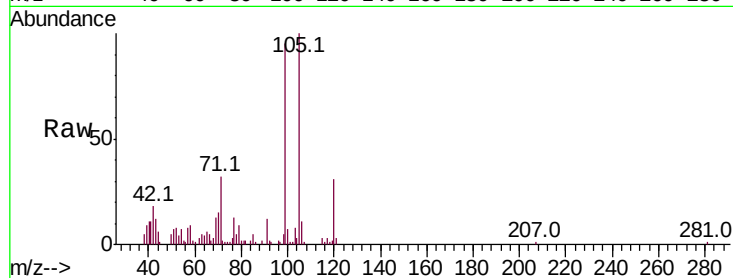

Abundance Ion 77.00 (76.70 to 77.70): BM022841.D (-667) (-)

Ion 105.00 (104.70 to 105.70): BM022841.D (-667) (-)

Ion 106.00 (105.70 to 106.70): BM022841.D (-667) (-)

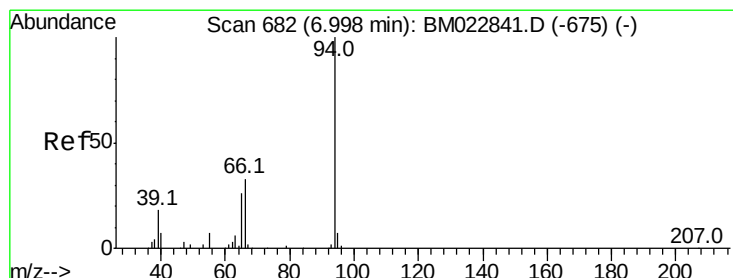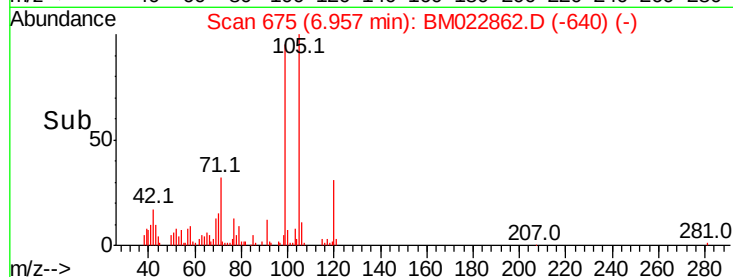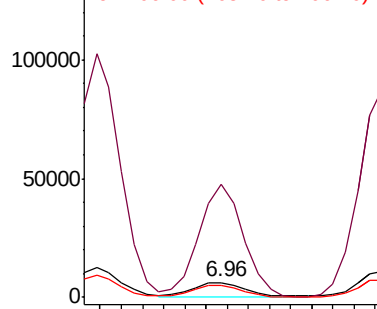

#6

Phenol

Concen: 1.674 ng/ul

RT: 6.99 min Scan# 681

Delta R.T. -0.01 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52


Tgt Ion: 94 Resp: 33617

Ion Ratio Lower Upper

94 100

65 26.8 20.9 31.3



66 35.9 27.2 40.8

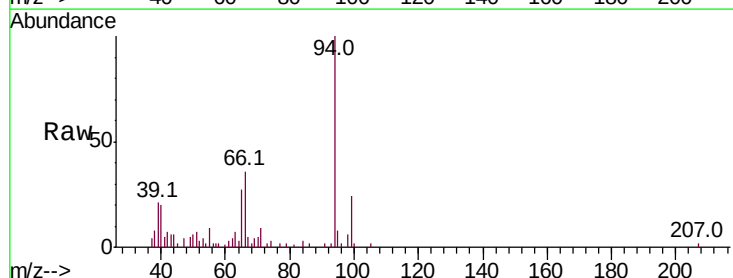


Abundance Ion 94.00 (93.70 to 94.70): BM022841.D (-675) (-)

Ion 65.00 (64.70 to 65.70): BM022841.D (-675) (-)

Ion 66.00 (65.70 to 66.70): BM022841.D (-675) (-)

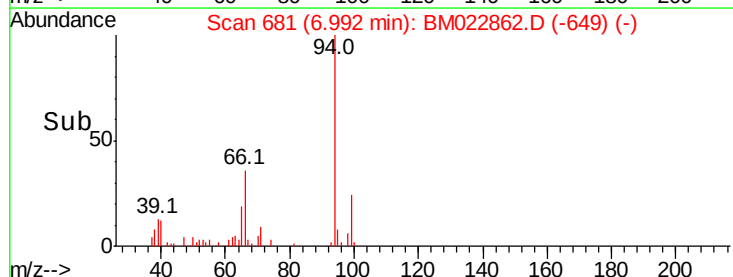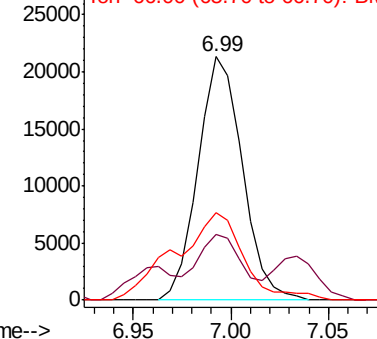

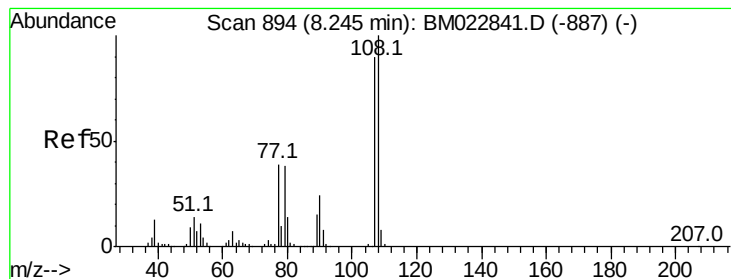

#11

2-Methylphenol

Concen: 5.635 ng/ul

RT: 8.25 min Scan# 894

Delta R.T. -0.01 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52

Instrument :

BNA_M


ClientSampleId :

Tot Ion:108 Resp: 87200

Ion Ratio Lower Upper

108 100

107 87.4 71.0 106.4

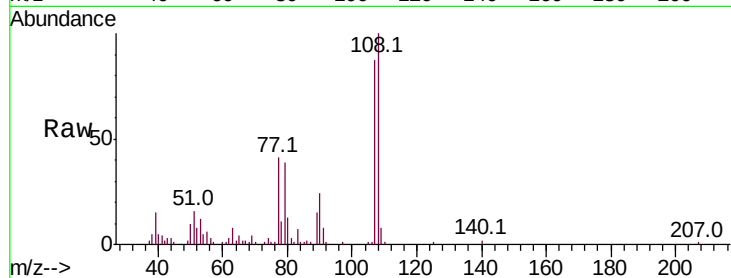

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

60000

50000

40000

30000



20000

10000

0

8.20 8.25 8.30

Time-->

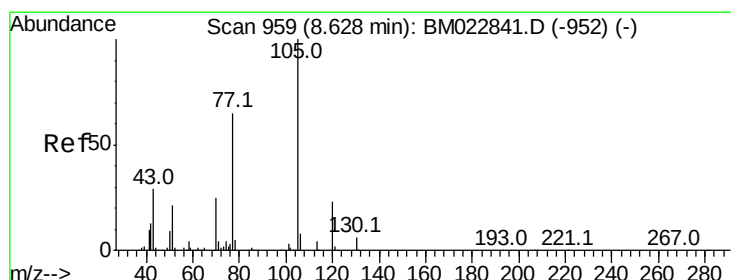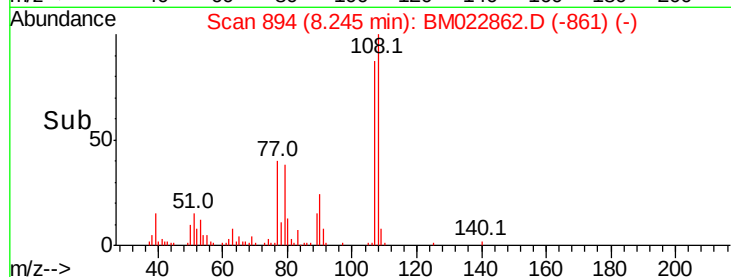

#14

Acetophenone

Concen: 1.707 ng/ul

RT: 8.61 min Scan# 956

Delta R.T. -0.02 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52


Tgt Ion:105 Resp: 40927

Ion Ratio Lower Upper

105 100

77 18.5 59.4 89.0#

51 6.8 19.4 29.0#

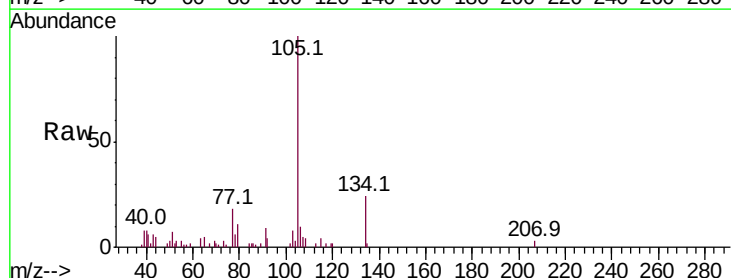

Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 51.00 (50.70 to 51.70): BM0

40000

30000


20000


10000

0

8.55 8.60 8.65

Time-->

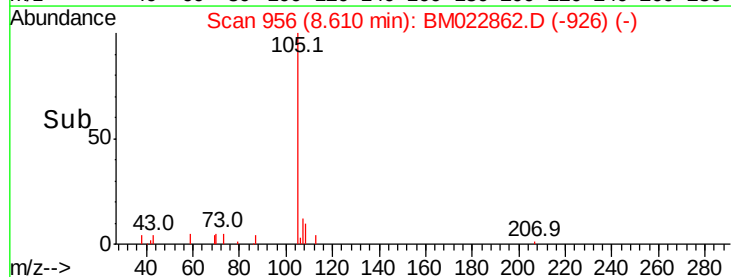

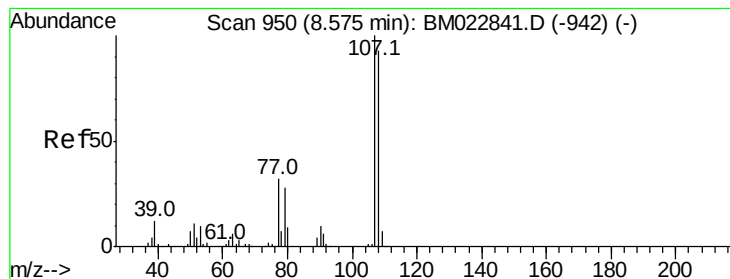

#16

4-Methylphenol

Concen: 8.802 ng/ul

RT: 8.57 min Scan# 949

Delta R.T. -0.01 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52

Instrument :

BNA_M


ClientSampleId :

Tot Ion:108 Resp: 150618

Ion Ratio Lower Upper

108 100

107 103.4 87.9 131.9

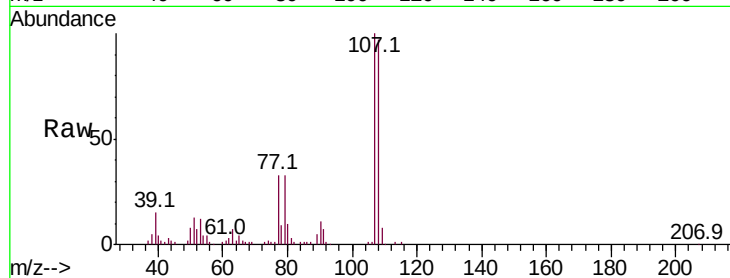

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

8.57

100000

80000

60000



40000

20000

0

Time-->

8.50 8.55 8.60 8.65

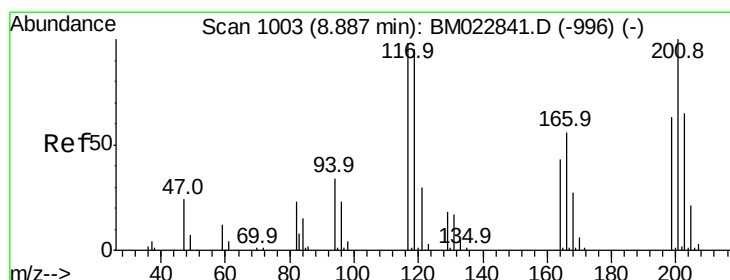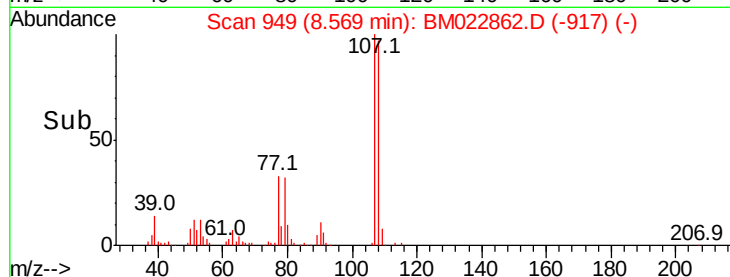

#17

Hexachloroethane

Concen: 4.455 ng/ul

RT: 8.91 min Scan# 1007

Delta R.T. 0.02 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52


Tgt Ion:117 Resp: 28010

Ion Ratio Lower Upper

117 100

201 0.0 82.5 123.7#

199 0.0 51.6 77.4#

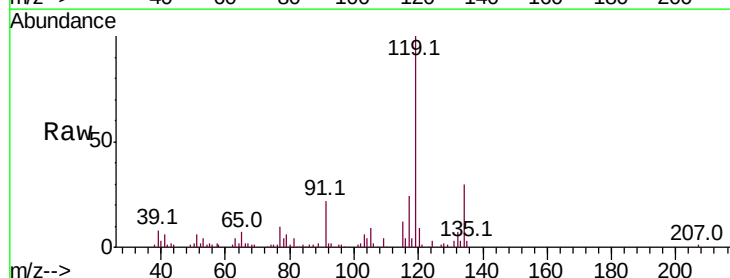

Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

60000

50000

40000

30000


20000


10000

0

Time-->

8.85 8.90 8.95

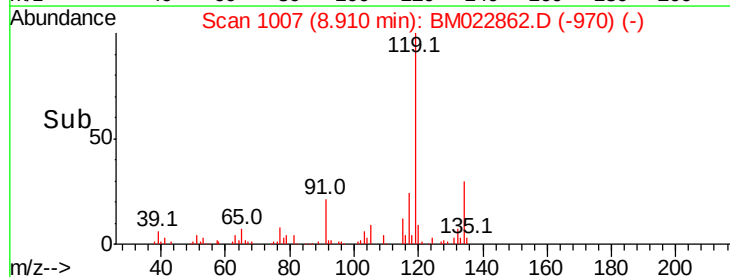

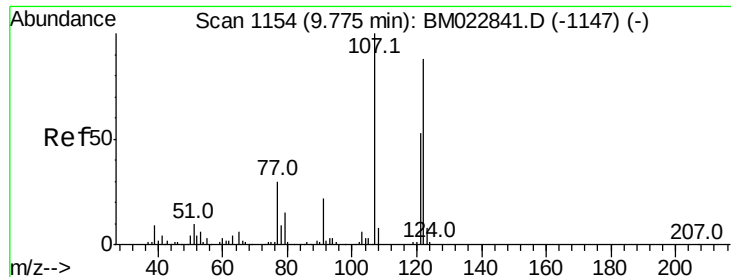

#24

2,4-Dimethylphenol

Concen: 12.551 ng/ul

RT: 9.77 min Scan# 1153

Delta R.T. -0.01 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52

Instrument :

BNA_M

ClientSampleId :


Tot Ion:107 Resp: 231061

Ion Ratio Lower Upper

107 100

121 53.1 43.0 64.4




122 89.3 71.4 107.0

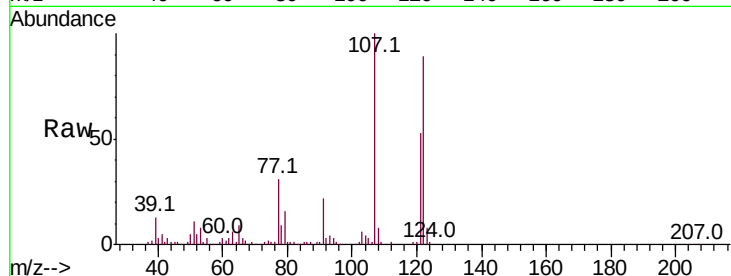

Abundance Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

Ion 122.00 (121.70 to 122.70): E

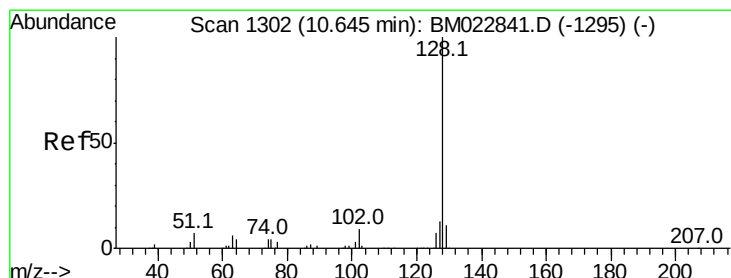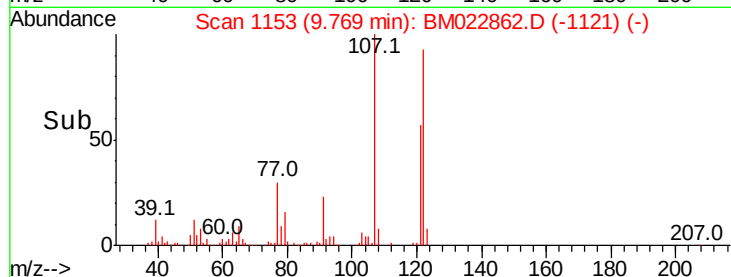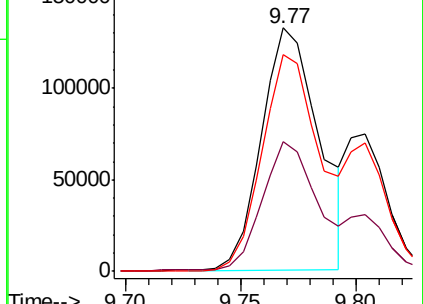

#28

Naphthalene

Concen: 6.267 ng/ul

RT: 10.65 min Scan# 1302

Delta R.T. -0.01 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52


Tgt Ion:128 Resp: 332002

Ion Ratio Lower Upper

128 100

129 11.5 8.6 13.0



127 13.2 10.2 15.4

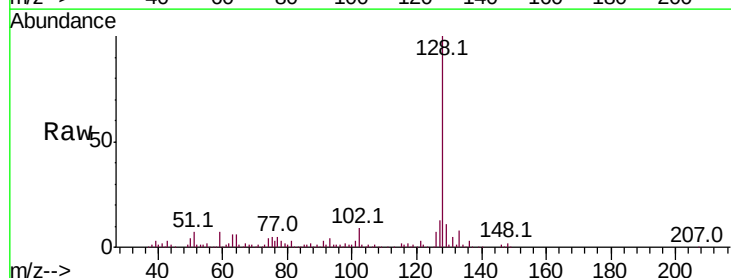


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



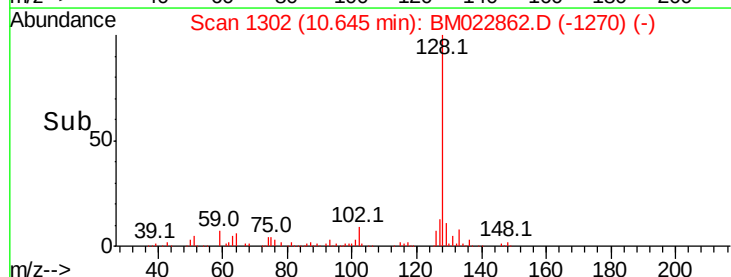
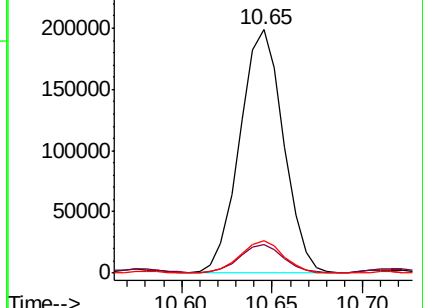


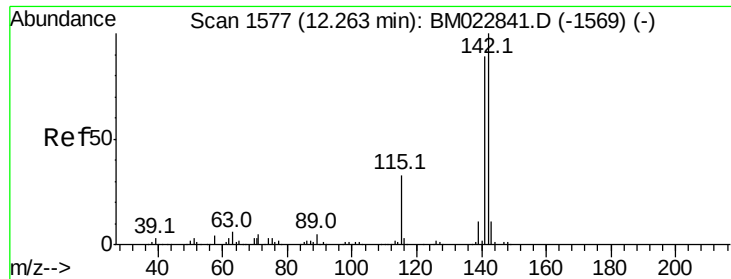

#34
2-Methylnaphthalene
Concen: 5.625 ng/ul
RT: 12.26 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BM022862.D
Acq: 01 Oct 2019 19:52




Instrument :
BNA_M
ClientSampleId :


Tot Ion:142 Resp: 223430
Ion Ratio Lower Upper
142 100
141 90.0 71.2 106.8

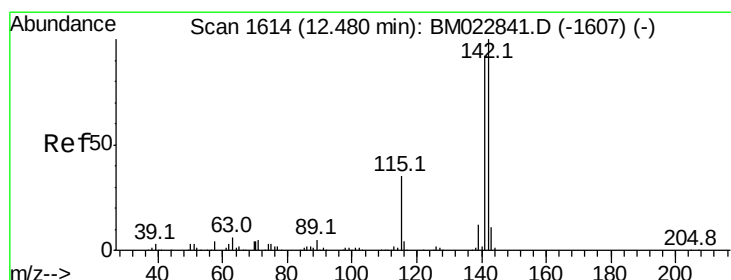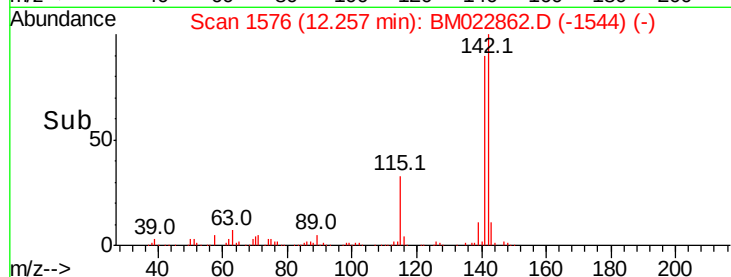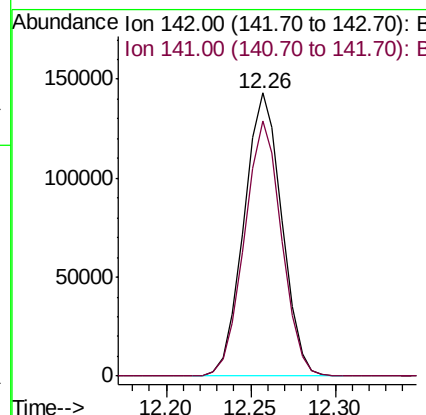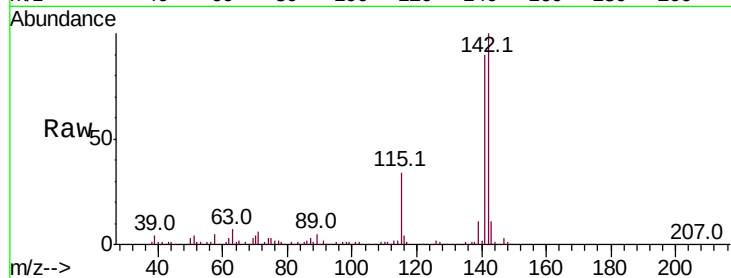

#35
1-Methylnaphthalene
Concen: 4.361 ng/ul
RT: 12.47 min Scan# 1613
Delta R.T. -0.01 min
Lab File: BM022862.D
Acq: 01 Oct 2019 19:52

Tgt Ion:142 Resp: 165426
Ion Ratio Lower Upper
142 100
141 90.0 73.0 109.6
116 3.6 2.9 4.3

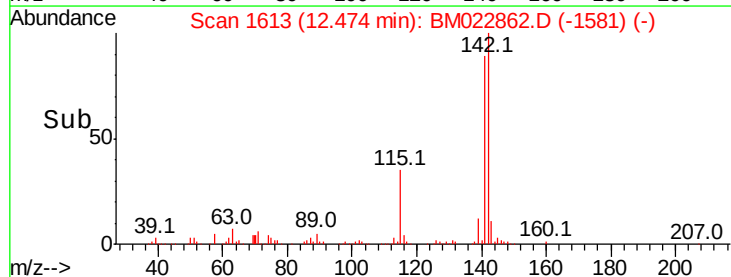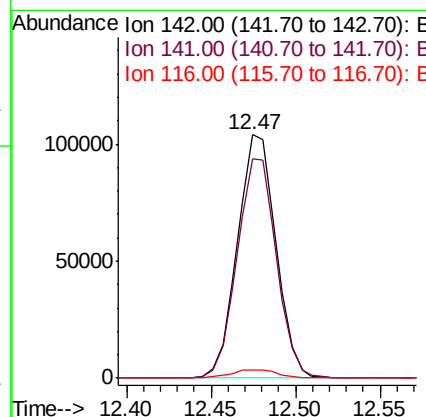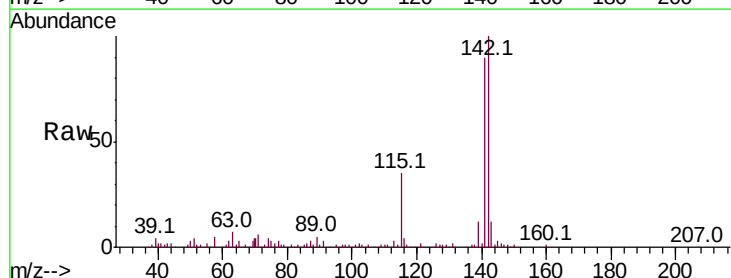

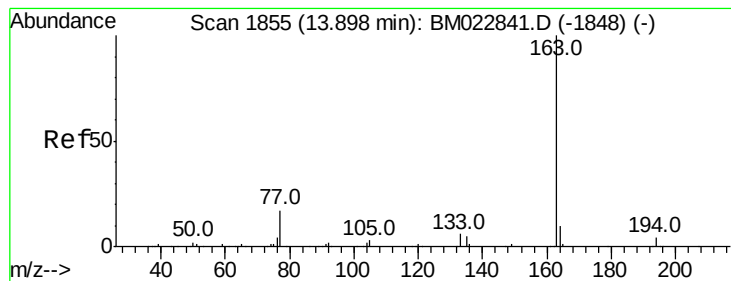

#45

Dimethylphthalate

Concen: 1.394 ng/ul

RT: 13.89 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BM022862.D

Acq: 01 Oct 2019 19:52

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 70256

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.7 8.1 12.1

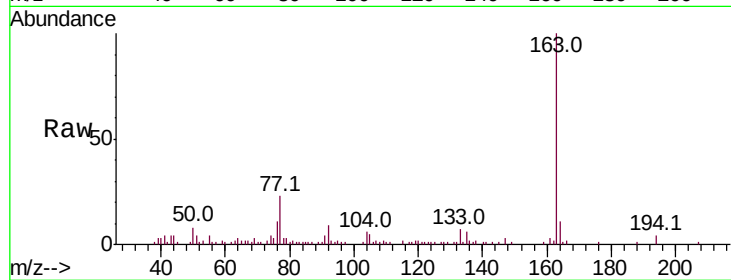

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

