

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100119\
 Data File : BM022883.D
 Acq On : 02 Oct 2019 09:12
 Operator : JU
 Sample : K4932-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 02 10:50:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 27 18:03:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	319777	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.59	136	1409489	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.44	164	850220	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.17	188	1505153	20.00	ng/ul	-0.01
78) Chrysene-d12	21.36	240	1077034	20.00	ng/ul	-0.01
86) Perylene-d12	23.62	264	1217287	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	36658	4.96	ng/uL	0.00
5) Phenol-d5	6.97	99	184653	6.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	381212	24.65	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.33	132	475203	20.89	ng/ul	-0.01
13) 4-Methylphenol-d8	8.50	113	334771	14.47	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	291205	26.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	325979	27.44	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.22	165	583922	24.69	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.72	131	576691	20.07	ng/ul	-0.01
44) Dimethylphthalate-d6	13.85	166	1856495	28.13	ng/ul	0.00
47) Acenaphthylene-d8	14.13	160	2084769	27.36	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.63	143	74919	5.75	ng/ul	0.00
58) Fluorene-d10	15.43	176	1533956	27.28	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.54	200	250421	25.57	ng/ul	-0.01
71) Anthracene-d10	17.27	188	2232864	30.38	ng/ul	-0.01
79) Pyrene-d10	19.57	212	2068214	35.68	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.48	264	1944095	30.87	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
4) Benzaldehyde	6.95	77	39523	3.087	ng/ul#	1
6) Phenol	7.00	94	143243	4.836	ng/ul	99
11) 2-Methylphenol	8.25	108	108941	4.772	ng/ul	100
14) Acetophenone	8.61	105	116291	3.288	ng/ul#	38
16) 4-Methylphenol	8.57	108	251795	9.975	ng/ul	98
24) 2,4-Dimethylphenol	9.77	107	336617	12.726	ng/ul	99
28) Naphthalene	10.65	128	1480334	19.447	ng/ul	99
34) 2-Methylnaphthalene	12.26	142	596341	10.449	ng/ul	100
35) 1-Methylnaphthalene	12.47	142	614207	11.268	ng/ul	100
45) Dimethylphthalate	13.89	163	1307819	19.294	ng/ul	99
50) Acenaphthene	14.50	153	76589	1.337	ng/ul	99
70) Phenanthrene	17.22	178	116947	1.302	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100119\
Data File : BM022883.D
Acq On : 02 Oct 2019 09:12
Operator : JU
Sample : K4932-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 02 10:50:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 27 18:03:27 2019
Response via : Initial Calibration

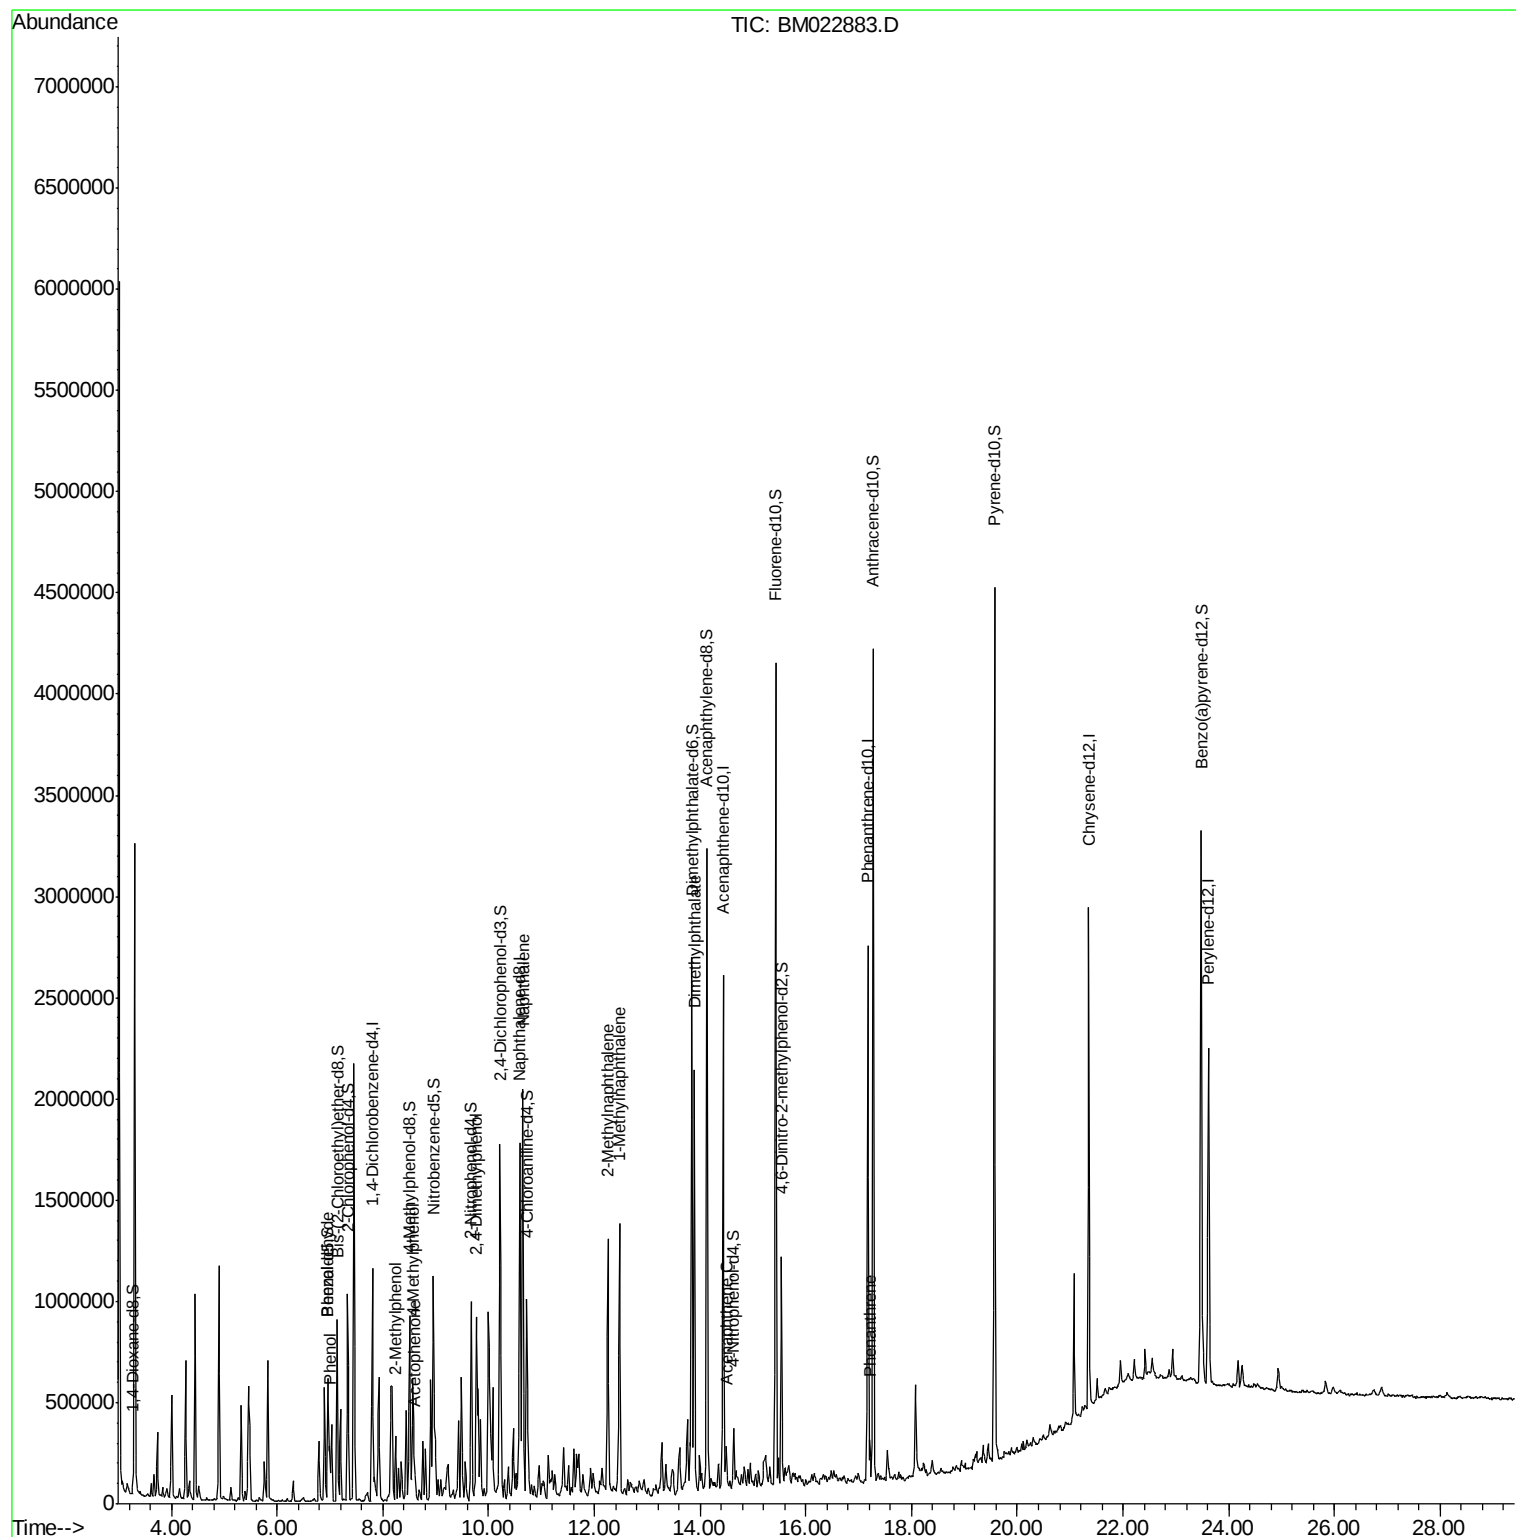

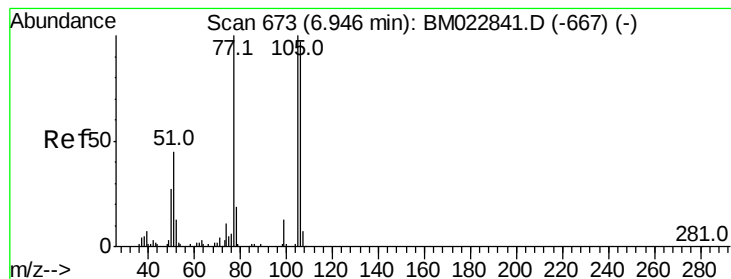

#4

Benzaldehyde

Concen: 3.087 ng/ul

RT: 6.95 min Scan# 674

Delta R.T. -0.00 min

Lab File: BM022883.D

Acq: 02 Oct 2019 09:12

Instrument :

BNA_M

ClientSampled :





Tot Ion: 77 Resp: 39523

Ion Ratio Lower Upper

77 100

105 702.7 80.6 120.8#

106 85.0 77.0 115.6

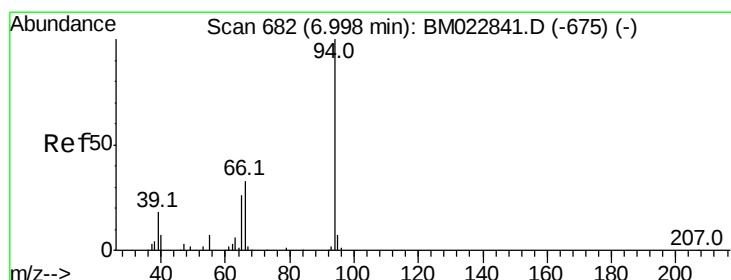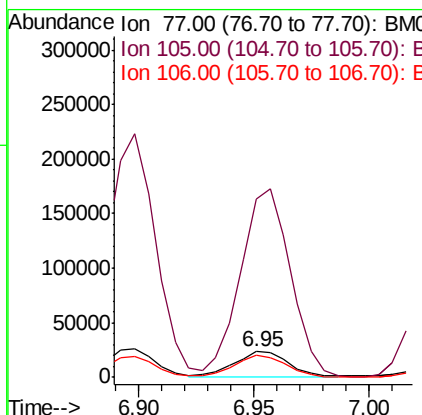

#6

Phenol

Concen: 4.836 ng/ul

RT: 7.00 min Scan# 682

Delta R.T. -0.01 min

Lab File: BM022883.D

Acq: 02 Oct 2019 09:12




Tgt Ion: 94 Resp: 143243


Ion Ratio Lower Upper

94 100

65 26.9 20.9 31.3

66 33.6 27.2 40.8

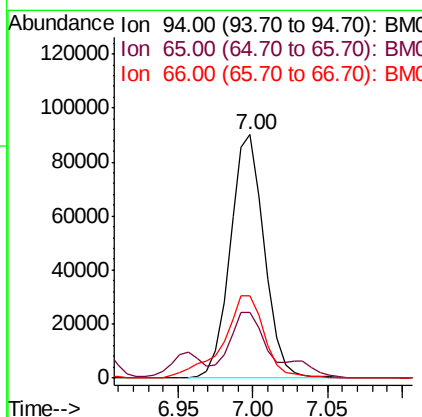



#11

2-Methylphenol

Concen: 4.772 ng/ul

RT: 8.25 min Scan# 894

Delta R.T. -0.01 min

Lab File: BM022883.D

Acq: 02 Oct 2019 09:12

Instrument :

BNA_M


ClientSampleId :

Tot Ion:108 Resp: 108941

Ion Ratio Lower Upper

108 100

107 88.6 71.0 106.4

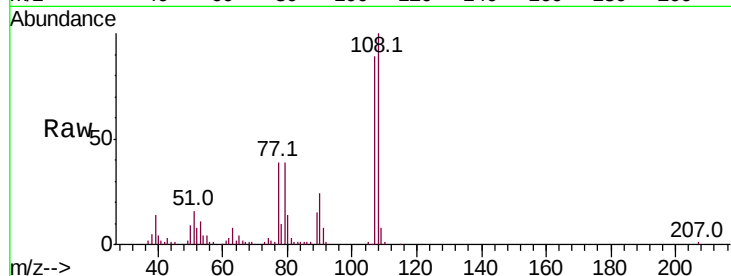

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

8.25

60000



40000

20000

0

8.20 8.25 8.30

Time-->



#14

Acetophenone

Concen: 3.288 ng/ul

RT: 8.61 min Scan# 956

Delta R.T. -0.02 min

Lab File: BM022883.D

Acq: 02 Oct 2019 09:12


Tgt Ion:105 Resp: 116291

Ion Ratio Lower Upper

105 100

77 15.5 59.4 89.0#

51 5.2 19.4 29.0#



Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 51.00 (50.70 to 51.70): BM0

8.61

60000


40000


20000

0

8.50 8.60 8.70

Time-->



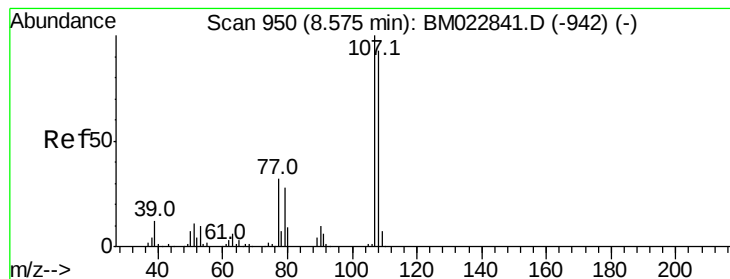

#16

4-Methylphenol

Concen: 9.975 ng/ul

RT: 8.57 min Scan# 949

Delta R.T. -0.01 min

Lab File: BM022883.D

Acq: 02 Oct 2019 09:12

Instrument :

BNA_M


ClientSampleId :

Tot Ion:108 Resp: 251795

Ion Ratio Lower Upper




108 100

107 107.9 87.9 131.9

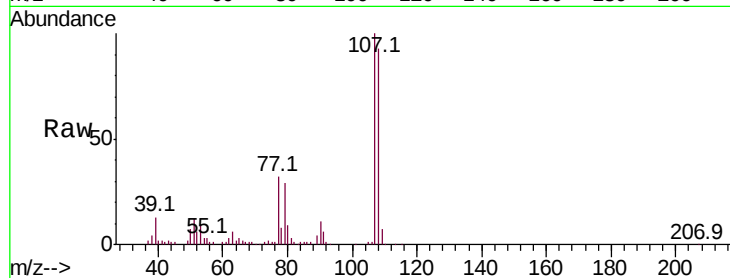

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

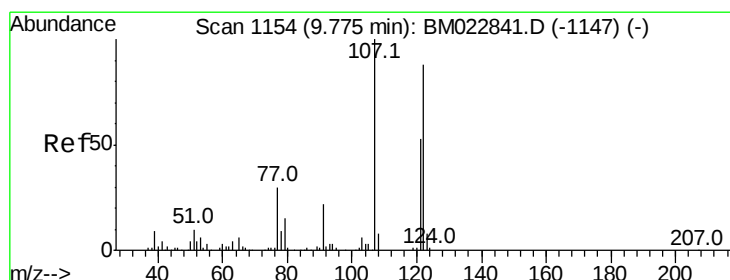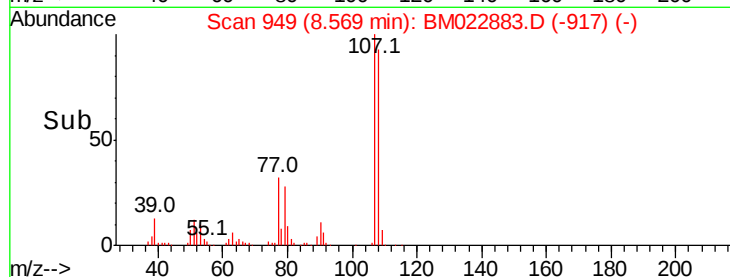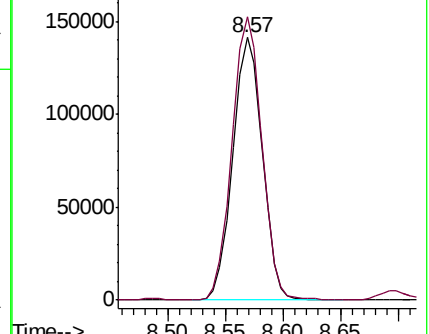

#24

2,4-Dimethylphenol

Concen: 12.726 ng/ul

RT: 9.77 min Scan# 1153

Delta R.T. -0.01 min

Lab File: BM022883.D

Acq: 02 Oct 2019 09:12


Tgt Ion:107 Resp: 336617

Ion Ratio Lower Upper

107 100

121 52.1 43.0 64.4



122 89.0 71.4 107.0

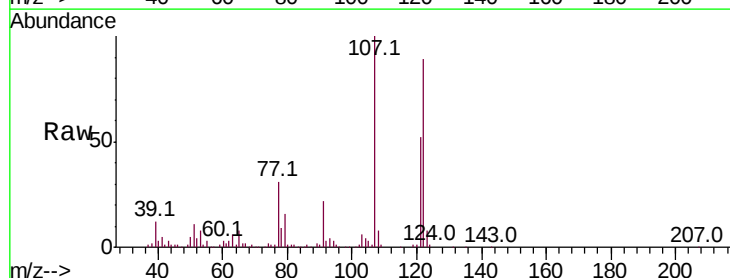


Abundance Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

Ion 122.00 (121.70 to 122.70): E

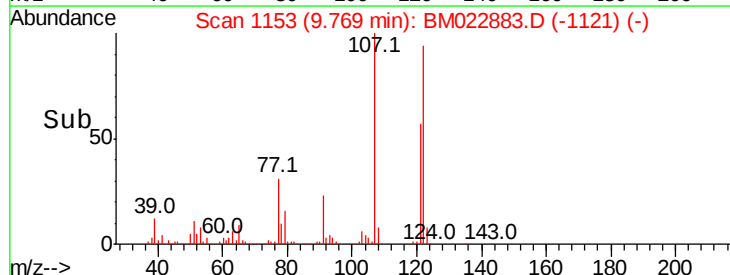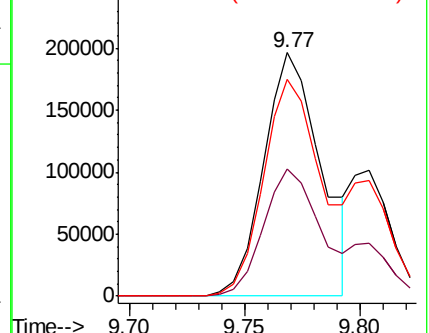







#28
Naphthalene
Concen: 19.447 ng/ul
RT: 10.65 min Scan# 1302
Delta R.T. -0.01 min
Lab File: BM022883.D
Acq: 02 Oct 2019 09:12

Instrument :
BNA_M
ClientSampleId :

Tot Ion:128 Resp: 1480334
Ion Ratio Lower Upper
128 100
129 11.1 8.6 13.0
127 12.9 10.2 15.4

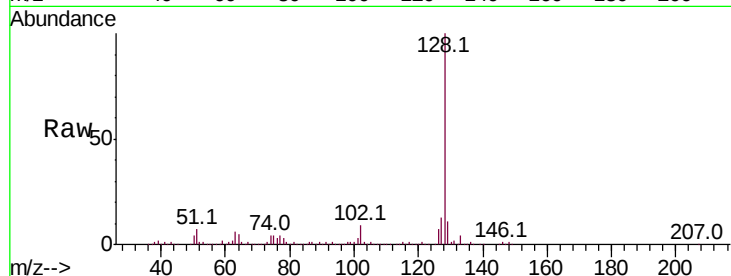


Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E


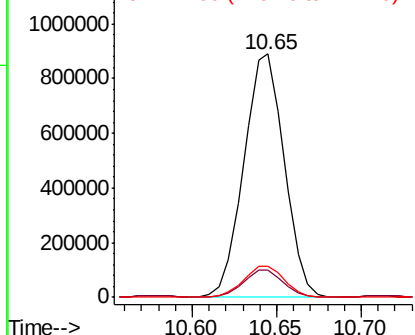



#34
2-Methylnaphthalene
Concen: 10.449 ng/ul
RT: 12.26 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BM022883.D
Acq: 02 Oct 2019 09:12

Tgt Ion:142 Resp: 596341
Ion Ratio Lower Upper
142 100
141 89.0 71.2 106.8



Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E




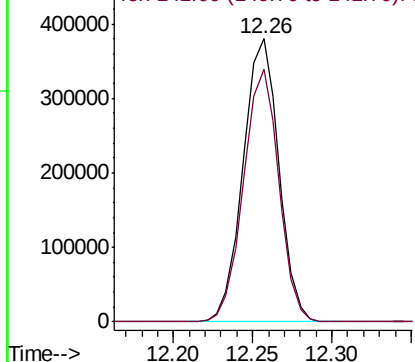




#35
1-Methylnaphthalene
Concen: 11.268 ng/ul
RT: 12.47 min Scan# 1613
Delta R.T. -0.01 min
Lab File: BM022883.D
Acq: 02 Oct 2019 09:12




Instrument :
BNA_M
ClientSampled :


Tot Ion:142 Resp: 614207
Ion Ratio Lower Upper
142 100
141 91.4 73.0 109.6
116 3.7 2.9 4.3

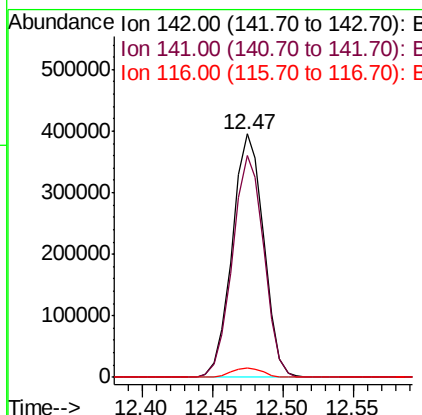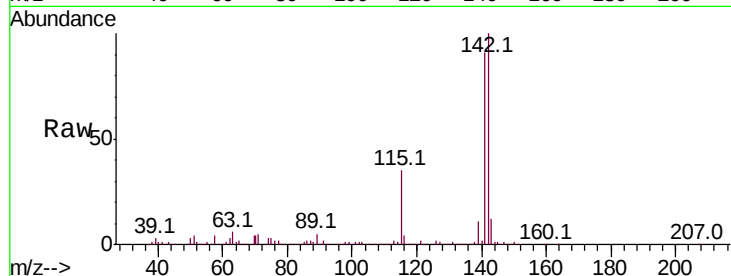

#45
Dimethylphthalate
Concen: 19.294 ng/ul
RT: 13.89 min Scan# 1854
Delta R.T. -0.01 min
Lab File: BM022883.D
Acq: 02 Oct 2019 09:12

Tgt Ion:163 Resp: 1307819
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.0
164 10.5 8.1 12.1

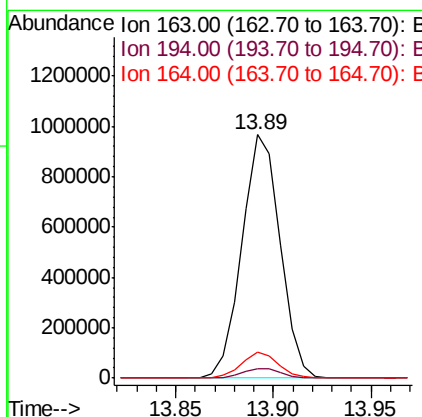



#50

Acenaphthene

Concen: 1.337 ng/ul

RT: 14.50 min Scan# 1957

Delta R.T. -0.02 min

Lab File: BM022883.D

Acq: 02 Oct 2019 09:12

Instrument :

BNA_M

ClientSampleId :


Tot Ion:153 Resp: 76589

Ion Ratio Lower Upper




153 100

152 46.3 38.1 57.1

154 89.9 71.1 106.7



Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

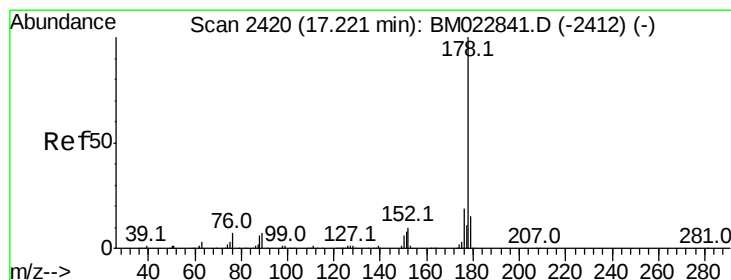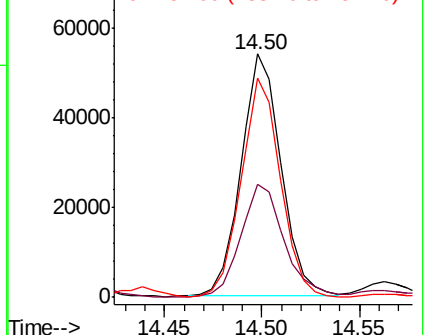

#70

Phenanthrene

Concen: 1.302 ng/ul

RT: 17.22 min Scan# 2419

Delta R.T. -0.01 min

Lab File: BM022883.D

Acq: 02 Oct 2019 09:12


Tgt Ion:178 Resp: 116947

Ion Ratio Lower Upper

178 100

179 15.5 12.4 18.6

176 18.6 15.3 22.9



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

