

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100119\
 Data File : BM022905.D
 Acq On : 02 Oct 2019 22:37
 Operator : JU
 Sample : K4895-17
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 03 01:00:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 27 18:03:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	281647	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.59	136	1195077	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.43	164	673178	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.17	188	1128082	20.00	ng/ul	-0.01
78) Chrysene-d12	21.35	240	860156	20.00	ng/ul	-0.02
86) Perylene-d12	23.61	264	1020959	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	34308	5.27	ng/uL	0.00
5) Phenol-d5	6.97	99	162754	6.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	331294	24.32	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.33	132	419785	20.95	ng/ul	-0.01
13) 4-Methylphenol-d8	8.50	113	283962	13.94	ng/ul	-0.01
19) Nitrobenzene-d5	8.95	128	244623	26.52	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.67	143	267747	26.59	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.21	165	498952	24.88	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.72	131	525004	21.55	ng/ul	-0.01
44) Dimethylphthalate-d6	13.84	166	1585685	30.35	ng/ul	-0.01
47) Acenaphthylene-d8	14.13	160	1754200	29.08	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.63	143	66044	6.40	ng/ul	0.00
58) Fluorene-d10	15.43	176	1312045	29.47	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.54	200	209142	28.49	ng/ul	-0.02
71) Anthracene-d10	17.27	188	1849030	33.57	ng/ul	-0.02
79) Pyrene-d10	19.56	212	1773258	38.30	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.47	264	1806767	34.21	ng/ul	-0.03

Target Compounds


					Ovalue	
4) Benzaldehyde	6.95	77	18883	1.674	ng/ul#	1
6) Phenol	6.99	94	44475	1.705	ng/ul	98
14) Acetophenone	8.60	105	55311	1.776	ng/ul#	40
16) 4-Methylphenol	8.57	108	29842	1.342	ng/ul	93
17) Hexachloroethane	8.91	117	39901	4.884	ng/ul#	6
28) Naphthalene	10.64	128	1022214	15.838	ng/ul	99
34) 2-Methylnaphthalene	12.25	142	411358	8.501	ng/ul	99
35) 1-Methylnaphthalene	12.47	142	280348	6.066	ng/ul	100
45) Dimethylphthalate	13.89	163	739214	13.773	ng/ul	100
70) Phenanthrene	17.22	178	79696	1.184	ng/ul	97
72) Anthracene	17.22	178	80058	1.167	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100119\
Data File : BM022905.D
Acq On : 02 Oct 2019 22:37
Operator : JU
Sample : K4895-17
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 03 01:00:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 27 18:03:27 2019
Response via : Initial Calibration

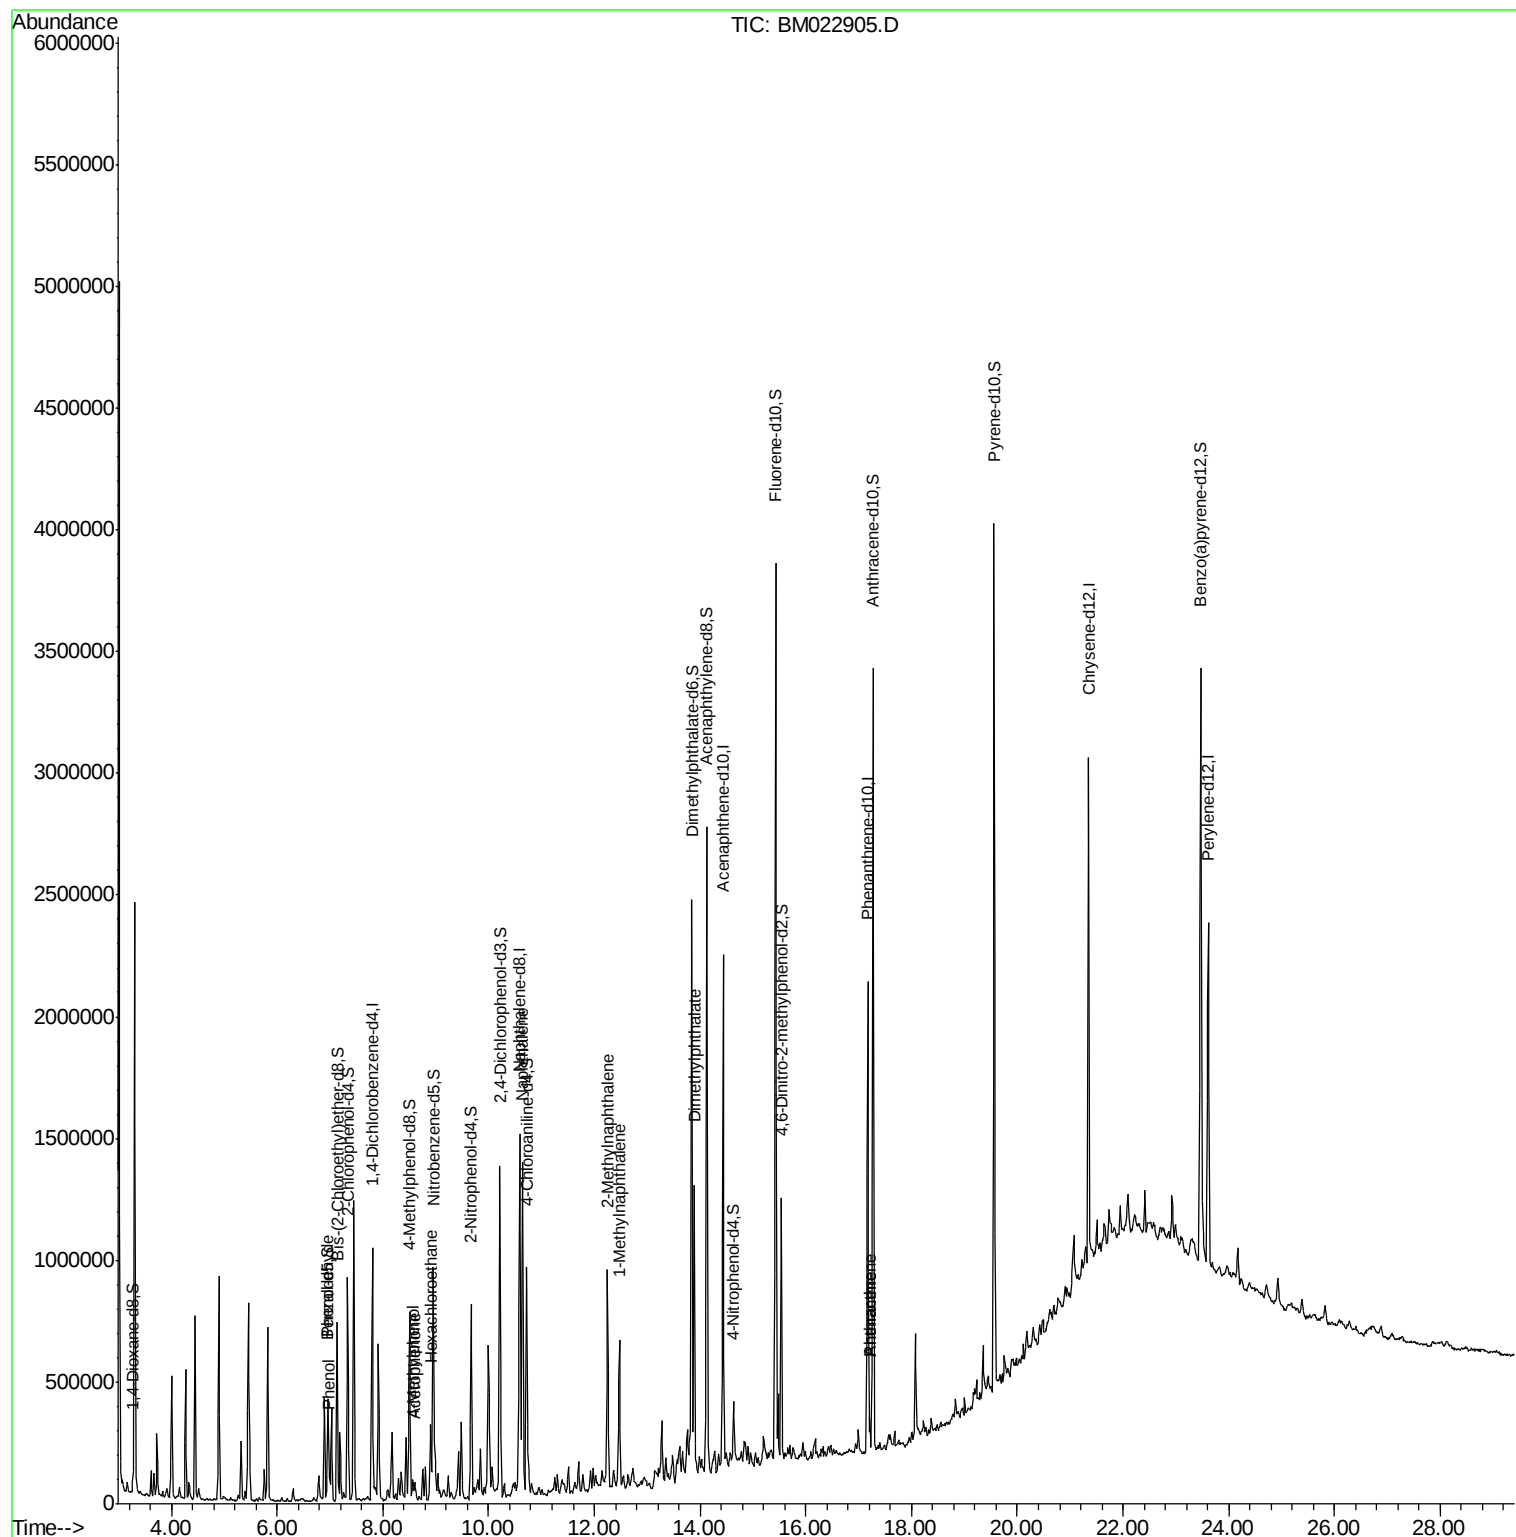

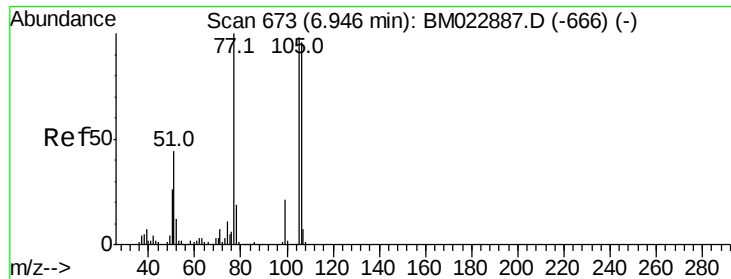

#4

Benzaldehyde

Concen: 1.674 ng/ul

RT: 6.95 min Scan# 674

Delta R.T. -0.00 min

Lab File: BM022905.D

Acq: 02 Oct 2019 22:37

Instrument :

BNA_M

ClientSampled :





Tot Ion: 77 Resp: 18883

Ion Ratio Lower Upper

77 100

105 729.4 80.6 120.8#

106 86.1 77.0 115.6

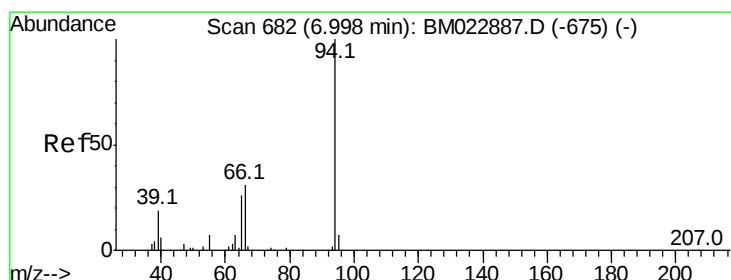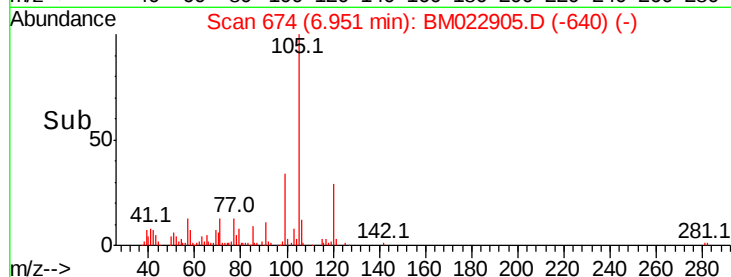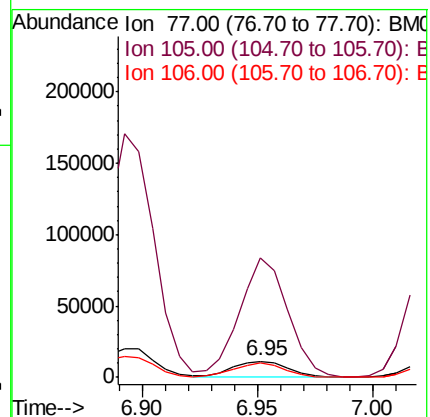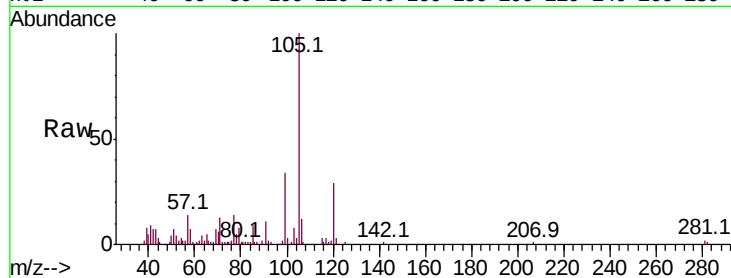

#6

Phenol

Concen: 1.705 ng/ul

RT: 6.99 min Scan# 681

Delta R.T. -0.01 min

Lab File: BM022905.D

Acq: 02 Oct 2019 22:37




Tgt Ion: 94 Resp: 44475


Ion Ratio Lower Upper

94 100

65 26.8 20.9 31.3

66 35.3 27.2 40.8

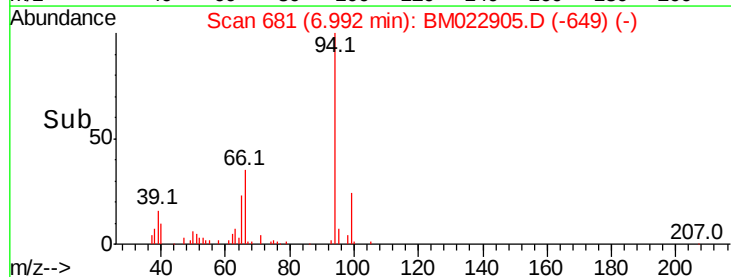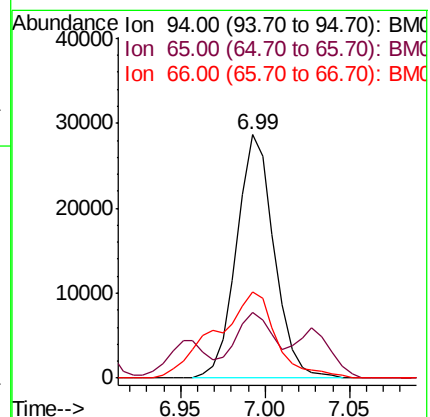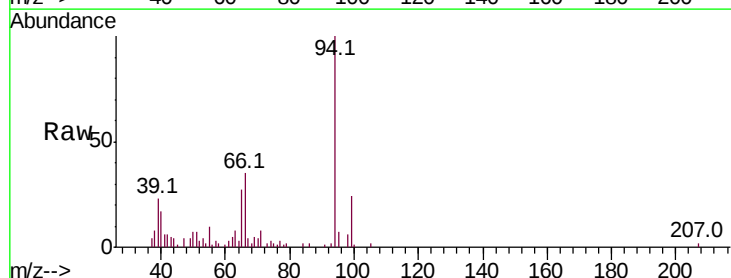

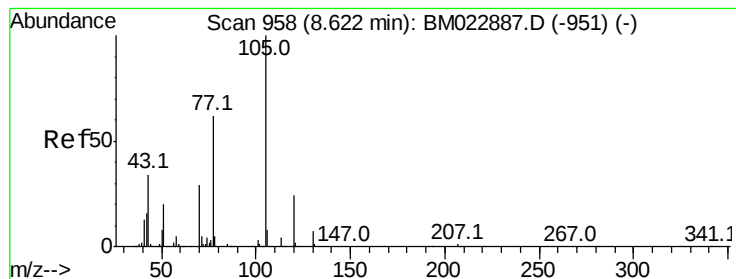

#14

Acetophenone

Concen: 1.776 ng/ul

RT: 8.60 min Scan# 955

Delta R.T. -0.03 min

Lab File: BM022905.D

Acq: 02 Oct 2019 22:37

Instrument :

BNA_M

ClientSampled :


Tot Ion:105 Resp: 55311

Ion Ratio Lower Upper

105 100

77 16.9 59.4 89.0#




51 6.0 19.4 29.0#

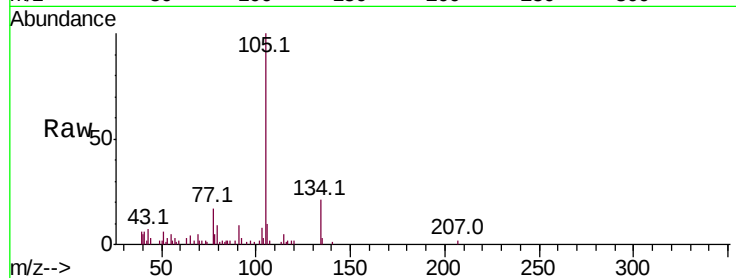

Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 51.00 (50.70 to 51.70): BM0

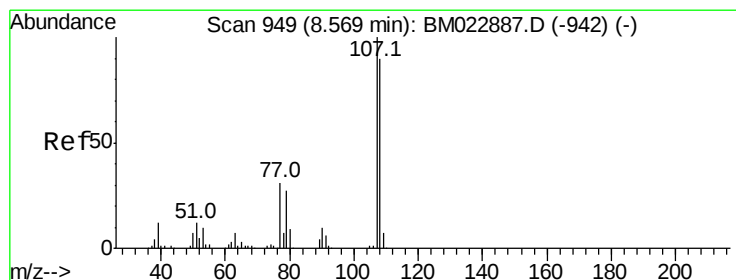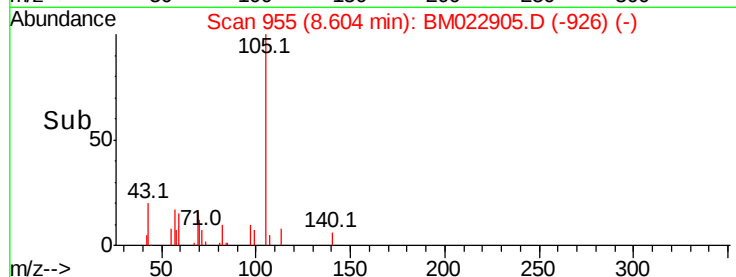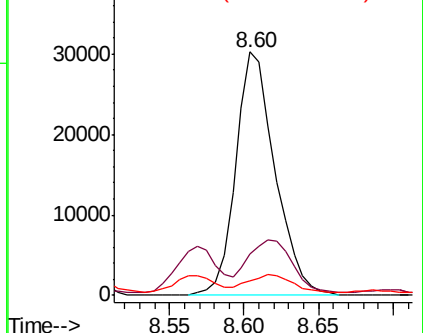

#16

4-Methylphenol

Concen: 1.342 ng/ul

RT: 8.57 min Scan# 949

Delta R.T. -0.01 min

Lab File: BM022905.D


Acq: 02 Oct 2019 22:37

Tgt Ion:108 Resp: 29842

Ion Ratio Lower Upper



108 100


107 102.3 87.9 131.9

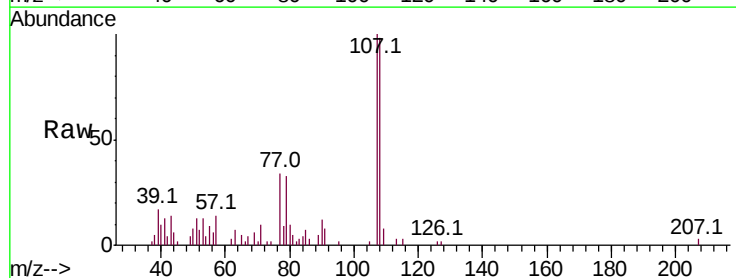

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

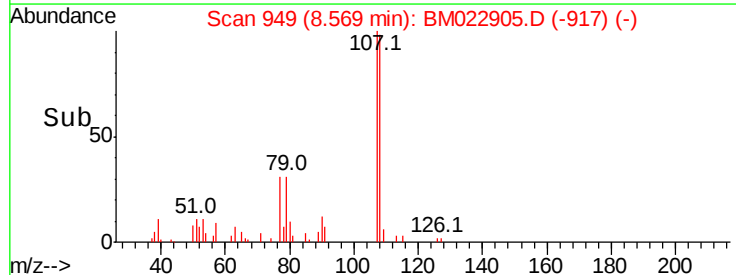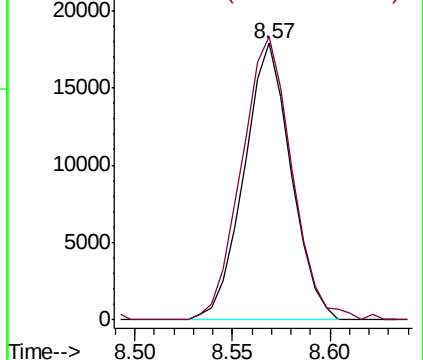

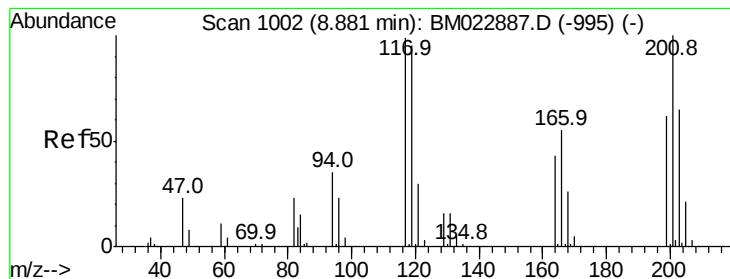

#17

Hexachloroethane

Concen: 4.884 ng/ul

RT: 8.91 min Scan# 1007

Delta R.T. 0.02 min

Lab File: BM022905.D

Acq: 02 Oct 2019 22:37

Instrument :

BNA_M

ClientSampleId :


Tot Ion:117 Resp: 39901

Ion Ratio Lower Upper

117 100

201 0.0 82.5 123.7#




199 0.0 51.6 77.4#

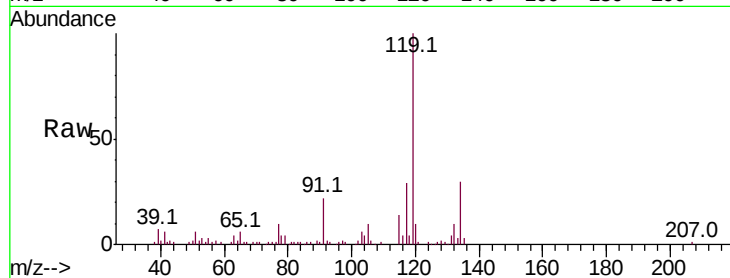

Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

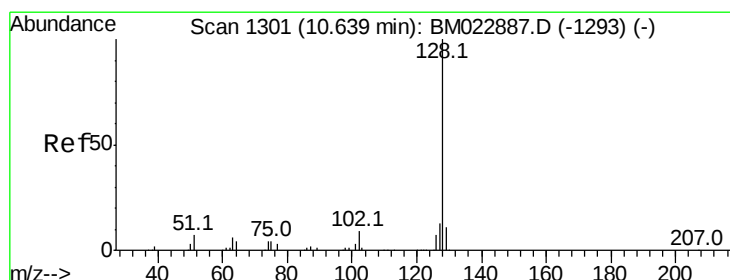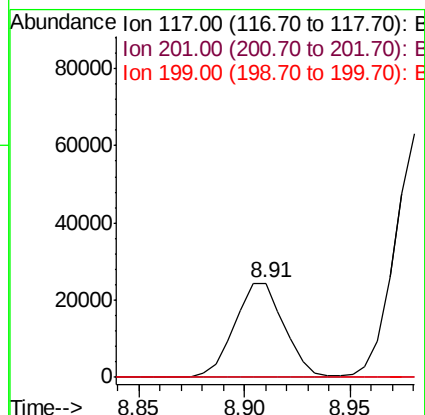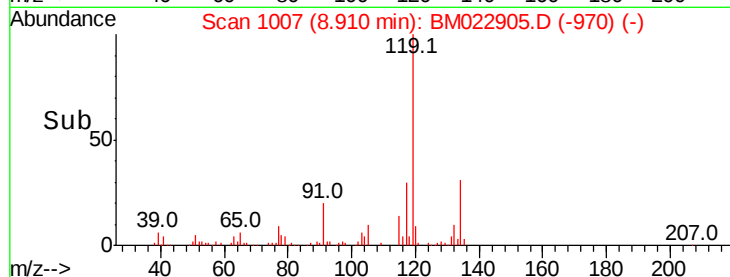

#28

Naphthalene

Concen: 15.838 ng/ul

RT: 10.64 min Scan# 1301

Delta R.T. -0.02 min

Lab File: BM022905.D

Acq: 02 Oct 2019 22:37


Tgt Ion:128 Resp: 1022214

Ion Ratio Lower Upper

128 100

129 11.3 8.6 13.0



127 13.0 10.2 15.4

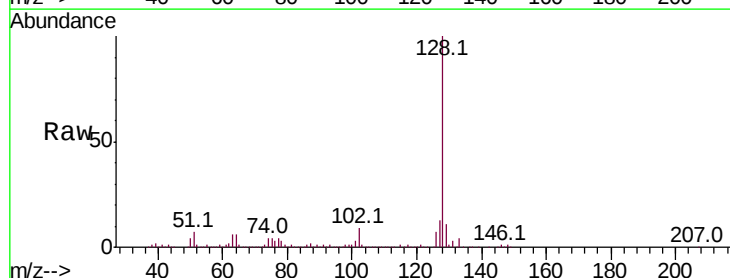


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



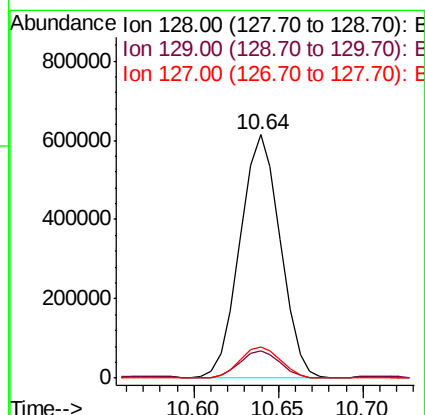
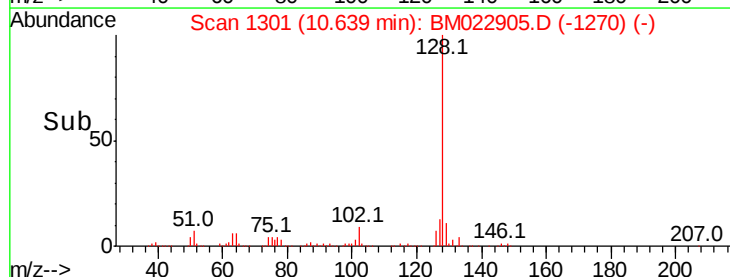


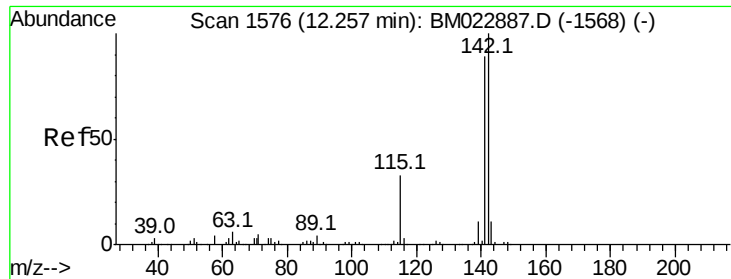

#34
 2-Methylnaphthalene
 Concen: 8.501 ng/ul
 RT: 12.25 min Scan# 1575
 Delta R.T. -0.02 min
 Lab File: BM022905.D
 Acq: 02 Oct 2019 22:37




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:142 Resp: 411358
 Ion Ratio Lower Upper
 142 100
 141 88.1 71.2 106.8

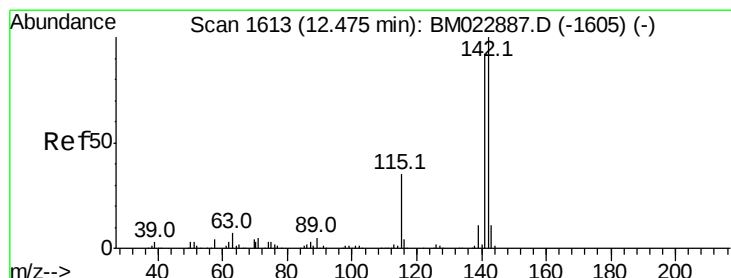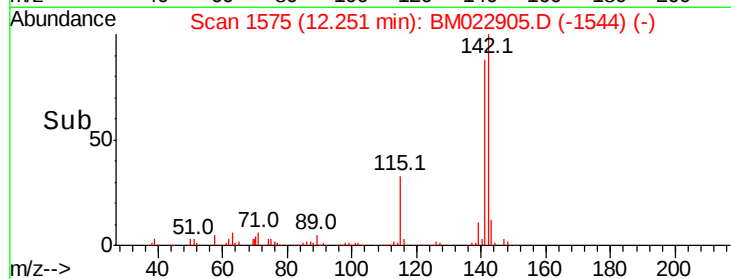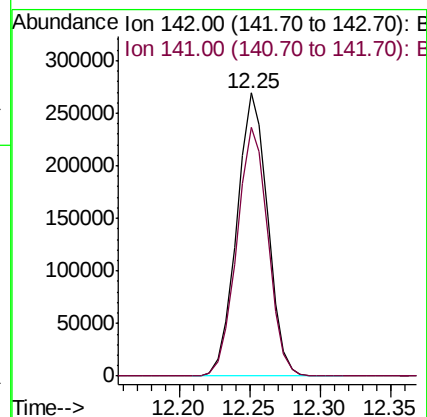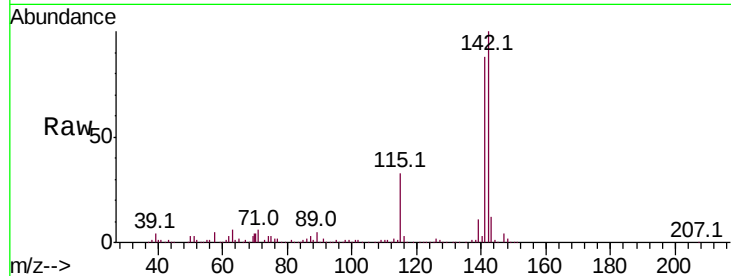

#35
 1-Methylnaphthalene
 Concen: 6.066 ng/ul
 RT: 12.47 min Scan# 1613
 Delta R.T. -0.01 min
 Lab File: BM022905.D
 Acq: 02 Oct 2019 22:37

Tgt Ion:142 Resp: 280348
 Ion Ratio Lower Upper
 142 100
 141 91.1 73.0 109.6
 116 3.7 2.9 4.3

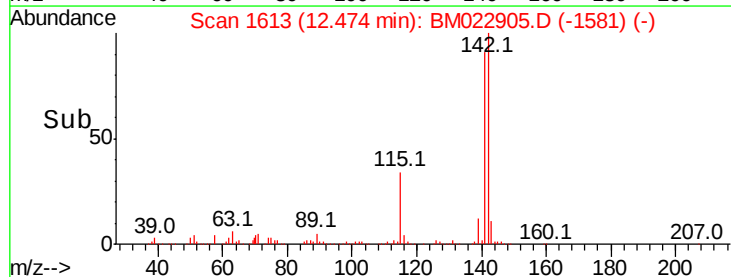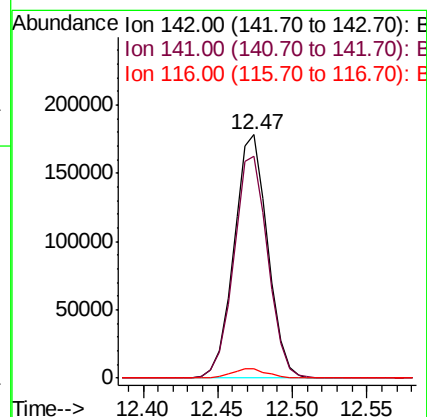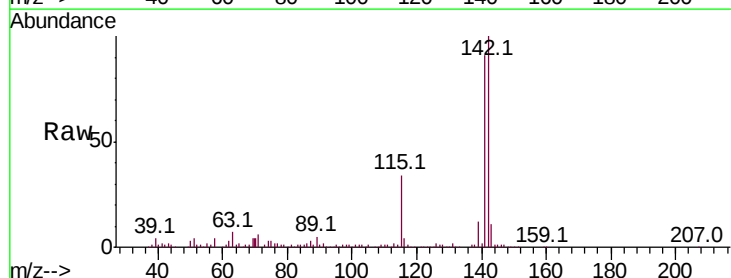

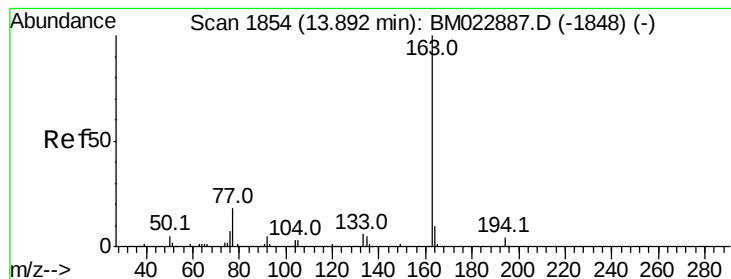

#45

Dimethylphthalate

Concen: 13.773 ng/ul

RT: 13.89 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BM022905.D

Acq: 02 Oct 2019 22:37

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 739214

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0




164 10.1 8.1 12.1

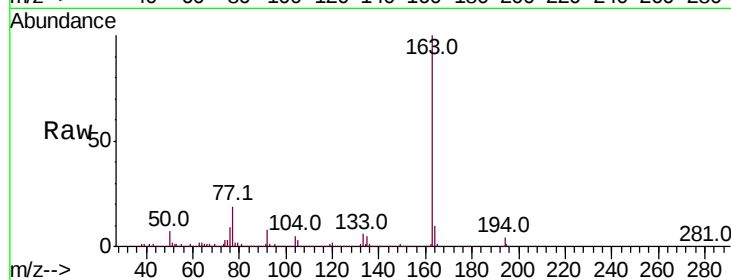

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

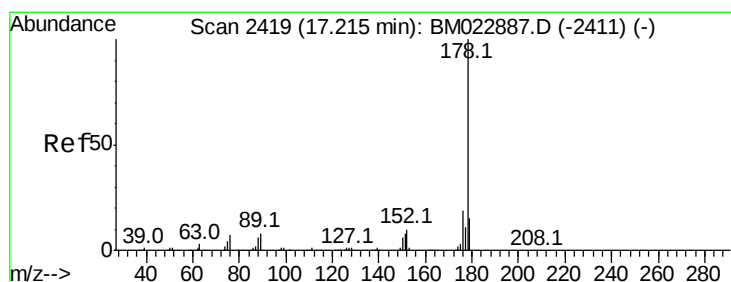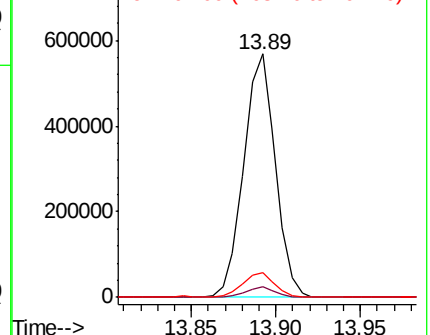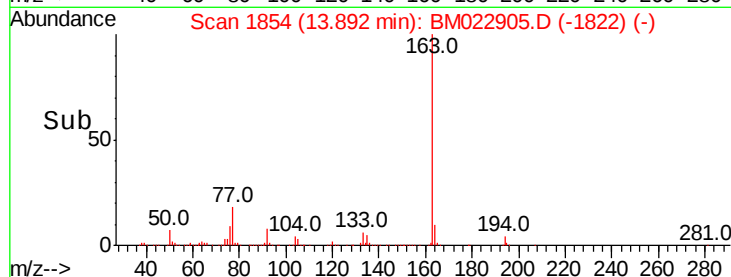

#70

Phenanthrene

Concen: 1.184 ng/ul

RT: 17.22 min Scan# 2419

Delta R.T. -0.01 min

Lab File: BM022905.D

Acq: 02 Oct 2019 22:37


Tgt Ion:178 Resp: 79696

Ion Ratio Lower Upper

178 100

179 17.2 12.4 18.6



176 20.1 15.3 22.9

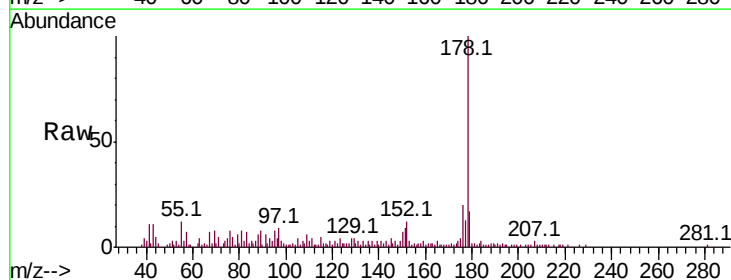


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

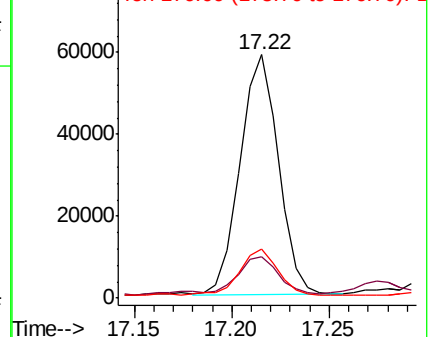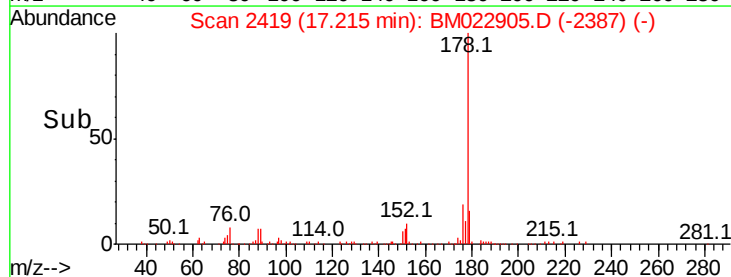


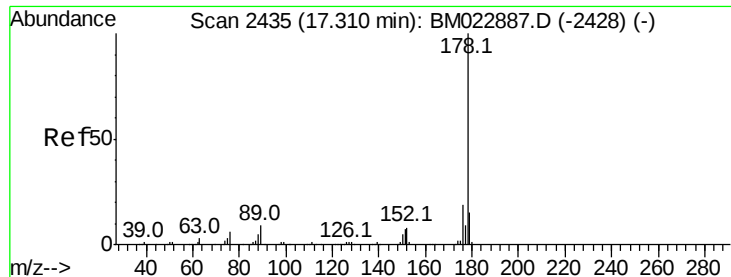

#72
 Anthracene
 Concen: 1.167 ng/ul
 RT: 17.22 min Scan# 2419
 Delta R.T. -0.11 min
 Lab File: BM022905.D
 Acq: 02 Oct 2019 22:37

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
178	100		
179	17.2	12.4	18.6
176	20.1	15.0	22.6

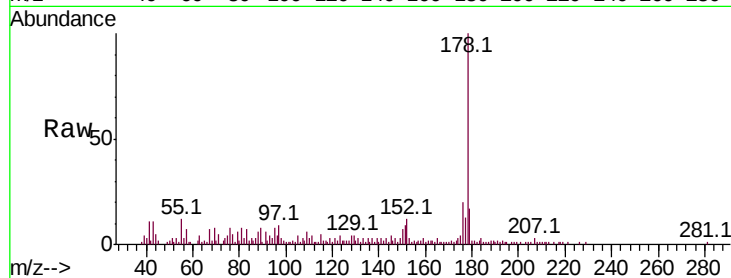

Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

