

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
 Data File : BM022866.D
 Acq On : 01 Oct 2019 22:18
 Operator : JU
 Sample : PB123400BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	45	48	61	rVB	56912	89277	1.44%	0.144%
2	3.916	154	158	169	rVB	29092	49936	0.80%	0.081%
3	4.005	170	173	179	rVB	10271	13354	0.22%	0.022%
4	4.099	186	189	195	rVB2	8160	11540	0.19%	0.019%
5	4.457	247	250	254	rVB2	5262	6736	0.11%	0.011%
6	4.934	327	331	336	rBV3	4408	7217	0.12%	0.012%
7	6.193	541	545	551	rVB2	7658	11563	0.19%	0.019%
8	6.969	670	677	690	rVB	391865	658048	10.60%	1.062%
9	7.134	698	705	724	rBV	804083	1304973	21.03%	2.106%
10	7.334	733	739	751	rBV	919558	1477466	23.80%	2.384%
11	7.804	812	819	827	rBV	894118	1396296	22.50%	2.253%
12	7.881	827	832	835	rVB2	9167	14751	0.24%	0.024%
13	8.504	931	938	949	rBV	863173	1356402	21.85%	2.189%
14	8.628	953	959	967	rVB	40670	67813	1.09%	0.109%
15	8.957	1007	1015	1024	rBV	1066232	1734490	27.95%	2.799%
16	9.404	1086	1091	1095	rBV2	12463	17478	0.28%	0.028%
17	9.463	1095	1101	1104	rVV4	10111	19458	0.31%	0.031%
18	9.516	1107	1110	1118	rVB3	12494	21423	0.35%	0.035%
19	9.675	1130	1137	1152	rBV	885700	1486552	23.95%	2.399%
20	10.216	1221	1229	1239	rBV	1370627	2248428	36.23%	3.628%
21	10.516	1275	1280	1286	rBV2	6245	11978	0.19%	0.019%
22	10.592	1286	1293	1300	rBV	1355645	2260962	36.43%	3.649%
23	10.728	1307	1316	1323	rBV	305284	521666	8.40%	0.842%
24	10.816	1328	1331	1335	rVB3	4796	6997	0.11%	0.011%
25	11.204	1393	1397	1405	rBV5	4261	8750	0.14%	0.014%
26	12.180	1558	1563	1569	rVB2	20832	31956	0.51%	0.052%
27	13.845	1840	1846	1851	rBV	2559740	3638090	58.62%	5.871%
28	13.892	1851	1854	1862	rVB	230037	294551	4.75%	0.475%
29	14.133	1888	1895	1909	rVB	2959016	4515026	72.74%	7.286%
30	14.351	1925	1932	1936	rBV3	4719	6311	0.10%	0.010%
31	14.439	1940	1947	1957	rVB	2310779	3308772	53.31%	5.339%
32	14.627	1973	1979	1988	rBV	364225	547925	8.83%	0.884%
33	14.851	2012	2017	2024	rBV3	15977	21829	0.35%	0.035%
34	15.298	2089	2093	2097	rBV	5218	7074	0.11%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
 Data File : BM022866.D
 Acq On : 01 Oct 2019 22:18
 Operator : JU
 Sample : PB123400BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

35	15.433	2109	2116	2128	rBV	3717221	5446346	87.75%	8.789%
36	15.545	2128	2135	2146	rBV	1141519	1531128	24.67%	2.471%
37	15.668	2152	2156	2161	rVB2	42254	53796	0.87%	0.087%
38	16.210	2243	2248	2253	rVB	12288	17468	0.28%	0.028%
39	16.963	2370	2376	2383	rBV3	7744	14936	0.24%	0.024%
40	17.174	2406	2412	2422	rBV2	2583695	3725092	60.02%	6.011%
41	17.274	2422	2429	2441	rVV	4172484	5881028	94.75%	9.490%
42	17.368	2441	2445	2449	rVB4	10879	14530	0.23%	0.023%
43	18.074	2560	2565	2574	rBV	119726	174253	2.81%	0.281%
44	19.009	2721	2724	2727	rBV3	5644	6646	0.11%	0.011%
45	19.204	2752	2757	2761	rBV	42559	58331	0.94%	0.094%
46	19.351	2779	2782	2789	rBV3	36220	49998	0.81%	0.081%
47	19.451	2795	2799	2804	rBV	33356	47313	0.76%	0.076%
48	19.568	2813	2819	2825	rBV	4648633	6206678	100.00%	10.016%
49	20.080	2904	2906	2909	rBV3	15513	19311	0.31%	0.031%
50	20.121	2911	2913	2916	rVB2	15260	15609	0.25%	0.025%
51	20.615	2995	2997	3001	rVB2	30841	28985	0.47%	0.047%
52	21.068	3070	3074	3085	rBV	429191	611555	9.85%	0.987%
53	21.356	3118	3123	3129	rBV	2413537	3021385	48.68%	4.876%
54	21.515	3147	3150	3155	rBV2	87880	91656	1.48%	0.148%
55	21.956	3222	3225	3230	rVB2	101729	128209	2.07%	0.207%
56	22.421	3301	3304	3309	rVB	130118	157929	2.54%	0.255%
57	22.939	3389	3392	3398	rVB	146629	188401	3.04%	0.304%
58	23.474	3477	3483	3499	rVB	2304395	4603254	74.17%	7.428%
59	23.621	3501	3508	3519	rVB	1405749	2700222	43.51%	4.357%


Sum of corrected areas: 61969147

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
Data File : BM022866.D
Acq On : 01 Oct 2019 22:18
Operator : JU
Sample : PB123400BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK00

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

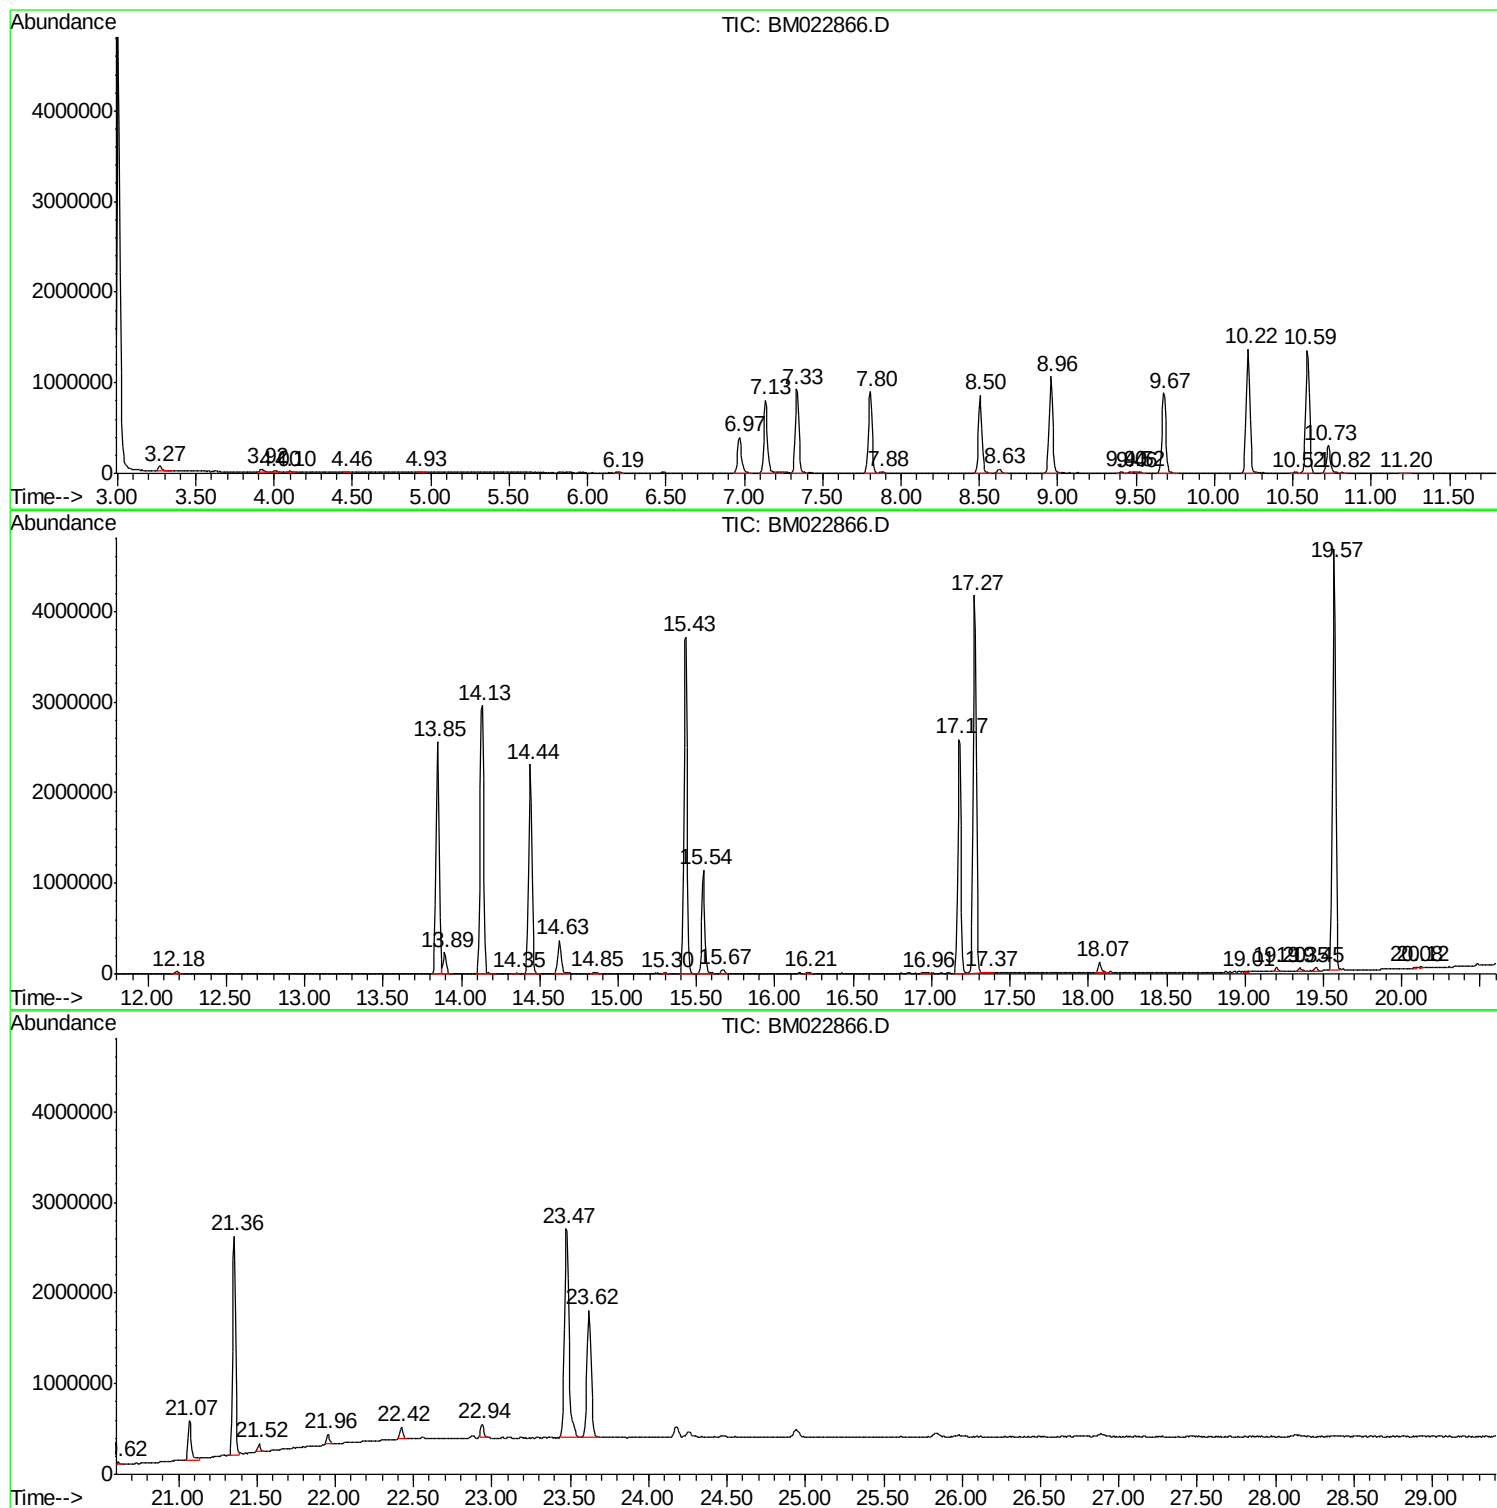

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
Data File : BM022866.D
Acq On : 01 Oct 2019 22:18
Operator : JU
Sample : PB123400BL
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
SBLK00

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.07 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.07	4.05 ng/ul	611555	Chrysene-d12		21.36	
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Octadecene	252	C18H36	000112-88-9	95
2		Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	94
3		Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
4		1-Heneicosyl formate	340	C22H44O2	077899-03-7	94
5		Cyclopentadecane	210	C15H30	000295-48-7	93

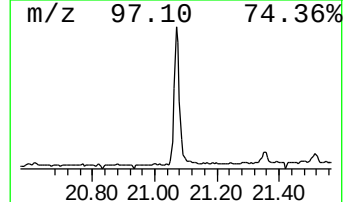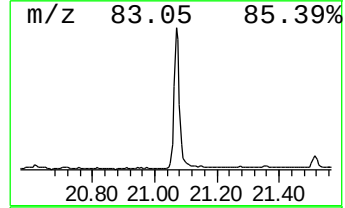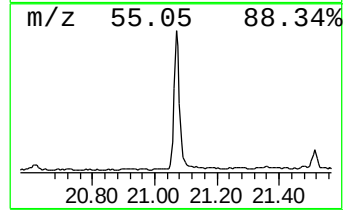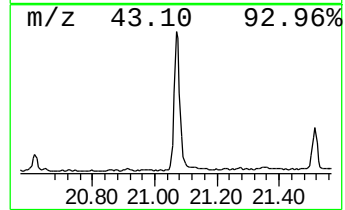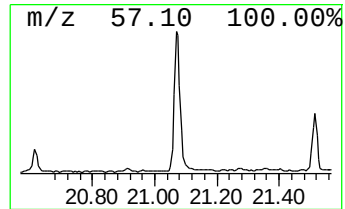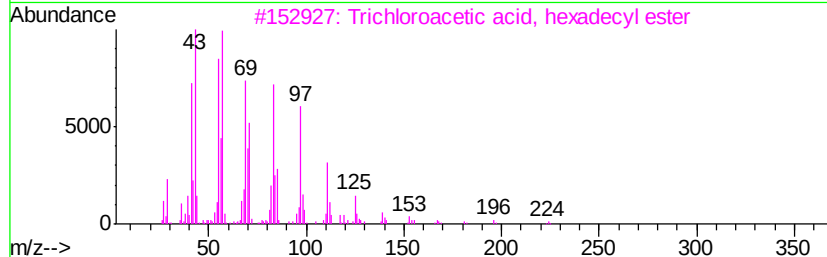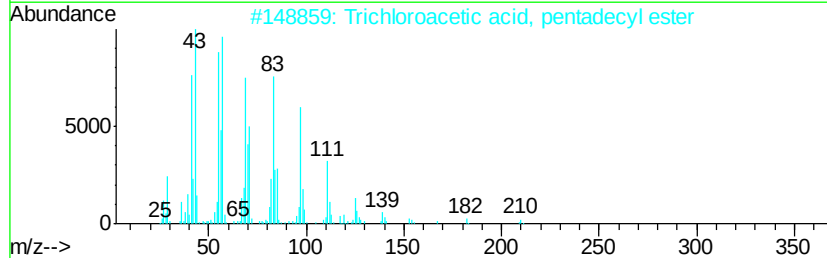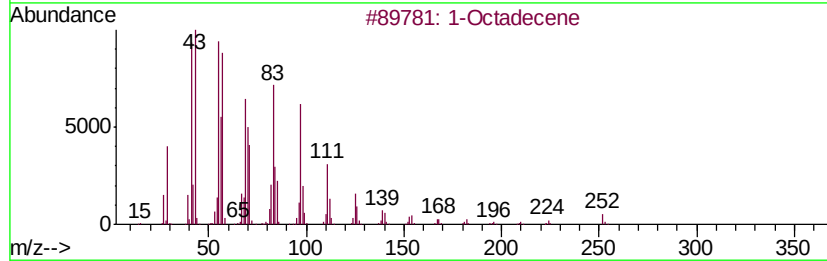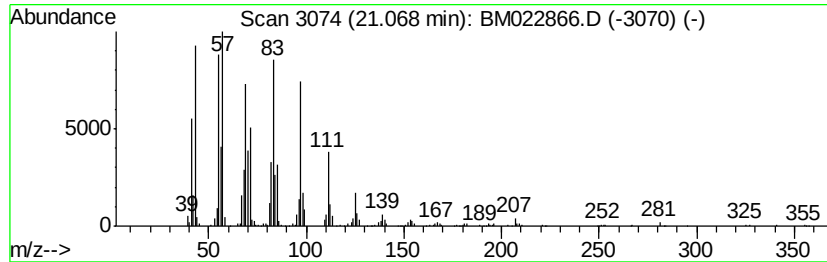

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
Data File : BM022866.D
Acq On : 01 Oct 2019 22:18
Operator : JU
Sample : PB123400BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK00

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Cyc...	21.07	4.0	ng/ul	611555	5	21.36	3021390	20.0