

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
 Data File : BM022911.D
 Acq On : 03 Oct 2019 02:16
 Operator : JU
 Sample : PB123379BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	45	49	60	rVB	21195	38380	0.79%	0.075%
2	3.916	153	158	163	rBV	26774	39895	0.82%	0.078%
3	4.004	169	173	178	rVB	10107	13246	0.27%	0.026%
4	4.099	186	189	193	rVB4	7630	10759	0.22%	0.021%
5	6.193	540	545	549	rBV2	5884	8254	0.17%	0.016%
6	6.475	589	593	601	rVB6	3792	6314	0.13%	0.012%
7	6.963	670	676	687	rBV	363432	631483	13.00%	1.235%
8	7.128	697	704	716	rBV	651414	1079159	22.22%	2.110%
9	7.334	731	739	749	rBV	824423	1298293	26.73%	2.539%
10	7.798	811	818	826	rBV	823043	1282786	26.41%	2.509%
11	7.869	827	830	835	rVB	8115	11021	0.23%	0.022%
12	8.504	931	938	951	rBV	740125	1221429	25.15%	2.389%
13	8.622	951	958	963	rVV	32590	52295	1.08%	0.102%
14	8.951	1006	1014	1024	rBV	885959	1436085	29.57%	2.808%
15	9.122	1040	1043	1048	rVB5	3225	5042	0.10%	0.010%
16	9.398	1085	1090	1094	rVV	9565	12761	0.26%	0.025%
17	9.457	1096	1100	1103	rVV4	8406	13753	0.28%	0.027%
18	9.510	1103	1109	1117	rVB3	9854	25367	0.52%	0.050%
19	9.669	1128	1136	1152	rBV	731014	1209461	24.90%	2.365%
20	10.210	1220	1228	1240	rBV	1188284	1945866	40.07%	3.805%
21	10.516	1273	1280	1285	rBV4	5261	10091	0.21%	0.020%
22	10.586	1285	1292	1300	rBV	1238467	2018184	41.56%	3.947%
23	10.722	1308	1315	1323	rBV	283827	492632	10.14%	0.963%
24	10.810	1326	1330	1339	rVB5	4002	9537	0.20%	0.019%
25	12.180	1558	1563	1568	rVB	16541	25680	0.53%	0.050%
26	13.845	1839	1846	1850	rBV	2176165	2984711	61.46%	5.837%
27	13.886	1850	1853	1864	rVB	235524	310466	6.39%	0.607%
28	14.127	1885	1894	1902	rBV	2440527	3673130	75.63%	7.183%
29	14.339	1927	1930	1936	rBV4	3462	5901	0.12%	0.012%
30	14.433	1939	1946	1956	rBV	1970709	2828074	58.23%	5.530%
31	14.627	1973	1979	1994	rBV	266318	415590	8.56%	0.813%
32	14.851	2011	2017	2020	rBV5	11059	14406	0.30%	0.028%
33	15.245	2078	2084	2088	rBV6	3012	5606	0.12%	0.011%
34	15.292	2088	2092	2096	rVB3	5000	5824	0.12%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
Data File : BM022911.D
Acq On : 03 Oct 2019 02:16
Operator : JU
Sample : PB123379BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK79

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Title : SVOA CALIBRATION

35	15.427	2108	2115	2123	rBV	3091641	4480770	92.26%	8.762%
36	15.539	2128	2134	2144	rBV	698568	934436	19.24%	1.827%
37	15.663	2149	2155	2159	rBV	31802	44766	0.92%	0.088%
38	16.157	2235	2239	2242	rBV5	3372	5279	0.11%	0.010%
39	16.204	2244	2247	2251	rVB3	9187	12446	0.26%	0.024%
40	16.957	2371	2375	2381	rVB2	5711	9422	0.19%	0.018%
41	17.168	2405	2411	2418	rBV2	2070683	2965660	61.07%	5.800%
42	17.268	2421	2428	2440	rBV2	3447050	4820487	99.26%	9.427%
43	17.362	2441	2444	2448	rVB4	6796	8364	0.17%	0.016%
44	17.415	2448	2453	2457	rBV6	4804	7261	0.15%	0.014%
45	18.068	2560	2564	2570	rBV	66000	86451	1.78%	0.169%
46	19.003	2720	2723	2727	rBV5	5359	6979	0.14%	0.014%
47	19.198	2752	2756	2759	rBV	34050	40892	0.84%	0.080%
48	19.345	2778	2781	2785	rBV4	23263	30607	0.63%	0.060%
49	19.451	2794	2799	2803	rBV	27449	40019	0.82%	0.078%
50	19.562	2812	2818	2831	rBV	3722343	4856548	100.00%	9.497%
51	21.068	3071	3074	3080	rVB3	70607	91070	1.88%	0.178%
52	21.350	3117	3122	3129	rBV	1931967	2421539	49.86%	4.735%
53	21.509	3146	3149	3152	rBV	74836	79325	1.63%	0.155%
54	21.944	3221	3223	3227	rVB	99912	102950	2.12%	0.201%
55	22.415	3300	3303	3309	rVB	139356	173892	3.58%	0.340%
56	22.927	3387	3390	3396	rVB	159869	220186	4.53%	0.431%
57	23.468	3475	3482	3495	rVB	2102500	4207653	86.64%	8.228%
58	23.609	3500	3506	3517	rVB	1253005	2347885	48.34%	4.591%


Sum of corrected areas: 51136368

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
Data File : BM022911.D
Acq On : 03 Oct 2019 02:16
Operator : JU
Sample : PB123379BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK79

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

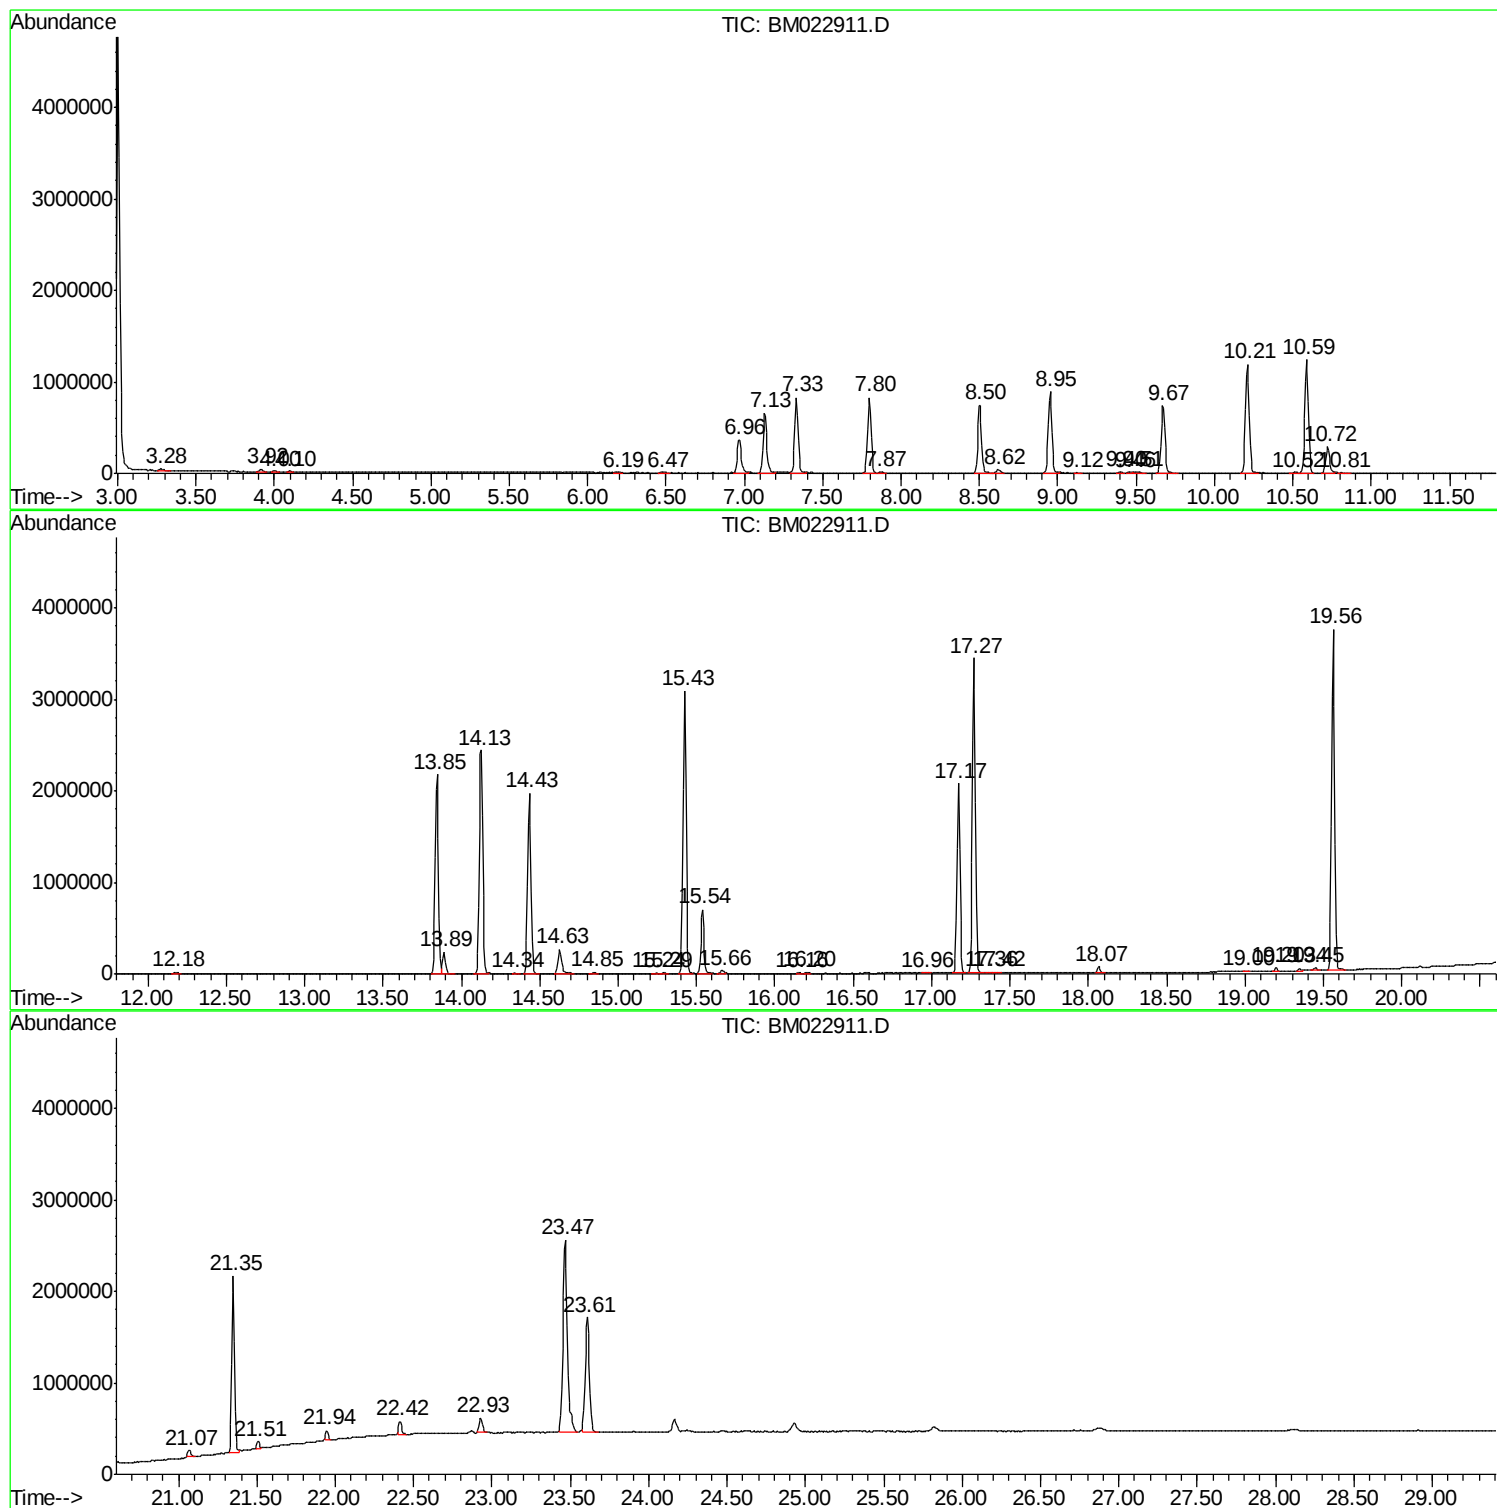

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
Data File : BM022911.D
Acq On : 03 Oct 2019 02:16
Operator : JU
Sample : PB123379BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK79

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100119\
Data File : BM022911.D
Acq On : 03 Oct 2019 02:16
Operator : JU
Sample : PB123379BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK79

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc