
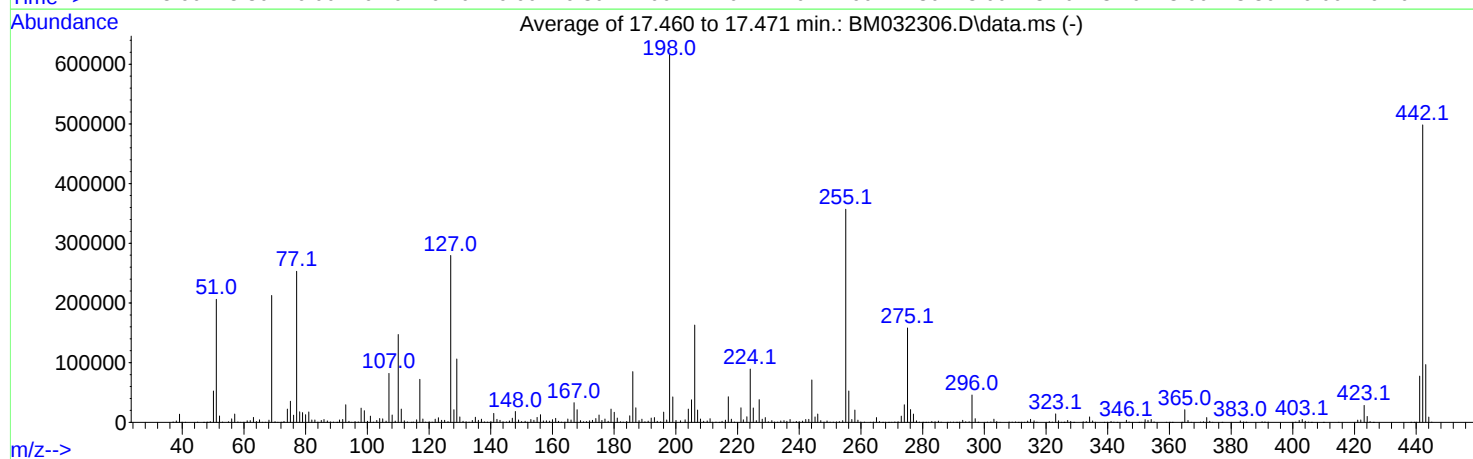


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100221\
 Data File : BM032306.D
 Acq On : 01 Oct 2021 09:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 18:34:58 2021

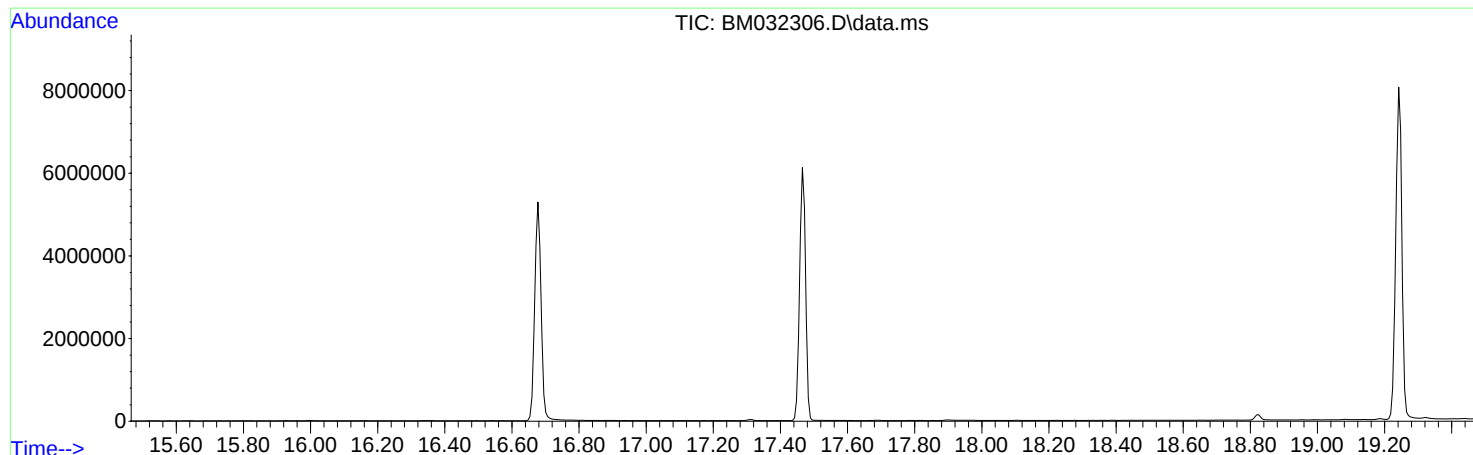




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	206241	PASS
68	69	0.00	2	1.7	3676	PASS
69	198	0.00	100	34.5	212551	PASS
70	69	0.00	2	0.5	1166	PASS
127	198	10	80	45.4	279552	PASS
197	198	0.00	2	0.6	3941	PASS
198	198	100	100	100.0	616277	PASS
199	198	5	9	6.9	42725	PASS
275	198	10	60	25.7	158203	PASS
365	198	1	100	3.4	21257	PASS
441	198	0.01	100	12.6	77381	PASS
442	442	50	100	100.0	498347	PASS
443	442	15	24	19.4	96848	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100221\
Data File : BM032306.D
Acq On : 01 Oct 2021 09:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 01 11:28:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 11:23:50 2021
Response via : Initial Calibration

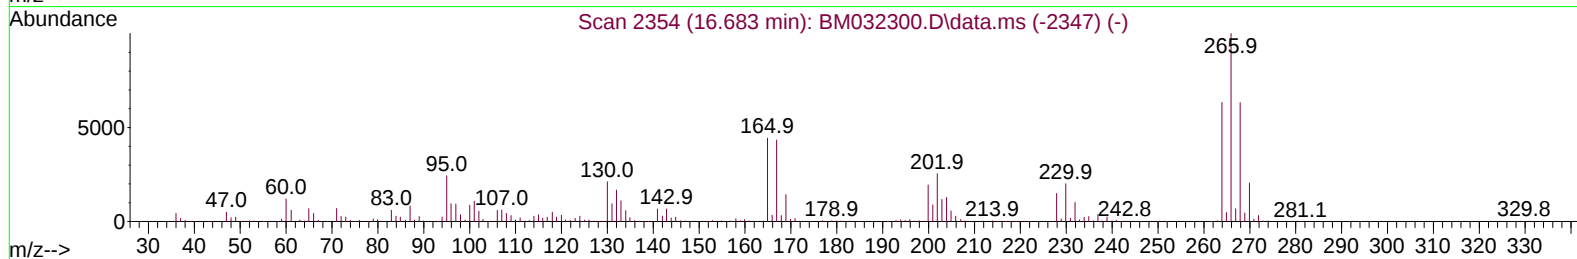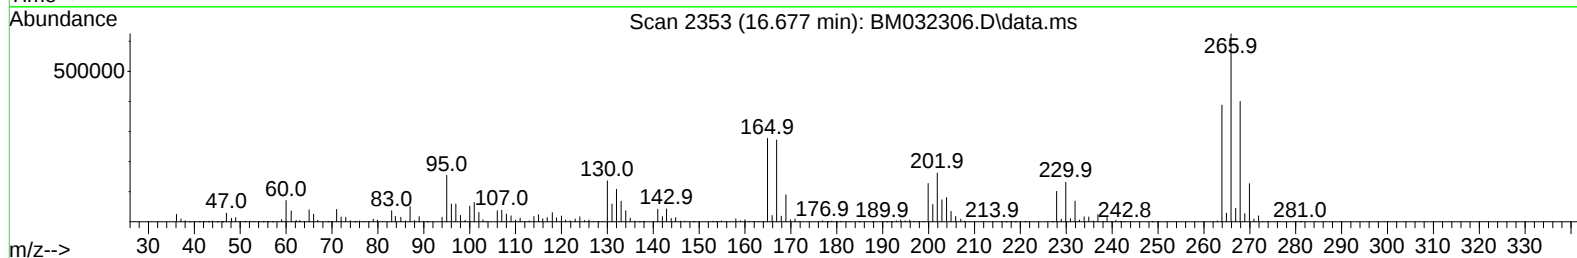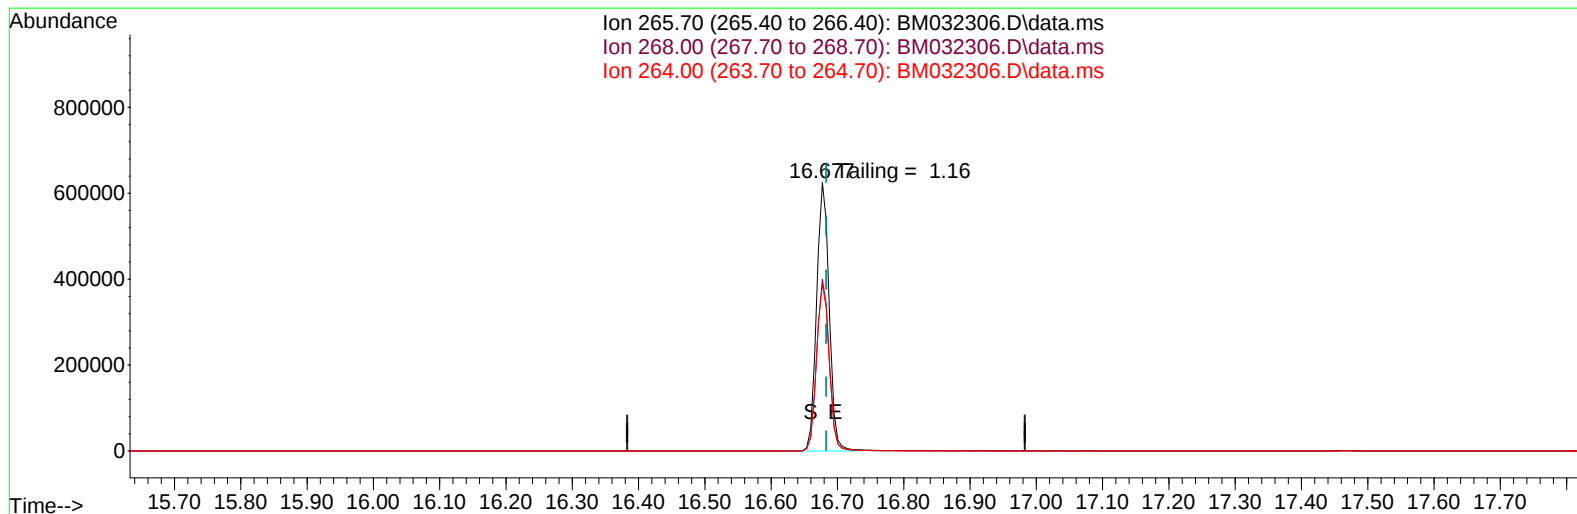

TIC: BM032306.D\data.ms

(70) Pentachlorophenol (C)

16.677min (-0.006) 0.00 ng




response 829600

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.04
264.00	65.10	62.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100221\
Data File : BM032306.D
Acq On : 01 Oct 2021 09:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 01 11:28:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 11:23:50 2021
Response via : Initial Calibration

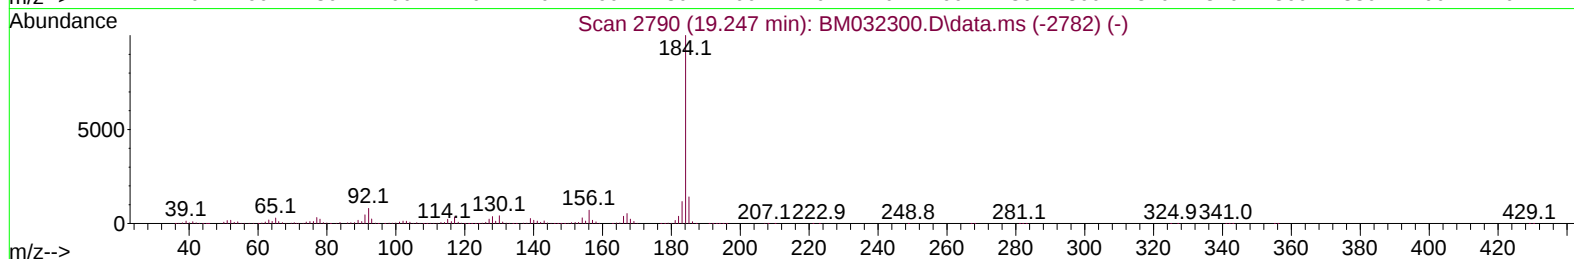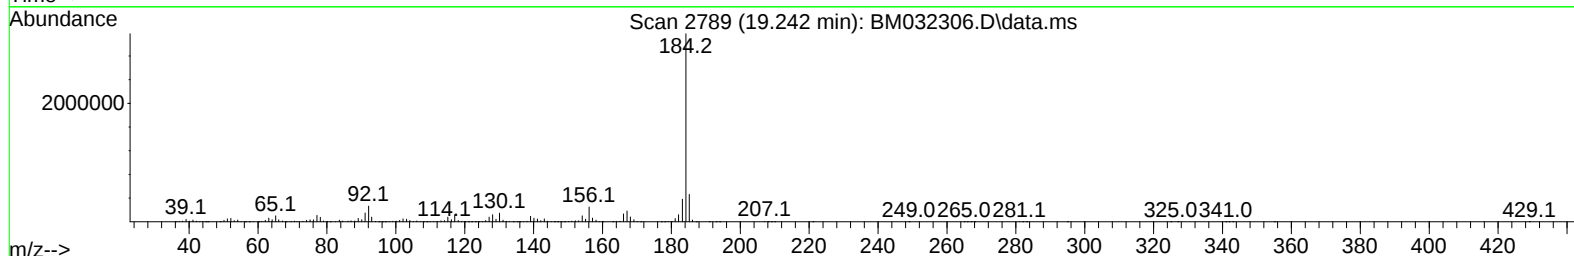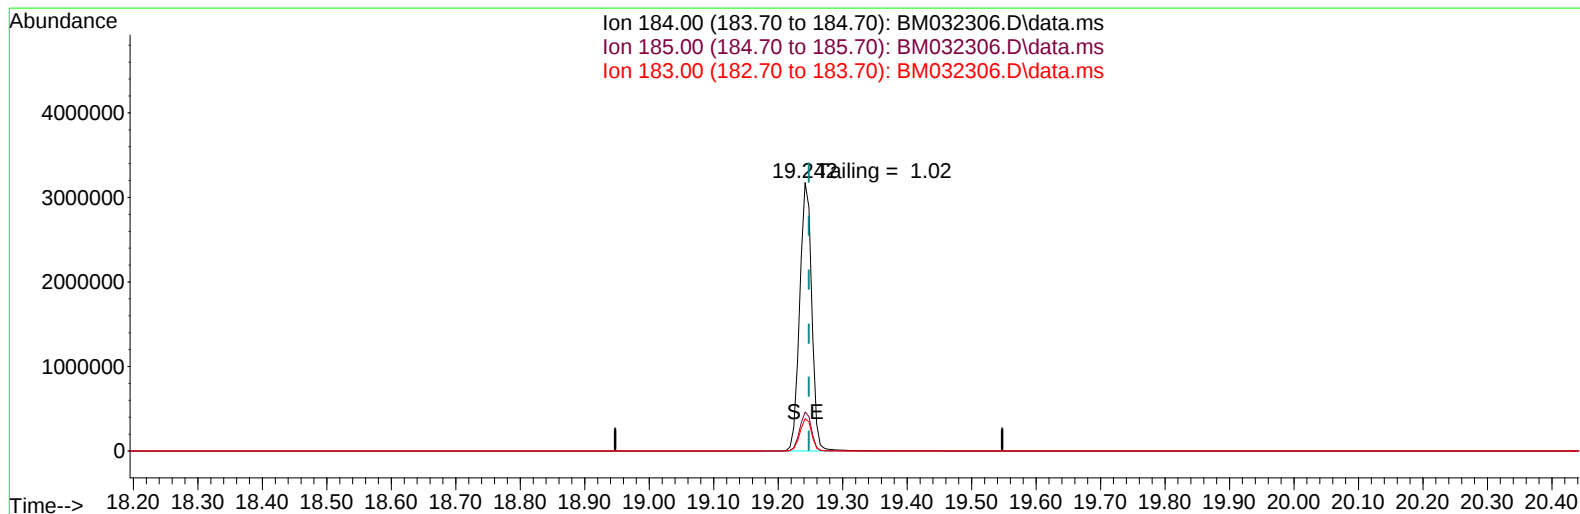

TIC: BM032306.D\data.ms

(77) Benzidine

19.242min (-0.006) 613952.67 ng

response 4123305

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.59
183.00	11.20	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/2/2021	BNA_M	<u>BM032306.D</u>
Compound Name	Response	Retention Time
DDT	2020039	20.48
DDD	34284	20.04
DDE	3632	19.54
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37916	2057955	1.84