
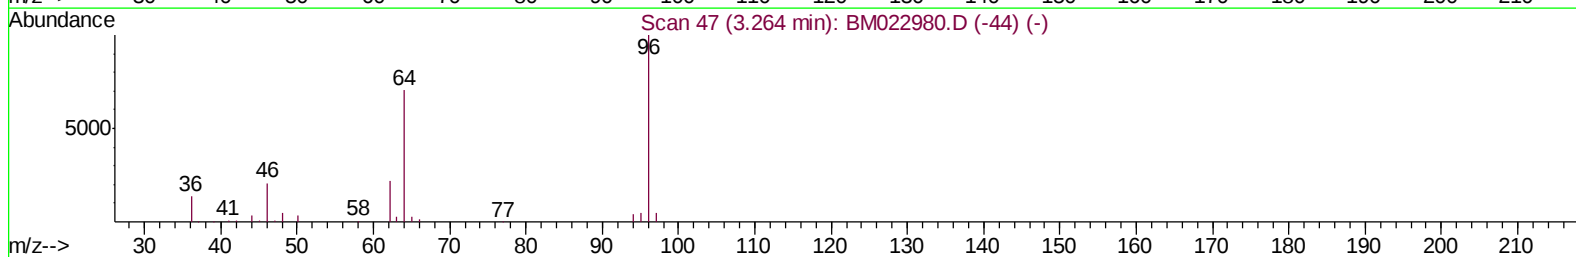
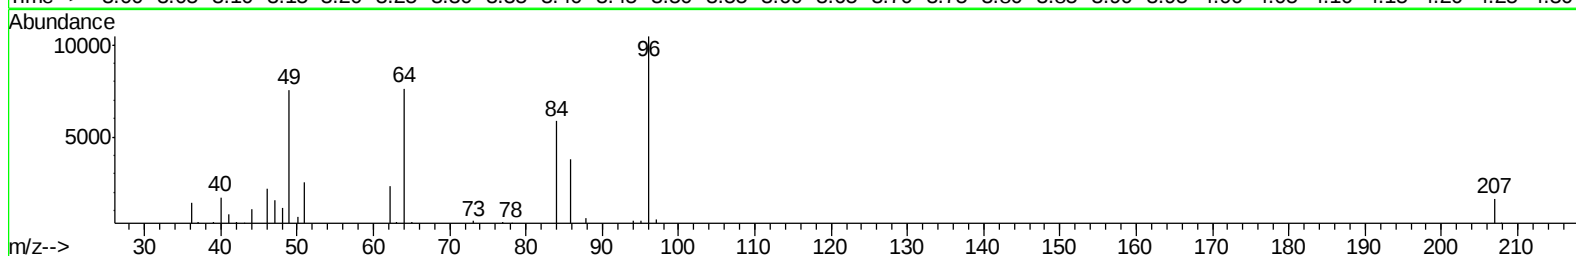


Data File : BM023001.D
Acq On : 05 Oct 2019 20:52
Operator : JU
Sample : K5050-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 06 23:35:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 16:45:59 2019
Response via : Initial Calibration

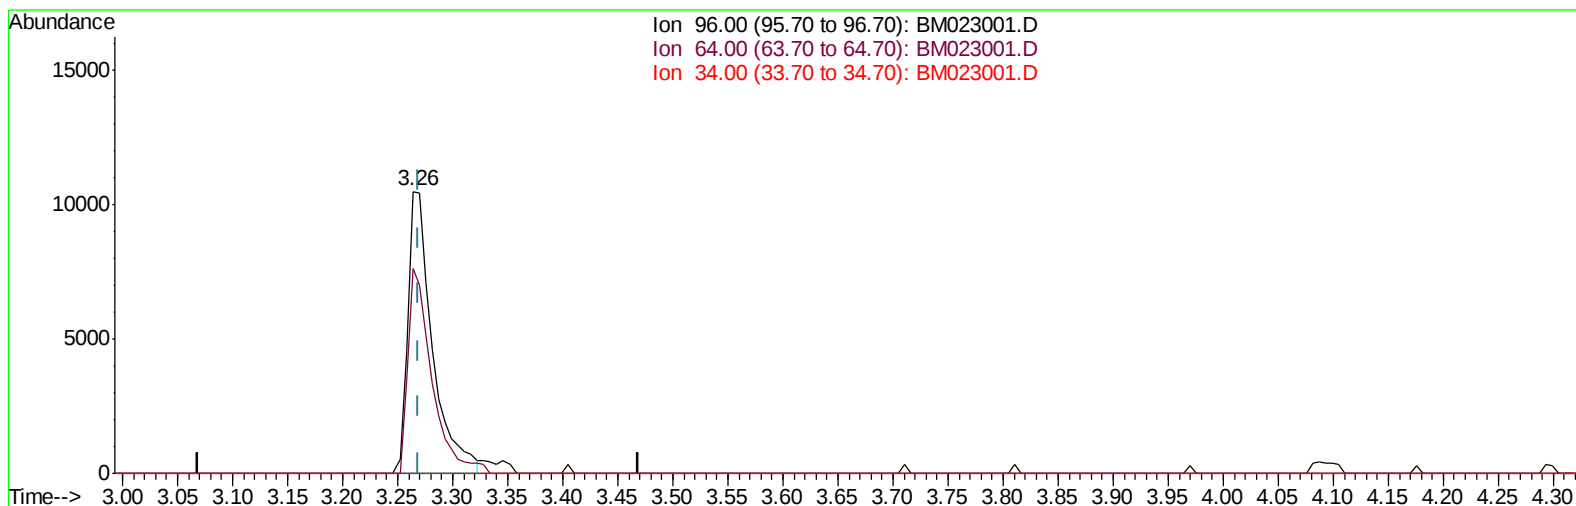

TIC: BM023001.D

(3) 1,4-Dioxane-d8 (S)

3.264min (-0.006) 3.07ng/uL

response 16479

Ion	Exp%	Act%
96.00	100	100
64.00	71.10	72.80
34.00	0.00	0.00
0.00	0.00	0.00