
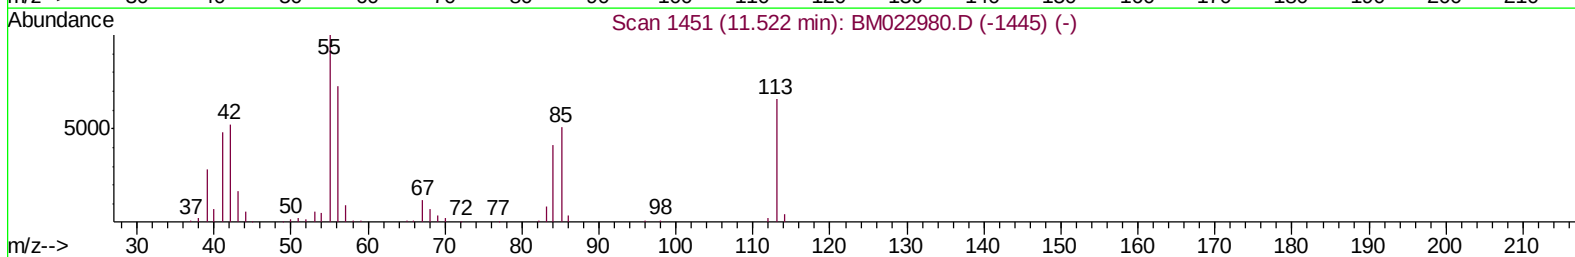
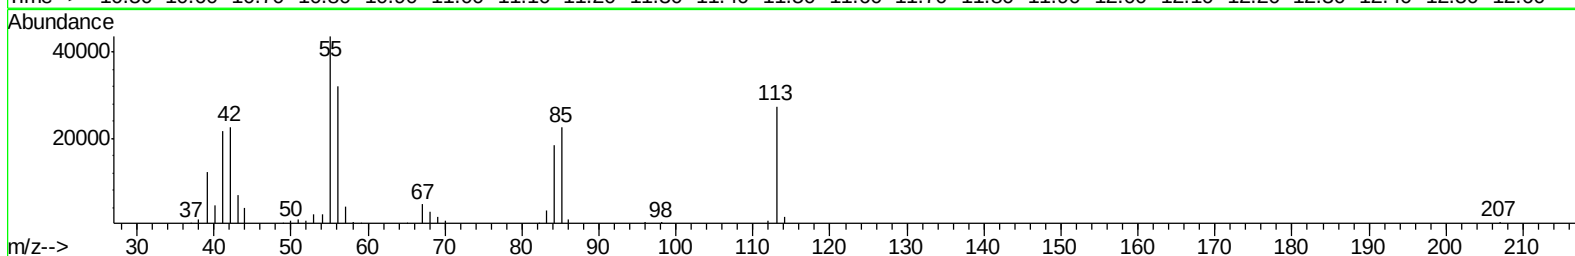


Data File : BM023006.D
Acq On : 05 Oct 2019 23:52
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Oct 07 02:45:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 07 01:10:23 2019
Response via : Initial Calibration

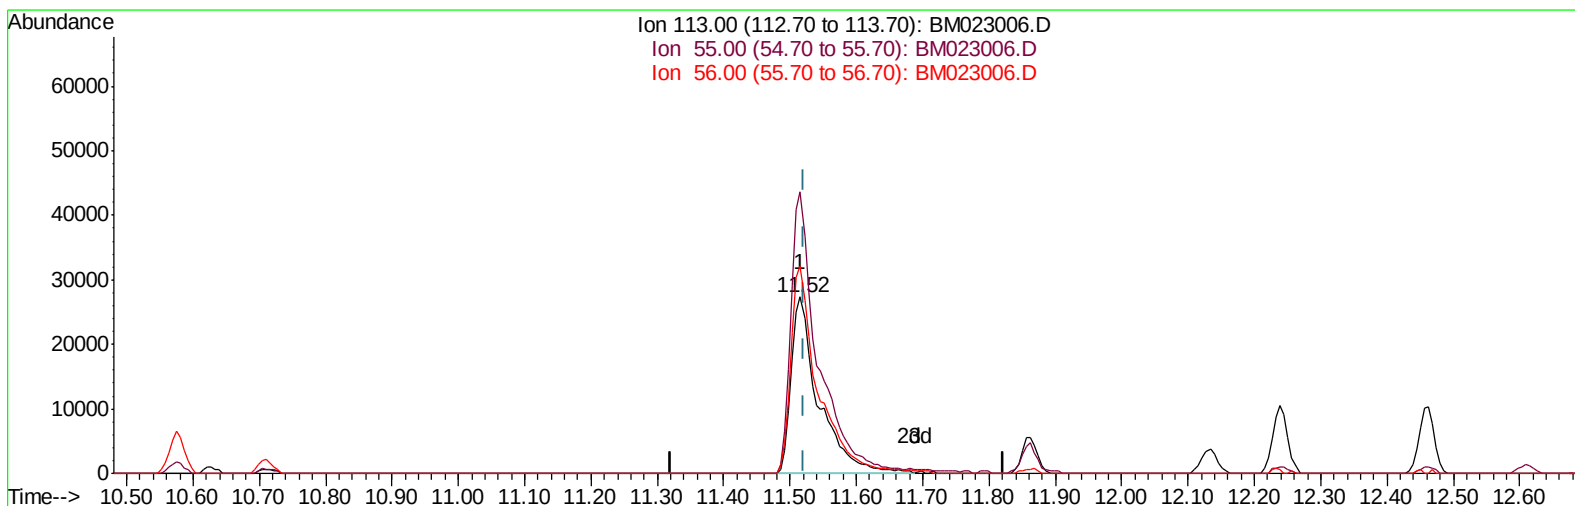

TIC: BM023006.D

(32) Caprolactam

11.516min (-0.006) 13.97ng/ul m

response 77104

Ion	Exp%	Act%
113.00	100	100
55.00	150.70	159.55
56.00	114.30	117.75
0.00	0.00	0.00