
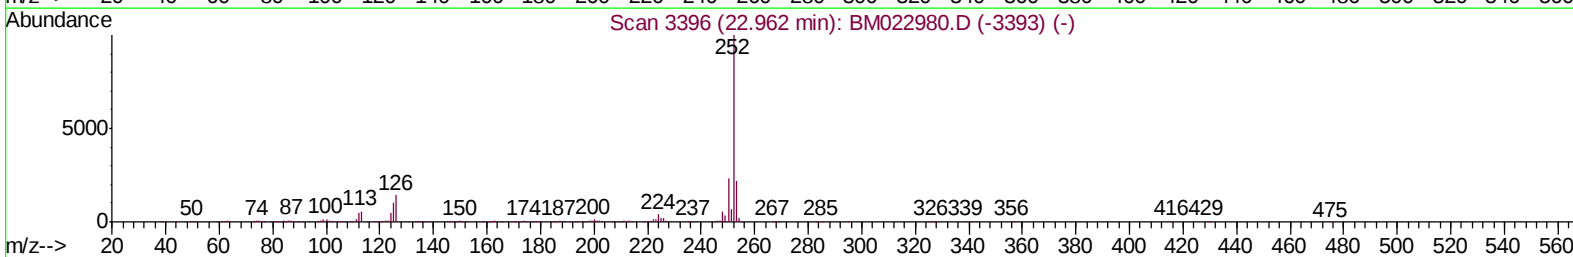
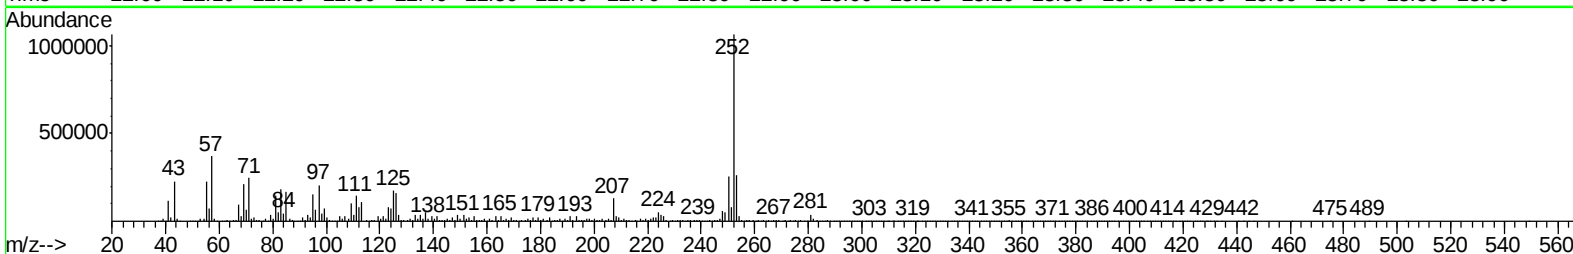


Data File : BM023018.D
Acq On : 06 Oct 2019 09:29
Operator : JU
Sample : K5057-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Oct 06 23:37:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 16:45:59 2019
Response via : Initial Calibration

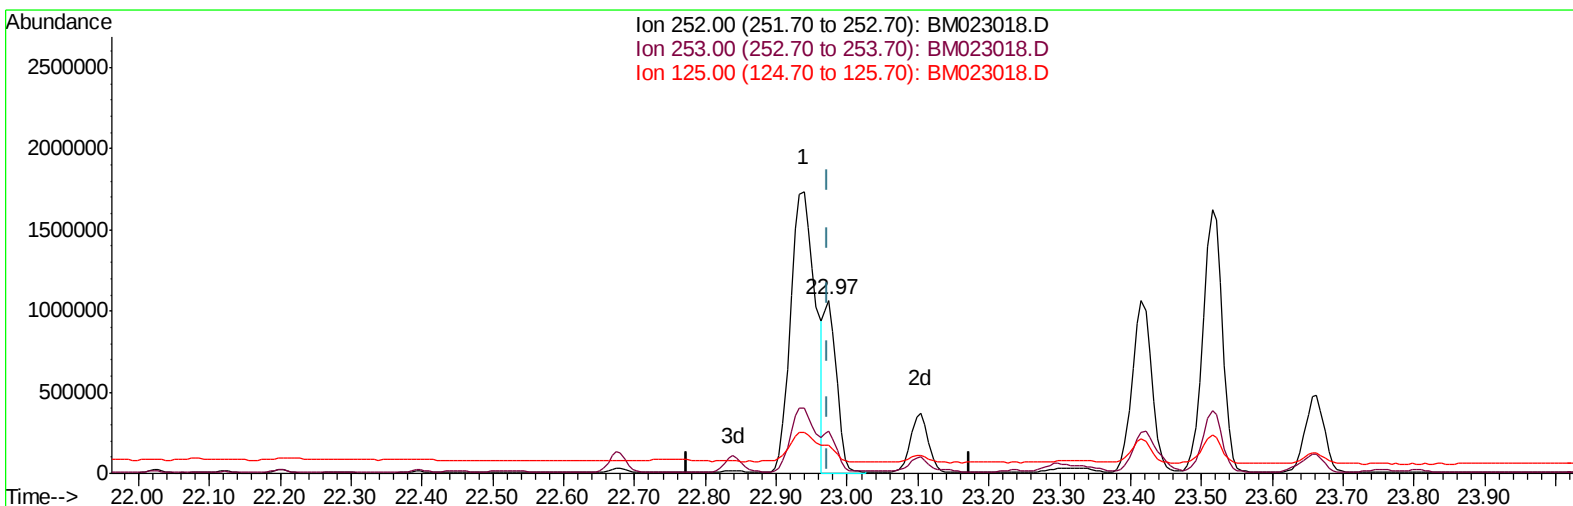

TIC: BM023018.D

(89) Benzo(k)fluoranthene

22.974min (+0.000) 17.94ng/ul m

response 1385198

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	24.47
125.00	9.90	16.35#
0.00	0.00	0.00