
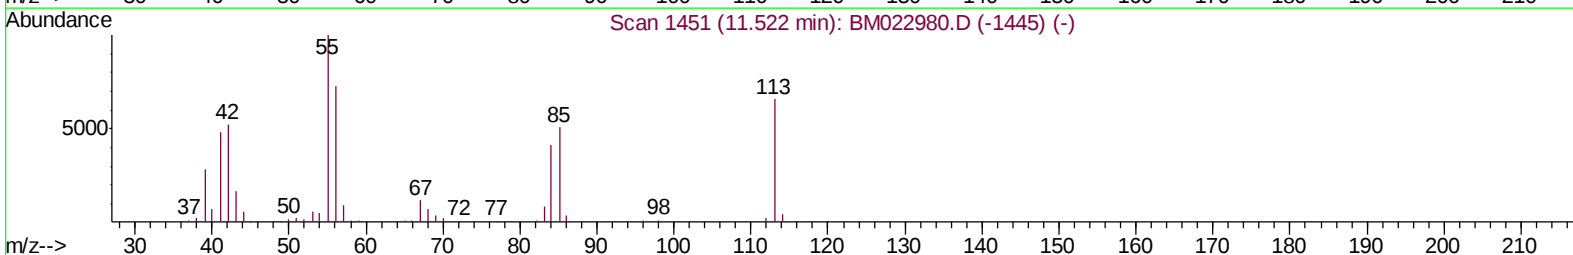
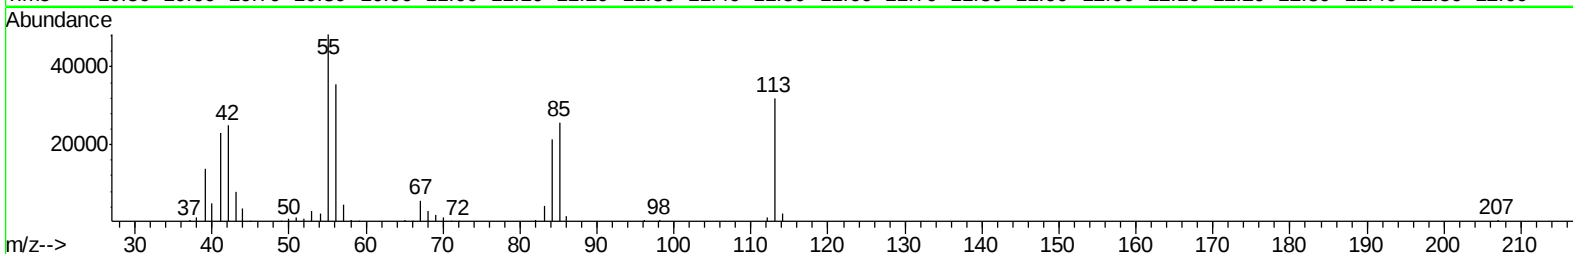


Data File : BM023029.D
Acq On : 06 Oct 2019 16:03
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 46 Sample Multiplier: 1

Quant Time: Oct 06 23:38:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 16:45:59 2019
Response via : Initial Calibration

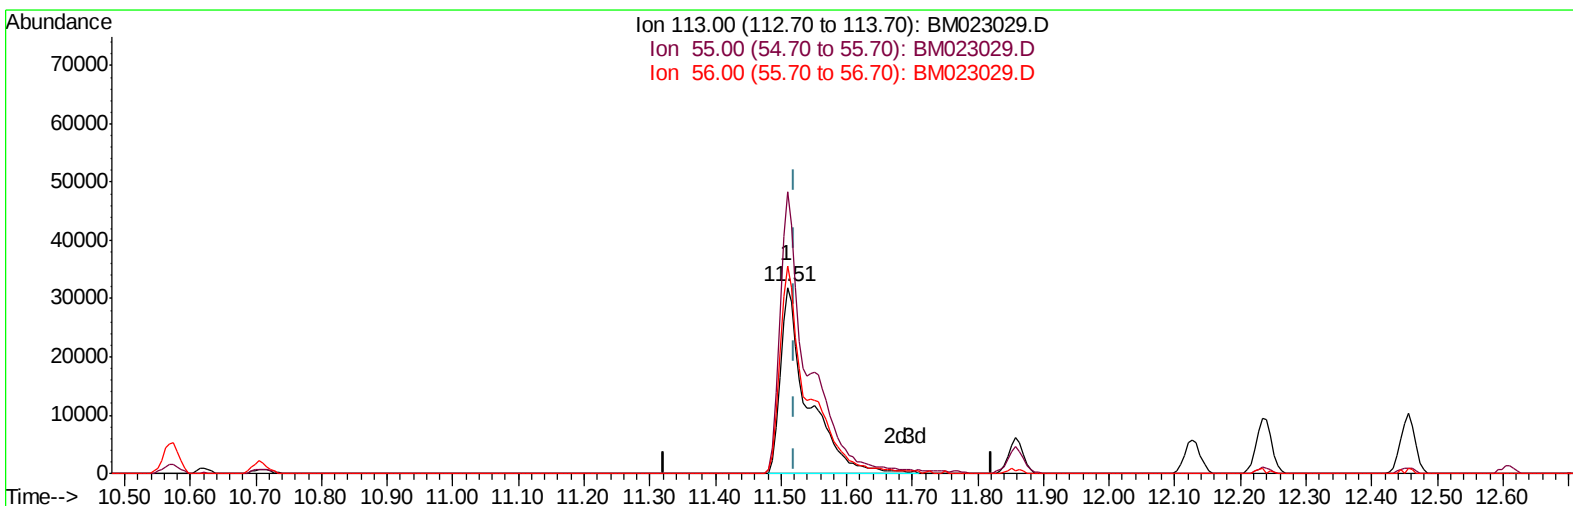

TIC: BM023029.D

(32) Caprolactam

11.510min (-0.012) 19.14ng/ul m

response 92842

Ion	Exp%	Act%
113.00	100	100
55.00	150.70	151.50
56.00	114.30	111.61
0.00	0.00	0.00