

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM022940.D
 Acq On : 04 Oct 2019 03:38
 Operator : JU
 Sample : K4988-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 04 04:36:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 02:36:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	247985	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1080603	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.43	164	665342	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	1338896	20.00	ng/ul	0.00
78) Chrysene-d12	21.35	240	1018889	20.00	ng/ul	0.00
86) Perylene-d12	23.61	264	971557	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	18135	3.16	ng/uL	0.00
5) Phenol-d5	6.96	99	362204	16.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	214490	17.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	312241	17.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	243806	13.59	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	155591	18.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	167751	18.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	320710	17.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	310432	14.09	ng/ul	0.00
44) Dimethylphthalate-d6	13.84	166	991686	19.20	ng/ul	0.00
47) Acenaphthylene-d8	14.12	160	1170301	19.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	108939	10.68	ng/ul	0.00
58) Fluorene-d10	15.42	176	877475	19.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.54	200	78638	9.03	ng/ul	0.00
71) Anthracene-d10	17.27	188	1335685	20.43	ng/ul	0.00
79) Pyrene-d10	19.56	212	1451981	26.48	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.47	264	1084990	21.59	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.99	94	60607	2.639	ng/ul 98
45) Dimethylphthalate	13.89	163	379055	7.146	ng/ul 100
70) Phenanthrene	17.21	178	137268	1.718	ng/ul 99
77) Fluoranthene	19.23	202	358626	3.990	ng/ul 99
80) Pyrene	19.59	202	289712	4.011	ng/ul 98
83) Benzo(a)anthracene	21.33	228	126526	1.730	ng/ul 98
85) Chrysene	21.39	228	133566	1.980	ng/ul 98
88) Benzo(b)fluoranthene	22.93	252	165295	2.564	ng/ul# 92
89) Benzo(k)fluoranthene	22.93	252	165295	2.680	ng/ul# 91
91) Benzo(a)pyrene	23.51	252	108164	1.788	ng/ul# 91
92) Indeno(1,2,3-cd)pyrene	25.89	276	82031	1.277	ng/ul 96
94) Benzo(g,h,i)perylene	26.60	276	81755	1.577	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM022940.D
Acq On : 04 Oct 2019 03:38
Operator : JU
Sample : K4988-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 04 04:36:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 02:36:53 2019
Response via : Initial Calibration

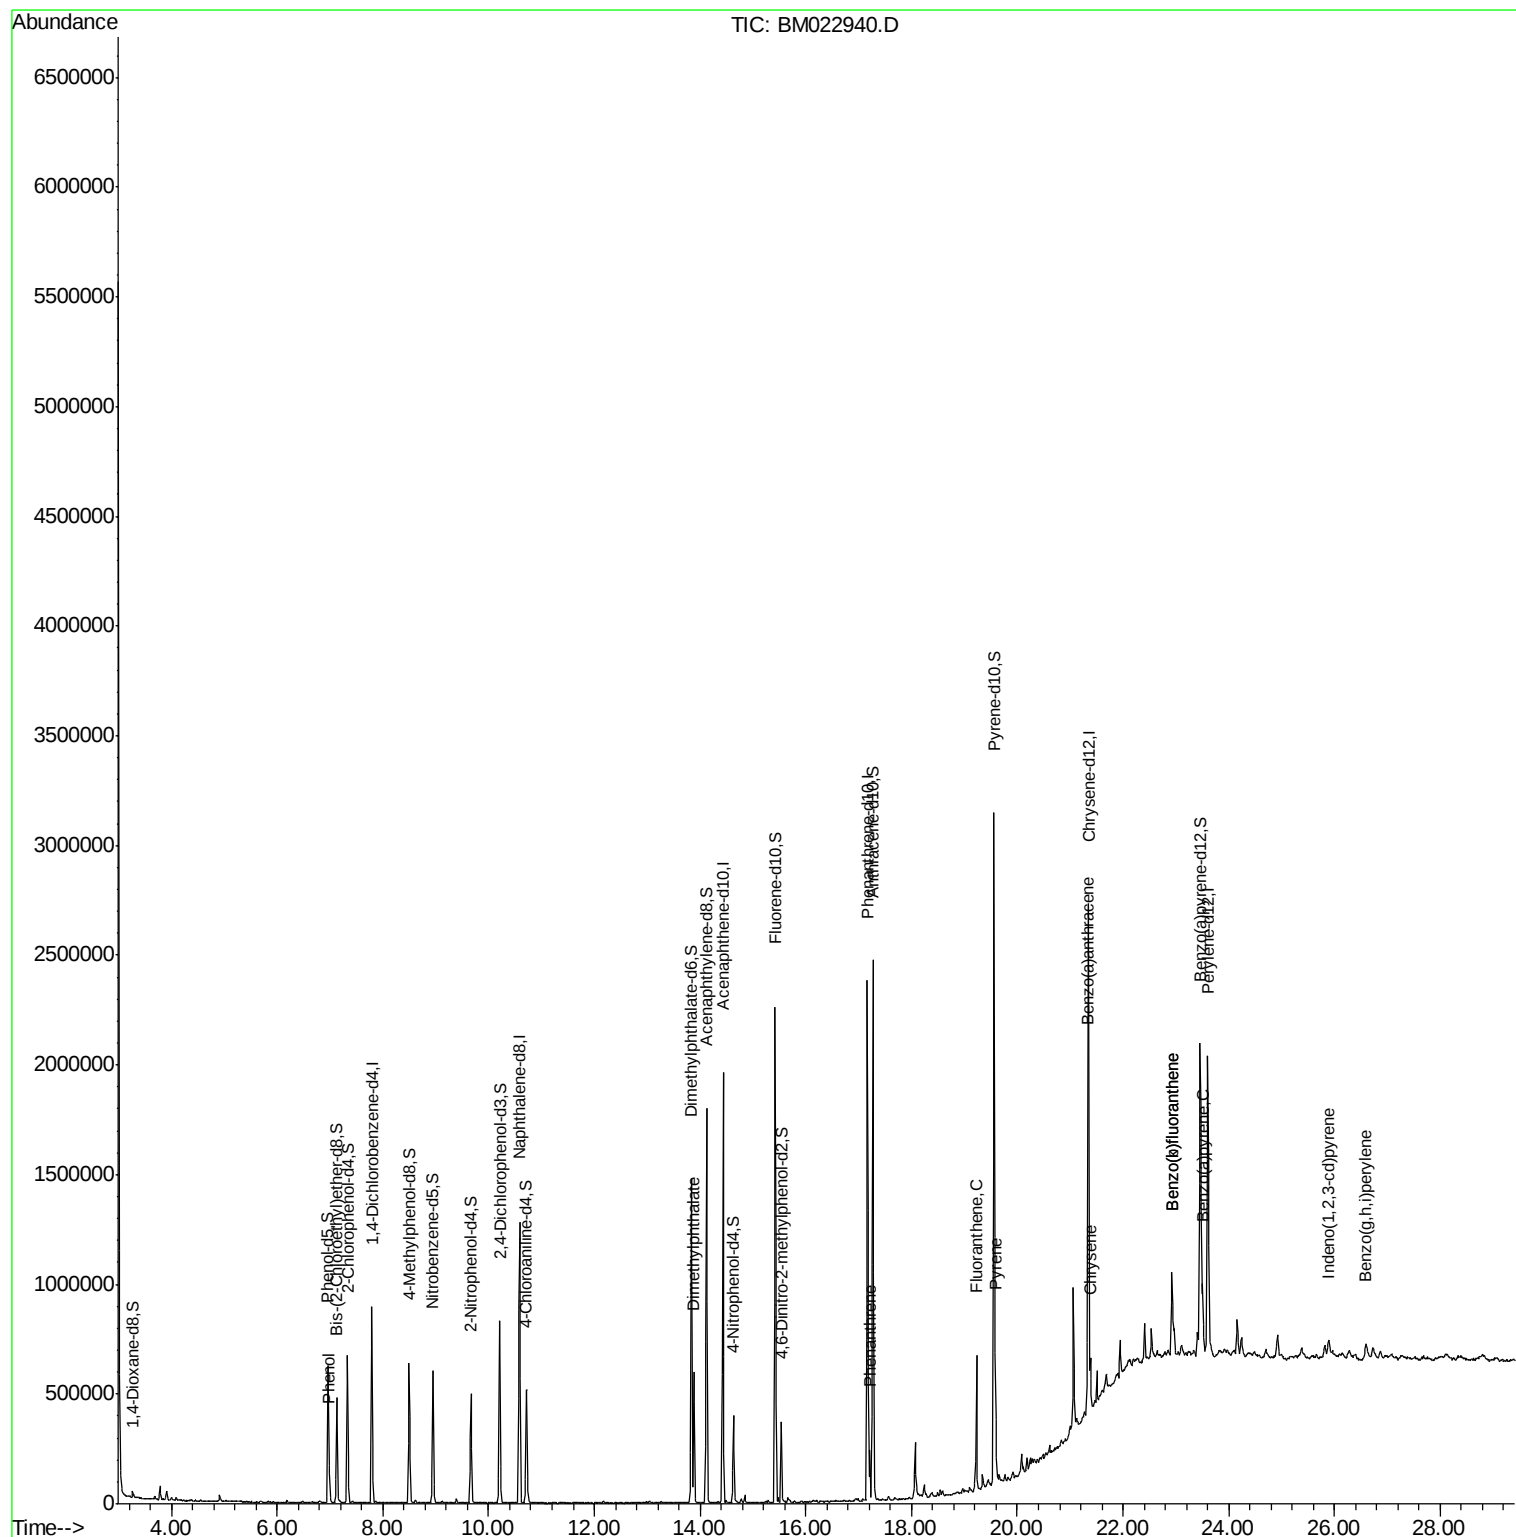

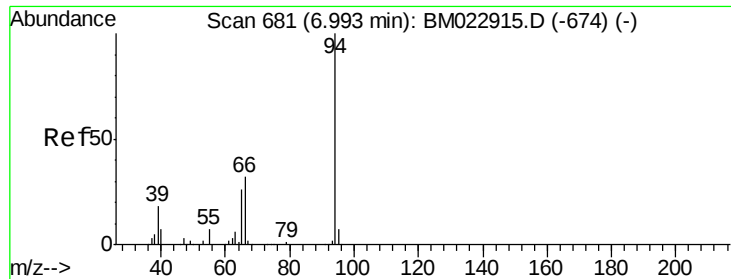





#6

Phenol

Concen: 2.639 ng/ul
 RT: 6.99 min Scan# 681
 Delta R.T. -0.00 min
 Lab File: BM022940.D
 Acq: 04 Oct 2019 03:38

Instrument :
 BNA_M
 ClientSampled :

Tot Ion	94	Resp	60607
Ion Ratio	Lower	Upper	
94	100		
65	27.8	20.9	31.3
66	34.8	27.2	40.8

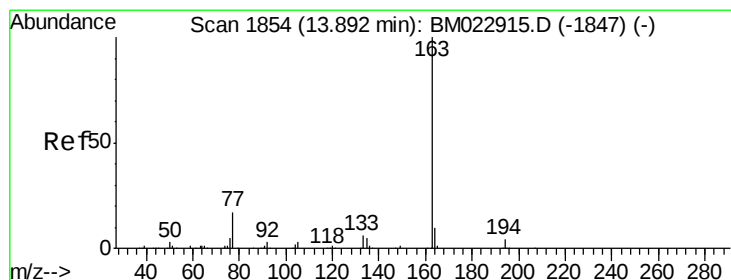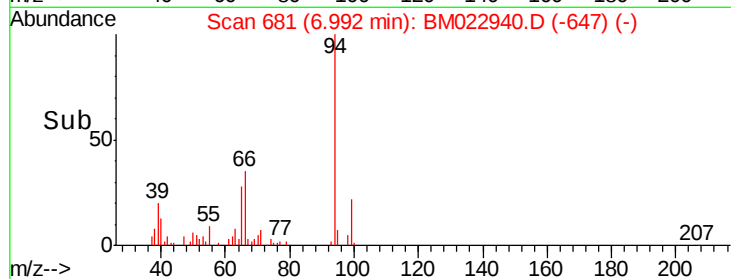
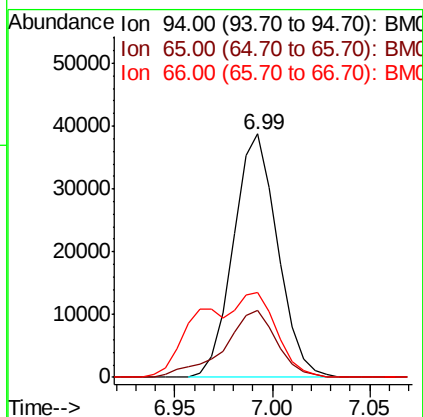
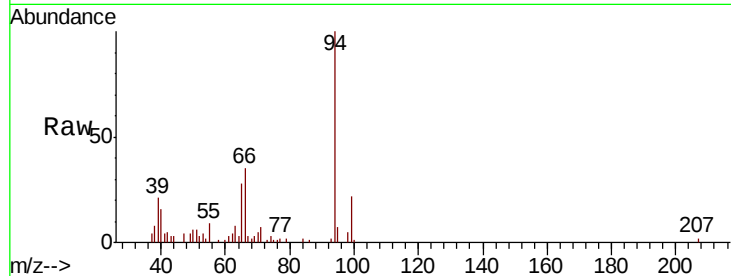



#45

Dimethylphthalate

Concen: 7.146 ng/ul
 RT: 13.89 min Scan# 1853
 Delta R.T. -0.01 min
 Lab File: BM022940.D
 Acq: 04 Oct 2019 03:38

Tgt Ion	163	Resp	379055
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.4	5.0
164	10.0	8.1	12.1

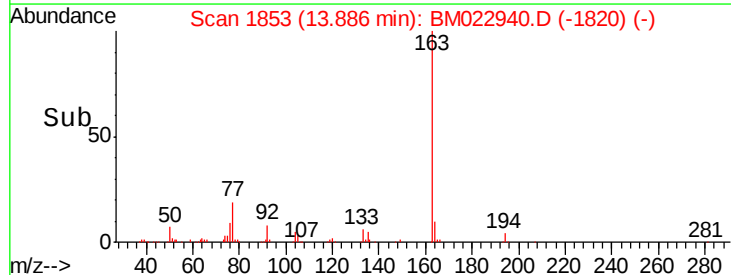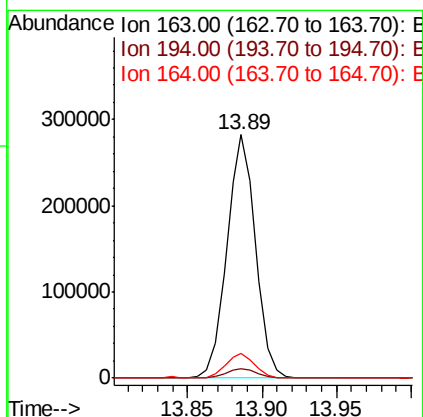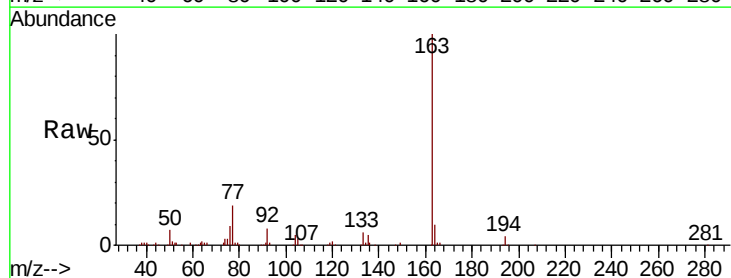

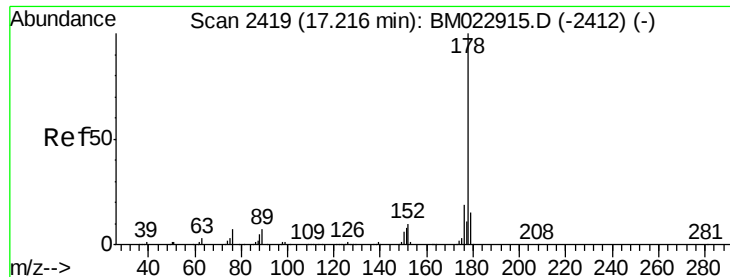

#70

Phenanthrene

Concen: 1.718 ng/ul

RT: 17.21 min Scan# 2418

Delta R.T. -0.01 min

Lab File: BM022940.D

Acq: 04 Oct 2019 03:38

Instrument :

BNA_M

ClientSampleId :


Tot Ion:178 Resp: 137268

Ion Ratio Lower Upper




178 100

179 15.8 12.4 18.6

176 19.3 15.3 22.9

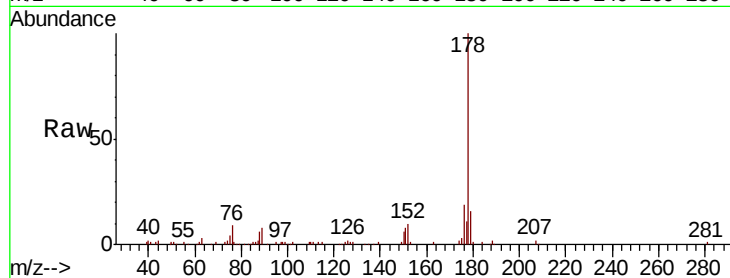

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

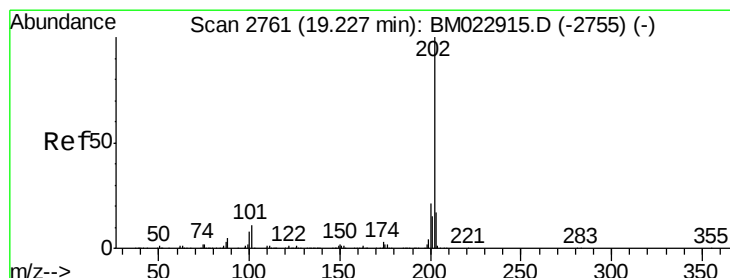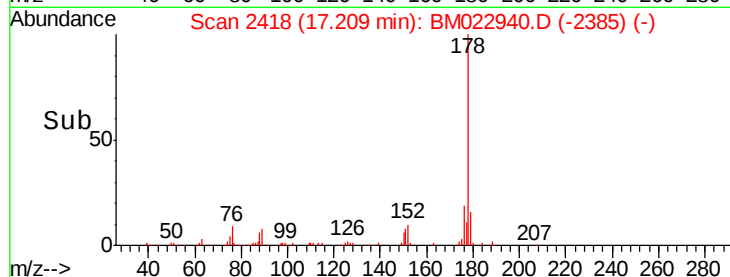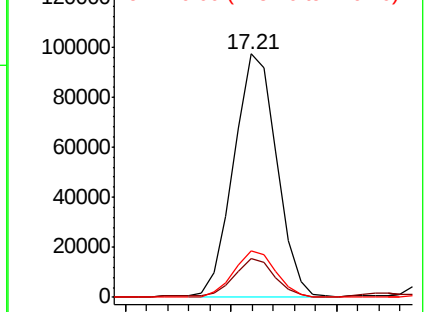

#77

Fluoranthene

Concen: 3.990 ng/ul

RT: 19.23 min Scan# 2761

Delta R.T. -0.00 min

Lab File: BM022940.D

Acq: 04 Oct 2019 03:38


Tgt Ion:202 Resp: 358626

Ion Ratio Lower Upper



202 100


101 10.4 8.6 12.8

100 7.6 6.4 9.6

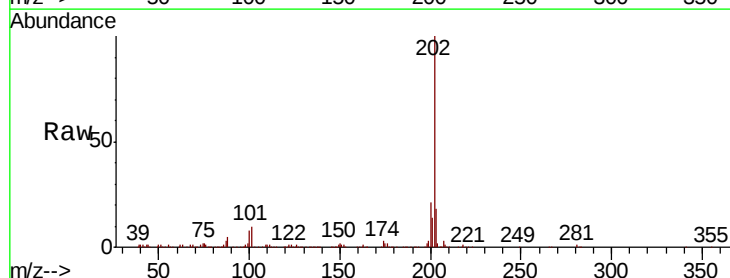

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

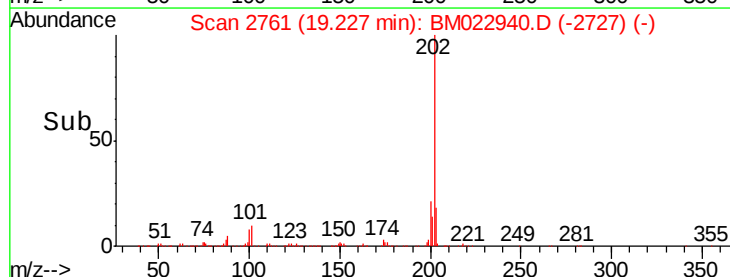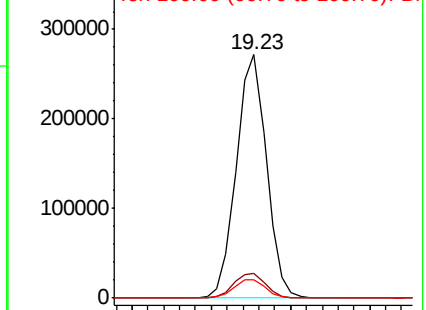


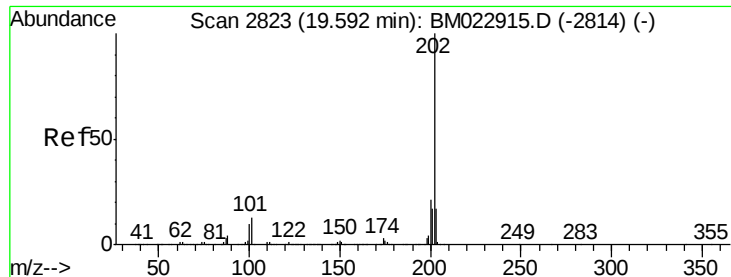




#80
 Pvrene
 Concen: 4.011 ng/ul
 RT: 19.59 min Scan# 2822
 Delta R.T. -0.01 min
 Lab File: BM022940.D
 Acq: 04 Oct 2019 03:38

Instrument :
 BNA_M
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
202	100		
101	12.9	9.7	14.5
100	10.7	7.8	11.8

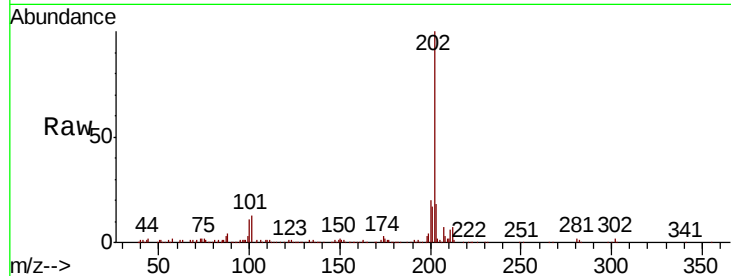


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

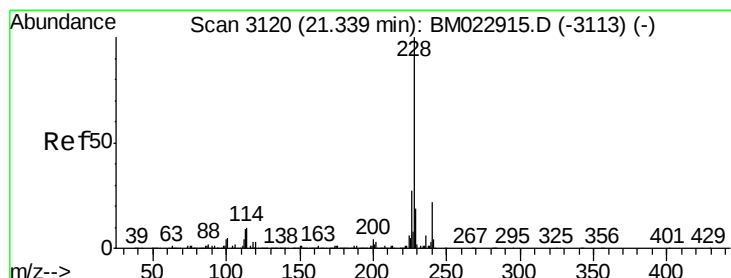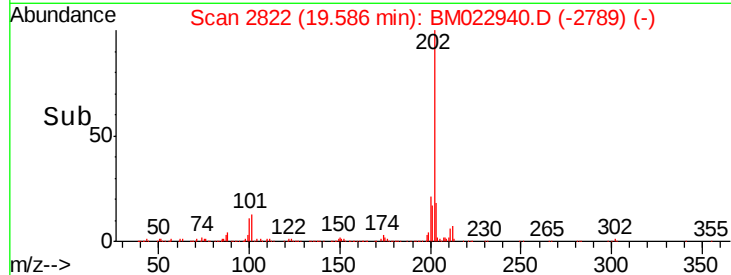
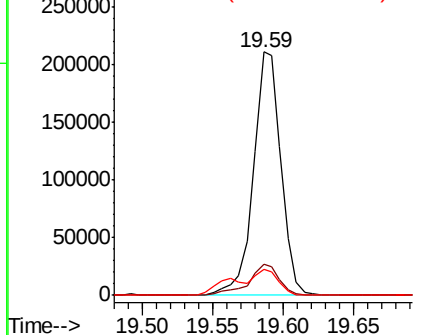



#83
 Benzo(a)anthracene
 Concen: 1.730 ng/ul
 RT: 21.33 min Scan# 3119
 Delta R.T. -0.01 min
 Lab File: BM022940.D
 Acq: 04 Oct 2019 03:38

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.3	15.8	23.8
226	27.5	22.4	33.6

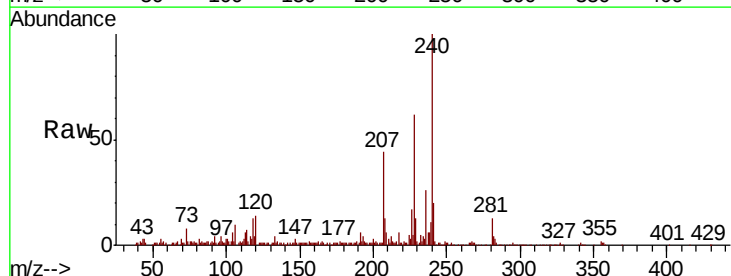

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 229.00 (228.70 to 229.70): E
 Ion 226.00 (225.70 to 226.70): E



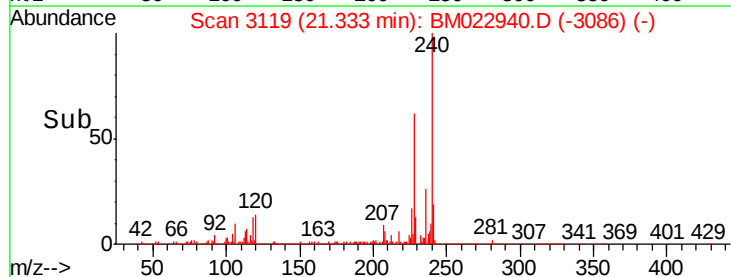
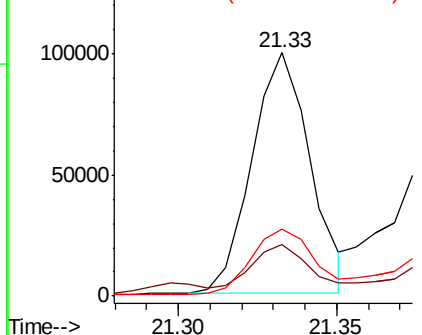


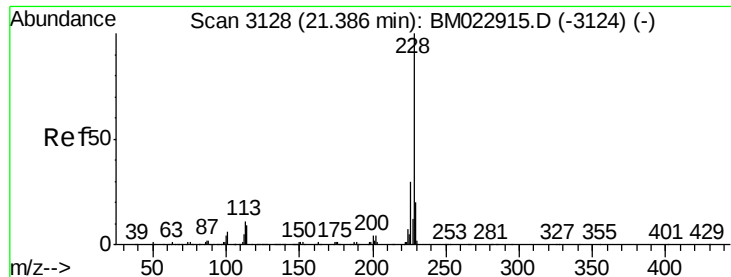

#85
Chrysene
Concen: 1.980 ng/ul
RT: 21.39 min Scan# 3128
Delta R.T. -0.00 min
Lab File: BM022940.D
Acq: 04 Oct 2019 03:38




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
228	100		
226	30.5	24.2	36.4
229	21.4	15.9	23.9

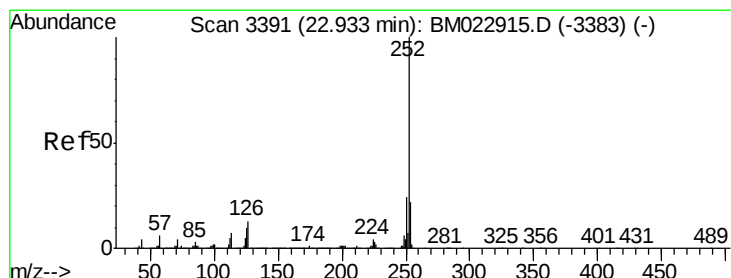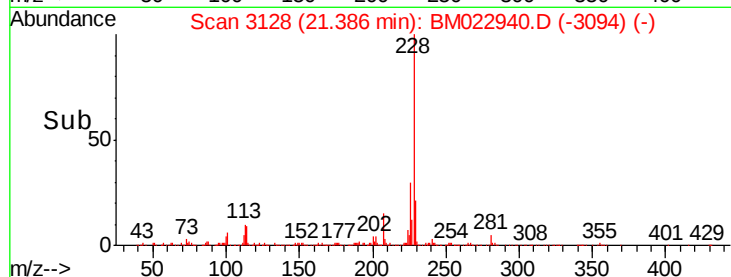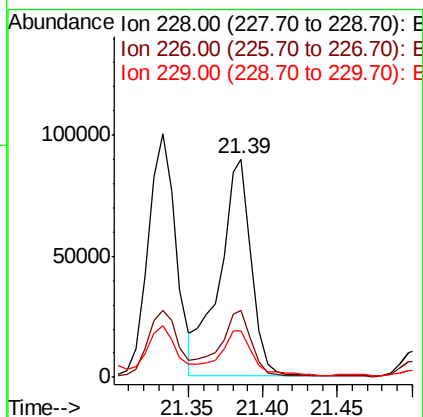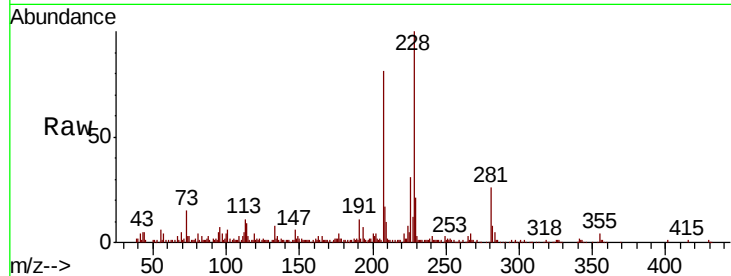

#88
Benzo(b)fluoranthene
Concen: 2.564 ng/ul
RT: 22.93 min Scan# 3390
Delta R.T. -0.01 min
Lab File: BM022940.D
Acq: 04 Oct 2019 03:38

Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.7	17.7	26.5
125	13.6	8.2	12.2#

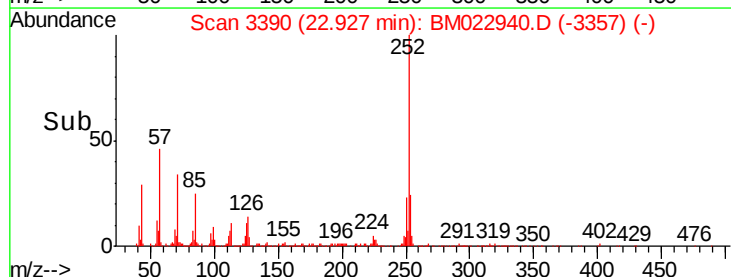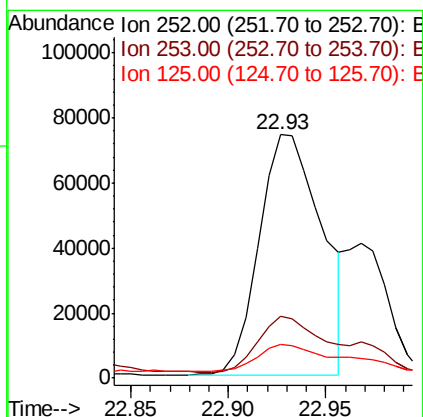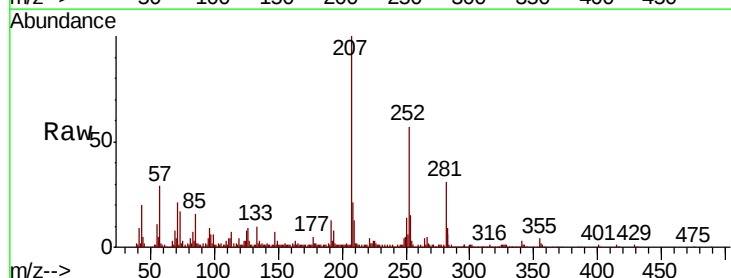

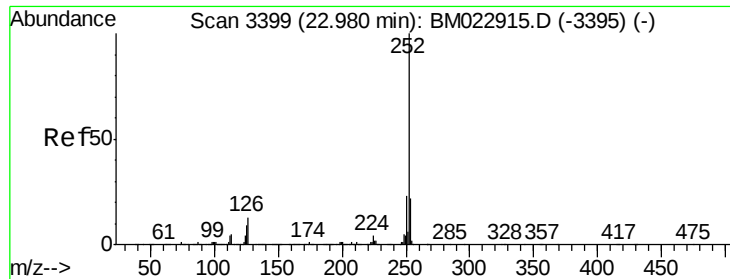

#89

Benzo(k)fluoranthene

Concen: 2.680 ng/ul

RT: 22.93 min Scan# 3390

Delta R.T. -0.05 min

Lab File: BM022940.D

Acq: 04 Oct 2019 03:38

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 165295

Ion Ratio Lower Upper

252 100

253 25.7 17.5 26.3




125 13.6 7.9 11.9#

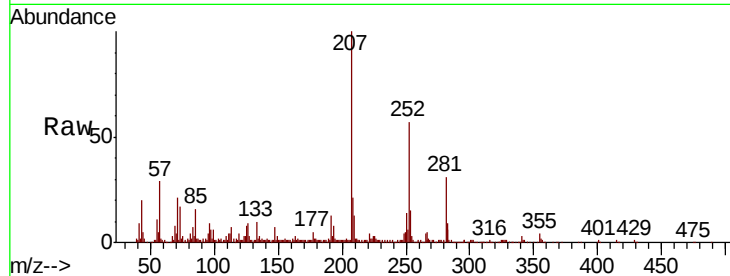

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

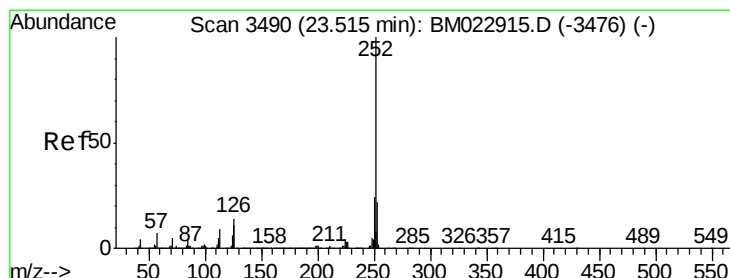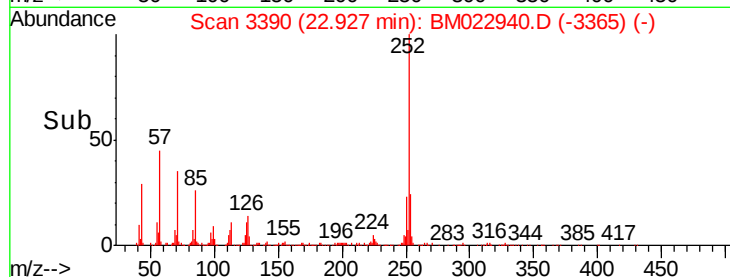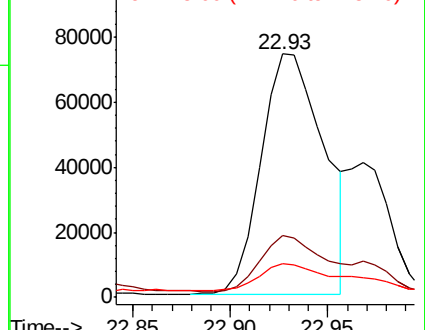

#91

Benzo(a)pyrene

Concen: 1.788 ng/ul

RT: 23.51 min Scan# 3489

Delta R.T. -0.01 min

Lab File: BM022940.D

Acq: 04 Oct 2019 03:38


Tgt Ion:252 Resp: 108164

Ion Ratio Lower Upper

252 100

253 25.5 17.6 26.4



125 15.4 8.7 13.1#

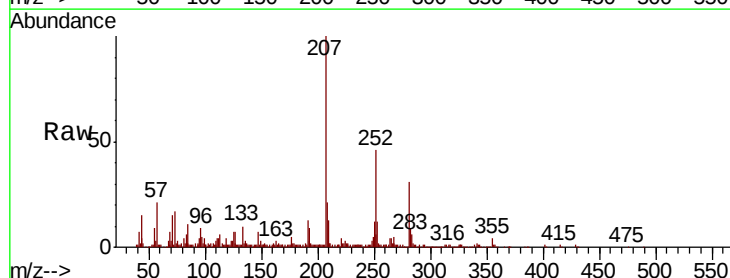


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

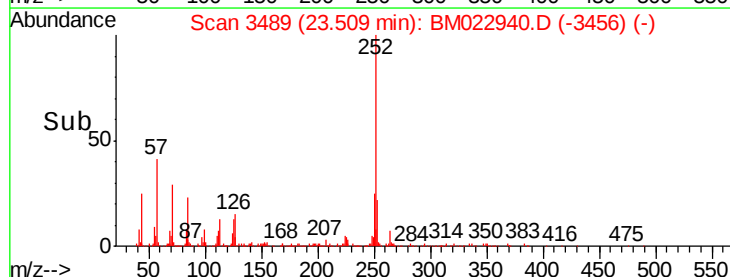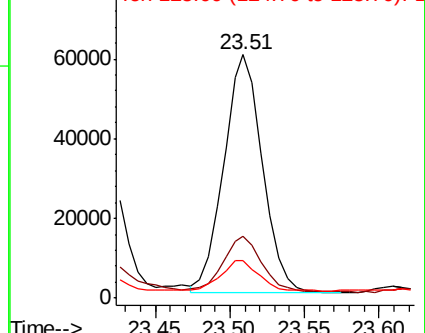




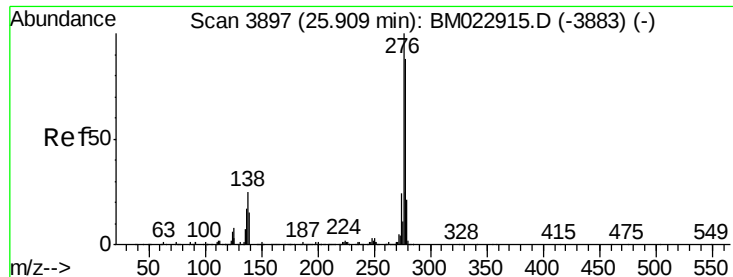


#92

Indeno(1,2,3-cd)pyrene
Concen: 1.277 ng/ul
RT: 25.89 min Scan# 3894
Delta R.T. -0.02 min
Lab File: BM022940.D
Acq: 04 Oct 2019 03:38

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
138	21.2	19.8	29.8
277	25.8	20.3	30.5

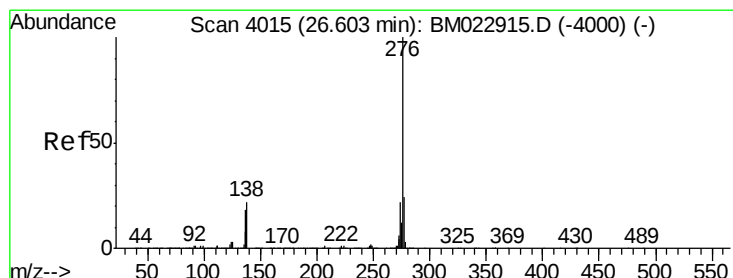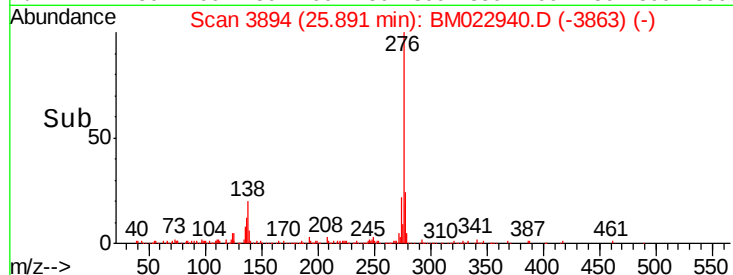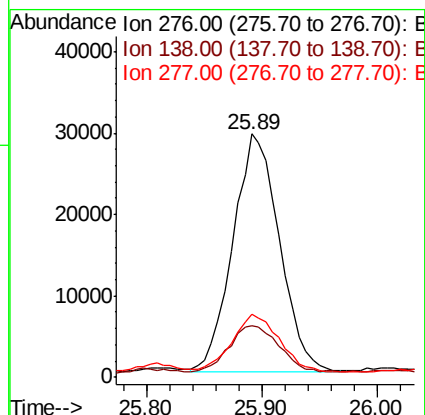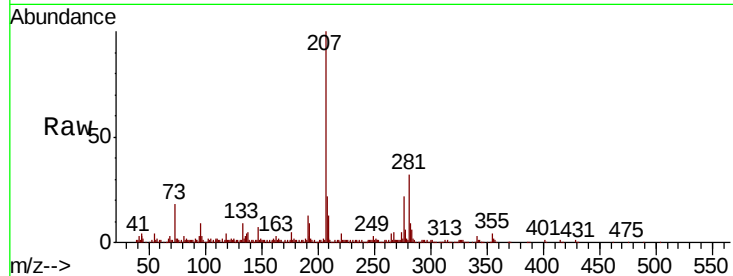

#94

Benzo(g,h,i)perylene
Concen: 1.577 ng/ul
RT: 26.60 min Scan# 4014
Delta R.T. -0.01 min
Lab File: BM022940.D
Acq: 04 Oct 2019 03:38

Tgt Ion	Ratio	Lower	Upper
276	100		
138	23.2	17.6	26.4
277	25.0	19.1	28.7

