

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM022941.D
 Acq On : 04 Oct 2019 04:14
 Operator : JU
 Sample : K4988-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNY7

Quant Time: Oct 04 05:31:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 04:31:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	220861	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	914047	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.43	164	502200	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	890927	20.00	ng/ul	0.00
78) Chrysene-d12	21.35	240	793595	20.00	ng/ul	0.00
86) Perylene-d12	23.61	264	946165	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	18152	3.55	ng/uL	0.00
5) Phenol-d5	6.96	99	324093	16.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	196014	18.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	284044	18.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	195417	12.23	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	136453	19.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	143559	18.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	260506	16.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	238052	12.78	ng/ul	0.00
44) Dimethylphthalate-d6	13.84	166	717889	18.42	ng/ul	0.00
47) Acenaphthylene-d8	14.12	160	878460	19.52	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	64427	8.37	ng/ul	0.00
58) Fluorene-d10	15.42	176	608036	18.30	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.54	200	48117	8.30	ng/ul	0.00
71) Anthracene-d10	17.27	188	808035	18.57	ng/ul	0.00
79) Pyrene-d10	19.56	212	894433	20.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.47	264	978301	19.99	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.99	94	55171	2.697 ng/ul	97
45) Dimethylphthalate	13.89	163	200748	5.014 ng/ul	99
70) Phenanthrene	17.21	178	215912	4.061 ng/ul	99
77) Fluoranthene	19.23	202	370567	6.197 ng/ul	100
80) Pyrene	19.59	202	304893	5.420 ng/ul	100
83) Benzo(a)anthracene	21.33	228	169394	2.973 ng/ul	99
85) Chrysene	21.39	228	166604	3.172 ng/ul	99
88) Benzo(b)fluoranthene	22.93	252	240562	3.831 ng/ul#	96
89) Benzo(k)fluoranthene	22.93	252	240562	4.005 ng/ul#	95
91) Benzo(a)pyrene	23.51	252	156383	2.655 ng/ul	98
92) Indeno(1,2,3-cd)pyrene	25.90	276	112458	1.797 ng/ul	95
94) Benzo(g,h,i)perylene	26.60	276	110183	2.183 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM022941.D
Acq On : 04 Oct 2019 04:14
Operator : JU
Sample : K4988-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNY7

Quant Time: Oct 04 05:31:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 04:31:57 2019
Response via : Initial Calibration

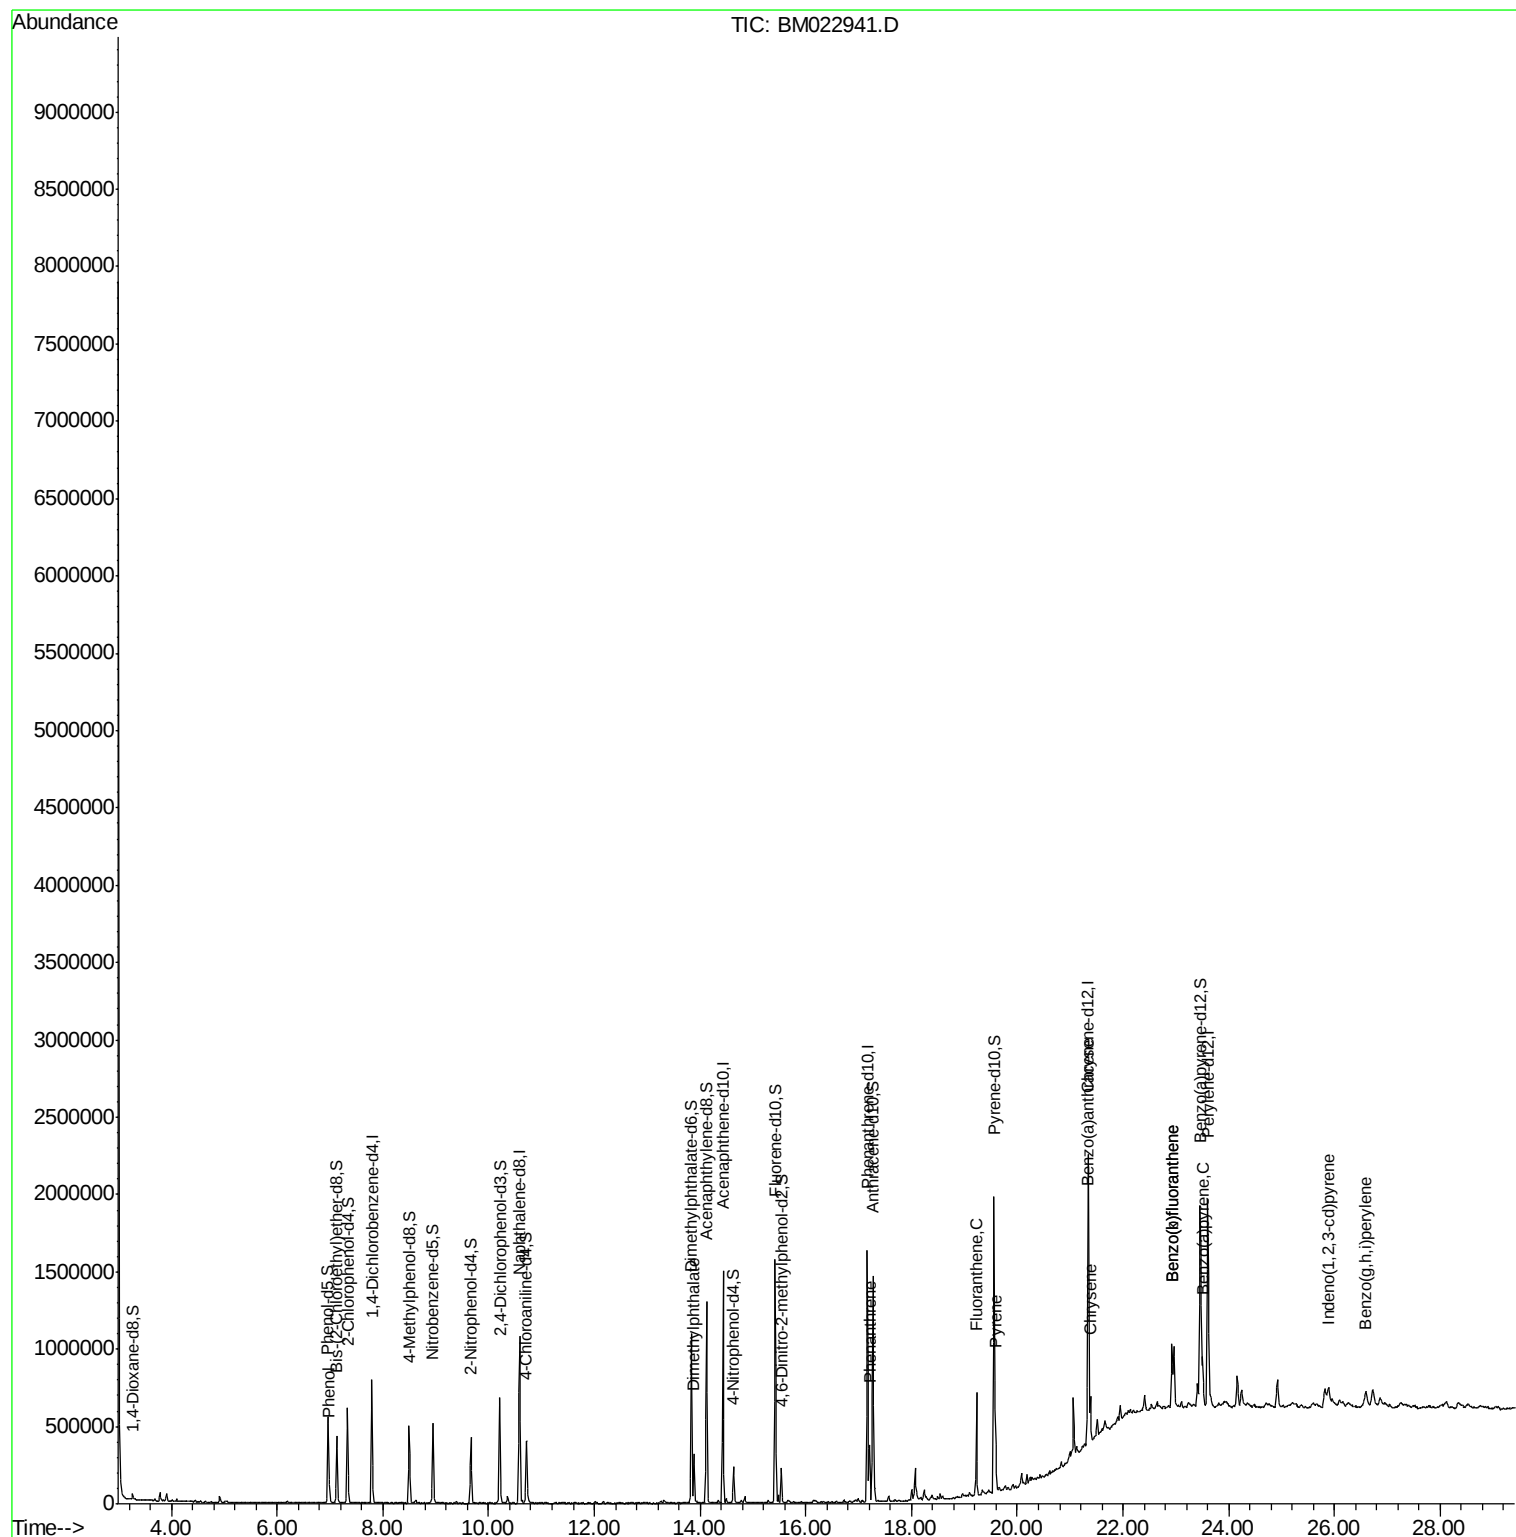

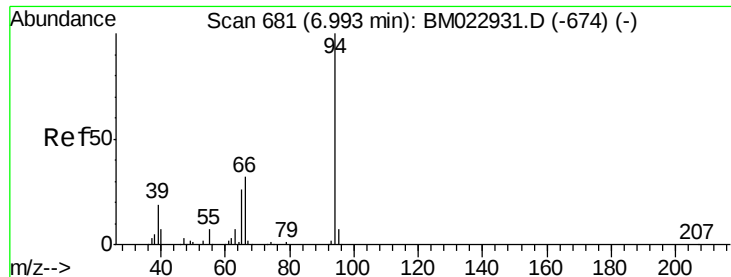





#6

Phenol

Concen: 2.697 ng/ul
 RT: 6.99 min Scan# 681
 Delta R.T. -0.00 min
 Lab File: BM022941.D
 Acq: 04 Oct 2019 04:14

Instrument :
 BNA_M
 ClientSampleId :
 ESNY7

Tot Ion	Ratio	Lower	Upper
94	100		
65	27.1	20.9	31.3
66	35.9	27.2	40.8

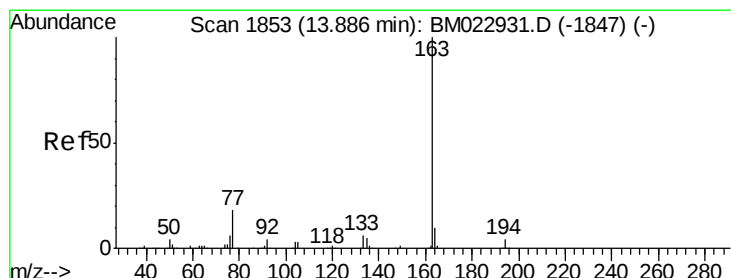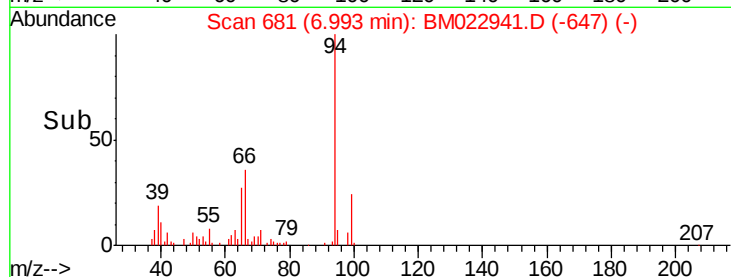
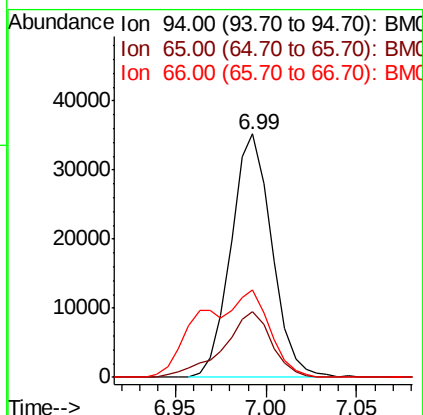
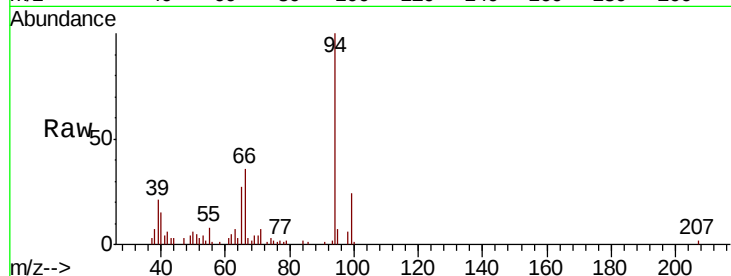



#45

Dimethylphthalate

Concen: 5.014 ng/ul
 RT: 13.89 min Scan# 1853
 Delta R.T. -0.01 min
 Lab File: BM022941.D
 Acq: 04 Oct 2019 04:14

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	9.6	8.1	12.1

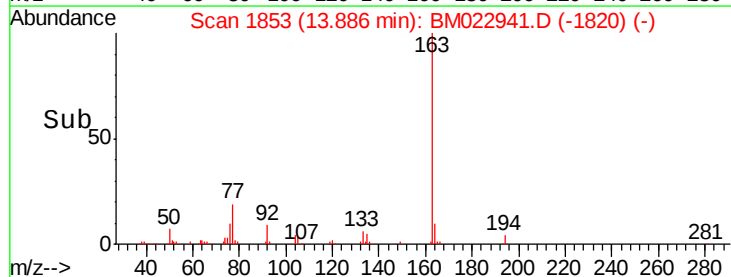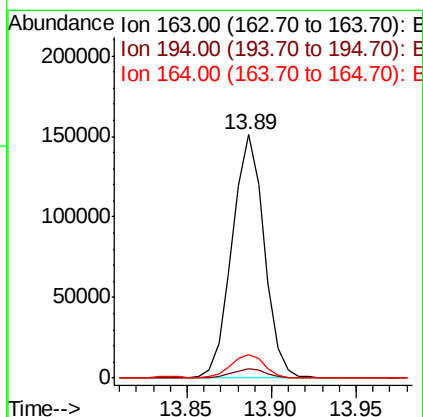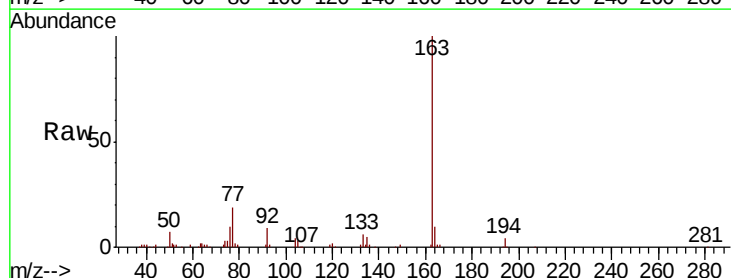

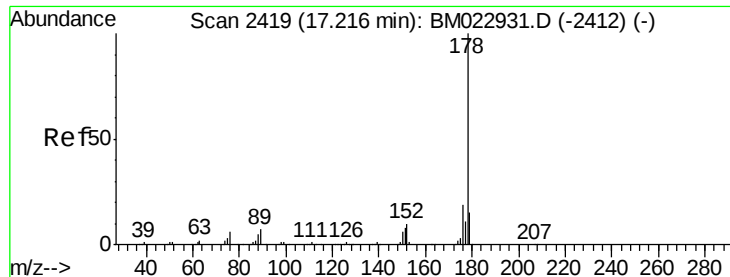

#70

Phenanthrene

Concen: 4.061 ng/ul

RT: 17.21 min Scan# 2418

Delta R.T. -0.01 min

Lab File: BM022941.D

Acq: 04 Oct 2019 04:14

Instrument :

BNA_M

ClientSampleId :

ESNY7


Tot Ion:178 Resp: 215912

Ion Ratio Lower Upper




178 100

179 15.3 12.4 18.6

176 18.8 15.3 22.9

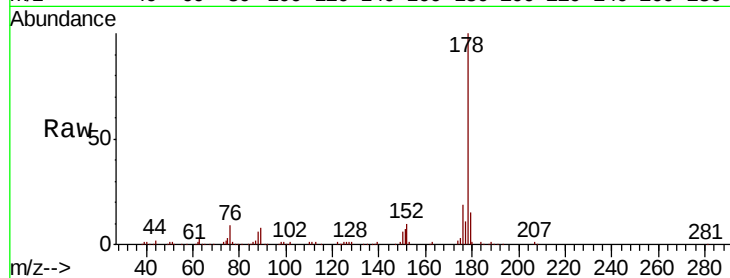

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

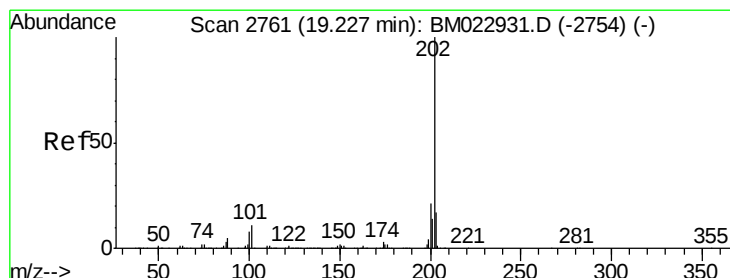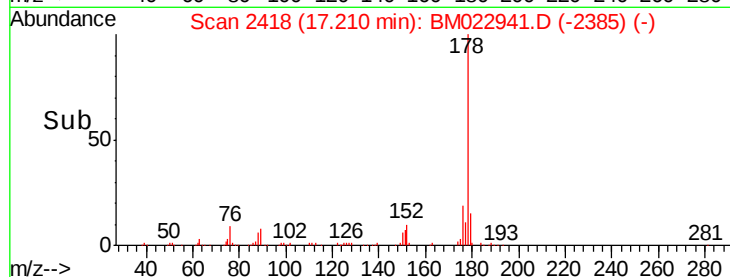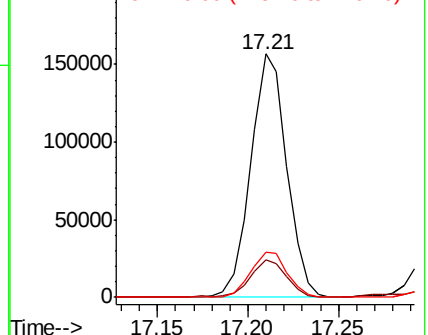

#77

Fluoranthene

Concen: 6.197 ng/ul

RT: 19.23 min Scan# 2761

Delta R.T. -0.00 min

Lab File: BM022941.D

Acq: 04 Oct 2019 04:14


Tgt Ion:202 Resp: 370567

Ion Ratio Lower Upper



202 100


101 10.6 8.6 12.8

100 8.2 6.4 9.6

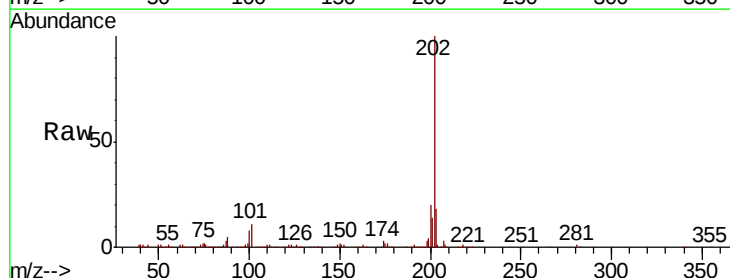

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

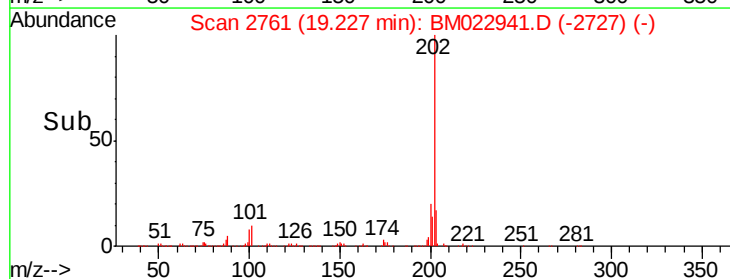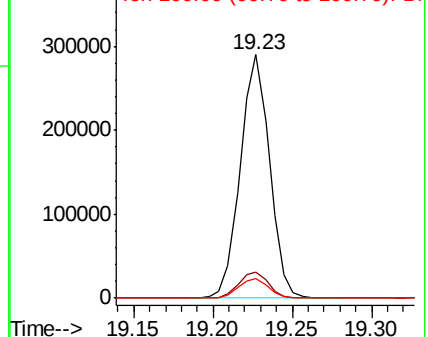


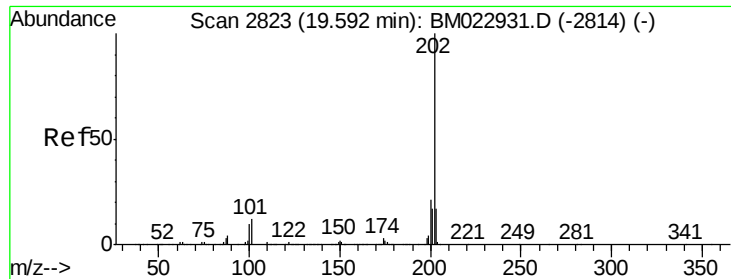

#80
Pvrene
Concen: 5.420 ng/ul
RT: 19.59 min Scan# 2823
Delta R.T. -0.00 min
Lab File: BM022941.D
Acq: 04 Oct 2019 04:14

Instrument :
BNA_M
ClientSampleId :
ESNY7

Tot Ion	Ratio	Lower	Upper
202	100		
101	12.1	9.7	14.5
100	9.8	7.8	11.8



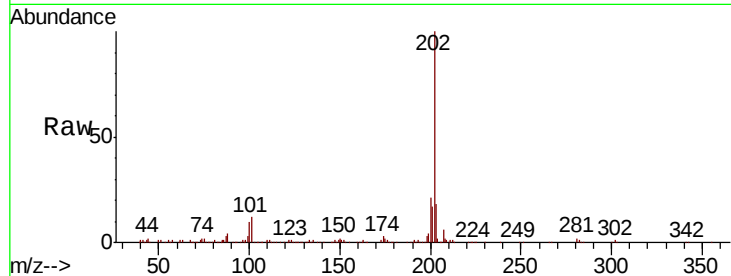


Abundance

Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

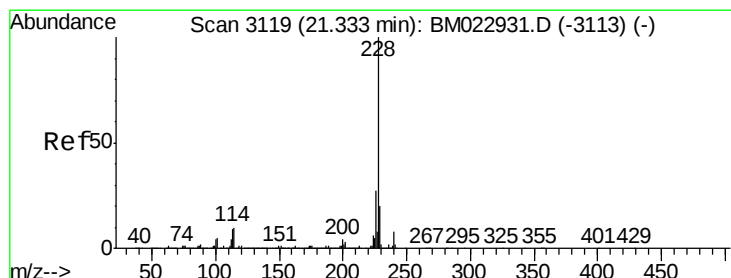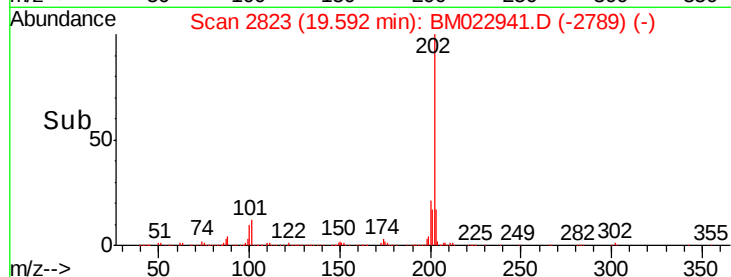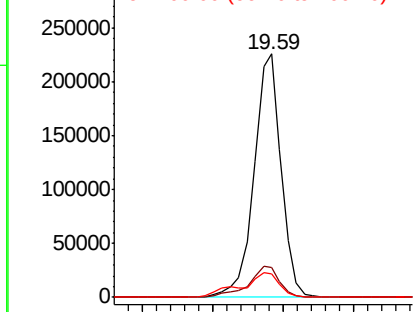

#83
Benzo(a)anthracene
Concen: 2.973 ng/ul
RT: 21.33 min Scan# 3119
Delta R.T. -0.01 min
Lab File: BM022941.D
Acq: 04 Oct 2019 04:14

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.3	15.8	23.8
226	27.6	22.4	33.6


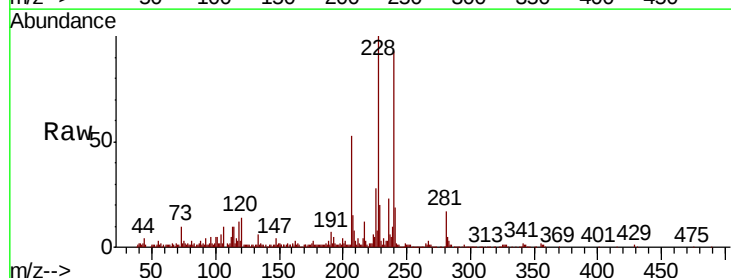



Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

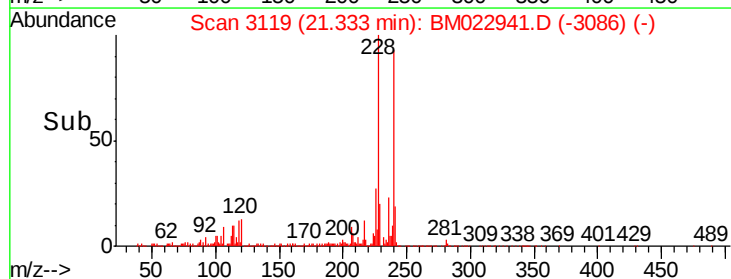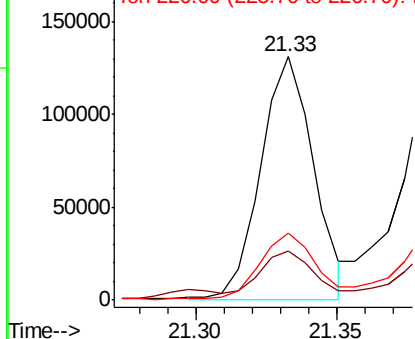

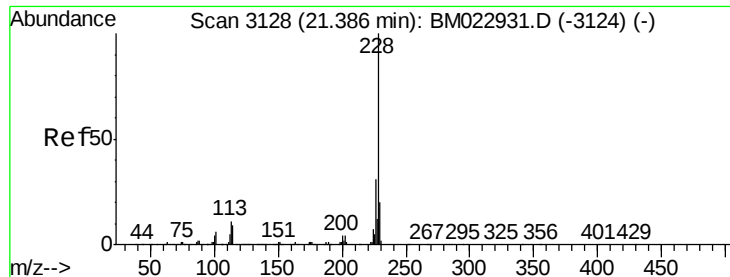

#85

Chrysene

Concen: 3.172 ng/ul

RT: 21.39 min Scan# 3128

Delta R.T. -0.00 min

Lab File: BM022941.D

Acq: 04 Oct 2019 04:14

Instrument :

BNA_M

ClientSampleId :

ESNY7


Tot Ion:228 Resp: 166604

Ion Ratio Lower Upper

228 100

226 30.0 24.2 36.4

229 20.9 15.9 23.9



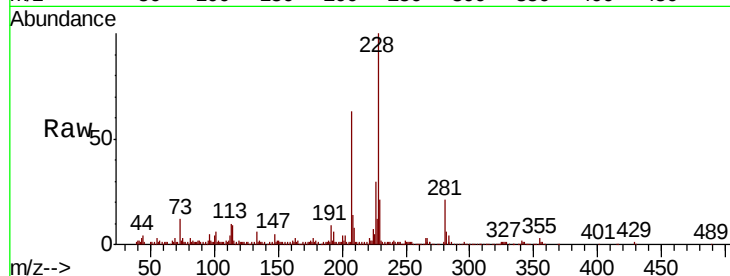


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

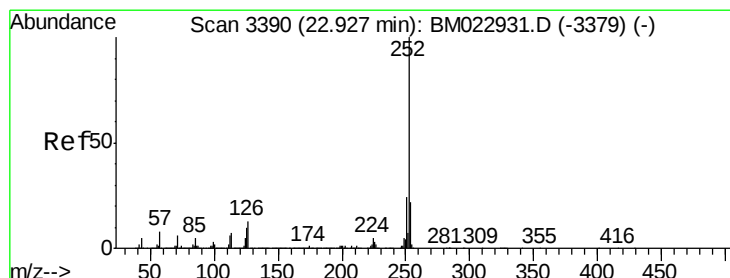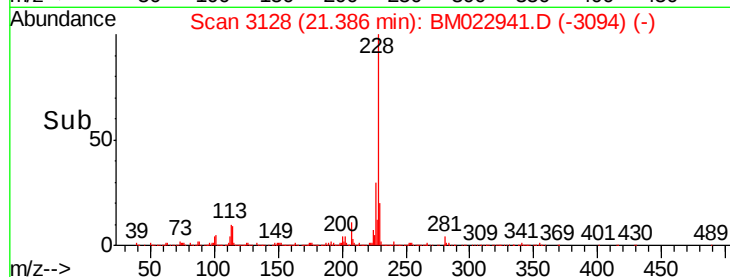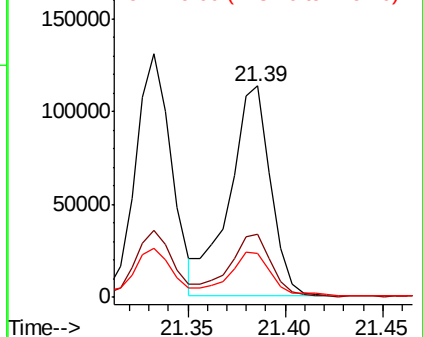

#88

Benzo(b)fluoranthene

Concen: 3.831 ng/ul

RT: 22.93 min Scan# 3391

Delta R.T. -0.00 min

Lab File: BM022941.D

Acq: 04 Oct 2019 04:14


Tgt Ion:252 Resp: 240562

Ion Ratio Lower Upper

252 100

253 23.9 17.7 26.5

125 12.3 8.2 12.2#


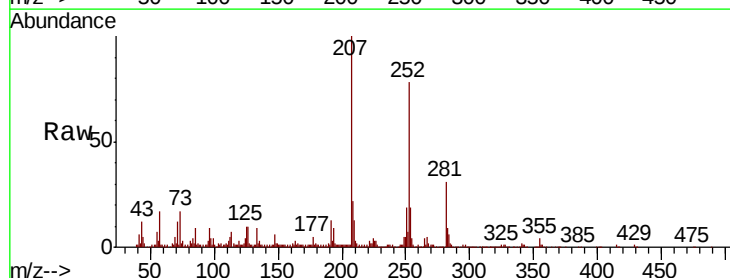



Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

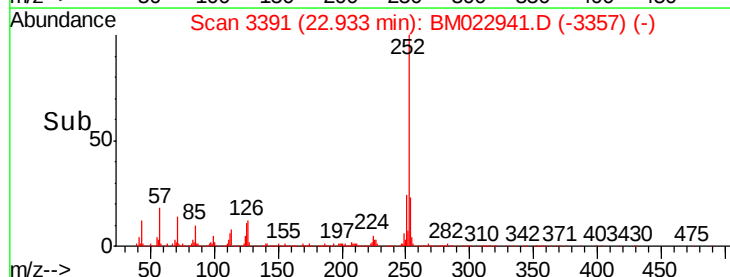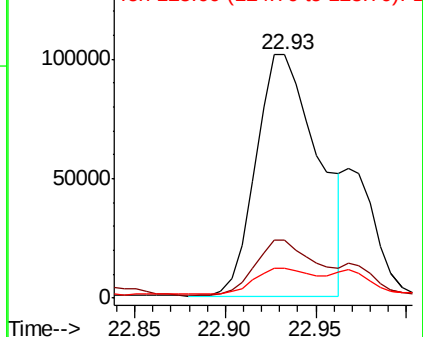

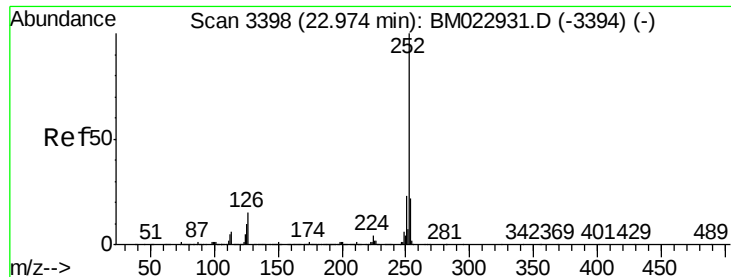

#89

Benzo(k)fluoranthene

Concen: 4.005 ng/ul

RT: 22.93 min Scan# 3391

Delta R.T. -0.05 min

Lab File: BM022941.D

Acq: 04 Oct 2019 04:14

Instrument :

BNA_M

ClientSampleId :

ESNY7


Tot Ion:252 Resp: 240562

Ion Ratio Lower Upper

252 100

253 23.9 17.5 26.3




125 12.3 7.9 11.9#

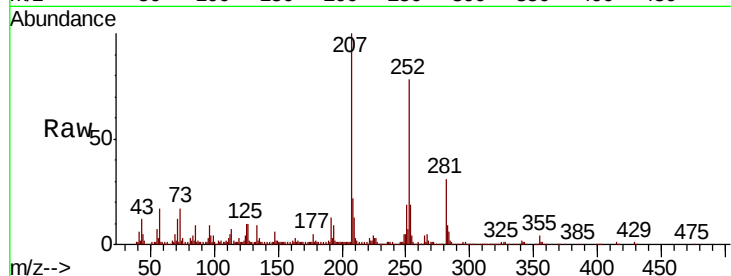

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

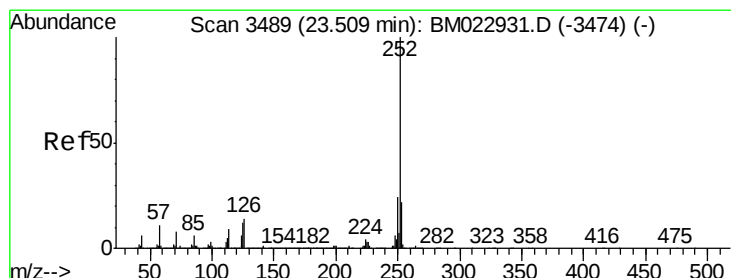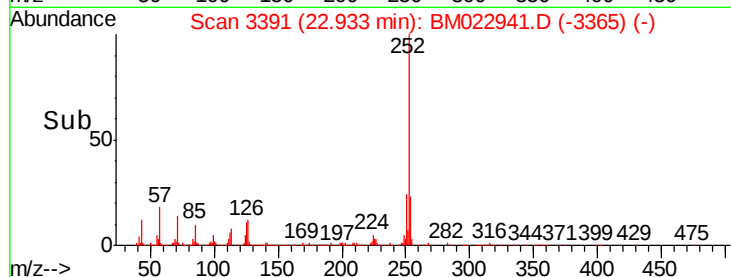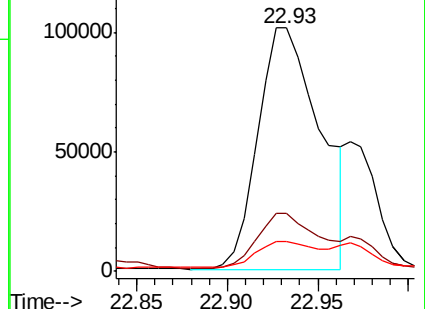

#91

Benzo(a)pyrene

Concen: 2.655 ng/ul

RT: 23.51 min Scan# 3489

Delta R.T. -0.01 min

Lab File: BM022941.D

Acq: 04 Oct 2019 04:14


Tgt Ion:252 Resp: 156383

Ion Ratio Lower Upper

252 100

253 22.9 17.6 26.4



125 12.2 8.7 13.1

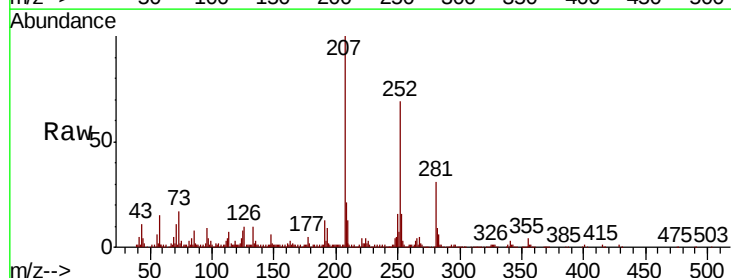


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

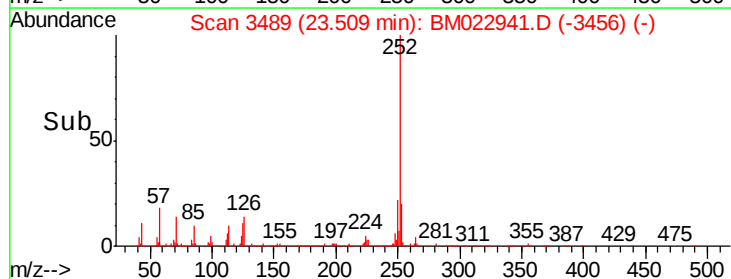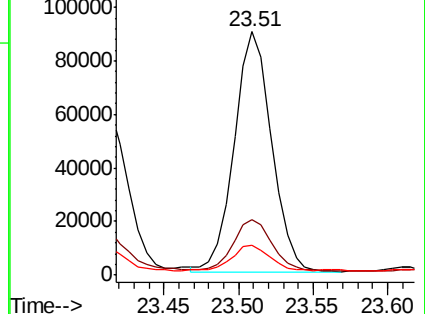




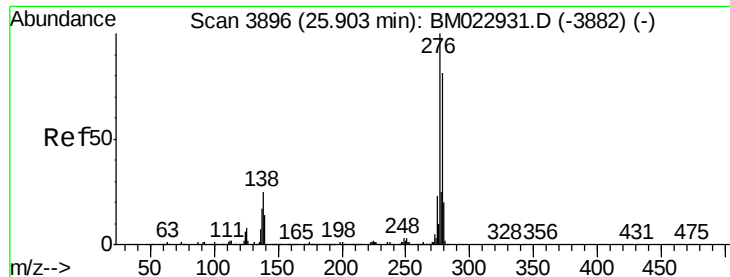


#92

Indeno(1,2,3-cd)pyrene
Concen: 1.797 ng/ul
RT: 25.90 min Scan# 3895
Delta R.T. -0.01 min
Lab File: BM022941.D
Acq: 04 Oct 2019 04:14

Instrument :
BNA_M
ClientSampleId :
ESNY7

Tot Ion	Ratio	Lower	Upper
276	100		
138	19.9	19.8	29.8
277	25.4	20.3	30.5

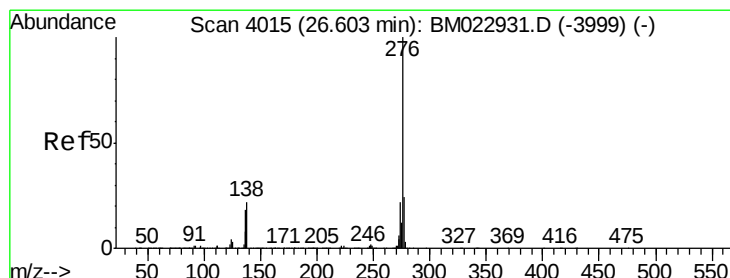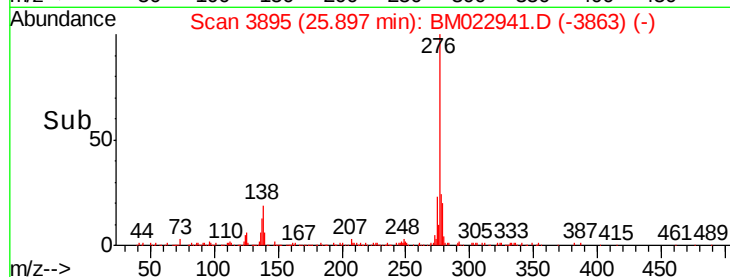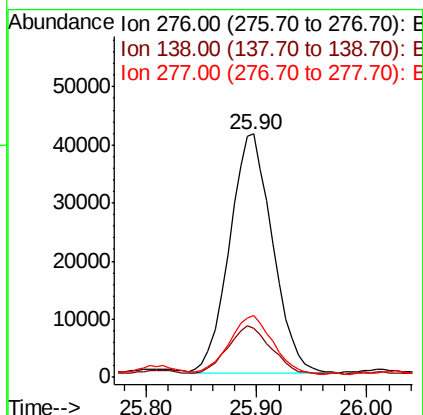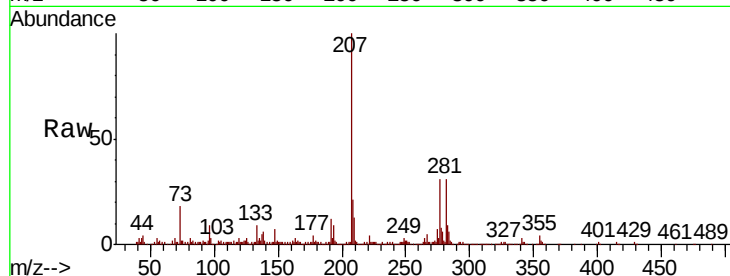

#94

Benzo(g,h,i)perylene
Concen: 2.183 ng/ul
RT: 26.60 min Scan# 4014
Delta R.T. -0.01 min
Lab File: BM022941.D
Acq: 04 Oct 2019 04:14

Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.7	17.6	26.4
277	25.5	19.1	28.7

