

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
 Data File : BM022949.D
 Acq On : 04 Oct 2019 09:43
 Operator : JU
 Sample : K5058-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAM0

Quant Time: Oct 04 16:54:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 27 18:03:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	185325	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.59	136	719722	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.43	164	386891	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.17	188	706321	20.00	ng/ul	-0.02
78) Chrysene-d12	21.35	240	678363	20.00	ng/ul	-0.02
86) Perylene-d12	23.62	264	801915	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	6011	1.40	ng/uL	0.00
5) Phenol-d5	6.96	99	93580	5.72	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.13	67	220373	24.59	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.33	132	273019	20.70	ng/ul	-0.02
13) 4-Methylphenol-d8	8.50	113	164192	12.25	ng/ul	-0.02
19) Nitrobenzene-d5	8.95	128	150326	27.06	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.67	143	160593	26.48	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.20	165	288218	23.87	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.73	131	15497	1.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.84	166	824565	27.46	ng/ul	-0.02
47) Acenaphthylene-d8	14.12	160	986076	28.44	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.63	143	22465	3.79	ng/ul	0.00
58) Fluorene-d10	15.42	176	695589	27.18	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.54	200	91348	19.87	ng/ul	-0.02
71) Anthracene-d10	17.27	188	1021221	29.61	ng/ul	-0.02
79) Pyrene-d10	19.56	212	1083940	29.69	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.47	264	1238938	29.87	ng/ul	-0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.89	163	40213	1.304	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM022949.D
Acq On : 04 Oct 2019 09:43
Operator : JU
Sample : K5058-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAM0

Quant Time: Oct 04 16:54:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 27 18:03:27 2019
Response via : Initial Calibration

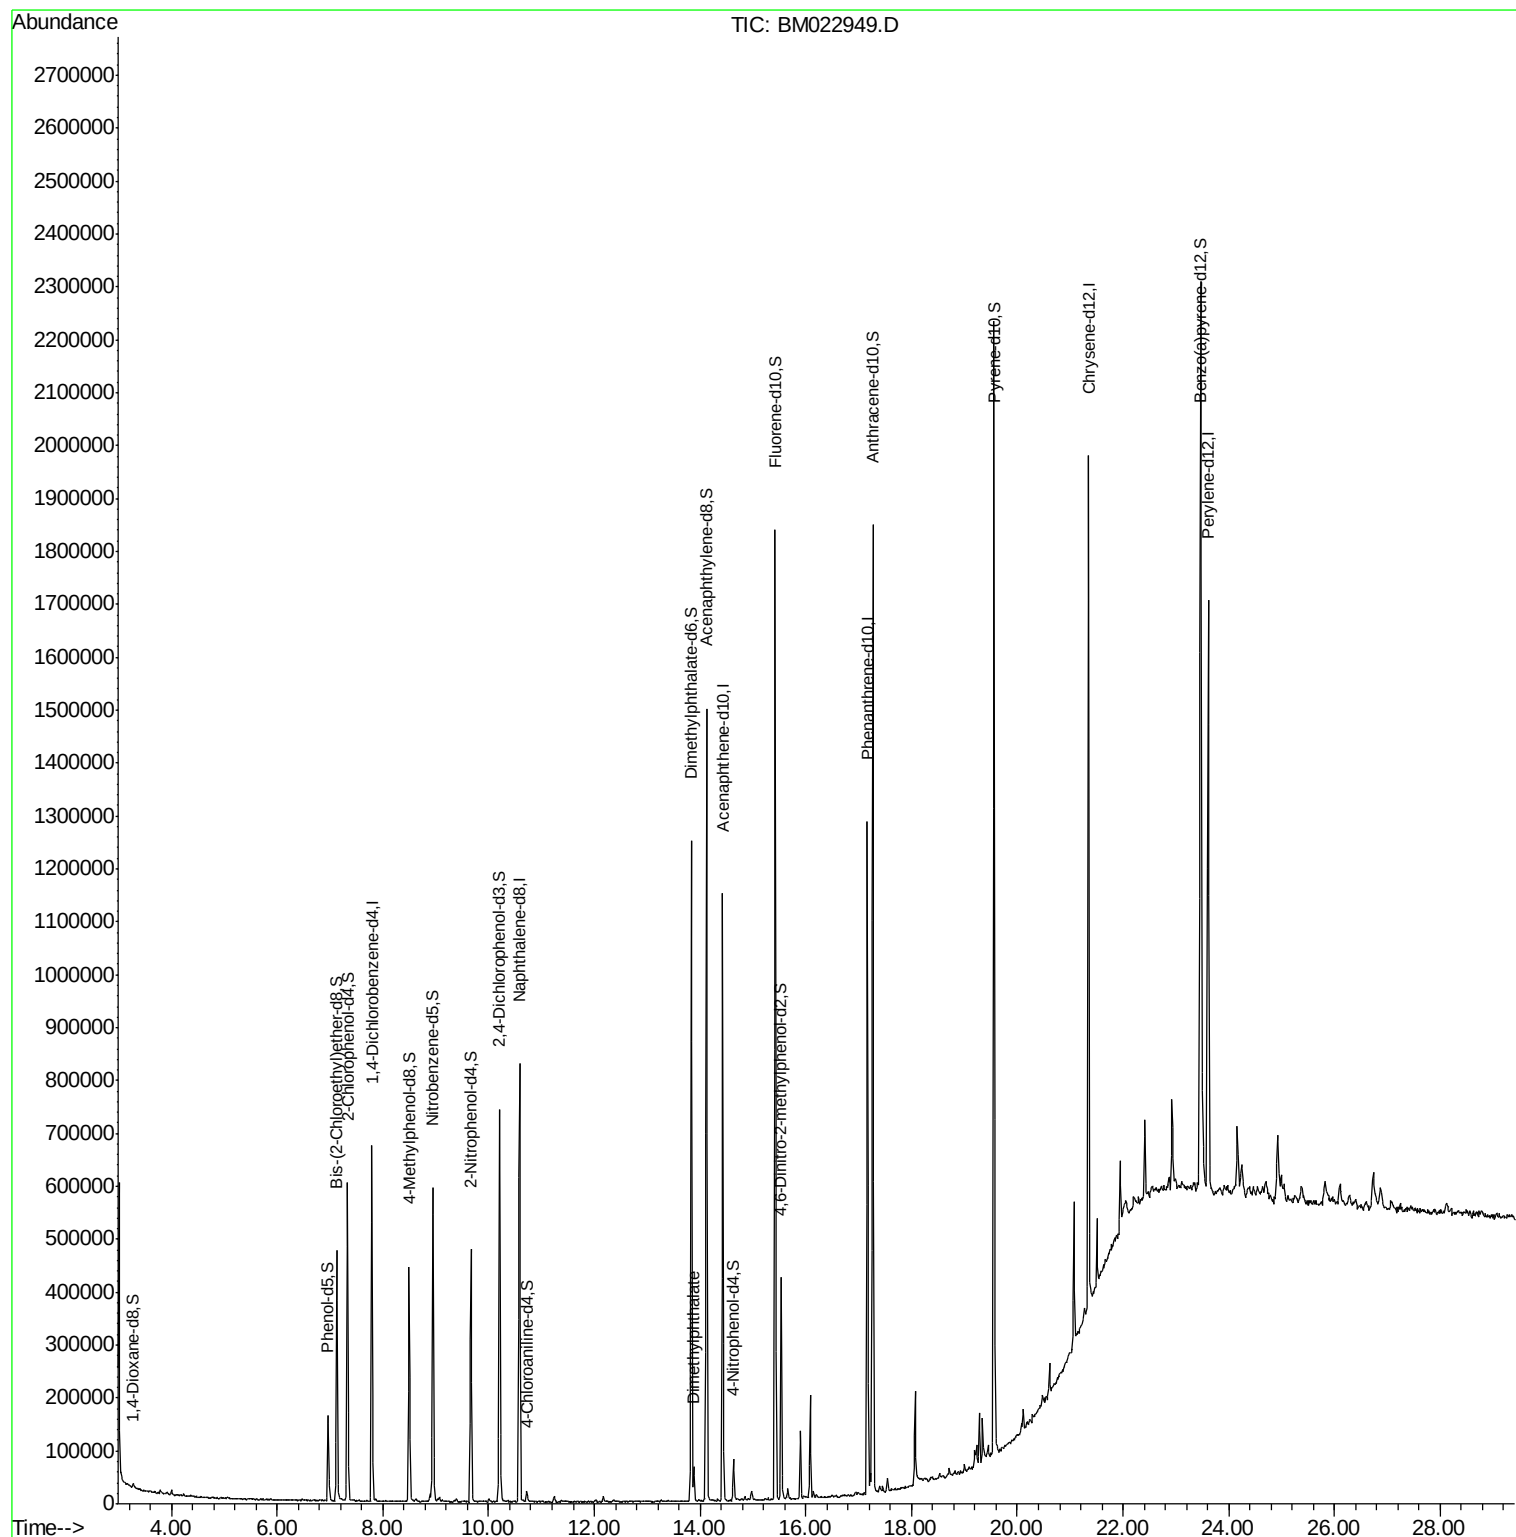

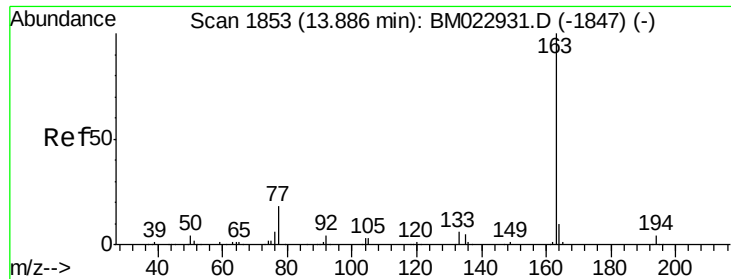

#45

Dimethylphthalate

Concen: 1.304 ng/ul

RT: 13.89 min Scan# 1853

Delta R.T. -0.02 min

Lab File: BM022949.D

Acq: 04 Oct 2019 09:43

Instrument :

BNA_M

ClientSampleId :

DBAM0


Tgt Ion:163 Resp: 40213

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 10.3 8.1 12.1

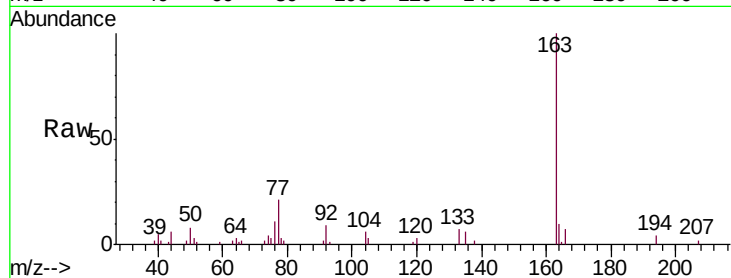

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

