

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM022973.D
 Acq On : 05 Oct 2019 00:29
 Operator : JU
 Sample : K5006-20
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETJX9

Quant Time: Oct 05 01:14:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 16:45:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	250613	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	1096460	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.43	164	642789	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.16	188	1094367	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	853157	20.00	ng/ul	-0.01
86) Perylene-d12	23.60	264	1004154	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	28185	4.86	ng/uL	0.00
5) Phenol-d5	6.96	99	124541	5.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	299827	24.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	356625	20.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	235874	13.01	ng/ul	-0.01
19) Nitrobenzene-d5	8.95	128	217963	25.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	235774	25.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	424640	23.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	43333	1.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.83	166	1400317	28.07	ng/ul	0.00
47) Acenaphthylene-d8	14.12	160	1573832	27.32	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	34966	3.55	ng/ul	0.00
58) Fluorene-d10	15.42	176	1106981	26.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.53	200	158322	22.23	ng/ul	0.00
71) Anthracene-d10	17.26	188	1644958	30.78	ng/ul	0.00
79) Pyrene-d10	19.56	212	1621281	35.31	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.46	264	1686322	32.46	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.88	163	217598	4.246	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM022973.D
Acq On : 05 Oct 2019 00:29
Operator : JU
Sample : K5006-20
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETJX9

Quant Time: Oct 05 01:14:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 16:45:59 2019
Response via : Initial Calibration

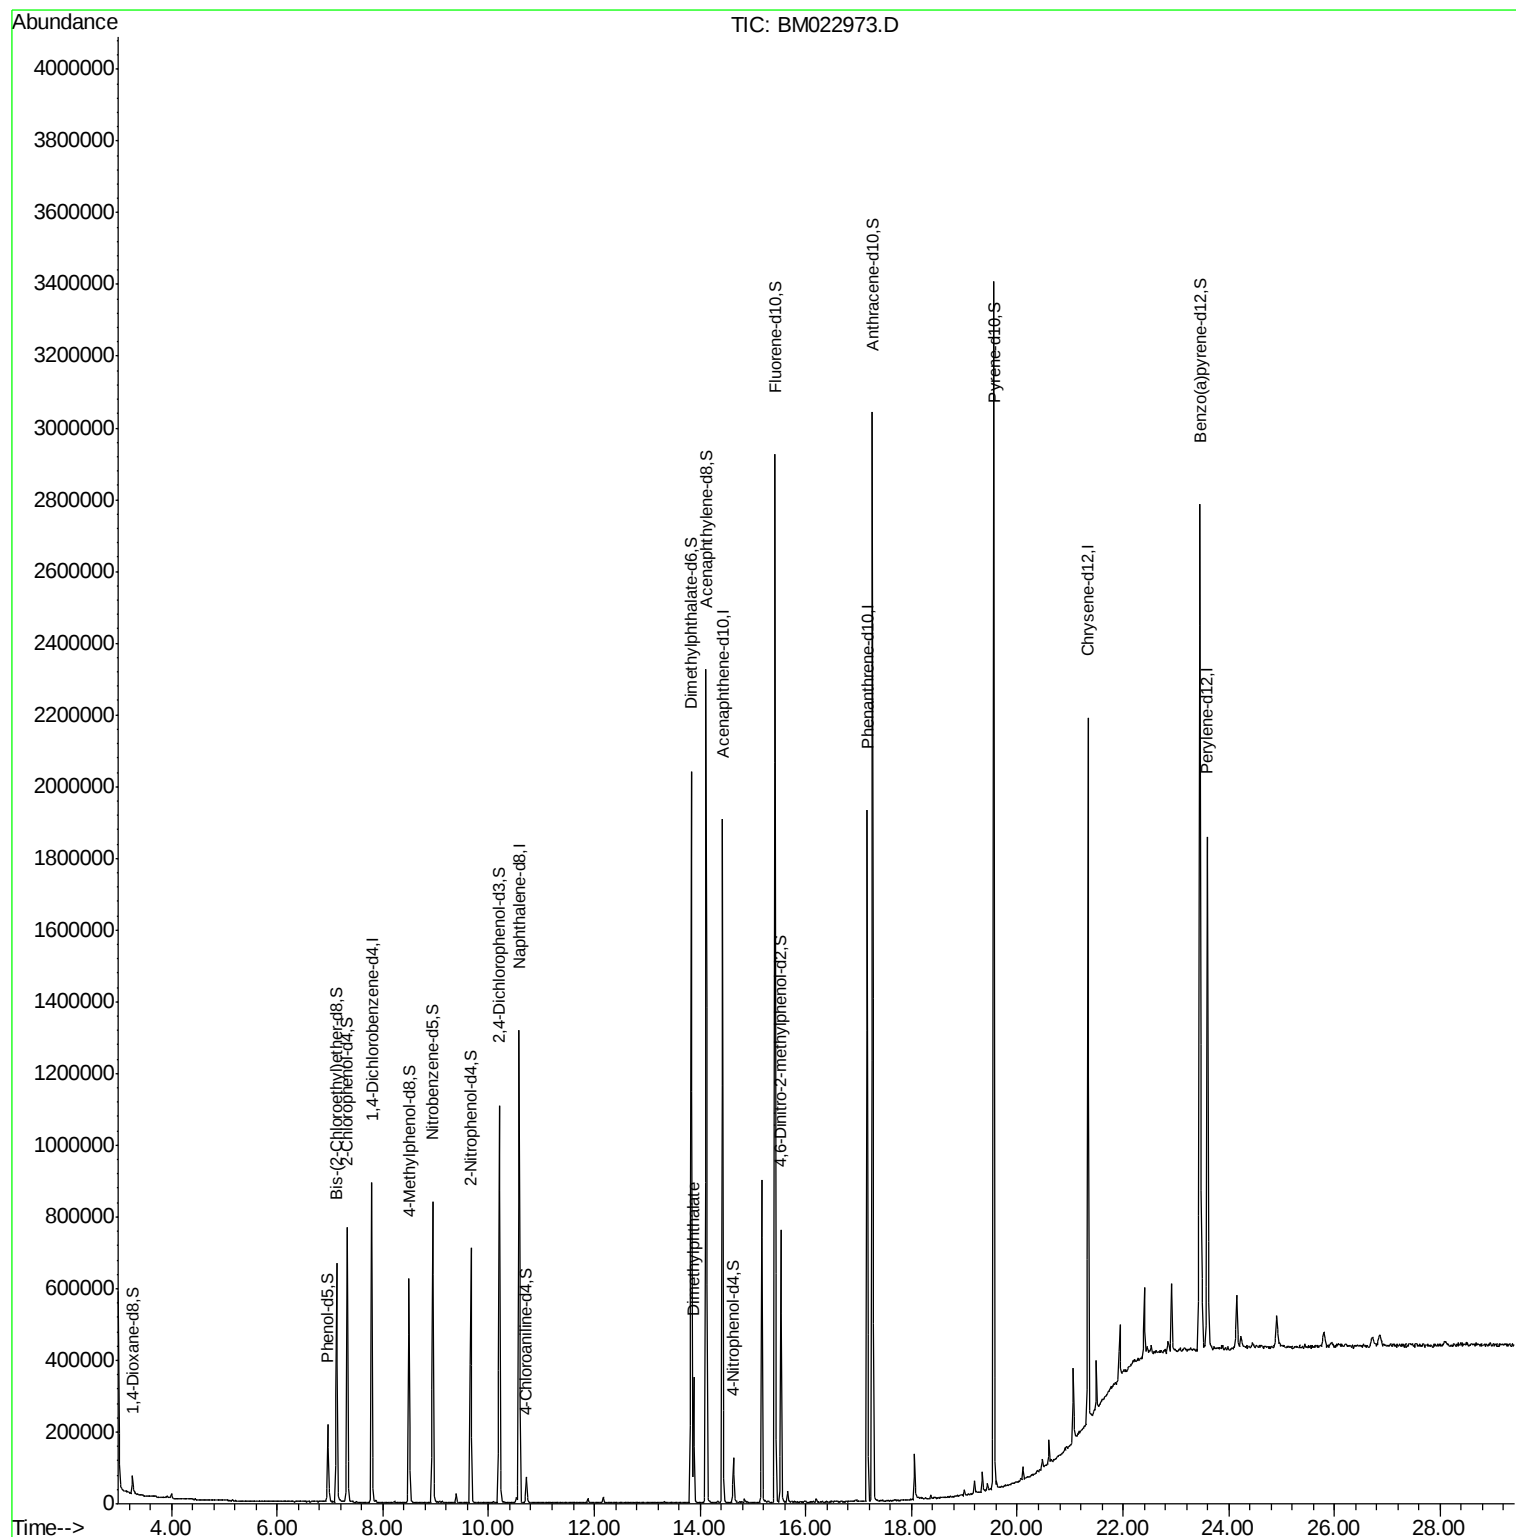

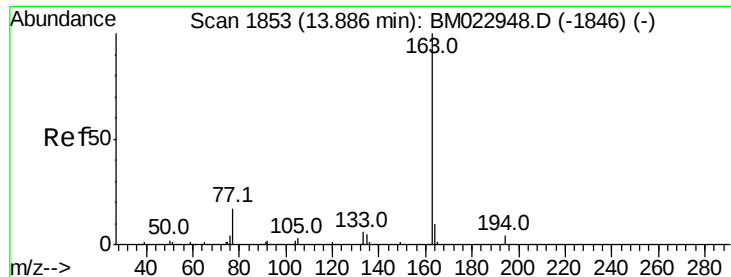

#45

Dimethylphthalate

Concen: 4.246 ng/ul

RT: 13.88 min Scan# 1852

Delta R.T. -0.01 min

Lab File: BM022973.D

Acq: 05 Oct 2019 00:29

Instrument :

BNA_M

ClientSampleId :

ETJX9


Tot Ion:163 Resp: 217598

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.5 8.1 12.1

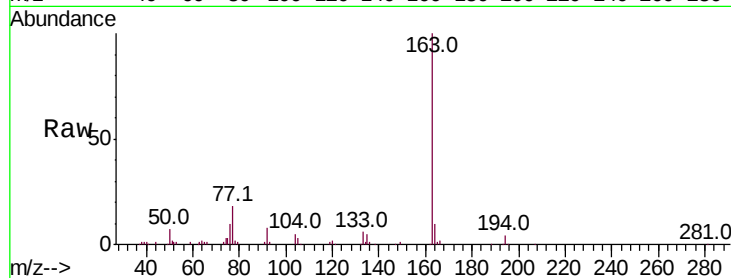

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

