

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023003.D
 Acq On : 05 Oct 2019 22:04
 Operator : JU
 Sample : K5057-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 06 23:35:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 16:45:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	249692	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1075734	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.42	164	619971	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.16	188	1065707	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	841537	20.00	ng/ul	-0.01
86) Perylene-d12	23.60	264	970170	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	19309	3.34	ng/uL	0.00
5) Phenol-d5	6.96	99	366211	16.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	219826	18.21	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.32	132	302827	17.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	297253	16.46	ng/ul	-0.01
19) Nitrobenzene-d5	8.94	128	144911	17.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	148800	16.41	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.20	165	295034	16.35	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.71	131	404938	18.47	ng/ul	0.00
44) Dimethylphthalate-d6	13.83	166	867493	18.03	ng/ul	0.00
47) Acenaphthylene-d8	14.12	160	1013781	18.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.62	143	68800	7.24	ng/ul	0.00
58) Fluorene-d10	15.42	176	719000	17.53	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.53	200	53804	7.76	ng/ul	-0.01
71) Anthracene-d10	17.26	188	977199	18.78	ng/ul	-0.01
79) Pyrene-d10	19.55	212	971922	21.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.46	264	988977	19.71	ng/ul	-0.01

Target Compounds


					Ovalue
6) Phenol	6.98	94	45859	1.983	ng/ul 98
45) Dimethylphthalate	13.88	163	299034	6.050	ng/ul 99
77) Fluoranthene	19.22	202	194532	2.719	ng/ul 98
80) Pyrene	19.58	202	177010	2.967	ng/ul 98
83) Benzo(a)anthracene	21.33	228	103009	1.705	ng/ul 98
85) Chrysene	21.38	228	111542	2.002	ng/ul 98
88) Benzo(b)fluoranthene	22.92	252	127224	1.976	ng/ul# 97
89) Benzo(k)fluoranthene	22.92	252	127224	2.065	ng/ul# 97
91) Benzo(a)pyrene	23.50	252	63657	1.054	ng/ul# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM023003.D
Acq On : 05 Oct 2019 22:04
Operator : JU
Sample : K5057-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 06 23:35:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 16:45:59 2019
Response via : Initial Calibration

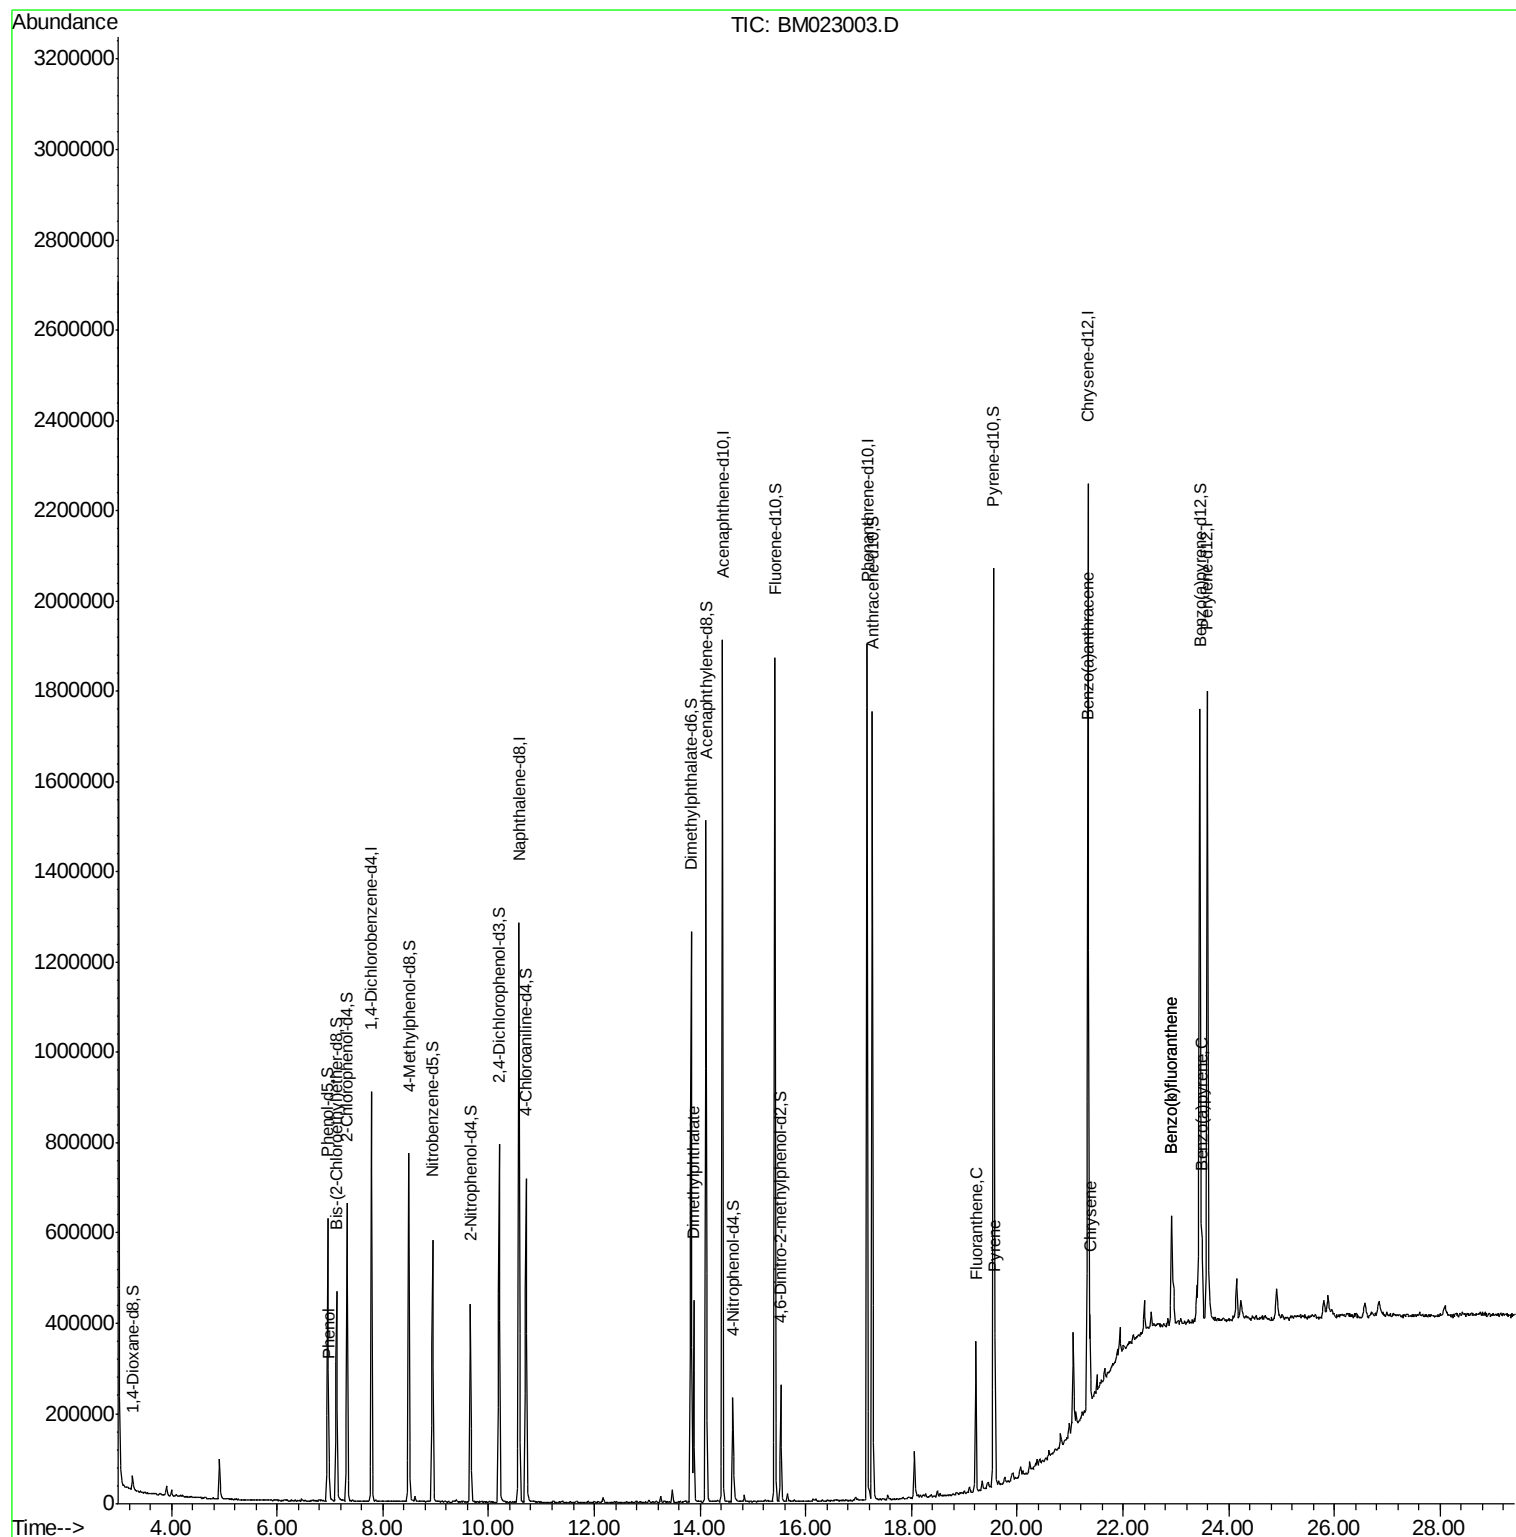

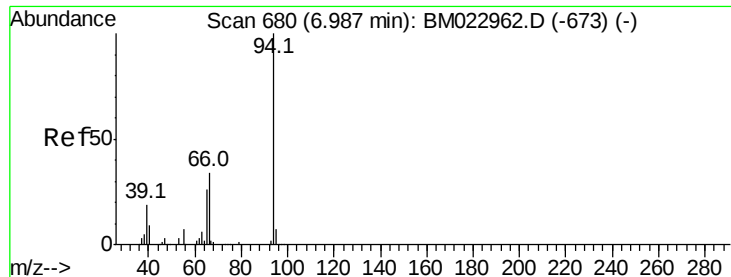

#6

Phenol

Concen: 1.983 ng/ul

RT: 6.98 min Scan# 679

Delta R.T. -0.01 min

Lab File: BM023003.D

Acq: 05 Oct 2019 22:04


Instrument :

BNA_M

ClientSampleId :

Tot Ion: 94 Resp: 45859

Ion	Ratio	Lower	Upper
94	100		
65	26.5	20.9	31.3
66	35.6	27.2	40.8



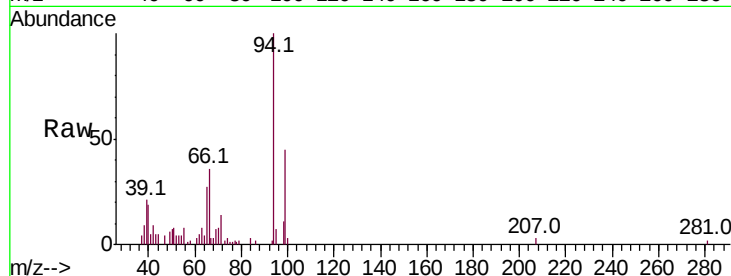


Abundance

Ion 94.00 (93.70 to 94.70): BM022962.D (-673) (-)

Ion 65.00 (64.70 to 65.70): BM022962.D (-673) (-)

Ion 66.00 (65.70 to 66.70): BM022962.D (-673) (-)

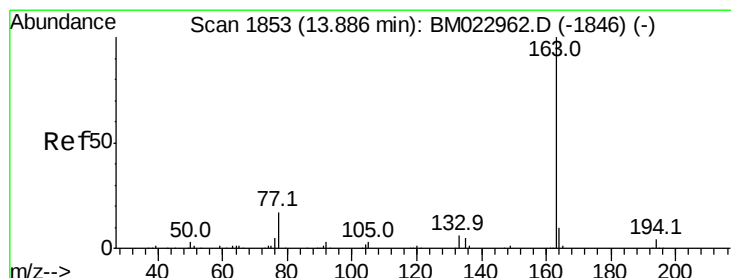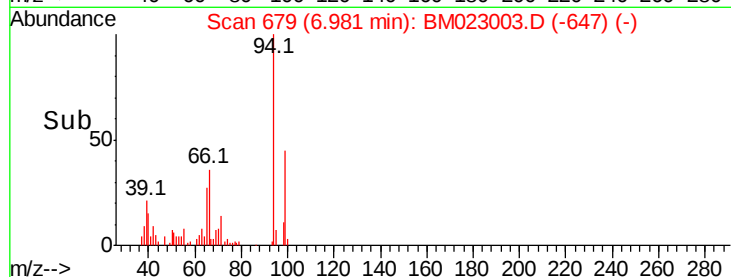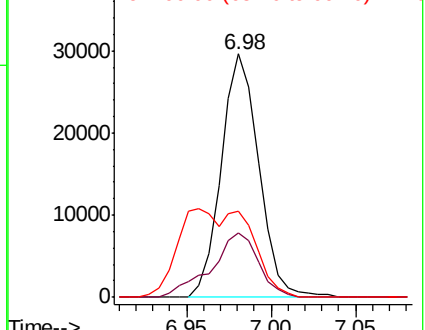

#45

Dimethylphthalate

Concen: 6.050 ng/ul

RT: 13.88 min Scan# 1852


Delta R.T. -0.01 min

Lab File: BM023003.D

Acq: 05 Oct 2019 22:04

Tgt Ion: 163 Resp: 299034

Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	9.9	8.1	12.1


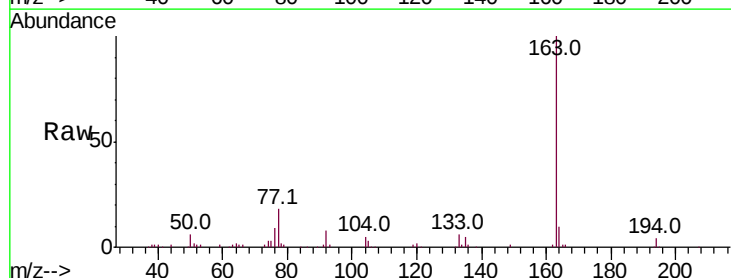



Abundance

Ion 163.00 (162.70 to 163.70): BM022962.D (-1846) (-)

Ion 194.00 (193.70 to 194.70): BM022962.D (-1846) (-)

Ion 164.00 (163.70 to 164.70): BM022962.D (-1846) (-)



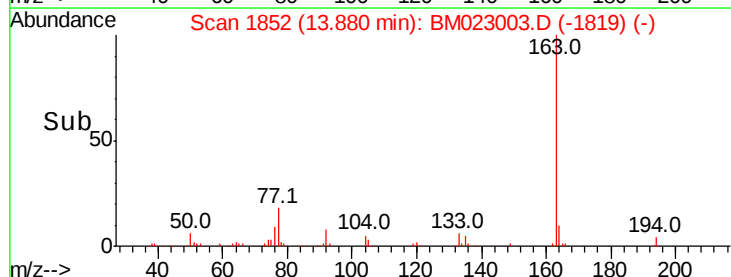
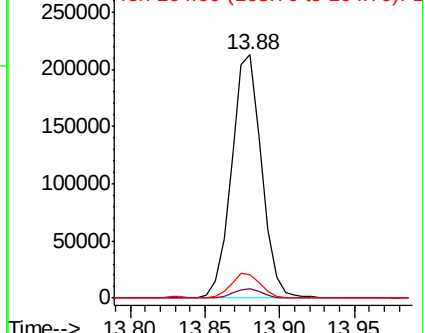


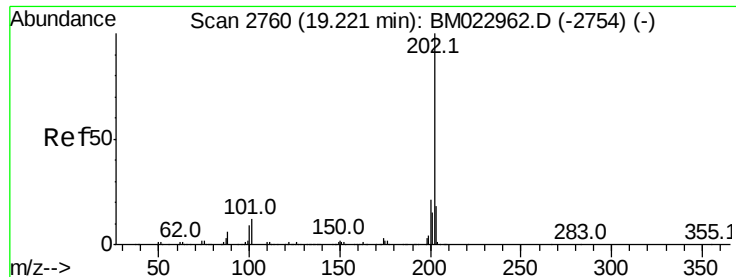

#77
 Fluoranthene
 Concen: 2.719 ng/ul
 RT: 19.22 min Scan# 2759
 Delta R.T. -0.01 min
 Lab File: BM023003.D
 Acq: 05 Oct 2019 22:04




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:	202	Resp:	194532
Ion	Ratio	Lower	Upper
202	100		
101	11.6	8.6	12.8
100	8.4	6.4	9.6

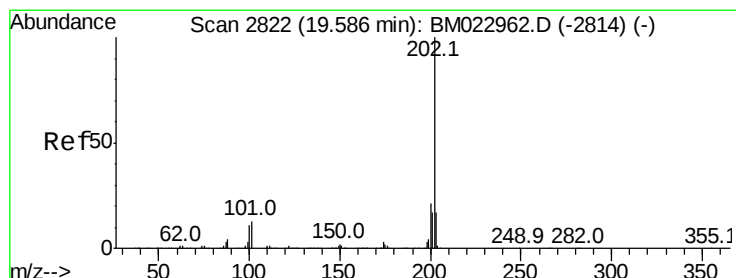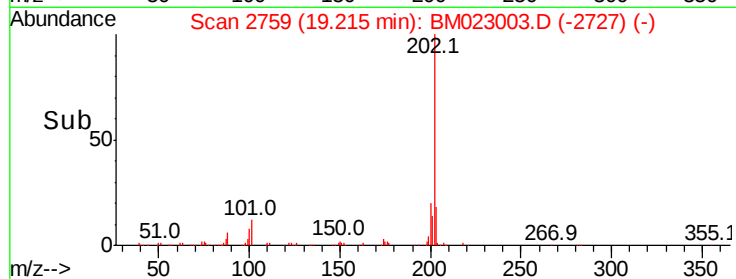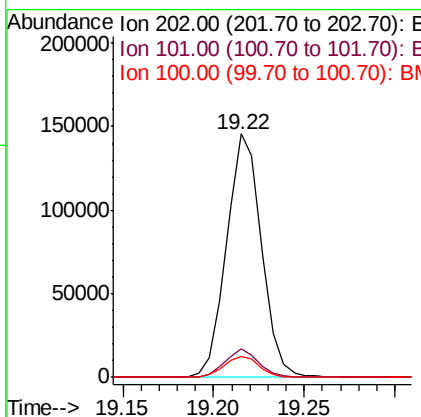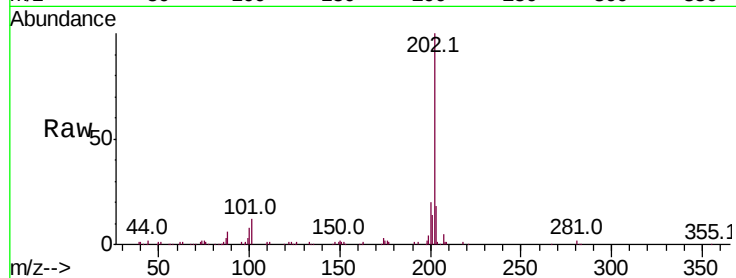

#80
 Pyrene
 Concen: 2.967 ng/ul
 RT: 19.58 min Scan# 2821
 Delta R.T. -0.01 min
 Lab File: BM023003.D
 Acq: 05 Oct 2019 22:04

Tgt Ion:	202	Resp:	177010
Ion	Ratio	Lower	Upper
202	100		
101	12.7	9.7	14.5
100	11.0	7.8	11.8

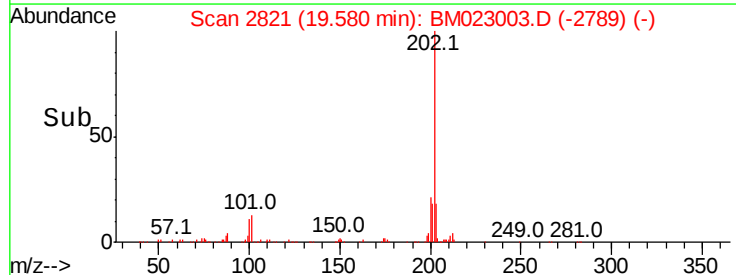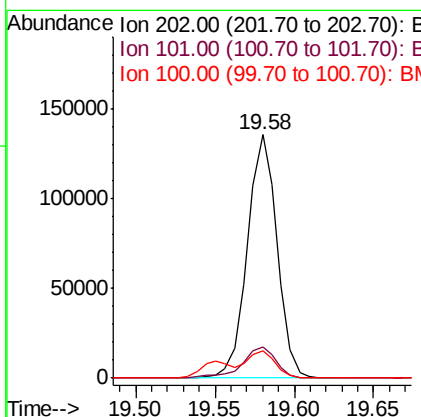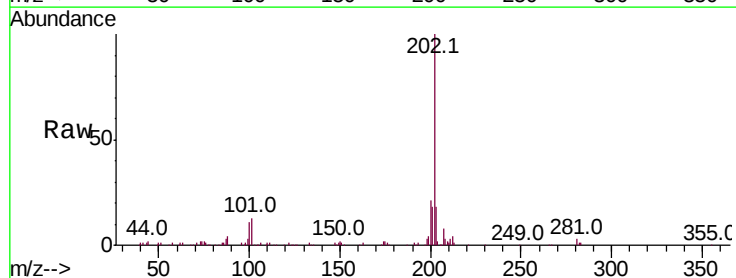


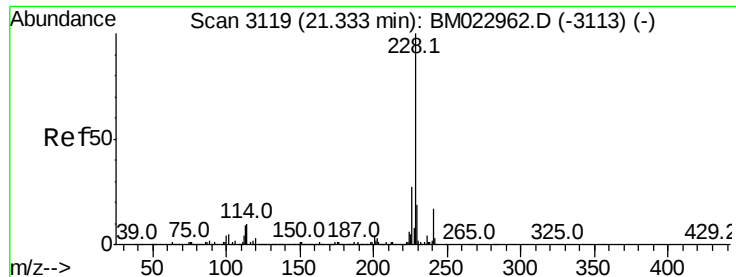

#83
Benzo(a)anthracene
Concen: 1.705 ng/ul
RT: 21.33 min Scan# 3118
Delta R.T. -0.01 min
Lab File: BM023003.D
Acq: 05 Oct 2019 22:04

Instrument :
BNA_M
ClientSampled :

Tot Ion	Ratio	Lower	Upper
228	100		
229	19.6	15.8	23.8
226	25.9	22.4	33.6



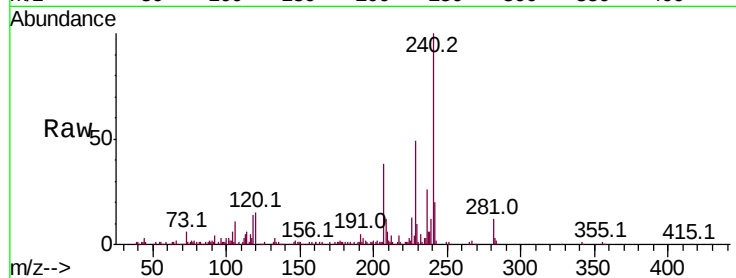


Abundance

Ion 228.00 (227.70 to 228.70): E


Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

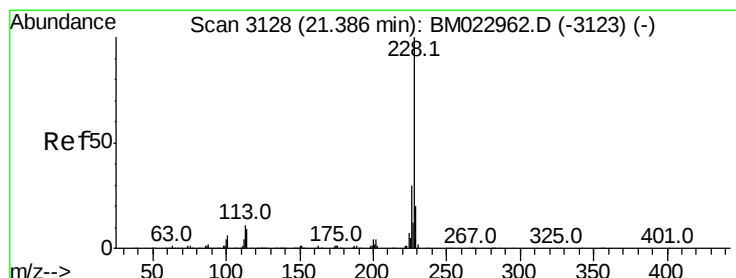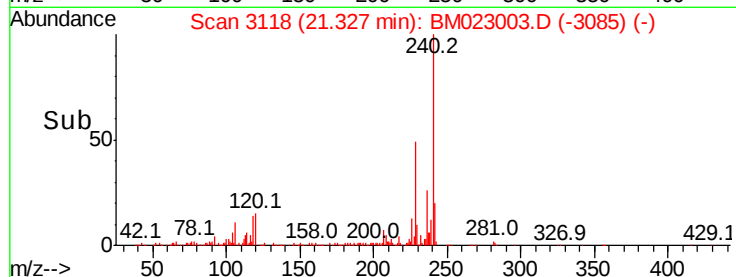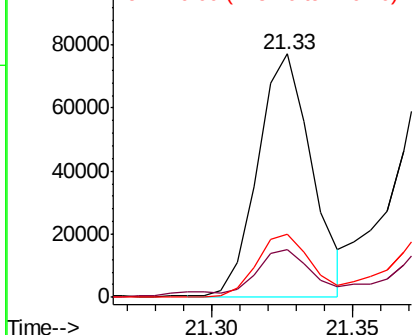

#85
Chrysene
Concen: 2.002 ng/ul
RT: 21.38 min Scan# 3127
Delta R.T. -0.01 min
Lab File: BM023003.D
Acq: 05 Oct 2019 22:04

Tgt Ion	Ratio	Lower	Upper
228	100		
226	29.0	24.2	36.4
229	20.1	15.9	23.9


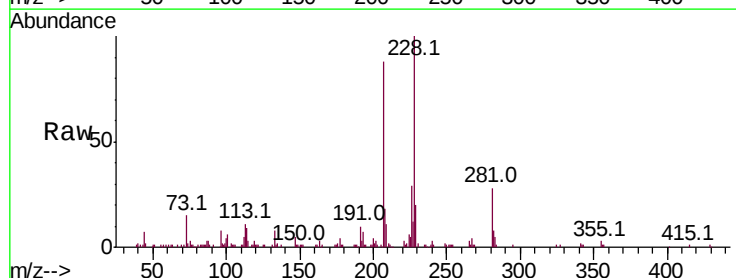



Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

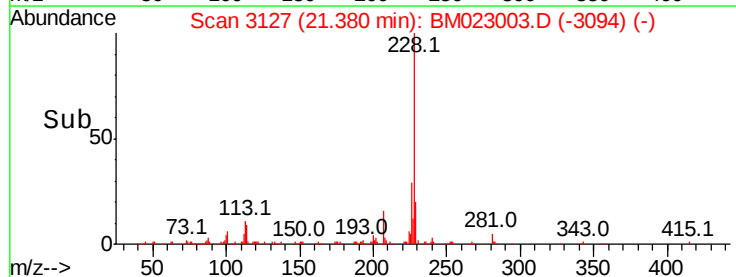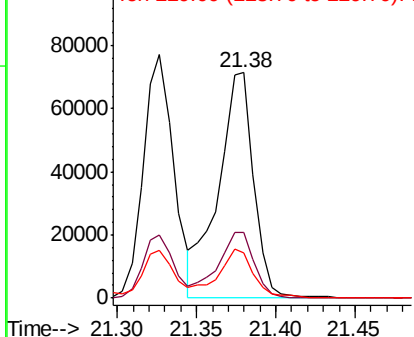

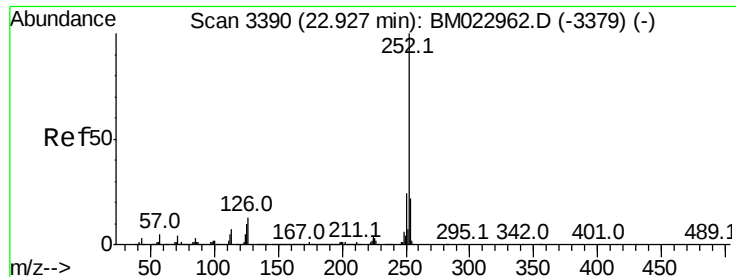

#88

Benzo(b)fluoranthene

Concen: 1.976 ng/ul

RT: 22.92 min Scan# 3389

Delta R.T. -0.01 min

Lab File: BM023003.D

Acq: 05 Oct 2019 22:04

Instrument :

BNA_M

ClientSampleId :





Tot Ion:252 Resp: 127224

Ion Ratio Lower Upper

252 100

253 22.7 17.7 26.5

125 12.5 8.2 12.2#

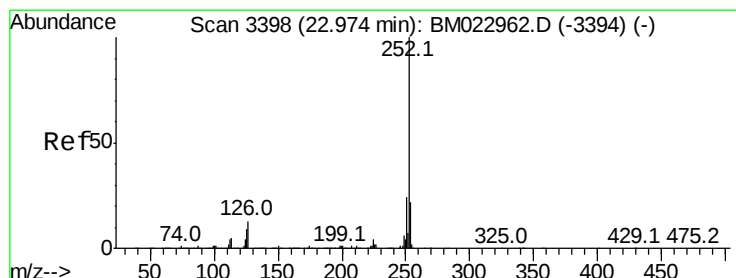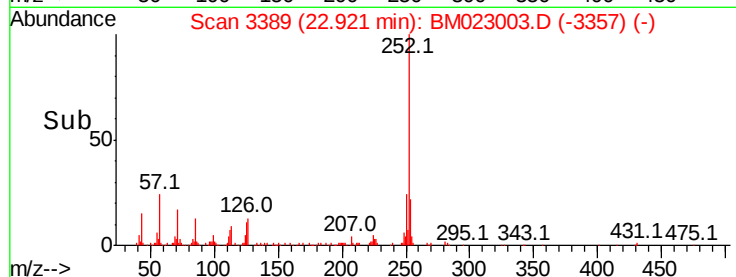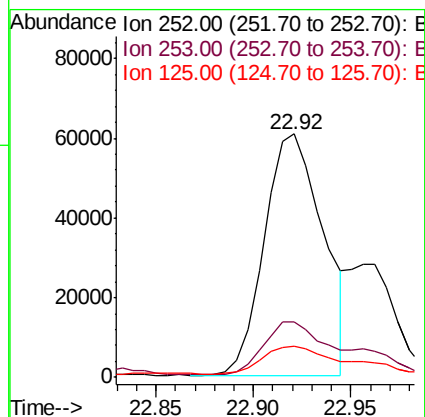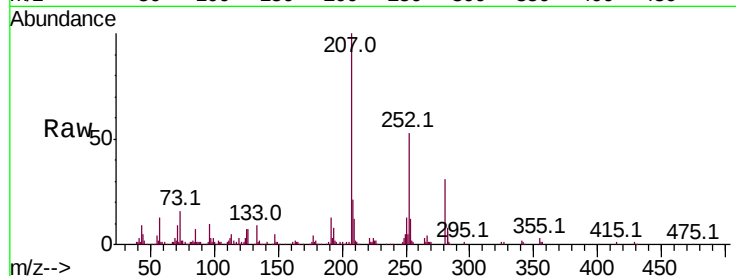

#89

Benzo(k)fluoranthene

Concen: 2.065 ng/ul

RT: 22.92 min Scan# 3389

Delta R.T. -0.05 min

Lab File: BM023003.D

Acq: 05 Oct 2019 22:04




Tgt Ion:252 Resp: 127224


Ion Ratio Lower Upper

252 100

253 22.7 17.5 26.3

125 12.5 7.9 11.9#

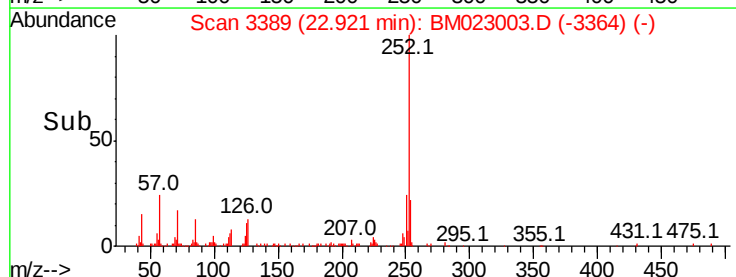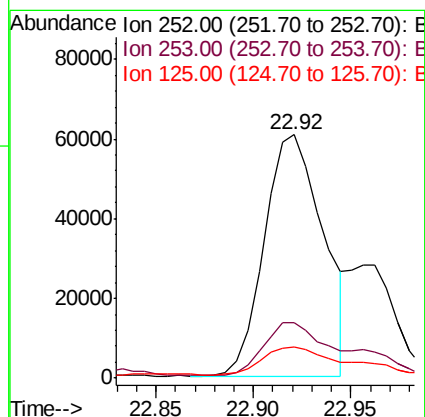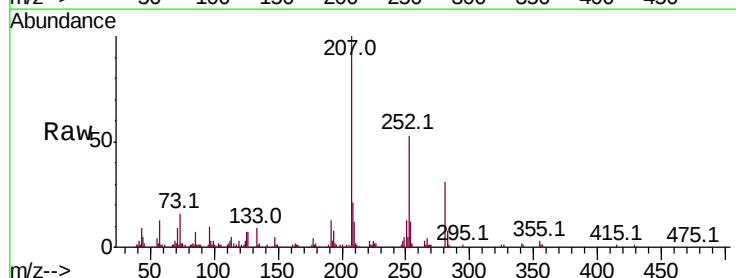

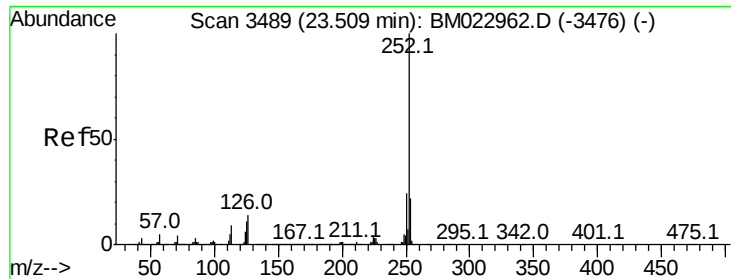

#91

Benzo(a)pyrene

Concen: 1.054 ng/ul

RT: 23.50 min Scan# 3487

Delta R.T. -0.02 min

Lab File: BM023003.D

Acq: 05 Oct 2019 22:04

Instrument :

BNA_M

ClientSampleId :

Tot Ion:	252	Resp:	63657
Ion Ratio	Lower	Upper	
252	100		
253	23.7	17.6	26.4
125	13.5	8.7	13.1#

