

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM022969.D
 Acq On : 04 Oct 2019 22:05
 Operator : JU
 Sample : K5006-16MS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETJX6MS

Quant Time: Oct 04 22:57:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 16:45:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	230756	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	993466	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.43	164	566880	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.16	188	979410	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	832628	20.00	ng/ul	0.00
86) Perylene-d12	23.60	264	985854	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	25167	4.72	ng/uL	0.00
5) Phenol-d5	6.96	99	125780	6.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	317162	28.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	372364	22.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	241750	14.48	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	233838	30.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	256682	30.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	443884	26.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	50099	2.47	ng/ul	0.00
44) Dimethylphthalate-d6	13.83	166	1409676	32.04	ng/ul	0.00
47) Acenaphthylene-d8	14.12	160	1617014	31.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	37884	4.36	ng/ul	0.00
58) Fluorene-d10	15.42	176	1112367	29.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.53	200	163720	25.69	ng/ul	0.00
71) Anthracene-d10	17.26	188	1599003	33.43	ng/ul	0.00
79) Pyrene-d10	19.56	212	1664240	37.14	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.46	264	1802021	35.33	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.99	94	146488	6.854	ng/ul 98
10) 2-Chlorophenol	7.36	128	374479	21.263	ng/ul 99
15) N-Nitroso-di-n-propylamine	8.60	70	375650	28.661	ng/ul 99
33) 4-Chloro-3-methylphenol	11.86	107	389559	22.426	ng/ul 99
45) Dimethylphthalate	13.88	163	196625	4.351	ng/ul 99
50) Acenaphthene	14.49	153	1114141	29.166	ng/ul 100
53) 4-Nitrophenol	14.64	109	30469	4.796	ng/ul 97
55) 2,4-Dinitrotoluene	14.79	165	353520	26.589	ng/ul 98
69) Pentachlorophenol	16.82	266	247136	28.917	ng/ul 99
80) Pyrene	19.59	202	2063314	34.958	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM022969.D
Acq On : 04 Oct 2019 22:05
Operator : JU
Sample : K5006-16MS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETJX6MS

Quant Time: Oct 04 22:57:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 16:45:59 2019
Response via : Initial Calibration

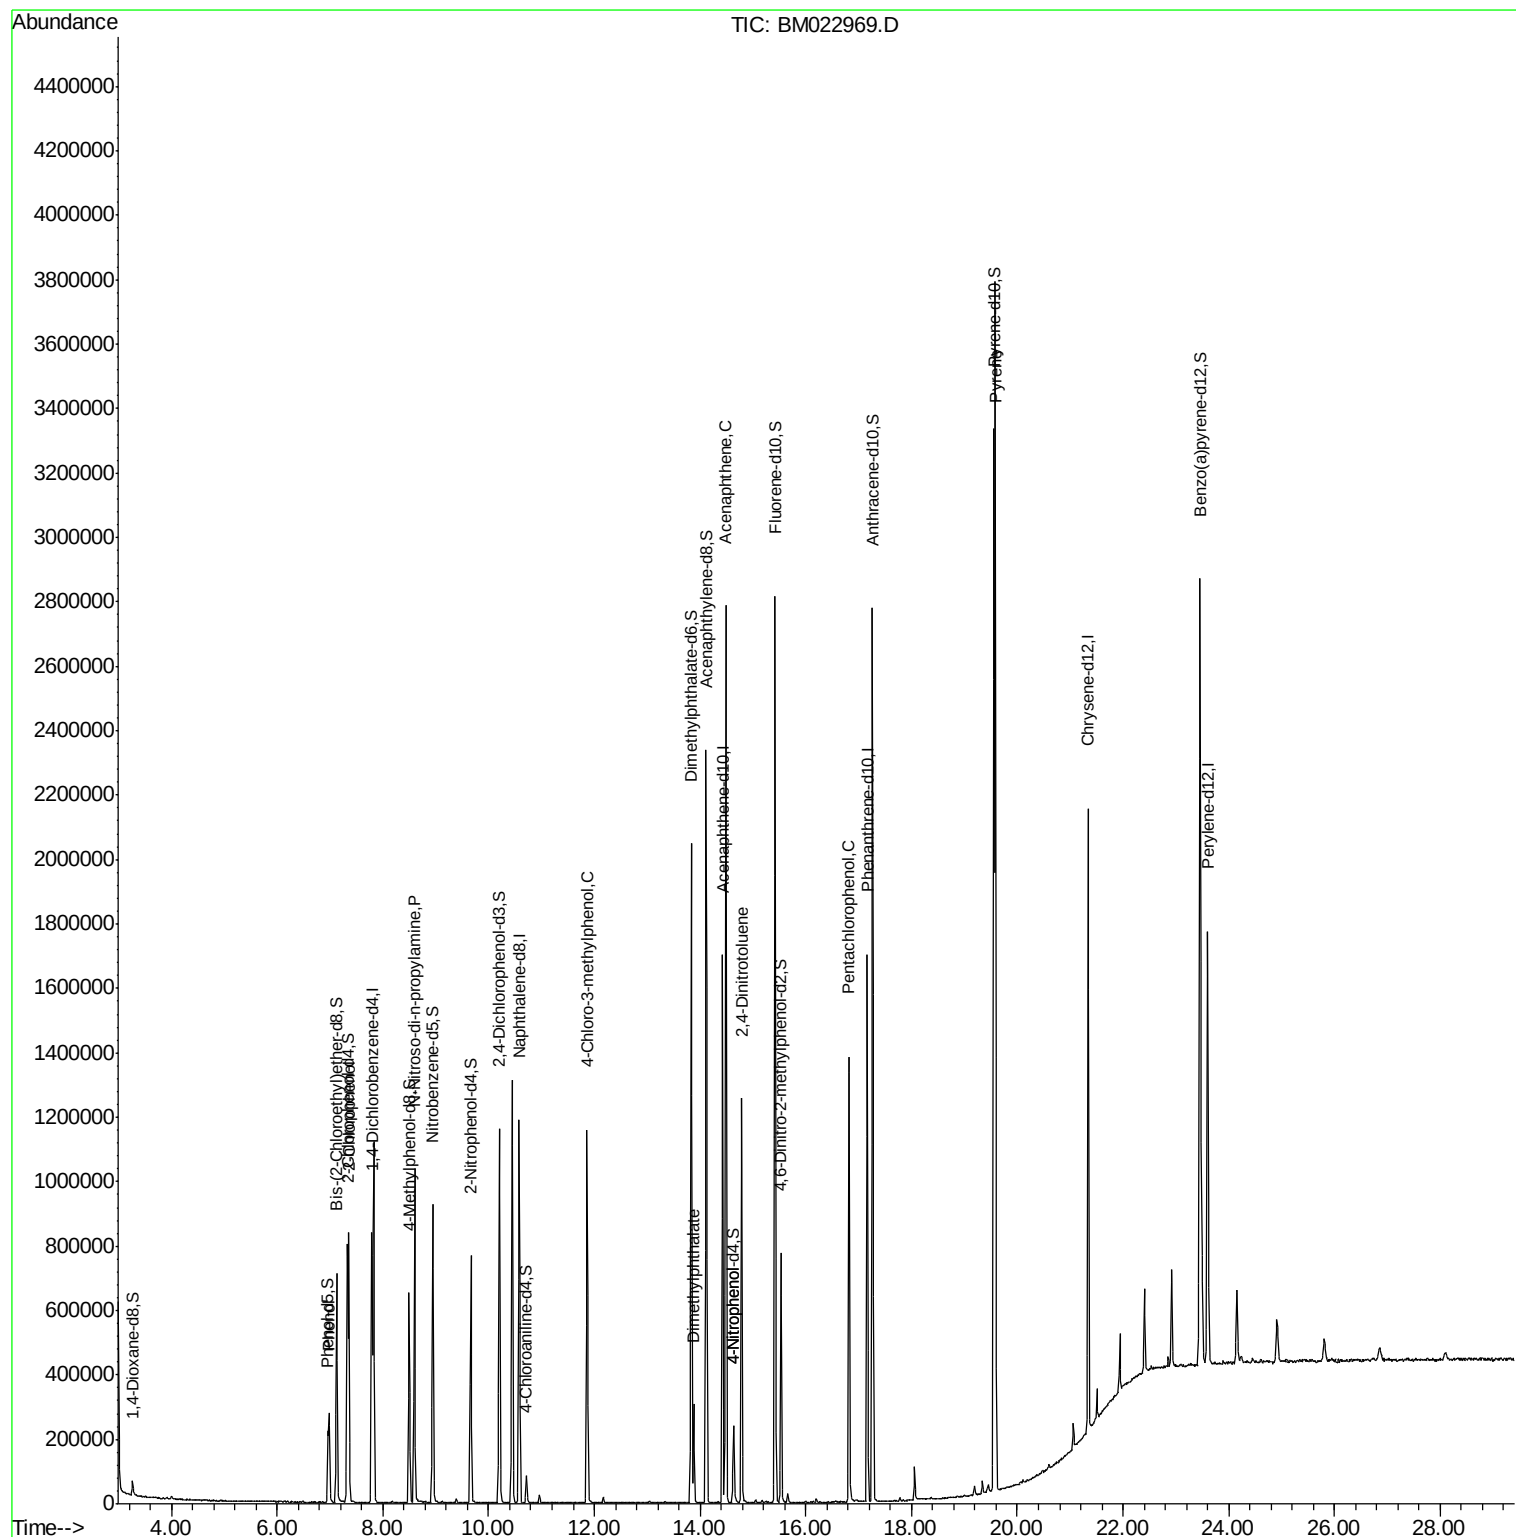

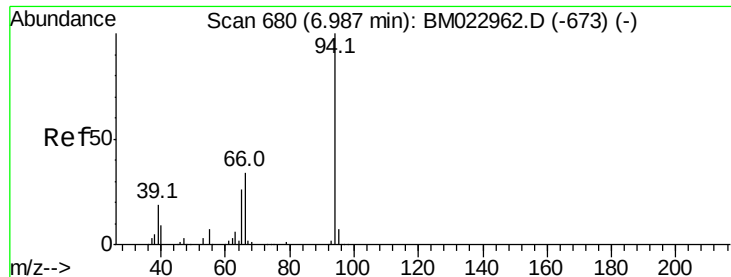

#6

Phenol

Concen: 6.854 ng/ul

RT: 6.99 min Scan# 680

Delta R.T. -0.01 min

Lab File: BM022969.D

Acq: 04 Oct 2019 22:05

Instrument :

BNA_M

ClientSampleId :

ETJX6MS


Tot Ion: 94 Resp: 146488

Ion Ratio Lower Upper

94 100

65 27.2 20.9 31.3




66 35.3 27.2 40.8

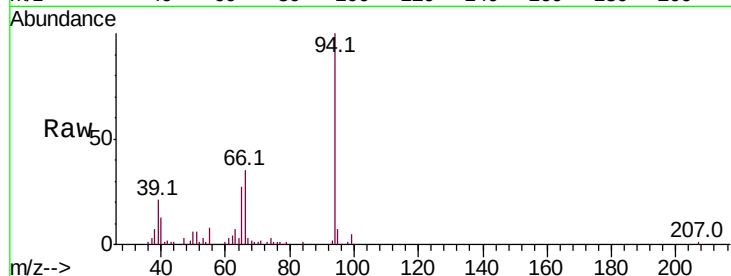

Abundance Ion 94.00 (93.70 to 94.70): BM022969.D (-647) (-)

Ion 65.00 (64.70 to 65.70): BM022969.D (-647) (-)

Ion 66.00 (65.70 to 66.70): BM022969.D (-647) (-)

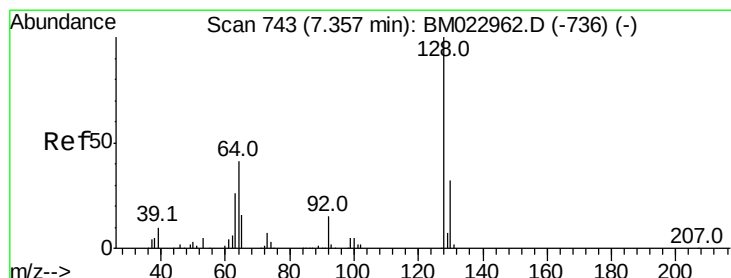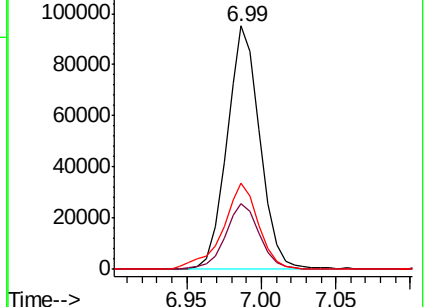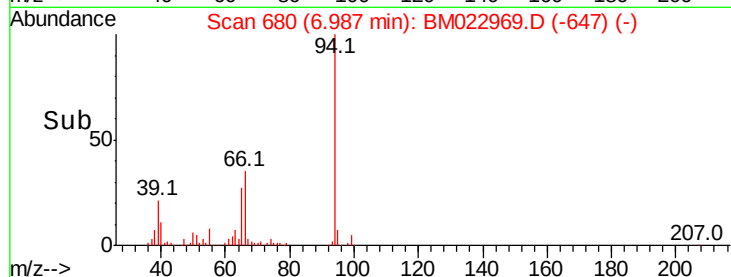

#10

2-Chlorophenol

Concen: 21.263 ng/ul

RT: 7.36 min Scan# 743

Delta R.T. -0.01 min

Lab File: BM022969.D

Acq: 04 Oct 2019 22:05


Tgt Ion:128 Resp: 374479

Ion Ratio Lower Upper

128 100

64 41.7 34.1 51.1



130 32.5 26.0 39.0

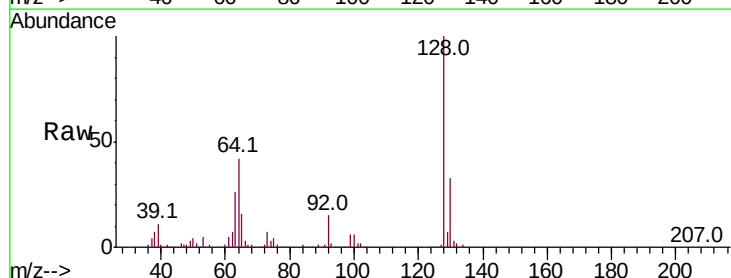


Abundance Ion 128.00 (127.70 to 128.70): BM022969.D (-710) (-)

Ion 64.00 (63.70 to 64.70): BM022969.D (-710) (-)

Ion 130.00 (129.70 to 130.70): BM022969.D (-710) (-)

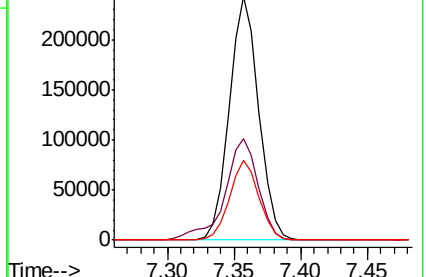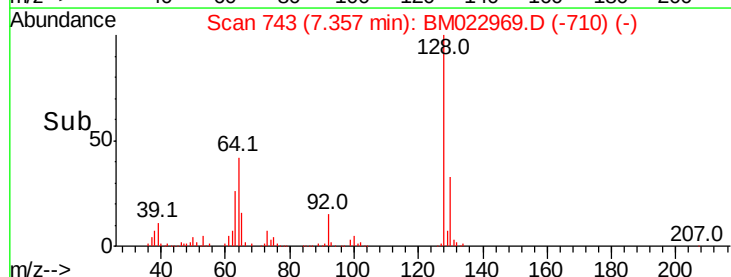


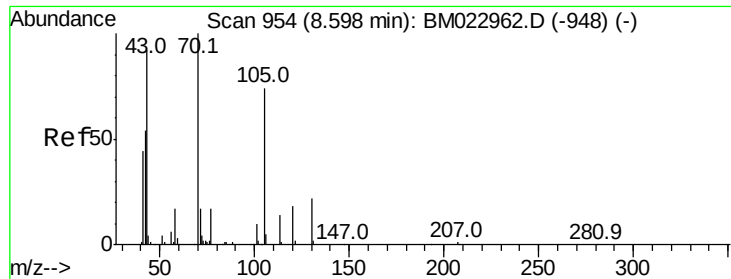




#15
N-Nitroso-di-n-propylamine
Concen: 28.661 ng/ul
RT: 8.60 min Scan# 954
Delta R.T. -0.01 min
Lab File: BM022969.D
Acq: 04 Oct 2019 22:05

Instrument :
BNA_M
ClientSampleId :
ETJX6MS

Tot Ion:	70	Resp:	375650
Ion	Ratio	Lower	Upper
70	100		
42	54.7	44.6	66.8
101	9.8	8.2	12.2
130	23.7	18.7	28.1

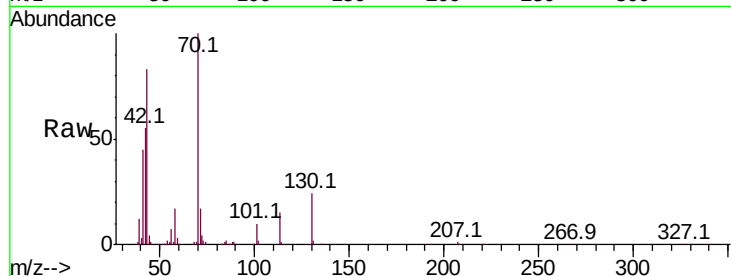


Abundance Ion 70.00 (69.70 to 70.70): BM0
Ion 42.00 (41.70 to 42.70): BM0
Ion 101.00 (100.70 to 101.70): E
Ion 130.00 (129.70 to 130.70): E

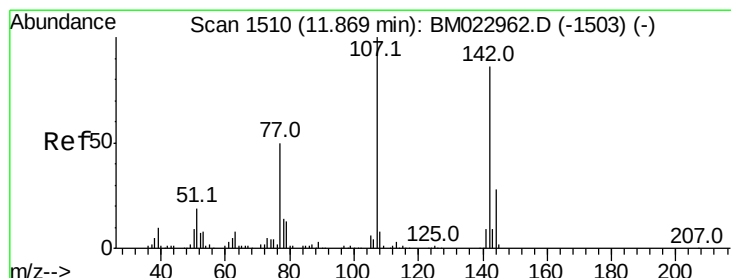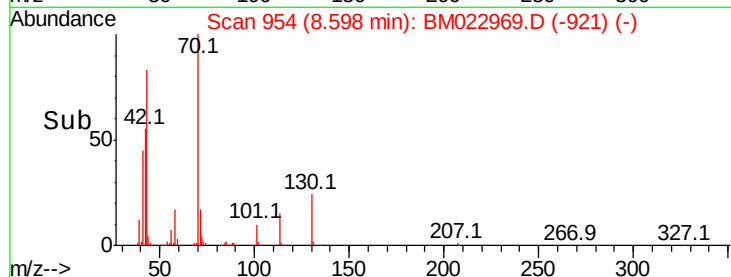
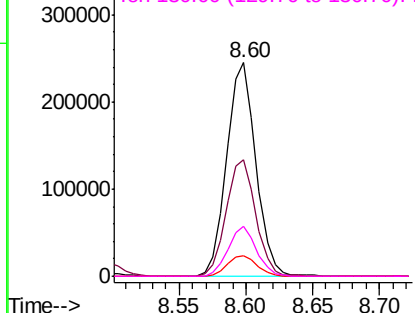



#33
4-Chloro-3-methylphenol
Concen: 22.426 ng/ul
RT: 11.86 min Scan# 1509
Delta R.T. -0.01 min
Lab File: BM022969.D
Acq: 04 Oct 2019 22:05

Tgt Ion:	107	Resp:	389559
Ion	Ratio	Lower	Upper
107	100		
144	27.8	22.5	33.7
142	85.1	68.9	103.3

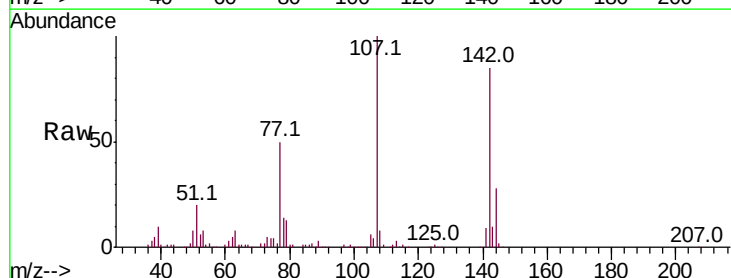

Abundance Ion 107.00 (106.70 to 107.70): E
Ion 144.00 (143.70 to 144.70): E
Ion 142.00 (141.70 to 142.70): E

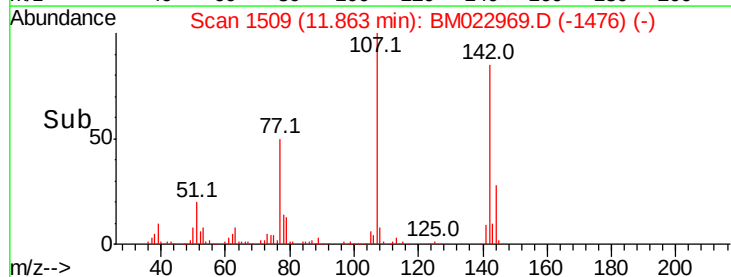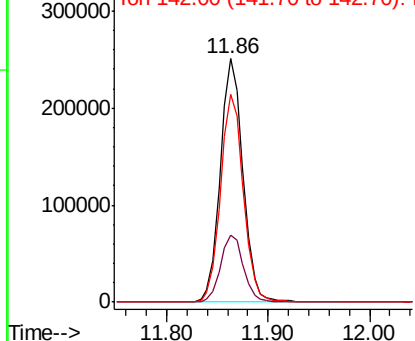


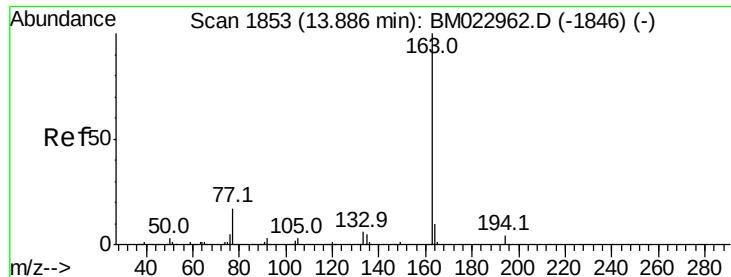

#45
Dimethylphthalate
Concen: 4.351 ng/ul
RT: 13.88 min Scan# 1852
Delta R.T. -0.01 min
Lab File: BM022969.D
Acq: 04 Oct 2019 22:05

Instrument :
BNA_M
ClientSampleId :
ETJX6MS

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	9.8	8.1	12.1



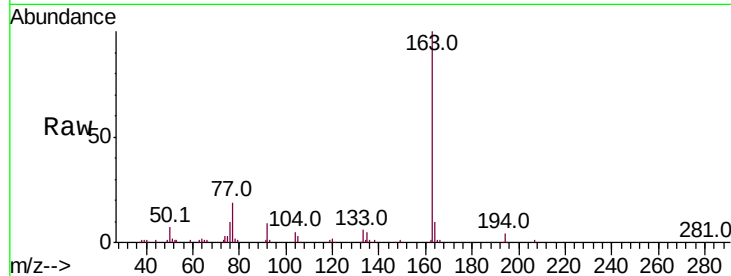


Abundance

Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

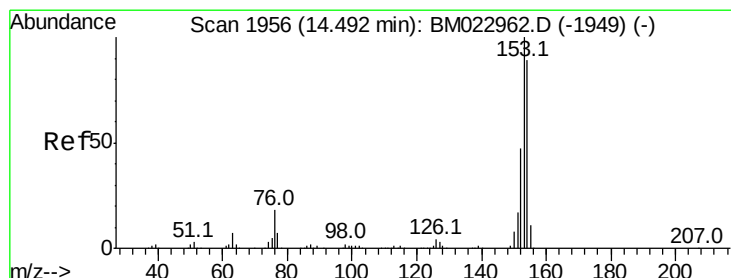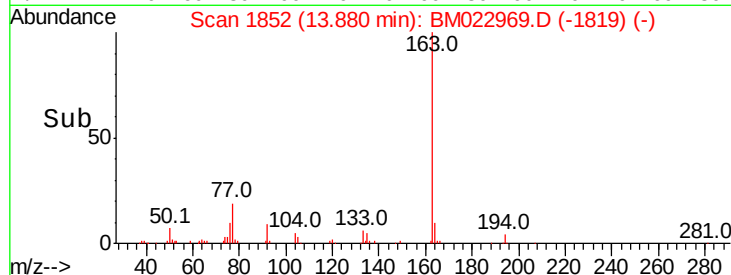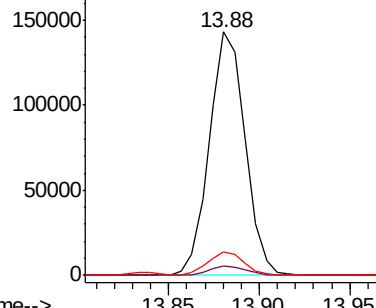

#50
Acenaphthene
Concen: 29.166 ng/ul
RT: 14.49 min Scan# 1956
Delta R.T. 0.00 min
Lab File: BM022969.D
Acq: 04 Oct 2019 22:05

Tgt Ion	Ratio	Lower	Upper
153	100		
152	47.6	38.1	57.1
154	88.4	71.1	106.7


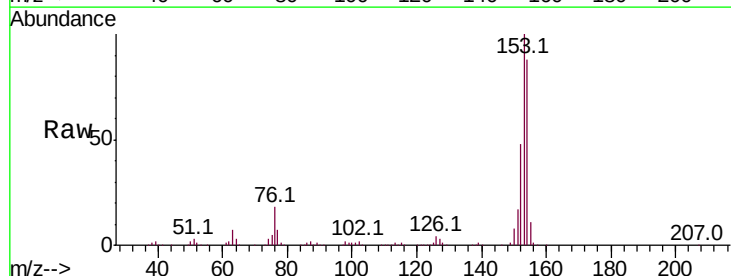



Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E



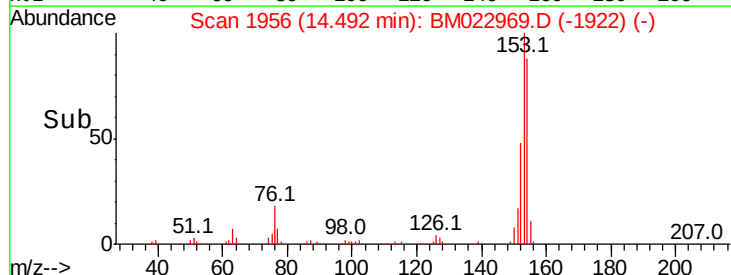
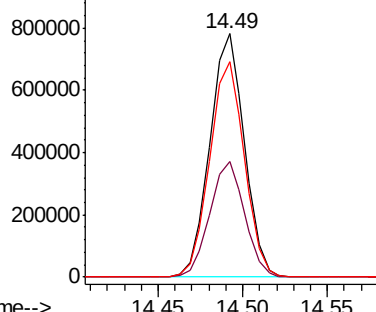


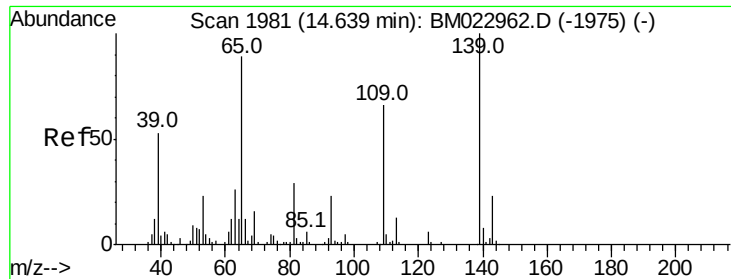

#53
4-Nitrophenol
Concen: 4.796 ng/ul
RT: 14.64 min Scan# 1981
Delta R.T. -0.01 min
Lab File: BM022969.D
Acq: 04 Oct 2019 22:05




Instrument :
BNA_M
ClientSampleId :
ETJX6MS


Tot Ion:109 Resp: 30469
Ion Ratio Lower Upper
109 100
139 150.1 119.5 179.3
65 138.0 105.0 157.4

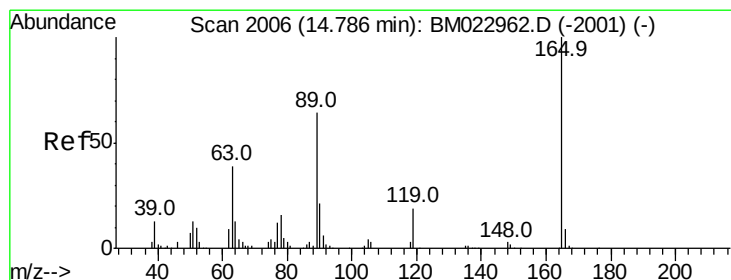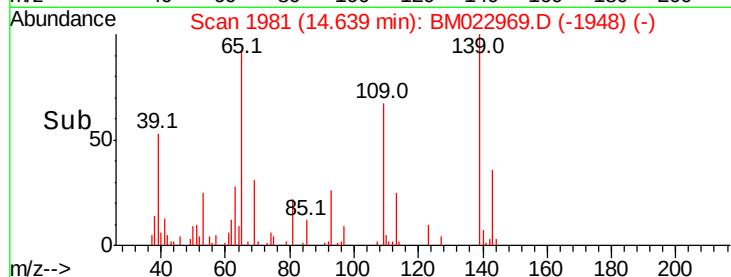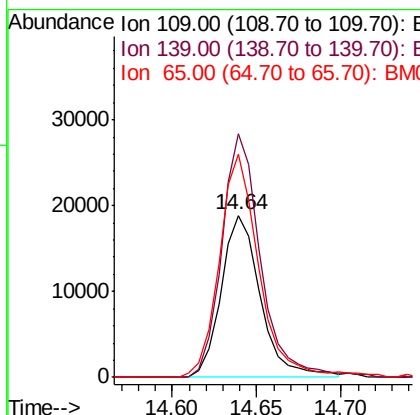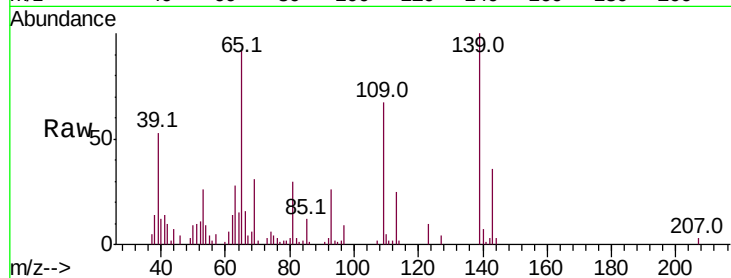

#55
2,4-Dinitrotoluene
Concen: 26.589 ng/ul
RT: 14.79 min Scan# 2006
Delta R.T. -0.01 min
Lab File: BM022969.D
Acq: 04 Oct 2019 22:05

Tgt Ion:165 Resp: 353520
Ion Ratio Lower Upper
165 100
63 38.7 29.8 44.6
182 2.8 2.2 3.4

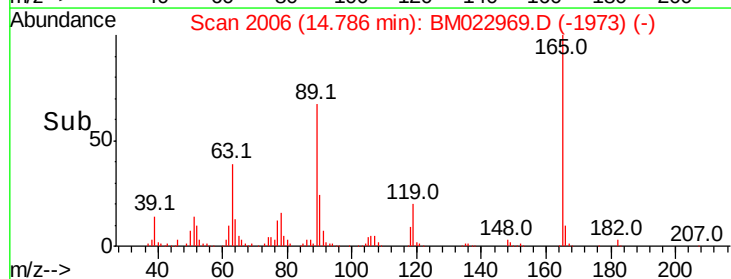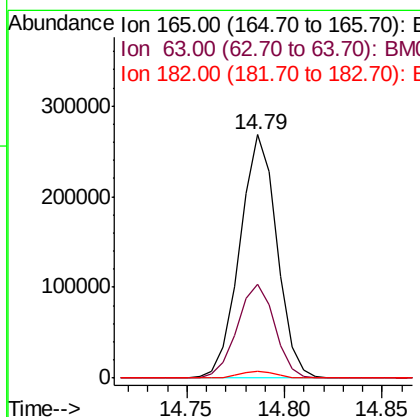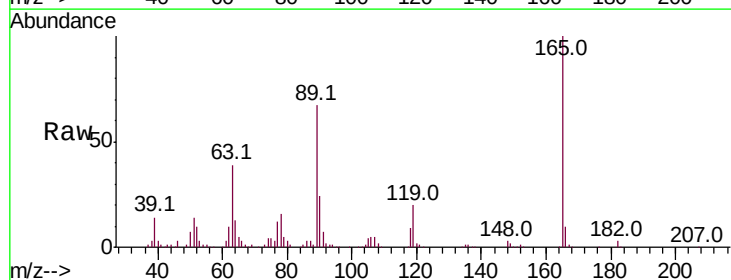

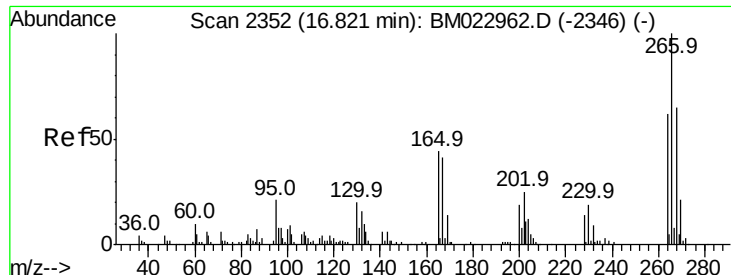

#69

Pentachlorophenol

Concen: 28.917 ng/ul

RT: 16.82 min Scan# 2352

Delta R.T. 0.00 min

Lab File: BM022969.D

Acq: 04 Oct 2019 22:05

Instrument :

BNA_M

ClientSampleId :

ETJX6MS


Tot Ion:266 Resp: 247136

Ion Ratio Lower Upper

266 100

264 63.1 50.8 76.2




268 63.6 51.4 77.0

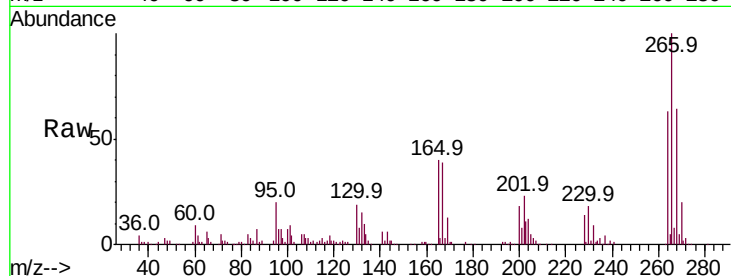

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

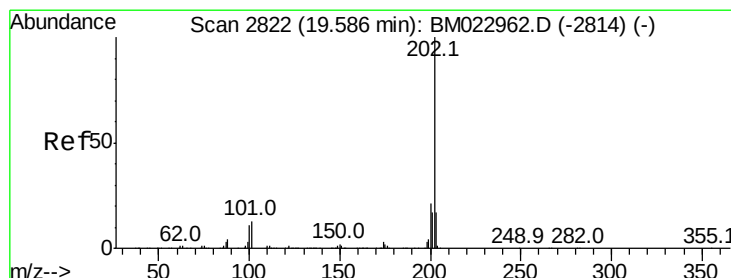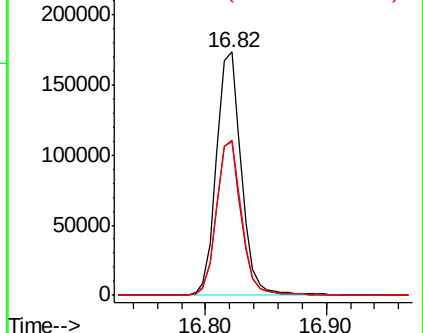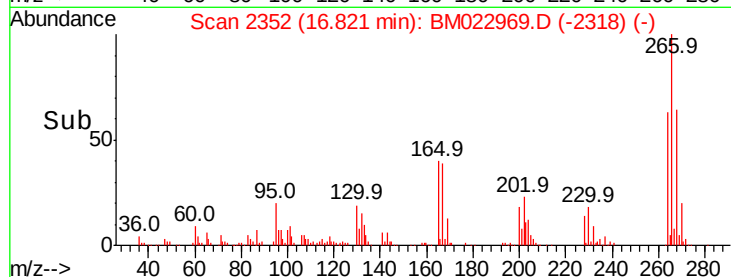

#80

Pyrene

Concen: 34.958 ng/ul

RT: 19.59 min Scan# 2822

Delta R.T. -0.01 min

Lab File: BM022969.D

Acq: 04 Oct 2019 22:05


Tgt Ion:202 Resp: 2063314

Ion Ratio Lower Upper

202 100

101 12.9 9.7 14.5

100 10.5 7.8 11.8

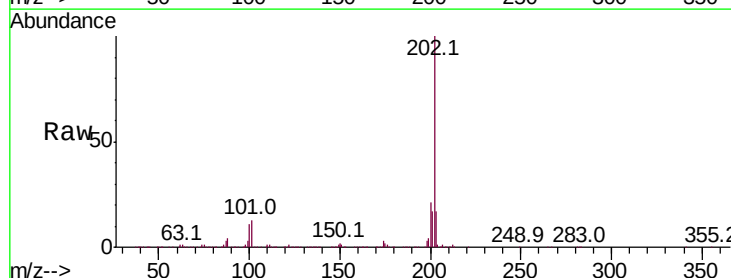

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

