

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023002.D
 Acq On : 05 Oct 2019 21:28
 Operator : JU
 Sample : K5050-20
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLME0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	44	47	56	rVB	43701	61983	1.84%	0.137%
2	3.999	168	172	176	rVB	10094	13756	0.41%	0.030%
3	6.469	588	592	597	rBV4	3529	4900	0.15%	0.011%
4	6.957	667	675	689	rBV	800778	1396930	41.43%	3.076%
5	7.122	696	703	717	rBV	594773	992844	29.45%	2.186%
6	7.322	730	737	750	rVB	857132	1338619	39.70%	2.948%
7	7.787	809	816	826	rBV	918931	1413435	41.92%	3.113%
8	7.857	826	828	835	rVB3	4968	6121	0.18%	0.013%
9	8.493	928	936	948	rBV	1005871	1631330	48.38%	3.593%
10	8.940	1004	1012	1022	rBV	761068	1245463	36.94%	2.743%
11	9.022	1022	1026	1031	rVB3	3339	5762	0.17%	0.013%
12	9.110	1037	1041	1046	rVB4	3458	5179	0.15%	0.011%
13	9.381	1081	1087	1095	rBV	8120	13016	0.39%	0.029%
14	9.657	1127	1134	1150	rBV	600699	988202	29.31%	2.176%
15	10.198	1219	1226	1243	rBV	1029462	1697424	50.34%	3.738%
16	10.575	1283	1290	1298	rBV	1306693	2130592	63.19%	4.692%
17	10.710	1303	1313	1331	rBV	958767	1659032	49.20%	3.654%
18	12.010	1530	1534	1537	rVB4	3215	4400	0.13%	0.010%
19	12.169	1555	1561	1566	rVB2	12836	22035	0.65%	0.049%
20	12.245	1569	1574	1578	rVB4	3271	5612	0.17%	0.012%
21	12.457	1608	1610	1615	rVB4	2287	3452	0.10%	0.008%
22	13.033	1705	1708	1713	rVB3	3509	4527	0.13%	0.010%
23	13.257	1740	1746	1751	rBV5	6206	9502	0.28%	0.021%
24	13.322	1753	1757	1763	rVB5	2328	4086	0.12%	0.009%
25	13.833	1837	1844	1848	rBV	1631102	2259685	67.02%	4.976%
26	13.875	1848	1851	1857	rVB	456383	630911	18.71%	1.389%
27	14.116	1883	1892	1904	rBV	1952138	2925619	86.77%	6.443%
28	14.333	1926	1929	1933	rVB2	6604	8875	0.26%	0.020%
29	14.422	1937	1944	1954	rBV	1918896	2786739	82.65%	6.137%
30	14.616	1971	1977	1996	rBV	387160	635135	18.84%	1.399%
31	14.839	2010	2015	2021	rVB3	15202	21650	0.64%	0.048%
32	14.963	2030	2036	2042	rBV4	9354	22184	0.66%	0.049%
33	15.233	2078	2082	2086	rVB2	3315	5565	0.17%	0.012%
34	15.280	2086	2090	2096	rVB	19978	26750	0.79%	0.059%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023002.D
 Acq On : 05 Oct 2019 21:28
 Operator : JU
 Sample : K5050-20
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLME0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

35	15.416	2106	2113	2123	rBV	2357502	3371820	100.00%	7.426%
36	15.527	2126	2132	2141	rBV	401609	539486	16.00%	1.188%
37	15.657	2149	2154	2158	rBV	22958	32936	0.98%	0.073%
38	15.692	2158	2160	2164	rVB3	2992	3626	0.11%	0.008%
39	16.139	2233	2236	2239	rBV2	7425	10170	0.30%	0.022%
40	16.198	2243	2246	2250	rVB3	7353	9541	0.28%	0.021%
41	16.310	2262	2265	2269	rVB3	2928	4734	0.14%	0.010%
42	16.568	2302	2309	2312	rBV6	4428	8576	0.25%	0.019%
43	16.933	2364	2371	2374	rBV3	8467	15163	0.45%	0.033%
44	17.163	2403	2410	2420	rBV	1953855	2731226	81.00%	6.015%
45	17.257	2420	2426	2437	rBV	2237190	3115741	92.41%	6.862%
46	17.545	2470	2475	2481	rBV7	10002	16157	0.48%	0.036%
47	17.668	2493	2496	2501	rVB4	3871	4823	0.14%	0.011%
48	17.933	2537	2541	2545	rVB6	4830	5815	0.17%	0.013%
49	18.057	2557	2562	2572	rBV	100070	145828	4.32%	0.321%
50	18.362	2611	2614	2616	rBV3	5285	7052	0.21%	0.016%
51	18.492	2632	2636	2640	rVB4	22349	26273	0.78%	0.058%
52	19.186	2750	2754	2758	rBV	18607	28063	0.83%	0.062%
53	19.339	2777	2780	2783	rBV4	14401	15845	0.47%	0.035%
54	19.439	2794	2797	2800	rBV	15807	17333	0.51%	0.038%
55	19.551	2810	2816	2824	rBV	2358261	3139489	93.11%	6.914%
56	21.056	3069	3072	3081	rBV3	98560	149139	4.42%	0.328%
57	21.339	3115	3120	3126	rBV	1954936	2438222	72.31%	5.370%
58	23.456	3473	3480	3492	rVB	1562494	3011893	89.33%	6.633%
59	23.597	3498	3504	3516	rVB	1357578	2577890	76.45%	5.677%


Sum of corrected areas: 45408156

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM023002.D
Acq On : 05 Oct 2019 21:28
Operator : JU
Sample : K5050-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLME0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

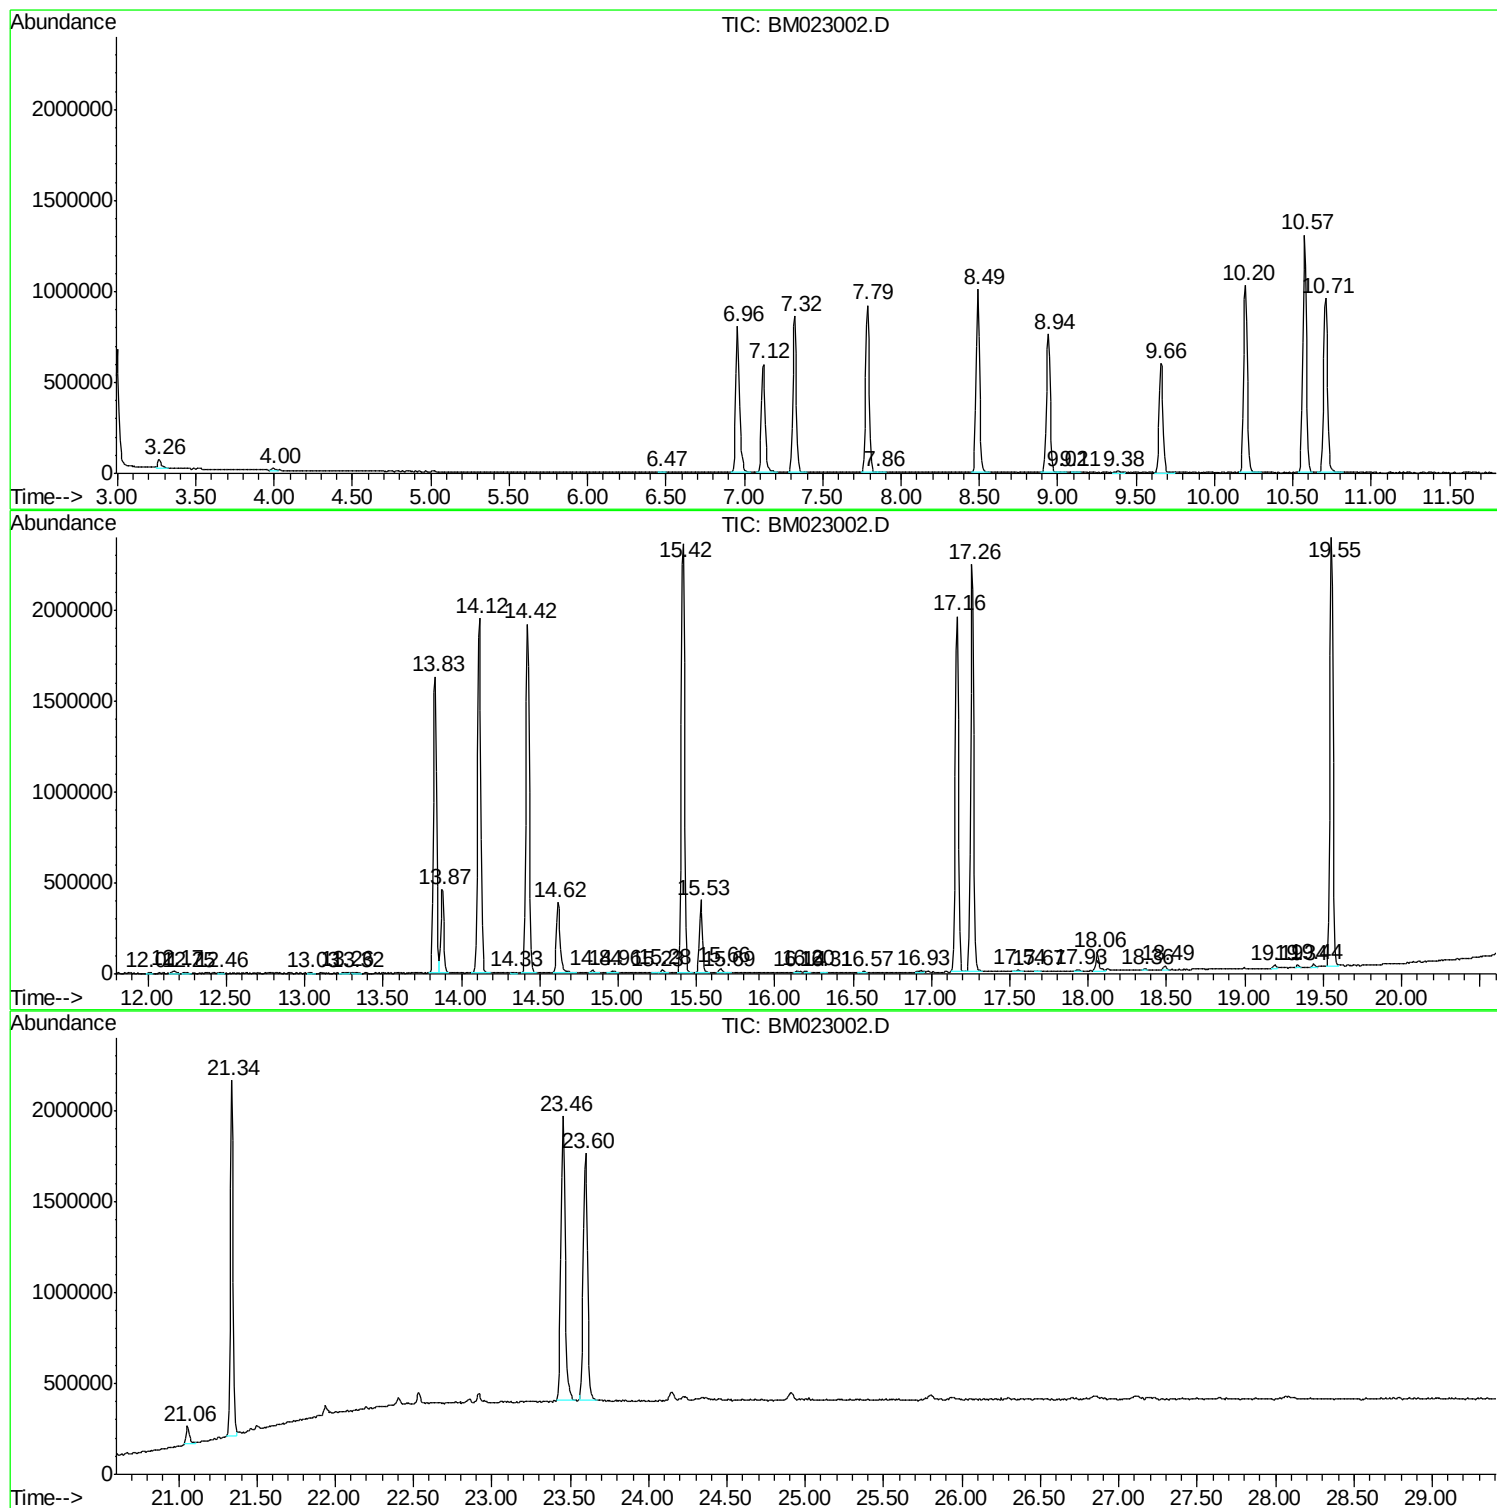

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023002.D
Acq On : 05 Oct 2019 21:28
Operator : JU
Sample : K5050-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLME0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023002.D
Acq On : 05 Oct 2019 21:28
Operator : JU
Sample : K5050-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLME0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc