

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023004.D
 Acq On : 05 Oct 2019 22:40
 Operator : JU
 Sample : K5057-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAH4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	45	47	58	rVB	28947	45447	1.78%	0.128%
2	3.910	153	157	167	rVB	17874	32145	1.26%	0.091%
3	3.993	167	171	176	rBV	11242	17165	0.67%	0.048%
4	4.910	323	327	336	rBV	58141	89851	3.52%	0.254%
5	6.469	588	592	594	rBV4	3156	4008	0.16%	0.011%
6	6.957	668	675	687	rBV2	547946	995697	38.98%	2.813%
7	7.122	696	703	716	rBV	400818	667843	26.14%	1.887%
8	7.322	730	737	748	rVV	571119	900517	35.25%	2.544%
9	7.416	751	753	758	rVB3	2889	3848	0.15%	0.011%
10	7.787	809	816	825	rBV	811008	1258534	49.26%	3.556%
11	7.863	825	829	834	rVB4	4277	7103	0.28%	0.020%
12	8.492	929	936	950	rBV	674204	1096892	42.94%	3.099%
13	8.610	952	956	963	rVB2	13158	23454	0.92%	0.066%
14	8.939	1005	1012	1022	rBV	505423	830326	32.50%	2.346%
15	9.063	1028	1033	1038	rBV2	5695	9179	0.36%	0.026%
16	9.110	1038	1041	1046	rVB5	3991	5133	0.20%	0.015%
17	9.381	1082	1087	1093	rVB2	4974	7672	0.30%	0.022%
18	9.657	1128	1134	1143	rBV	390233	631692	24.73%	1.785%
19	10.198	1219	1226	1235	rBV	701627	1134543	44.41%	3.206%
20	10.575	1283	1290	1298	rBV	1173716	1912202	74.85%	5.403%
21	10.710	1306	1313	1327	rBV	635250	1101615	43.12%	3.113%
22	11.369	1423	1425	1429	rBV4	1491	2567	0.10%	0.007%
23	12.163	1556	1560	1566	rVB2	7942	12848	0.50%	0.036%
24	12.245	1569	1574	1580	rVV4	2062	3008	0.12%	0.008%
25	12.463	1607	1611	1615	rVB3	2944	4947	0.19%	0.014%
26	12.786	1662	1666	1672	rVB3	2186	2728	0.11%	0.008%
27	13.039	1703	1709	1714	rVB4	3672	5611	0.22%	0.016%
28	13.327	1753	1758	1761	rVB3	3115	3442	0.13%	0.010%
29	13.833	1837	1844	1848	rBV	1168321	1630000	63.80%	4.605%
30	13.874	1848	1851	1861	rVB	431972	596972	23.37%	1.687%
31	14.116	1885	1892	1904	rVB	1369179	1997811	78.20%	5.645%
32	14.333	1926	1929	1931	rBV	3352	3043	0.12%	0.009%
33	14.421	1937	1944	1958	rBV	1769338	2554659	100.00%	7.218%
34	14.616	1972	1977	1996	rBV	264583	455019	17.81%	1.286%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM023004.D
Acq On : 05 Oct 2019 22:40
Operator : JU
Sample : K5057-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAH4

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Title : SVOA CALIBRATION

35	14.839	2010	2015	2020	rVB4	11376	15335	0.60%	0.043%
36	15.227	2078	2081	2086	rBV3	4529	6979	0.27%	0.020%
37	15.286	2086	2091	2094	rVV3	4182	6167	0.24%	0.017%
38	15.416	2106	2113	2121	rBV	1704569	2407392	94.24%	6.802%
39	15.527	2127	2132	2144	rBV	270300	372818	14.59%	1.053%
40	15.651	2149	2153	2159	rBV	14817	20561	0.80%	0.058%
41	16.139	2233	2236	2239	rBV3	5153	6207	0.24%	0.018%
42	16.198	2243	2246	2249	rVB2	4491	5861	0.23%	0.017%
43	16.568	2303	2309	2311	rBV2	4402	5363	0.21%	0.015%
44	16.945	2367	2373	2378	rBV4	5403	11990	0.47%	0.034%
45	17.062	2390	2393	2396	rBV4	2230	3430	0.13%	0.010%
46	17.162	2403	2410	2420	rBV2	1748287	2482277	97.17%	7.014%
47	17.257	2420	2426	2439	rBV	1587969	2257332	88.36%	6.378%
48	17.551	2471	2476	2483	rBV6	8844	16197	0.63%	0.046%
49	17.668	2492	2496	2500	rBV6	4195	7158	0.28%	0.020%
50	17.839	2521	2525	2527	rBV4	3442	3593	0.14%	0.010%
51	17.939	2537	2542	2548	rBV6	8101	15275	0.60%	0.043%
52	18.057	2557	2562	2571	rBV	71990	93215	3.65%	0.263%
53	18.127	2571	2574	2580	rVB3	4376	7916	0.31%	0.022%
54	18.357	2610	2613	2617	rBV3	4294	6503	0.25%	0.018%
55	18.492	2632	2636	2641	rVB2	11019	13836	0.54%	0.039%
56	19.186	2751	2754	2757	rBV3	14858	19153	0.75%	0.054%
57	19.221	2757	2760	2763	rVB	12161	14972	0.59%	0.042%
58	19.339	2777	2780	2785	rVB3	16869	17204	0.67%	0.049%
59	19.551	2810	2816	2824	rBV	1857131	2446991	95.79%	6.914%
60	21.062	3069	3073	3079	rBV2	97450	144445	5.65%	0.408%
61	21.339	3115	3120	3126	rBV	1761015	2183161	85.46%	6.168%
62	23.450	3473	3479	3493	rVB	1227338	2468375	96.62%	6.974%
63	23.597	3497	3504	3515	rVB	1204385	2285359	89.46%	6.457%


Sum of corrected areas: 35392586

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM023004.D
Acq On : 05 Oct 2019 22:40
Operator : JU
Sample : K5057-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAH4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

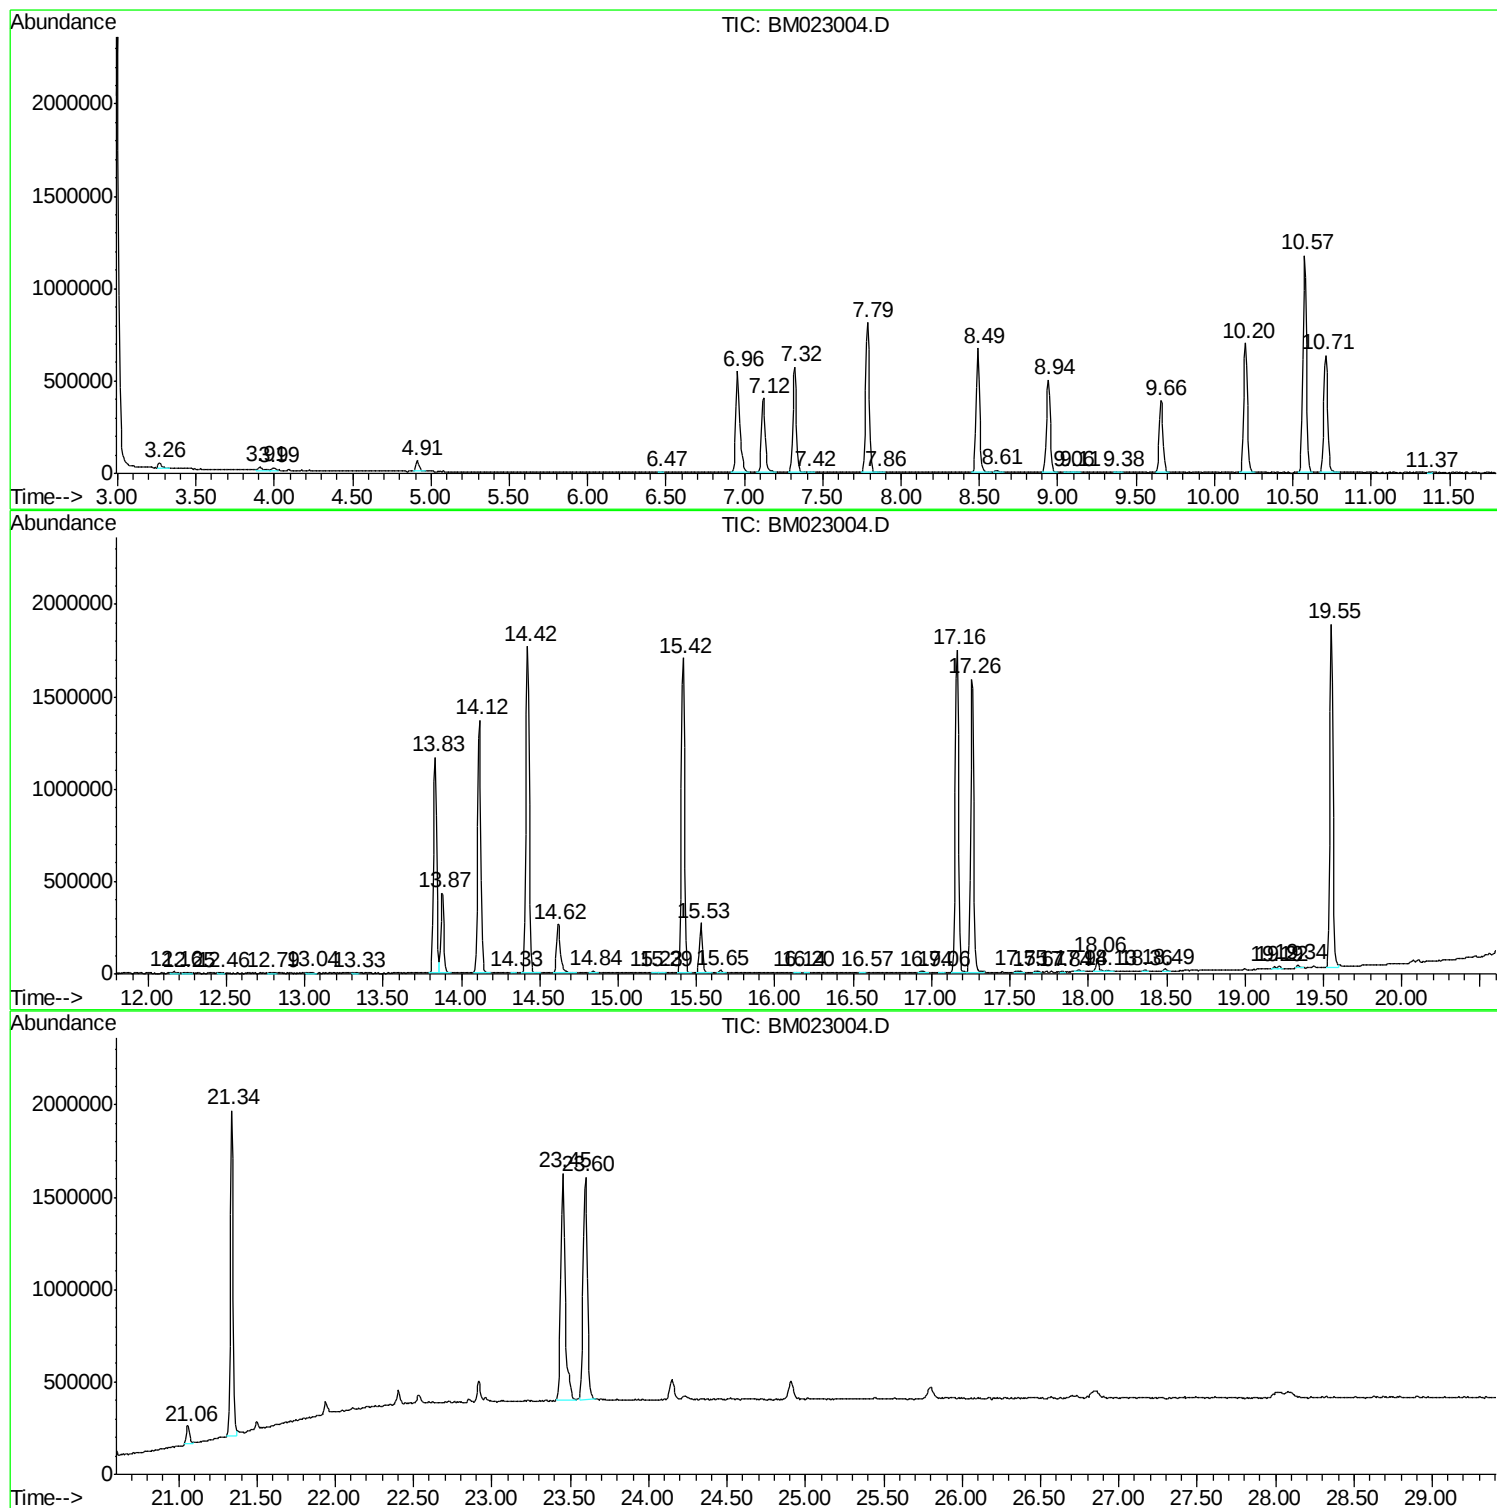

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023004.D
Acq On : 05 Oct 2019 22:40
Operator : JU
Sample : K5057-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAH4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023004.D
Acq On : 05 Oct 2019 22:40
Operator : JU
Sample : K5057-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAH4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc