

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023014.D
 Acq On : 06 Oct 2019 05:53
 Operator : JU
 Sample : K5057-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAJ9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	44	47	56	rVB	27318	39847	1.48%	0.109%
2	3.910	152	157	161	rBV	15437	22951	0.85%	0.063%
3	3.993	167	171	177	rBV	19308	25759	0.95%	0.070%
4	4.910	323	327	343	rVB	64118	101740	3.77%	0.278%
5	5.946	499	503	506	rBV5	1523	2911	0.11%	0.008%
6	6.469	588	592	595	rVB4	3317	4491	0.17%	0.012%
7	6.951	668	674	691	rBV2	518325	944391	34.99%	2.577%
8	7.122	696	703	723	rVV	389861	662025	24.53%	1.806%
9	7.322	730	737	747	rVV	550276	880156	32.61%	2.401%
10	7.416	751	753	757	rVB4	3264	4441	0.16%	0.012%
11	7.787	809	816	825	rBV	834173	1313821	48.68%	3.585%
12	7.863	825	829	834	rVB4	5403	8798	0.33%	0.024%
13	8.487	929	935	949	rBV	671003	1079335	39.99%	2.945%
14	8.610	952	956	962	rVB2	8586	15073	0.56%	0.041%
15	8.775	978	984	988	rBV4	2346	2763	0.10%	0.008%
16	8.939	1005	1012	1021	rBV	505654	831150	30.79%	2.268%
17	9.110	1037	1041	1046	rVB	8700	11440	0.42%	0.031%
18	9.381	1081	1087	1093	rVB2	6350	10711	0.40%	0.029%
19	9.657	1128	1134	1148	rBV	385576	633801	23.48%	1.729%
20	10.198	1218	1226	1241	rBV	673209	1140615	42.26%	3.112%
21	10.575	1282	1290	1301	rBV	1209455	1995206	73.92%	5.444%
22	10.710	1303	1313	1327	rBV	638714	1119492	41.48%	3.054%
23	12.163	1555	1560	1567	rVB3	8545	14518	0.54%	0.040%
24	12.786	1661	1666	1670	rBV4	3678	4858	0.18%	0.013%
25	13.039	1704	1709	1712	rVB3	4808	6799	0.25%	0.019%
26	13.263	1743	1747	1751	rVB4	2276	3379	0.13%	0.009%
27	13.322	1754	1757	1762	rVB2	2119	2879	0.11%	0.008%
28	13.833	1837	1844	1848	rBV	1161387	1642814	60.86%	4.482%
29	13.874	1848	1851	1862	rVB	413739	562022	20.82%	1.533%
30	14.116	1885	1892	1905	rVB	1388055	2044393	75.74%	5.578%
31	14.333	1925	1929	1933	rVB2	5739	6761	0.25%	0.018%
32	14.421	1937	1944	1954	rBV	1882534	2695098	99.85%	7.353%
33	14.616	1971	1977	1991	rBV	205976	364150	13.49%	0.994%
34	14.839	2010	2015	2019	rBV3	8222	12211	0.45%	0.033%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023014.D
 Acq On : 06 Oct 2019 05:53
 Operator : JU
 Sample : K5057-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAJ9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

35	15.227	2077	2081	2086	rBV4	5328	8960	0.33%	0.024%
36	15.280	2086	2090	2097	rVB3	4461	7603	0.28%	0.021%
37	15.415	2106	2113	2127	rBV	1701111	2465907	91.36%	6.728%
38	15.527	2127	2132	2140	rBV	261712	358055	13.27%	0.977%
39	15.651	2147	2153	2158	rBV	16318	21946	0.81%	0.060%
40	16.110	2224	2231	2235	rBV	32720	52221	1.93%	0.142%
41	16.192	2242	2245	2249	rVB2	5751	7631	0.28%	0.021%
42	16.310	2261	2265	2269	rVB4	2879	3949	0.15%	0.011%
43	16.410	2278	2282	2289	rBV3	2991	5315	0.20%	0.015%
44	16.492	2291	2296	2298	rBV2	1999	3058	0.11%	0.008%
45	16.939	2367	2372	2373	rBV2	5580	8222	0.30%	0.022%
46	17.092	2396	2398	2401	rVB3	3175	2938	0.11%	0.008%
47	17.162	2403	2410	2418	rBV2	1909858	2699131	100.00%	7.364%
48	17.257	2420	2426	2436	rBV2	1651934	2362545	87.53%	6.446%
49	17.451	2456	2459	2462	rBV3	2589	3462	0.13%	0.009%
50	17.662	2492	2495	2500	rBV4	3883	5165	0.19%	0.014%
51	18.056	2557	2562	2569	rBV	62196	83024	3.08%	0.227%
52	18.127	2569	2574	2578	rVB	7095	10864	0.40%	0.030%
53	18.362	2610	2614	2618	rBV7	5296	8031	0.30%	0.022%
54	18.992	2717	2721	2728	rBV6	6197	16341	0.61%	0.045%
55	19.186	2750	2754	2757	rBV2	13732	20586	0.76%	0.056%
56	19.339	2776	2780	2787	rBV5	19343	30075	1.11%	0.082%
57	19.445	2794	2798	2801	rBV	13735	18131	0.67%	0.049%
58	19.551	2810	2816	2824	rBV	1877276	2495029	92.44%	6.807%
59	21.056	3068	3072	3080	rBV	141234	219534	8.13%	0.599%
60	21.339	3115	3120	3129	rBV	1841748	2314230	85.74%	6.314%
61	21.933	3219	3221	3230	rVB2	80213	90095	3.34%	0.246%
62	22.403	3298	3301	3306	rVB2	104224	128282	4.75%	0.350%
63	22.915	3385	3388	3393	rVB	131209	170558	6.32%	0.465%
64	23.450	3473	3479	3491	rVB	1167612	2408635	89.24%	6.572%
65	23.591	3497	3503	3515	rVB	1241345	2411624	89.35%	6.580%


Sum of corrected areas: 36651946

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM023014.D
Acq On : 06 Oct 2019 05:53
Operator : JU
Sample : K5057-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAJ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

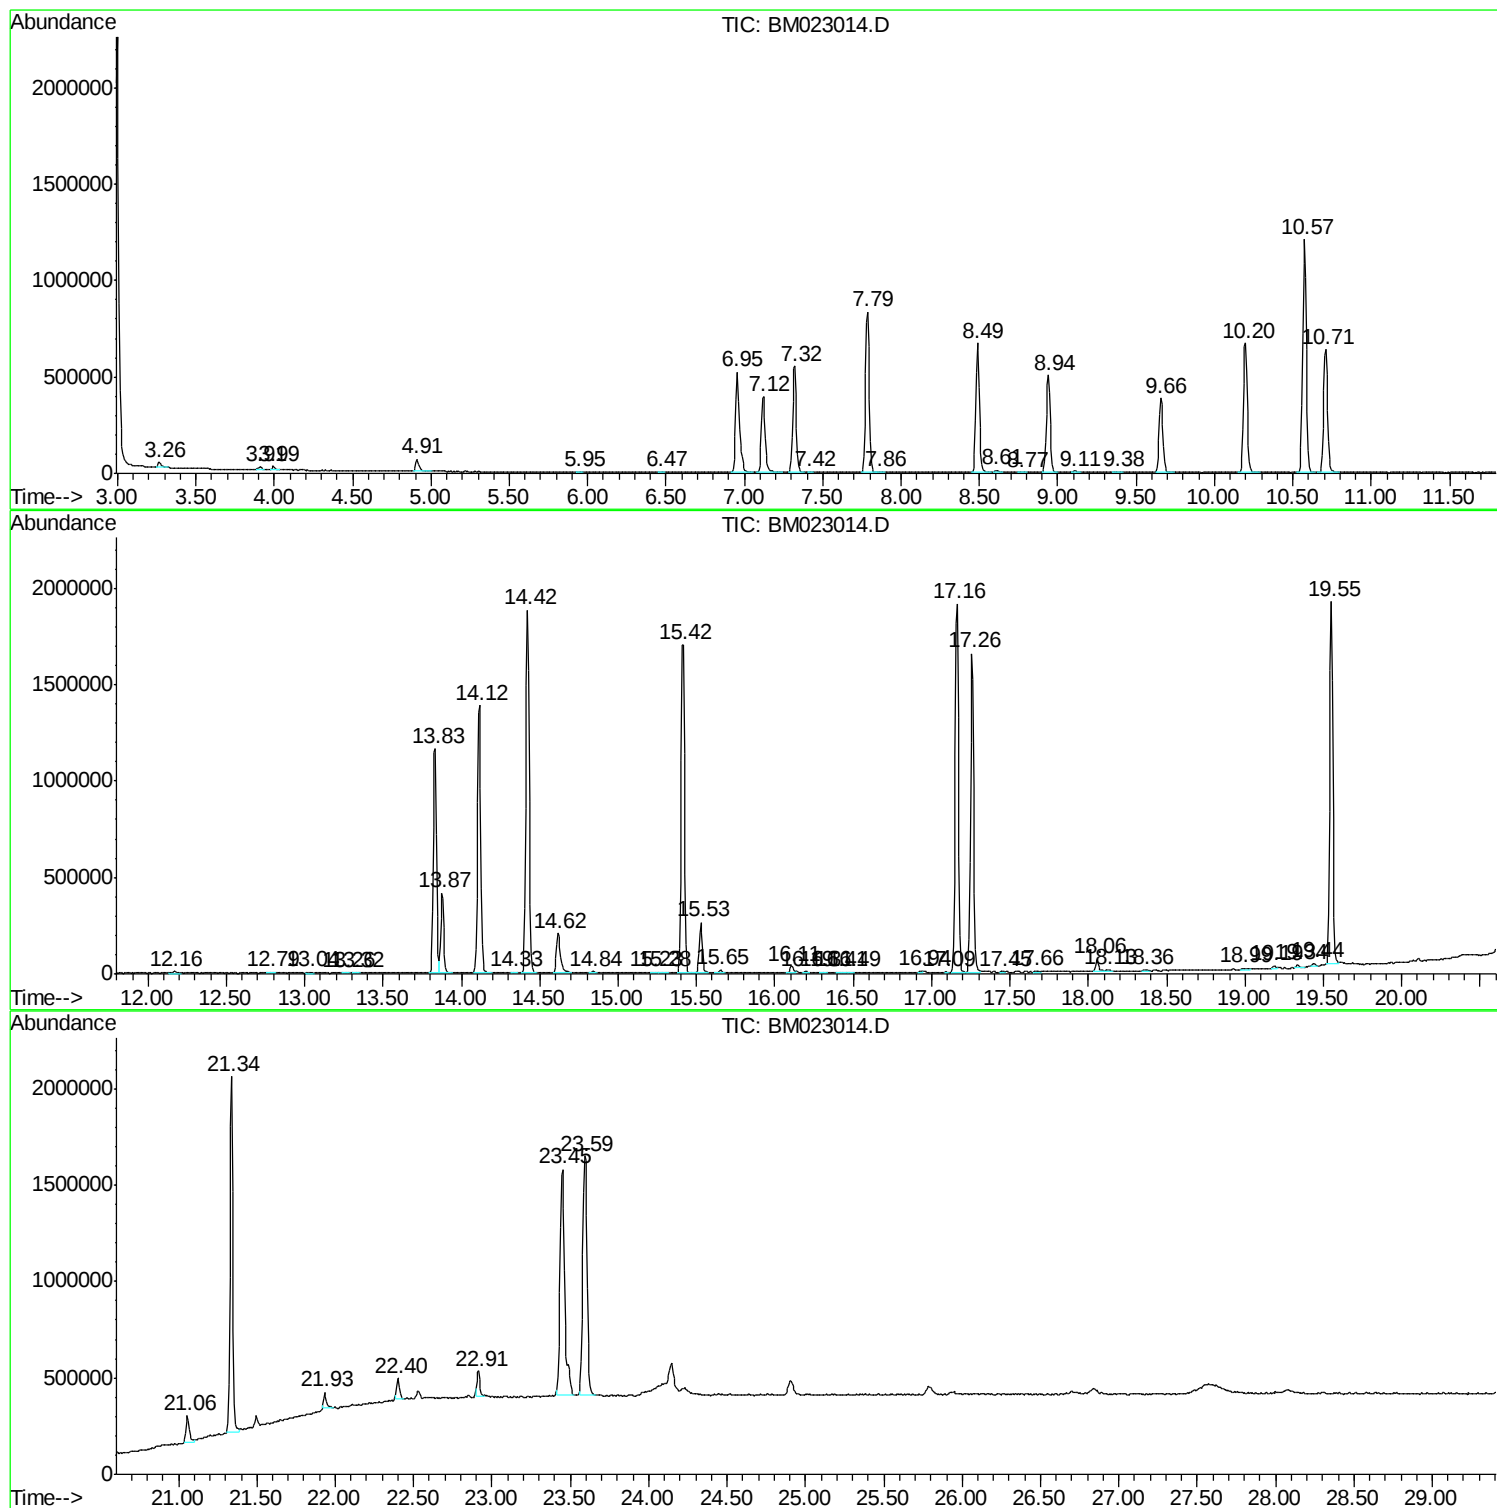

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023014.D
Acq On : 06 Oct 2019 05:53
Operator : JU
Sample : K5057-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAJ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023014.D
Acq On : 06 Oct 2019 05:53
Operator : JU
Sample : K5057-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAJ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc