

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023015.D
 Acq On : 06 Oct 2019 06:29
 Operator : JU
 Sample : K5057-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	45	47	59	rVB	29223	47982	1.73%	0.128%
2	3.904	152	156	164	rVB2	17980	29761	1.07%	0.079%
3	3.993	167	171	176	rBV	11825	16025	0.58%	0.043%
4	4.910	322	327	336	rBV	84864	125426	4.52%	0.334%
5	6.175	539	542	546	rVB4	1988	2820	0.10%	0.008%
6	6.463	587	591	598	rVB4	4513	6500	0.23%	0.017%
7	6.951	668	674	689	rBV2	559820	1009411	36.36%	2.689%
8	7.116	695	702	715	rBV	433654	713716	25.71%	1.901%
9	7.316	729	736	747	rBV	588238	947241	34.12%	2.523%
10	7.416	750	753	758	rVB3	3846	4862	0.18%	0.013%
11	7.787	809	816	825	rBV	880877	1398230	50.36%	3.725%
12	7.857	825	828	833	rVB	6137	8374	0.30%	0.022%
13	8.486	928	935	948	rBV	703828	1139384	41.04%	3.035%
14	8.610	952	956	963	rVB2	10743	19134	0.69%	0.051%
15	8.763	979	982	985	rBV3	2217	2796	0.10%	0.007%
16	8.939	1002	1012	1025	rBV	539753	891035	32.10%	2.374%
17	9.110	1038	1041	1045	rBV4	3109	3527	0.13%	0.009%
18	9.381	1082	1087	1094	rVB2	6403	10902	0.39%	0.029%
19	9.657	1127	1134	1147	rBV	411066	668276	24.07%	1.780%
20	10.198	1219	1226	1242	rBV	704019	1180090	42.51%	3.144%
21	10.575	1282	1290	1298	rBV	1285463	2106949	75.89%	5.613%
22	10.710	1305	1313	1326	rBV	665132	1175113	42.33%	3.130%
23	12.163	1553	1560	1568	rVB2	8890	15973	0.58%	0.043%
24	12.786	1663	1666	1670	rVB3	2118	2923	0.11%	0.008%
25	13.027	1705	1707	1715	rBV3	2978	4505	0.16%	0.012%
26	13.257	1743	1746	1750	rBV4	2587	3631	0.13%	0.010%
27	13.469	1779	1782	1789	rVB3	2509	3936	0.14%	0.010%
28	13.827	1837	1843	1848	rBV	1170378	1671953	60.22%	4.454%
29	13.874	1848	1851	1860	rVV	457858	615429	22.17%	1.639%
30	14.110	1885	1891	1901	rBV	1405548	2090313	75.29%	5.568%
31	14.327	1926	1928	1934	rVB2	2605	3470	0.12%	0.009%
32	14.421	1937	1944	1953	rBV	1910247	2776219	100.00%	7.396%
33	14.621	1972	1978	1986	rBV	56508	106006	3.82%	0.282%
34	14.845	2011	2016	2019	rBV4	7389	9775	0.35%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023015.D
 Acq On : 06 Oct 2019 06:29
 Operator : JU
 Sample : K5057-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

35	15.227	2078	2081	2086	rBV3	3661	5465	0.20%	0.015%
36	15.280	2086	2090	2093	rVB4	3789	4755	0.17%	0.013%
37	15.410	2106	2112	2127	rVB	1698164	2455507	88.45%	6.541%
38	15.527	2127	2132	2138	rBV	79774	112236	4.04%	0.299%
39	15.651	2149	2153	2158	rBV	15706	19882	0.72%	0.053%
40	16.139	2233	2236	2240	rVV3	3570	4414	0.16%	0.012%
41	16.192	2242	2245	2250	rVB3	6439	7167	0.26%	0.019%
42	16.945	2367	2373	2377	rBV3	6865	12156	0.44%	0.032%
43	17.092	2396	2398	2402	rVB3	2653	3136	0.11%	0.008%
44	17.162	2403	2410	2420	rVV	1897610	2711485	97.67%	7.223%
45	17.256	2420	2426	2440	rVV	1707860	2358066	84.94%	6.282%
46	17.345	2440	2441	2445	rVB2	2882	2845	0.10%	0.008%
47	17.668	2490	2496	2499	rBV5	2423	3187	0.11%	0.008%
48	18.056	2557	2562	2567	rBV	50984	70359	2.53%	0.187%
49	18.362	2610	2614	2616	rVB3	4085	4844	0.17%	0.013%
50	18.992	2719	2721	2725	rVB3	8071	7897	0.28%	0.021%
51	19.186	2750	2754	2758	rBV2	16227	22747	0.82%	0.061%
52	19.339	2776	2780	2783	rBV3	19350	22296	0.80%	0.059%
53	19.439	2794	2797	2801	rVB	10733	13079	0.47%	0.035%
54	19.550	2810	2816	2823	rBV	1882643	2472178	89.05%	6.586%
55	20.103	2907	2910	2915	rBV	25808	30204	1.09%	0.080%
56	20.597	2992	2994	2998	rVB	32366	30850	1.11%	0.082%
57	21.062	3069	3073	3079	rBV2	91897	130872	4.71%	0.349%
58	21.339	3115	3120	3126	rBV	1999161	2458744	88.56%	6.550%
59	21.497	3144	3147	3152	rVB2	88850	86827	3.13%	0.231%
60	21.933	3219	3221	3226	rVB	102872	109335	3.94%	0.291%
61	22.403	3298	3301	3307	rVB	125166	151847	5.47%	0.405%
62	22.915	3385	3388	3394	rVB	143038	191564	6.90%	0.510%
63	23.450	3473	3479	3493	rVB	1270097	2607218	93.91%	6.945%
64	23.597	3497	3504	3515	rVB2	1357720	2615759	94.22%	6.968%


Sum of corrected areas: 37538608

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM023015.D
Acq On : 06 Oct 2019 06:29
Operator : JU
Sample : K5057-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAK2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

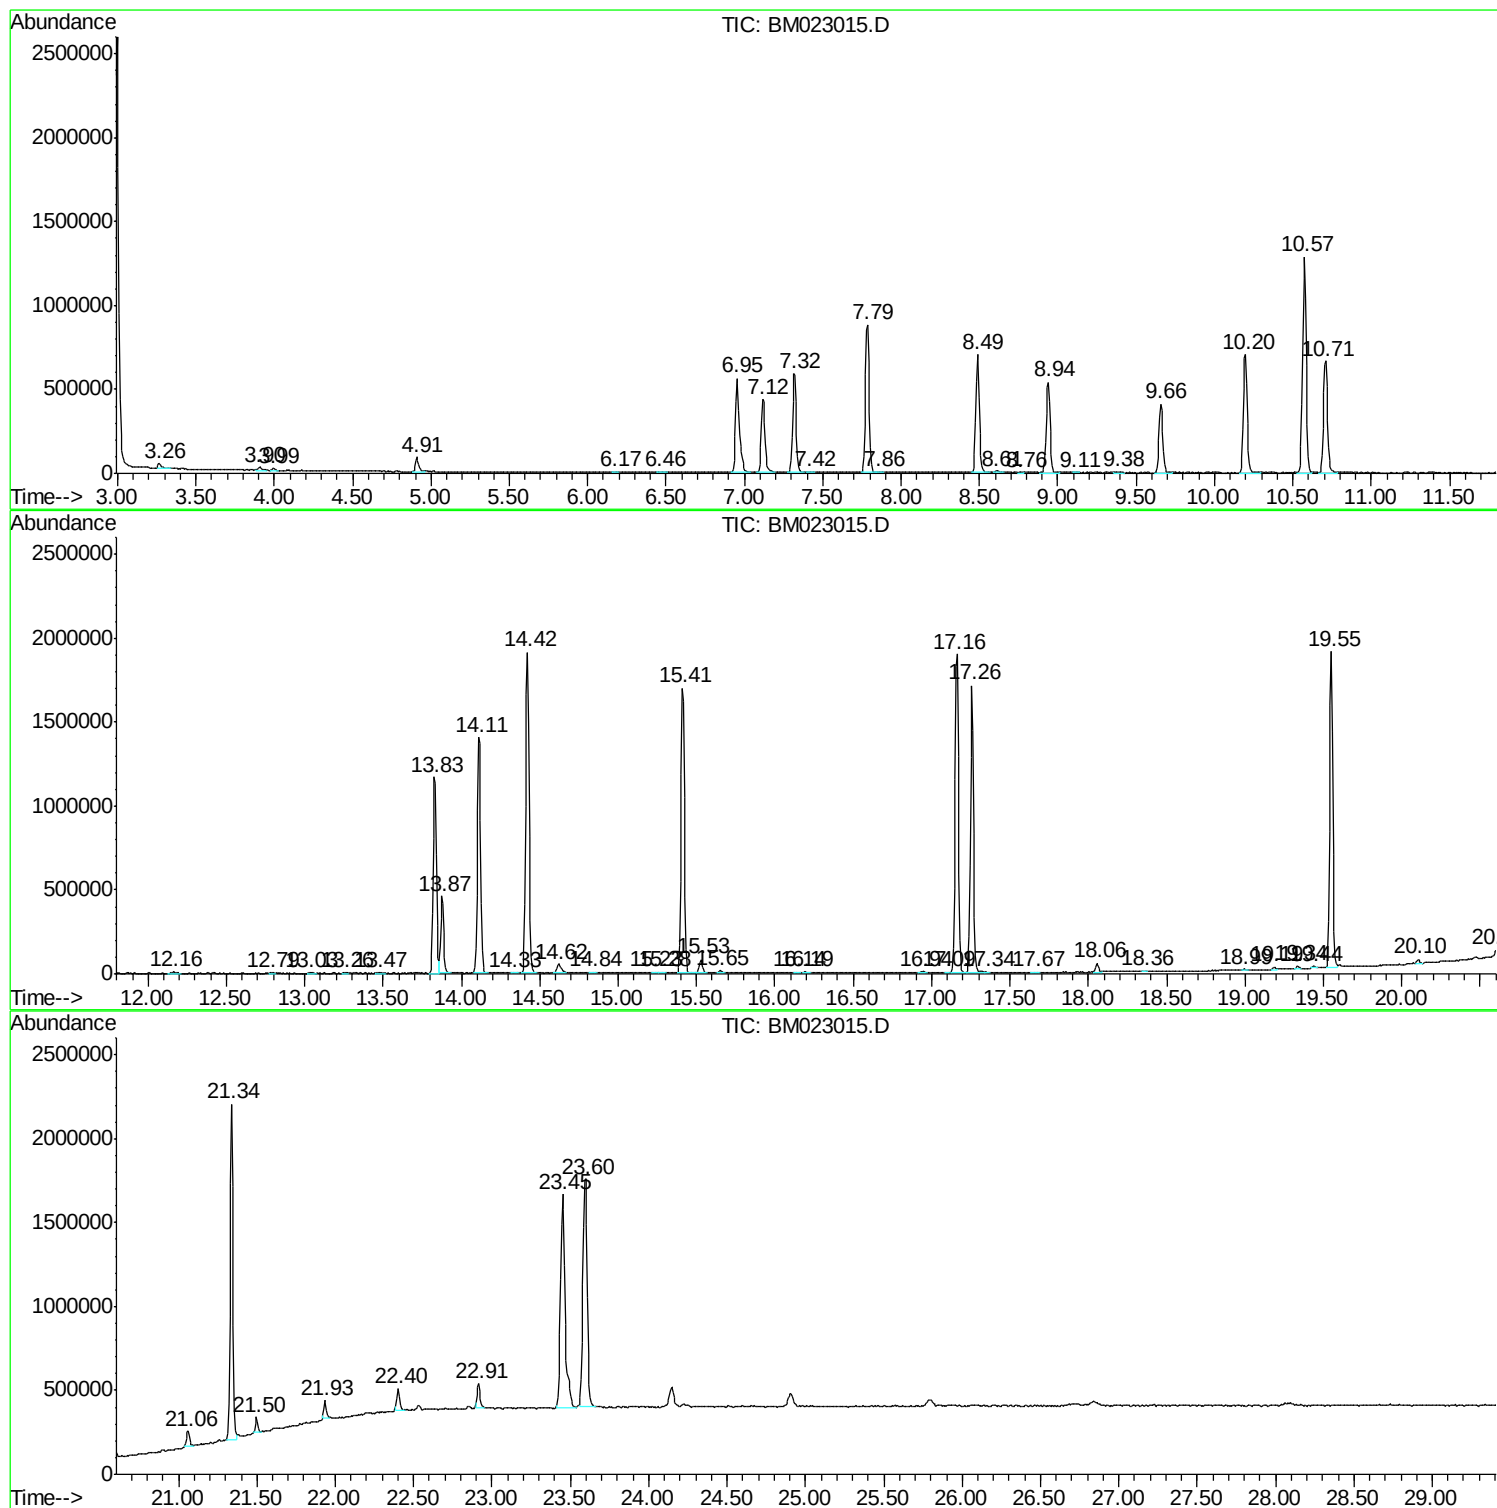

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023015.D
Acq On : 06 Oct 2019 06:29
Operator : JU
Sample : K5057-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAK2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023015.D
Acq On : 06 Oct 2019 06:29
Operator : JU
Sample : K5057-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAK2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc