

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023024.D
 Acq On : 06 Oct 2019 13:04
 Operator : JU
 Sample : K5057-18
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	45	47	58	rVB	19680	28575	0.79%	0.070%
2	3.905	152	156	165	rVV2	13952	24132	0.66%	0.059%
3	3.993	167	171	175	rVB	12707	17813	0.49%	0.044%
4	4.910	322	327	340	rBV	51476	91084	2.51%	0.223%
5	6.463	587	591	596	rBV5	4206	6869	0.19%	0.017%
6	6.951	667	674	690	rBV2	390223	699017	19.23%	1.709%
7	7.116	694	702	711	rBV	370538	598643	16.47%	1.463%
8	7.316	729	736	750	rVB	499040	783010	21.54%	1.914%
9	7.781	808	815	825	rBV	890670	1413322	38.88%	3.455%
10	7.857	825	828	833	rVB	6094	8896	0.24%	0.022%
11	8.487	928	935	948	rBV	590866	935737	25.74%	2.287%
12	8.610	951	956	963	rVB2	9909	19522	0.54%	0.048%
13	8.934	1004	1011	1020	rBV	471704	769291	21.16%	1.880%
14	9.110	1034	1041	1045	rVB6	3934	5757	0.16%	0.014%
15	9.381	1083	1087	1092	rVB	5410	7513	0.21%	0.018%
16	9.657	1127	1134	1146	rBV	351113	571615	15.72%	1.397%
17	10.192	1218	1225	1235	rBV	601786	995342	27.38%	2.433%
18	10.575	1282	1290	1301	rVB	1269242	2168335	59.64%	5.300%
19	10.704	1305	1312	1326	rBV	605371	1059662	29.15%	2.590%
20	11.322	1414	1417	1423	rBV3	2057	3941	0.11%	0.010%
21	12.163	1552	1560	1566	rBV3	7998	14270	0.39%	0.035%
22	13.033	1704	1708	1712	rVB3	4117	5983	0.16%	0.015%
23	13.322	1751	1757	1763	rBV	81513	120830	3.32%	0.295%
24	13.827	1837	1843	1847	rBV	1253647	1700381	46.77%	4.156%
25	13.874	1847	1851	1864	rVB	793881	1098173	30.21%	2.684%
26	14.110	1884	1891	1904	rBV	1393107	2029956	55.84%	4.962%
27	14.327	1924	1928	1931	rVB2	2609	3875	0.11%	0.009%
28	14.421	1937	1944	1956	rBV	2138824	3147510	86.58%	7.694%
29	14.504	1956	1958	1966	rVB4	2353	4665	0.13%	0.011%
30	14.633	1973	1980	1989	rBV3	7238	17475	0.48%	0.043%
31	14.839	2008	2015	2018	rBV3	5081	7000	0.19%	0.017%
32	15.227	2076	2081	2087	rBV3	5063	8546	0.24%	0.021%
33	15.274	2087	2089	2095	rVB2	4301	5992	0.16%	0.015%
34	15.410	2106	2112	2122	rBV	1849303	2576676	70.88%	6.298%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
 Data File : BM023024.D
 Acq On : 06 Oct 2019 13:04
 Operator : JU
 Sample : K5057-18
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAK6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Title : SVOA CALIBRATION

35	15.527	2127	2132	2139	rBV4	19012	34334	0.94%	0.084%
36	15.651	2148	2153	2157	rBV2	15805	21465	0.59%	0.052%
37	16.139	2233	2236	2241	rBV2	7582	10724	0.29%	0.026%
38	16.192	2241	2245	2250	rVB4	5408	8686	0.24%	0.021%
39	16.410	2278	2282	2289	rBV8	3287	6868	0.19%	0.017%
40	16.945	2366	2373	2377	rBV4	6539	13797	0.38%	0.034%
41	17.157	2403	2409	2419	rBV2	2514930	3635471	100.00%	8.887%
42	17.257	2419	2426	2438	rVV	2047046	2829986	77.84%	6.918%
43	17.351	2439	2442	2445	rVV3	9828	11974	0.33%	0.029%
44	17.392	2445	2449	2453	rVV	6721	10553	0.29%	0.026%
45	17.451	2455	2459	2463	rVB3	3765	6103	0.17%	0.015%
46	17.551	2470	2476	2483	rBV4	9677	15404	0.42%	0.038%
47	17.662	2494	2495	2499	rVB3	3668	3732	0.10%	0.009%
48	17.721	2499	2505	2508	rBV3	2084	5144	0.14%	0.013%
49	18.051	2557	2561	2570	rBV	48282	69635	1.92%	0.170%
50	18.121	2570	2573	2579	rVB	5763	9370	0.26%	0.023%
51	18.362	2610	2614	2617	rBV5	4871	7941	0.22%	0.019%
52	18.921	2704	2709	2714	rBV3	18136	33773	0.93%	0.083%
53	18.992	2718	2721	2724	rVV4	6876	10500	0.29%	0.026%
54	19.186	2750	2754	2757	rBV	20638	25307	0.70%	0.062%
55	19.339	2776	2780	2783	rBV4	17309	23626	0.65%	0.058%
56	19.439	2794	2797	2801	rVB	16329	19949	0.55%	0.049%
57	19.551	2810	2816	2823	rBV	2407491	3208286	88.25%	7.842%
58	20.103	2907	2910	2913	rBV	25906	28373	0.78%	0.069%
59	20.598	2992	2994	2998	rVB	35970	35194	0.97%	0.086%
60	21.056	3069	3072	3080	rBV	95545	136587	3.76%	0.334%
61	21.339	3115	3120	3128	rBV	2654260	3330186	91.60%	8.140%
62	21.497	3144	3147	3151	rBV	85392	95420	2.62%	0.233%
63	21.933	3218	3221	3230	rBV	109666	137208	3.77%	0.335%
64	22.397	3297	3300	3306	rVB	146420	186265	5.12%	0.455%
65	22.909	3384	3387	3392	rVB	155951	220139	6.06%	0.538%
66	23.450	3472	3479	3492	rVB	1308959	2740234	75.37%	6.698%
67	23.591	3497	3503	3514	rVB	1664825	3027728	83.28%	7.401%


Sum of corrected areas: 40909370

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100319\
Data File : BM023024.D
Acq On : 06 Oct 2019 13:04
Operator : JU
Sample : K5057-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DBAK6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

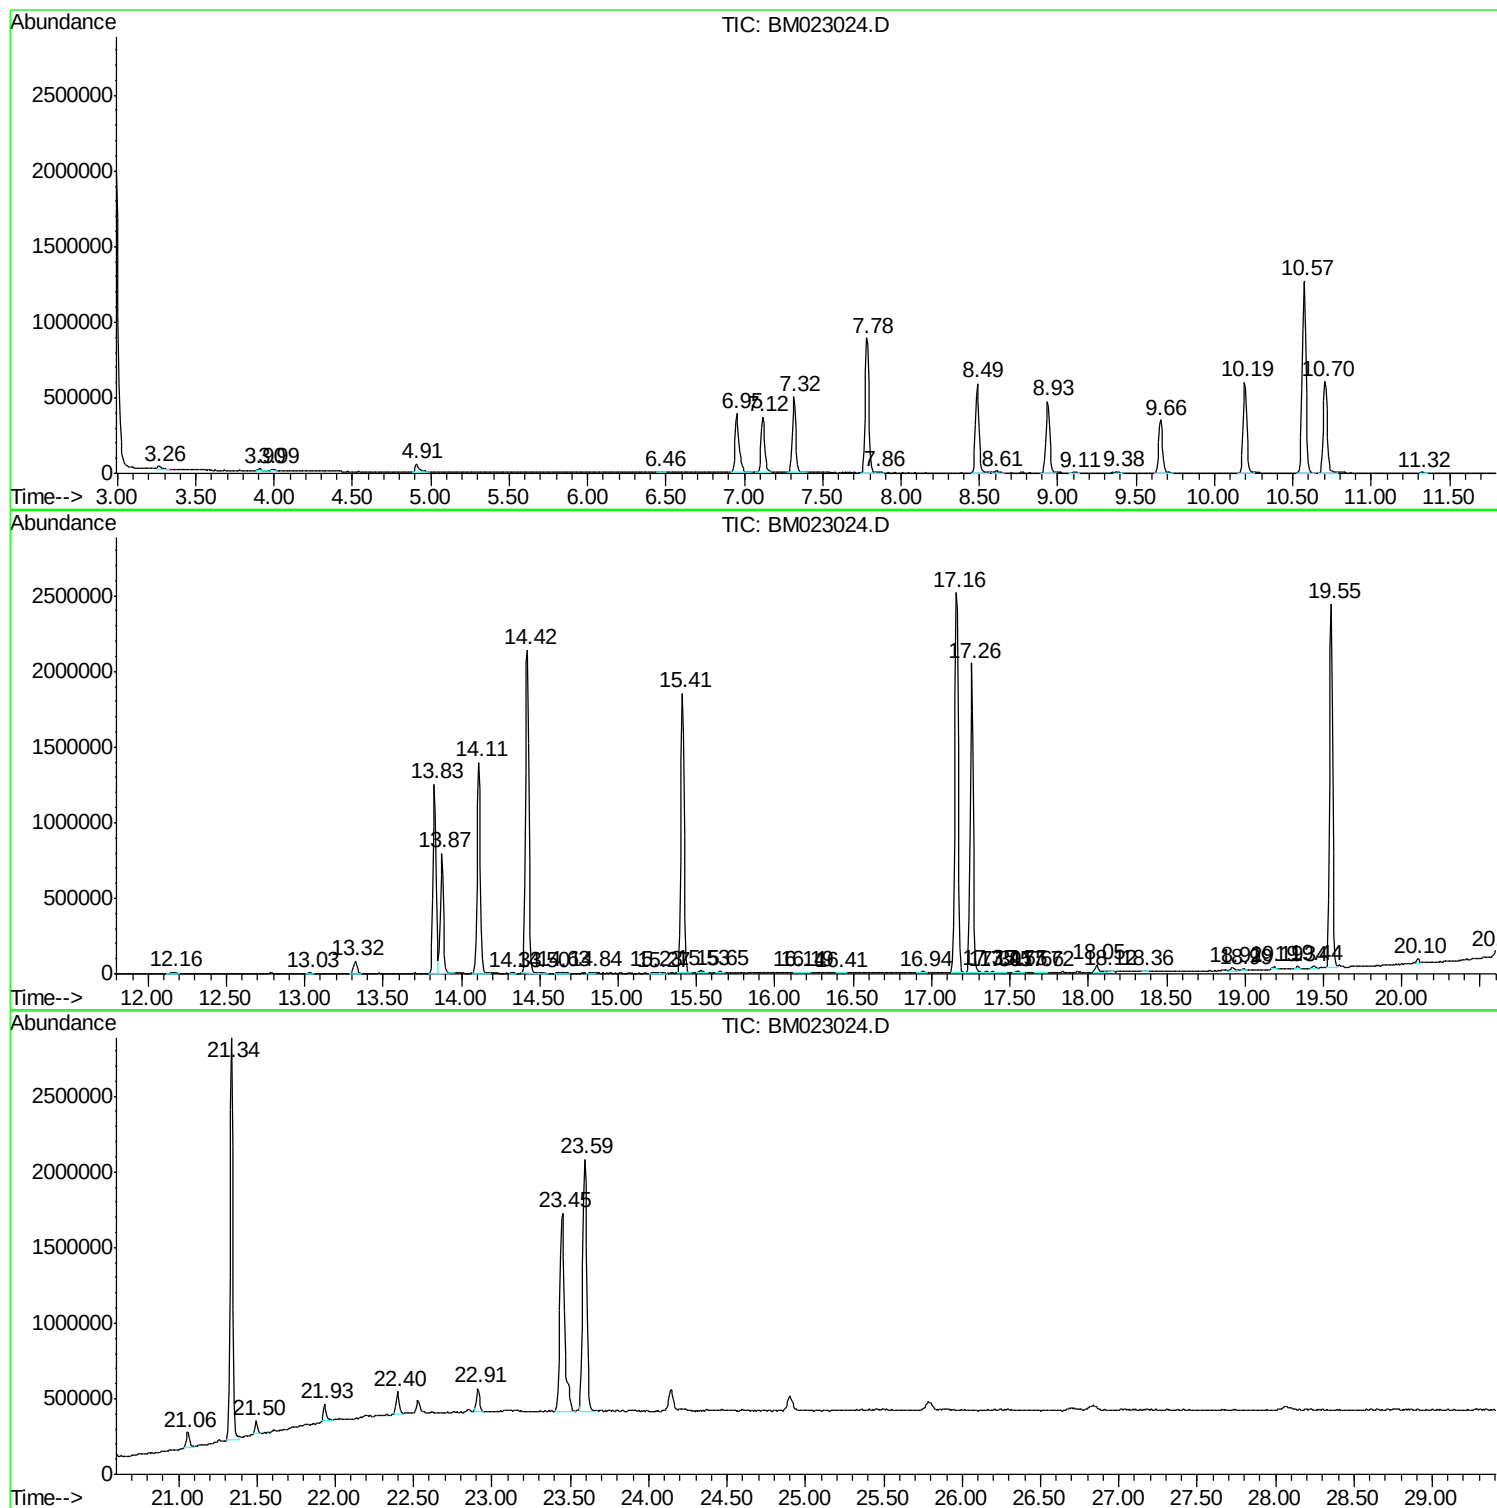

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023024.D
Acq On : 06 Oct 2019 13:04
Operator : JU
Sample : K5057-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAK6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100319\
Data File : BM023024.D
Acq On : 06 Oct 2019 13:04
Operator : JU
Sample : K5057-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAK6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc