



2-Nitrophenol

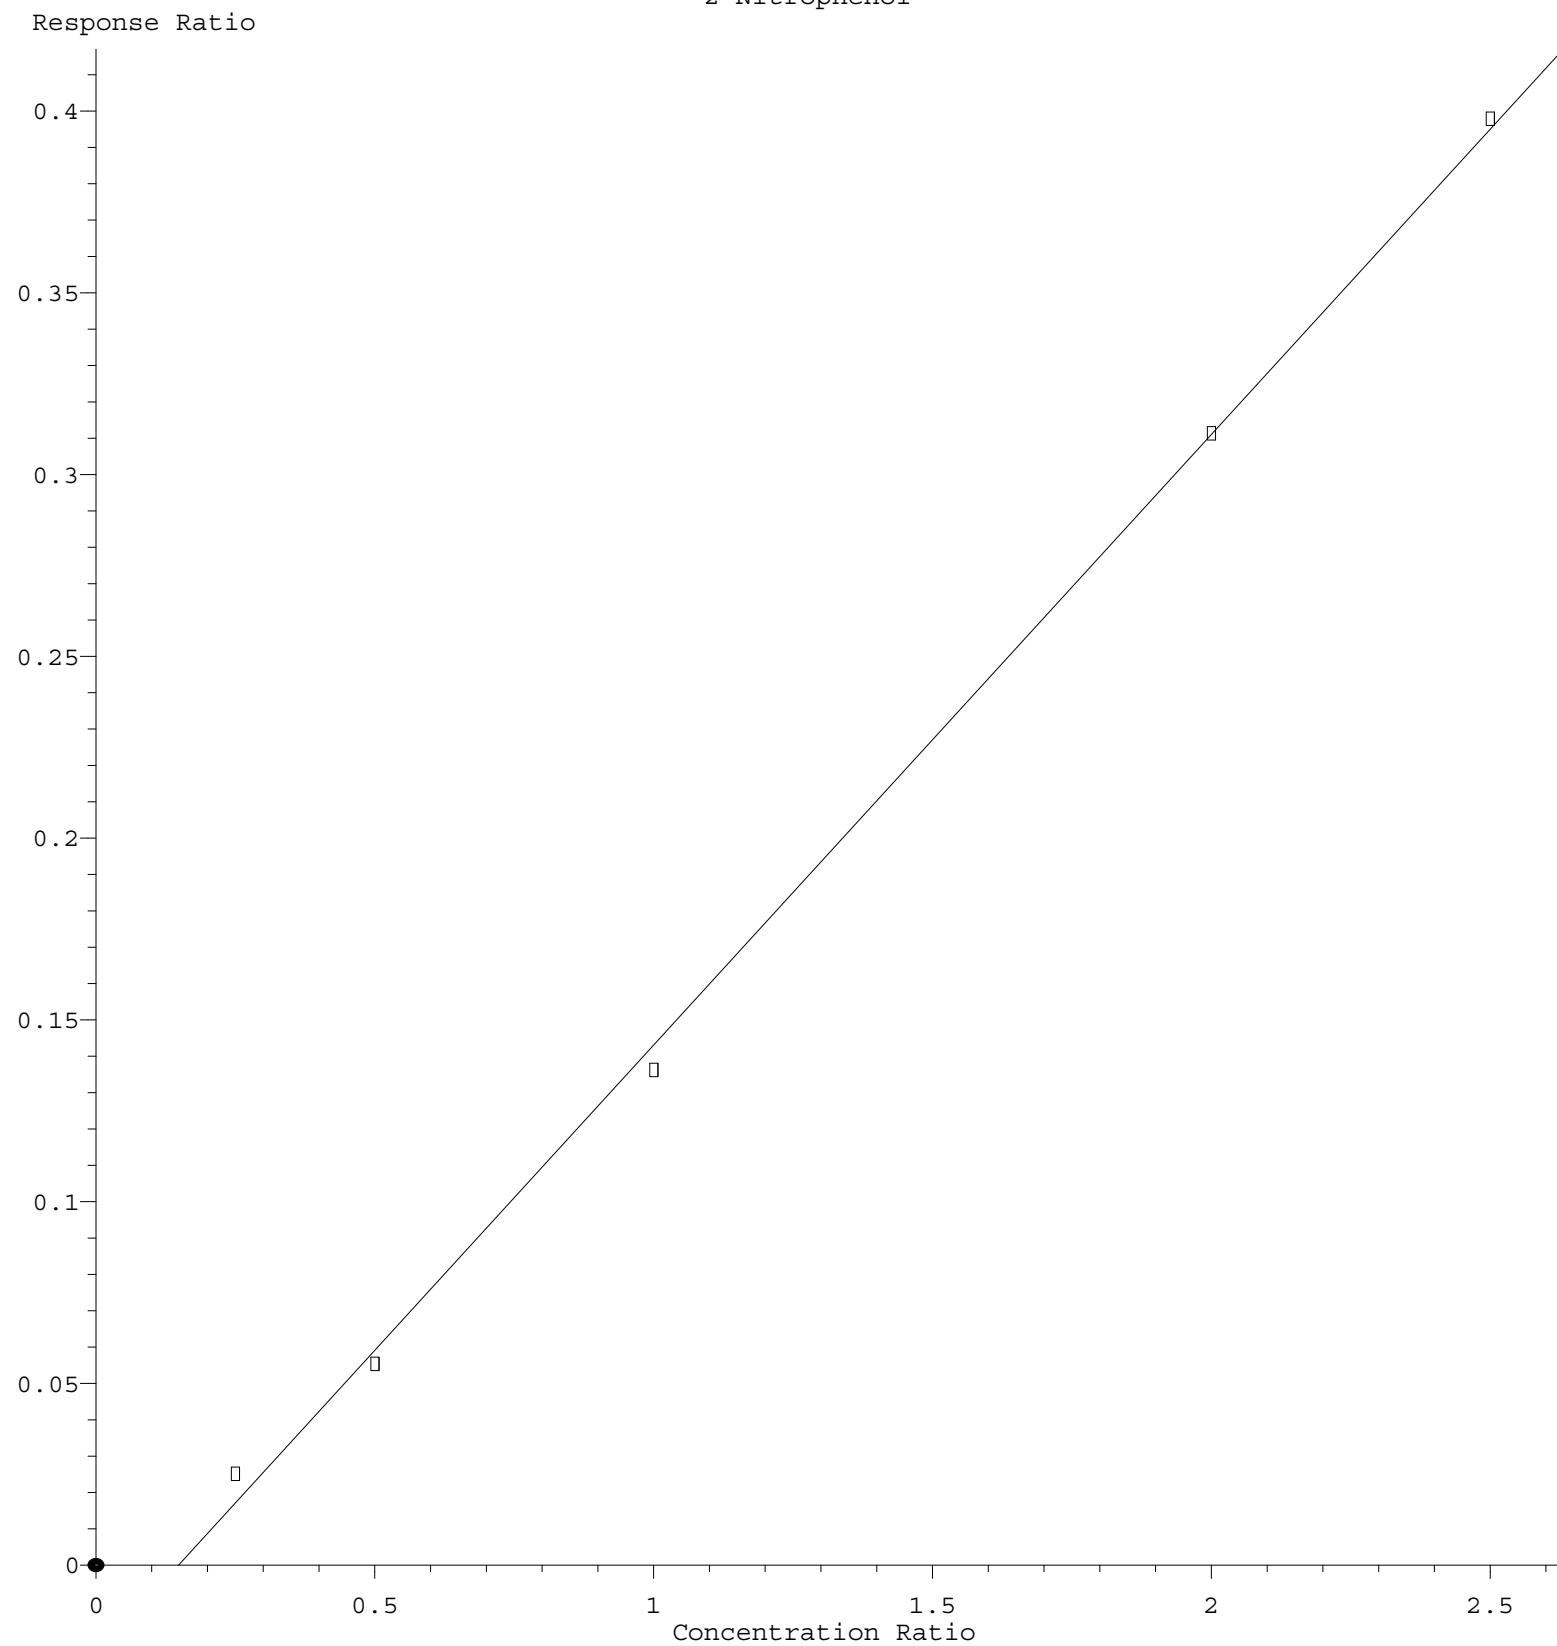

Response = $1.680 \times 10^{-1} \times \text{Amt} - 2.485 \times 10^{-2}$
 Coef of Det (r^2) = 0.998737 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M
 Calibration Table Last Updated: Tue Oct 04 03:17:03 2022

Di-n-octyl phthalate

Response Ratio

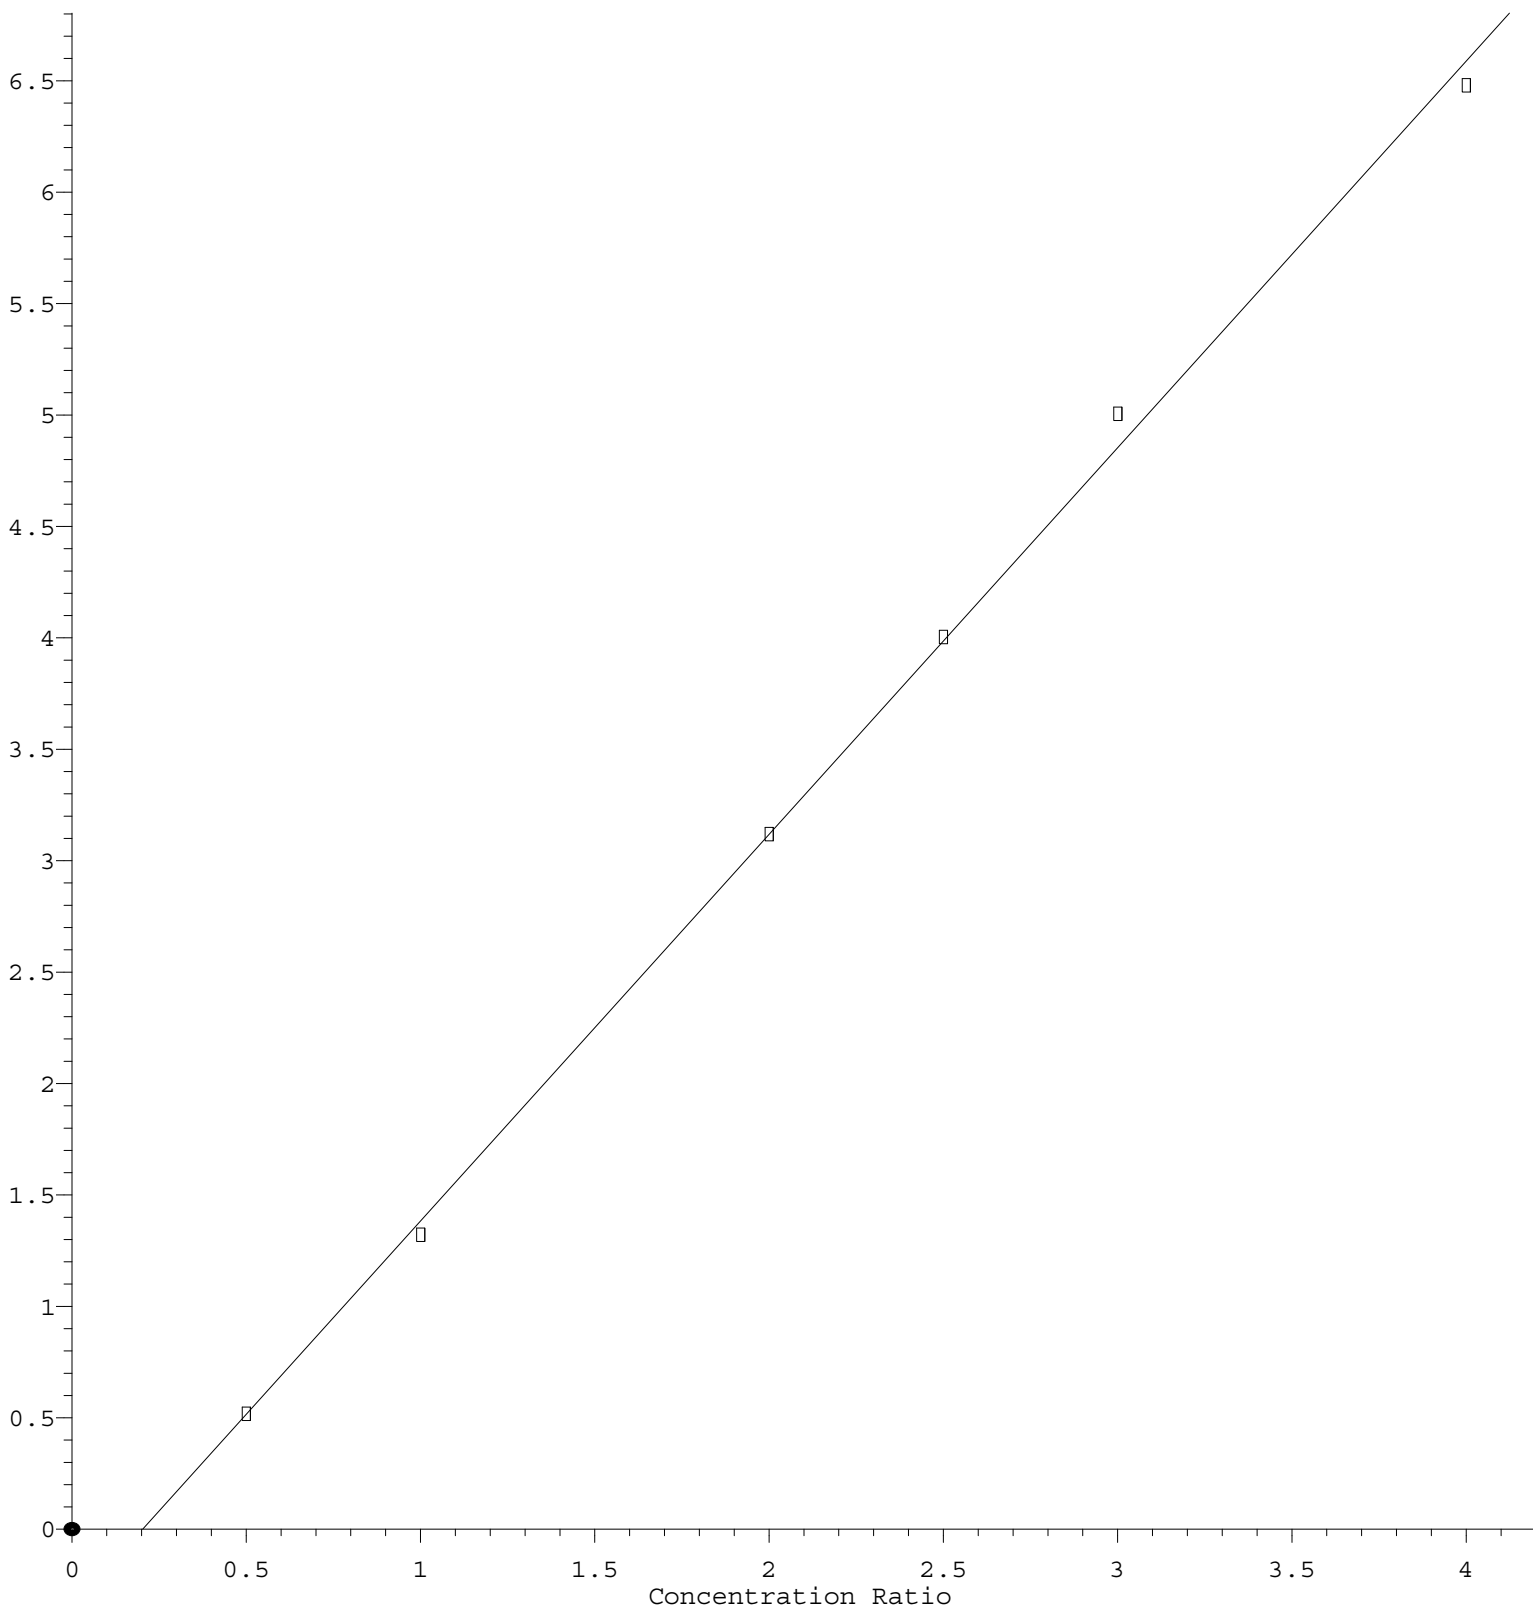

$$\text{Response} = 1.735\text{e}+000 * \text{Amt} - 3.519\text{e}-001$$


Coef of Det (r^2) = 0.998443 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M

Calibration Table Last Updated: Tue Oct 04 03:17:03 2022

Bis(2-ethylhexyl)phthalate

Response Ratio

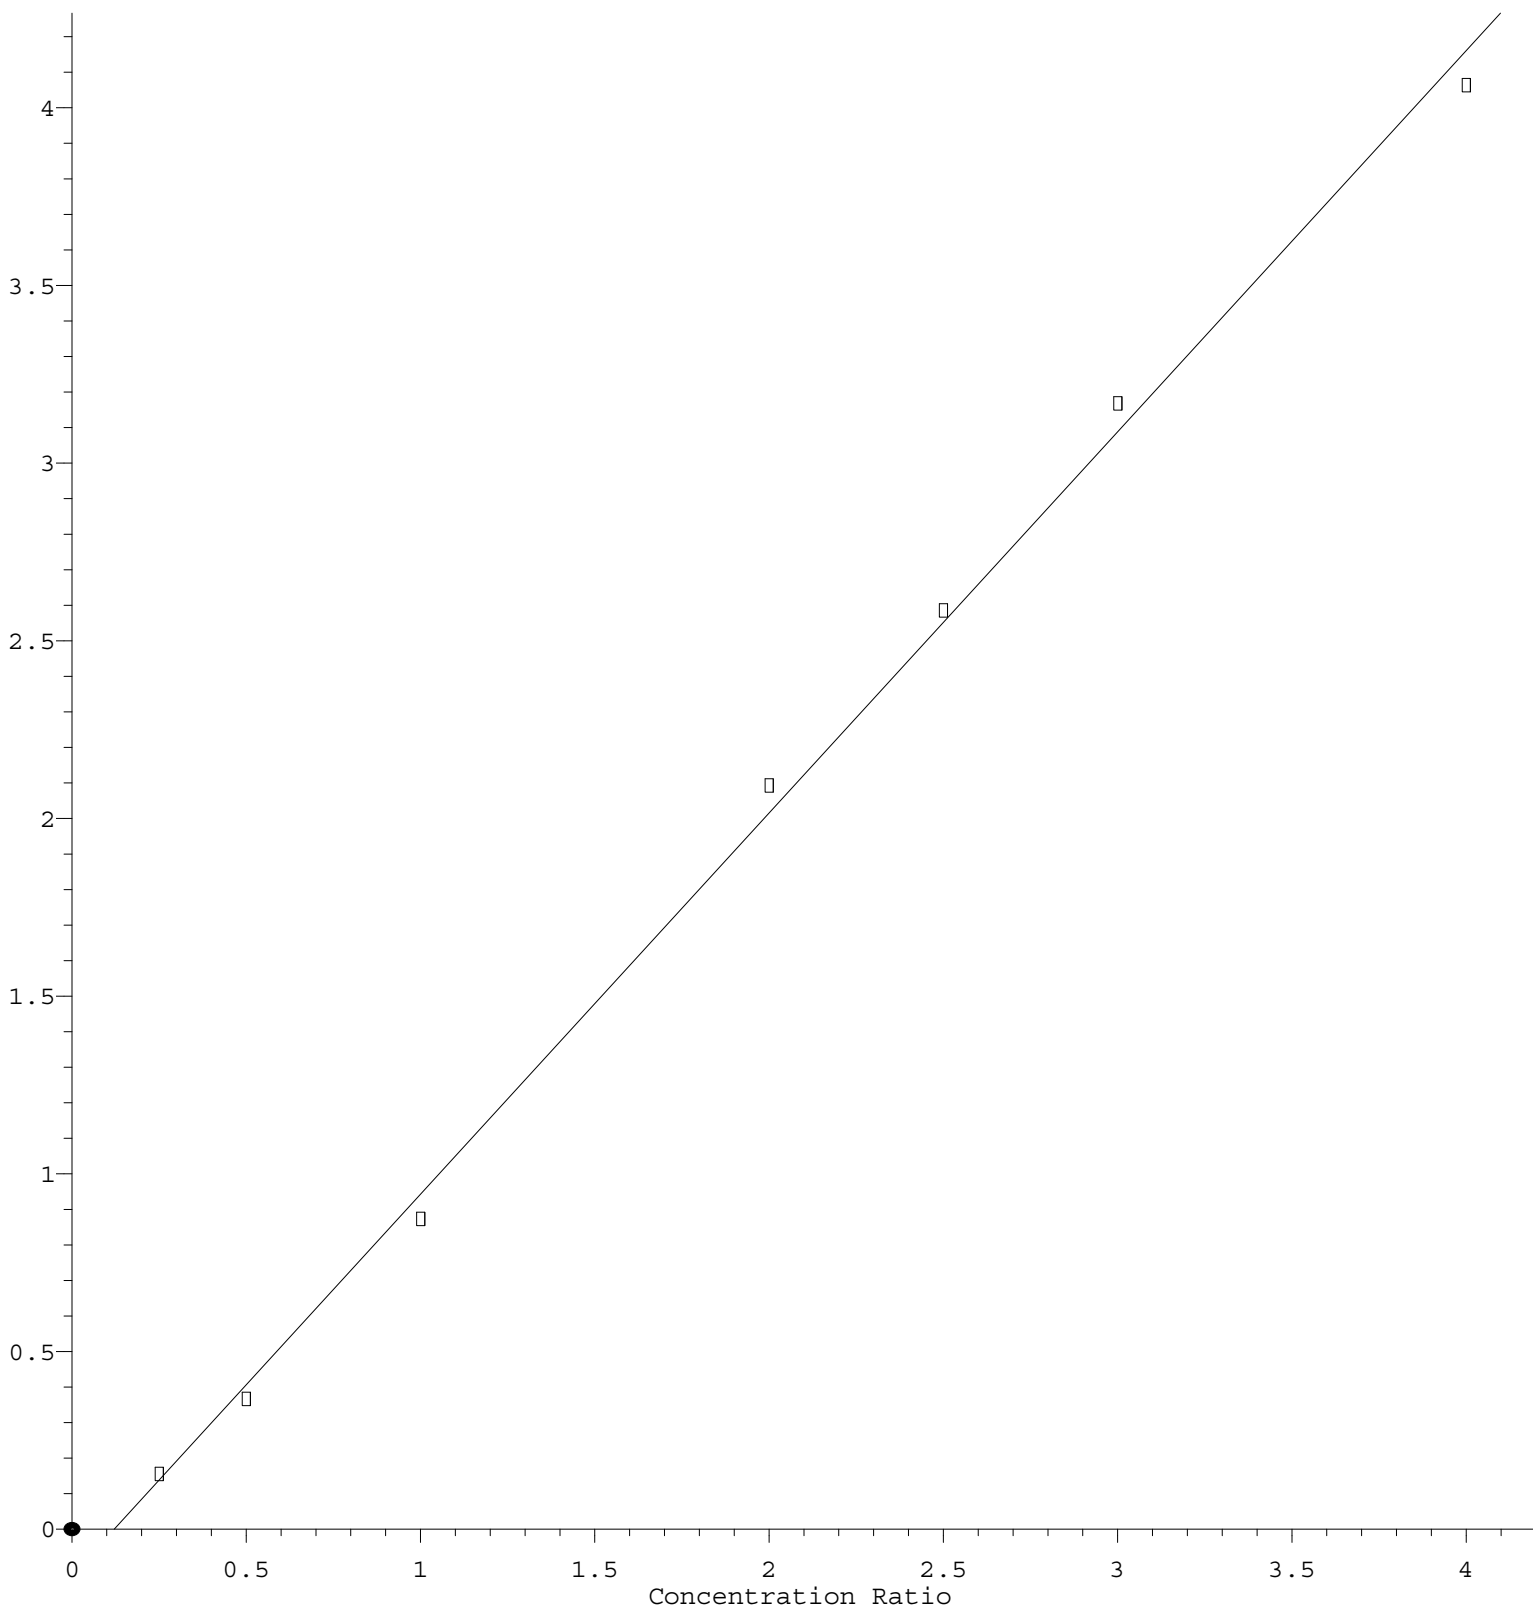

$$\text{Response} = 1.073\text{e}+000 * \text{Amt} - 1.300\text{e}-001$$


Coef of Det (r^2) = 0.997758 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M

Calibration Table Last Updated: Tue Oct 04 03:17:03 2022

Butylbenzylphthalate

Response Ratio

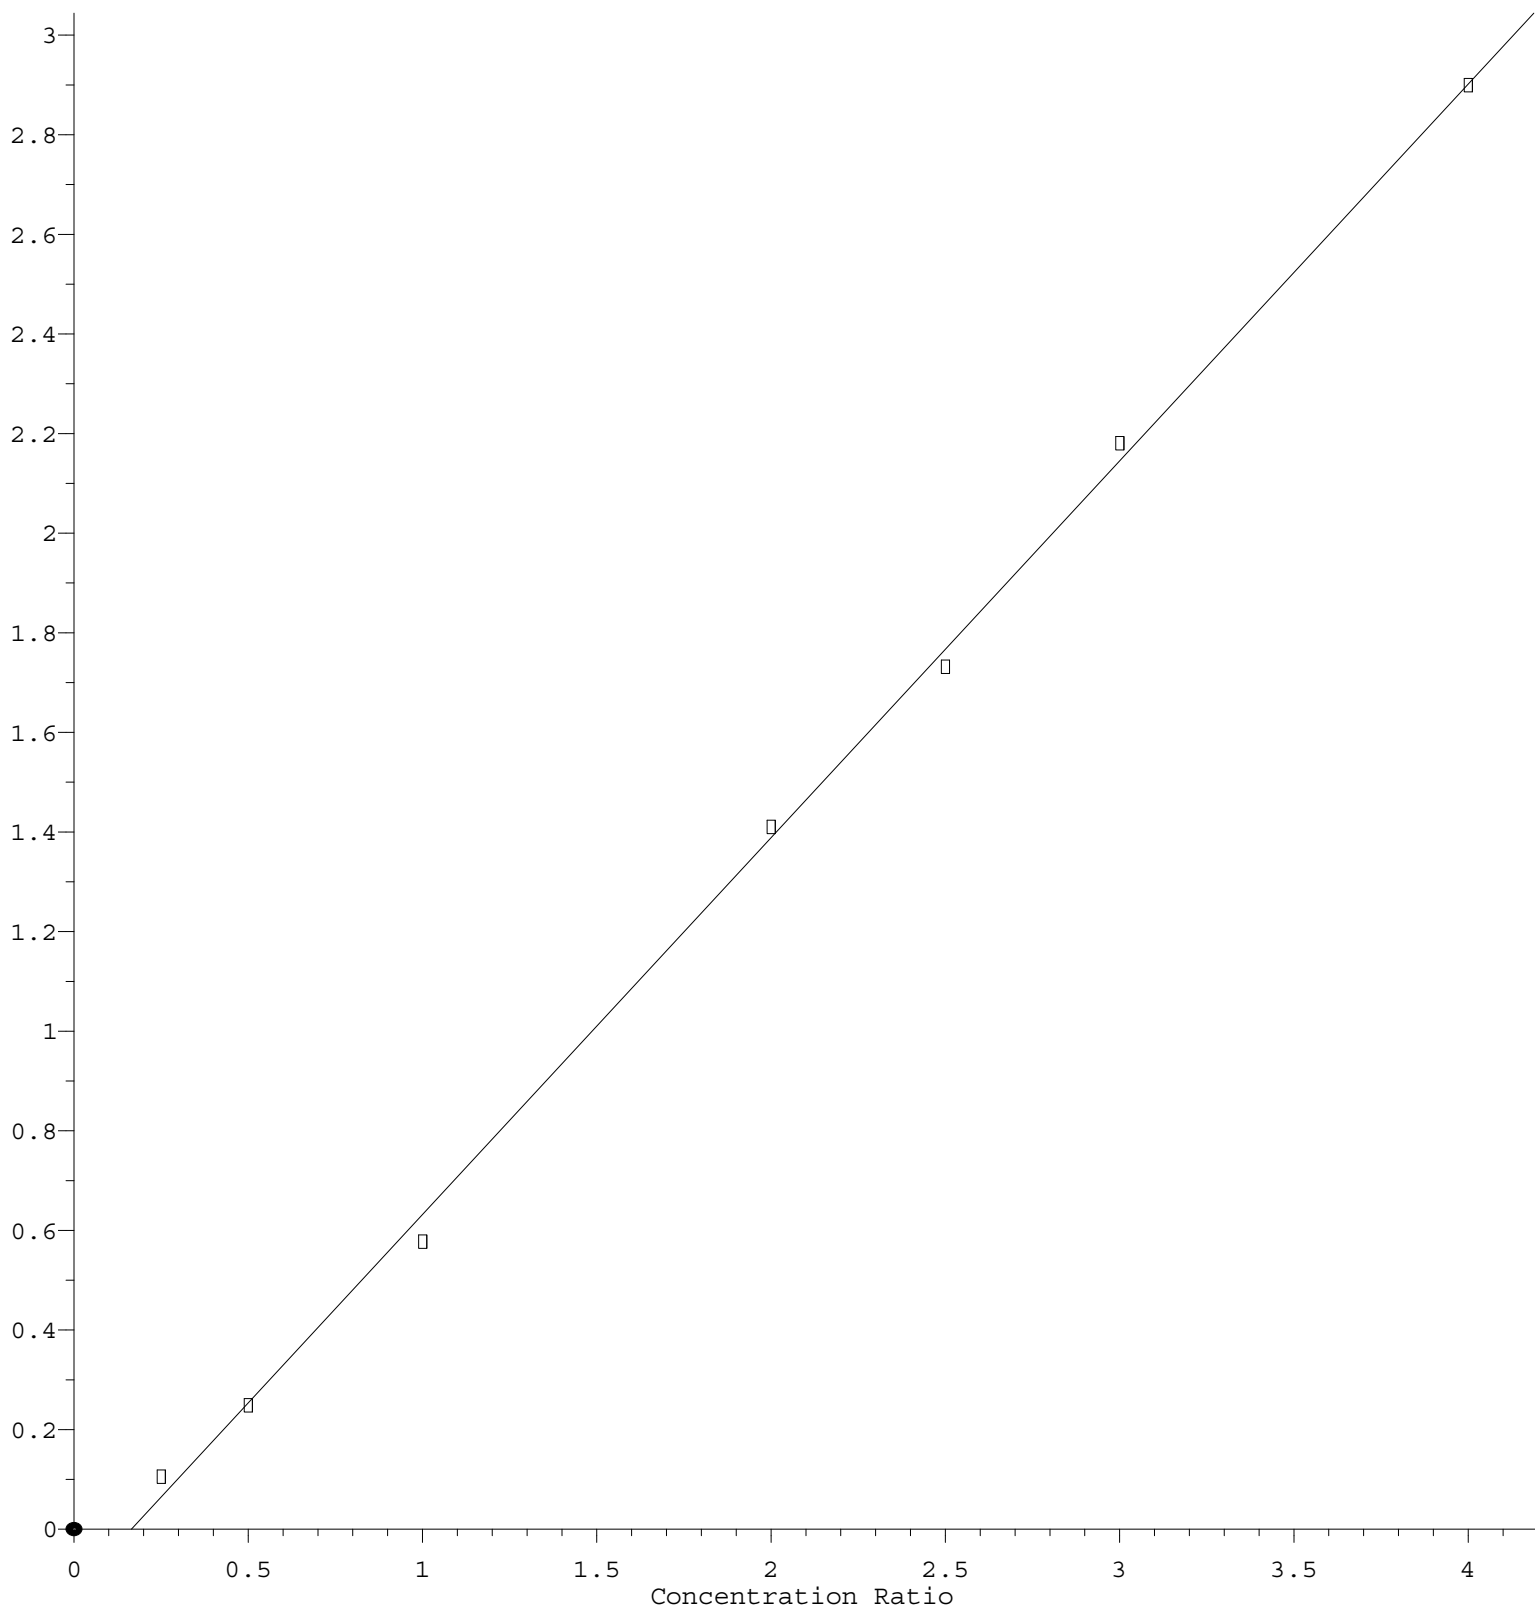


$$\text{Response} = 7.569\text{e-}001 * \text{Amt} - 1.251\text{e-}001$$

Coef of Det (r^2) = 0.998841 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M

Calibration Table Last Updated: Tue Oct 04 03:17:03 2022


4,6-Dinitro-2-methylphenol

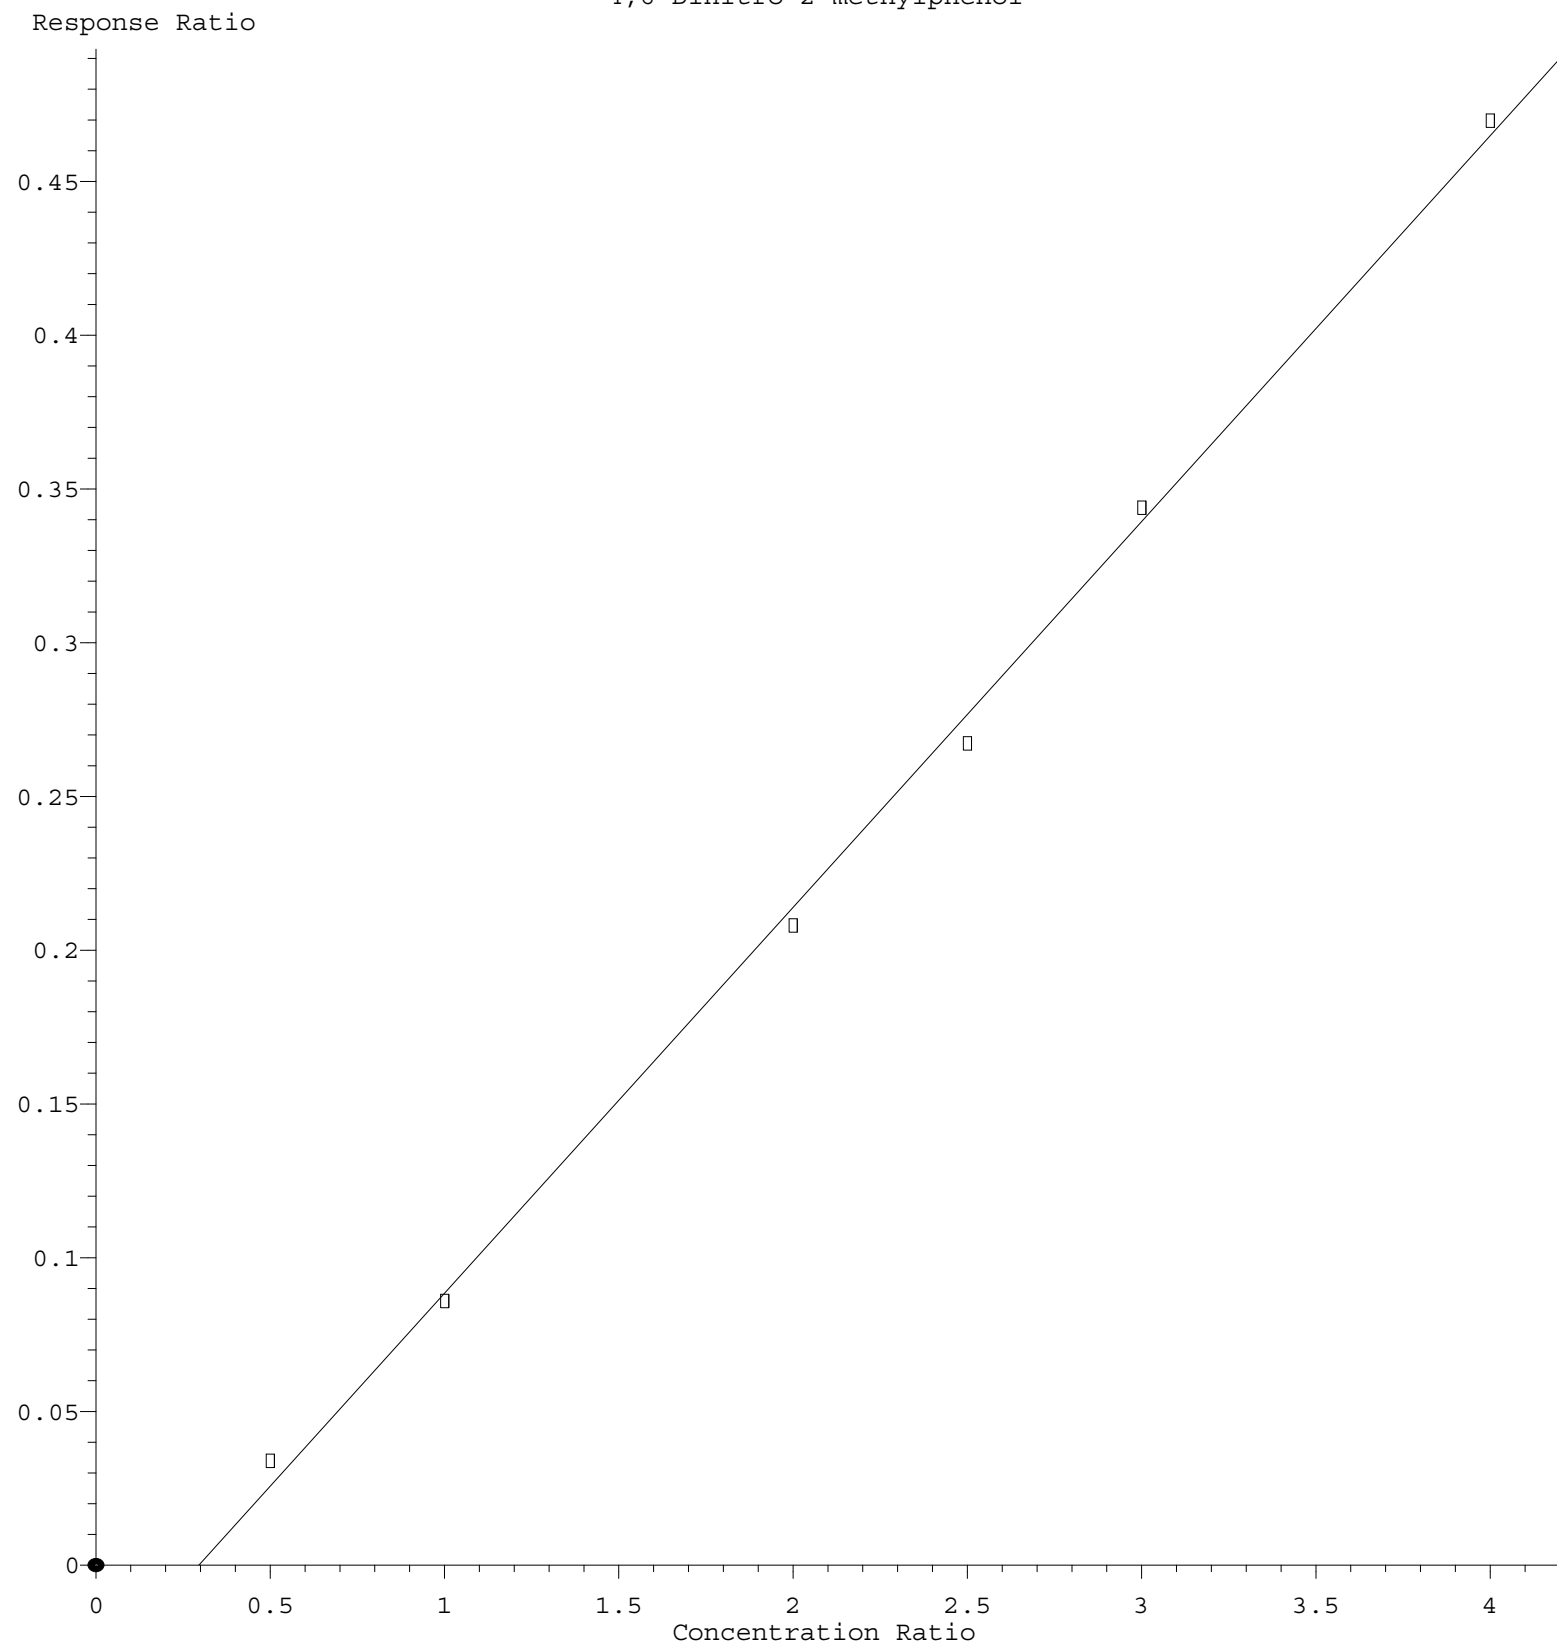

Response = 1.255e-001 * Amt - 3.704e-002
Coef of Det (r^2) = 0.998164 Curve Fit: Linear
Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M
Calibration Table Last Updated: Tue Oct 04 03:17:03 2022

4-Nitroaniline

Response Ratio

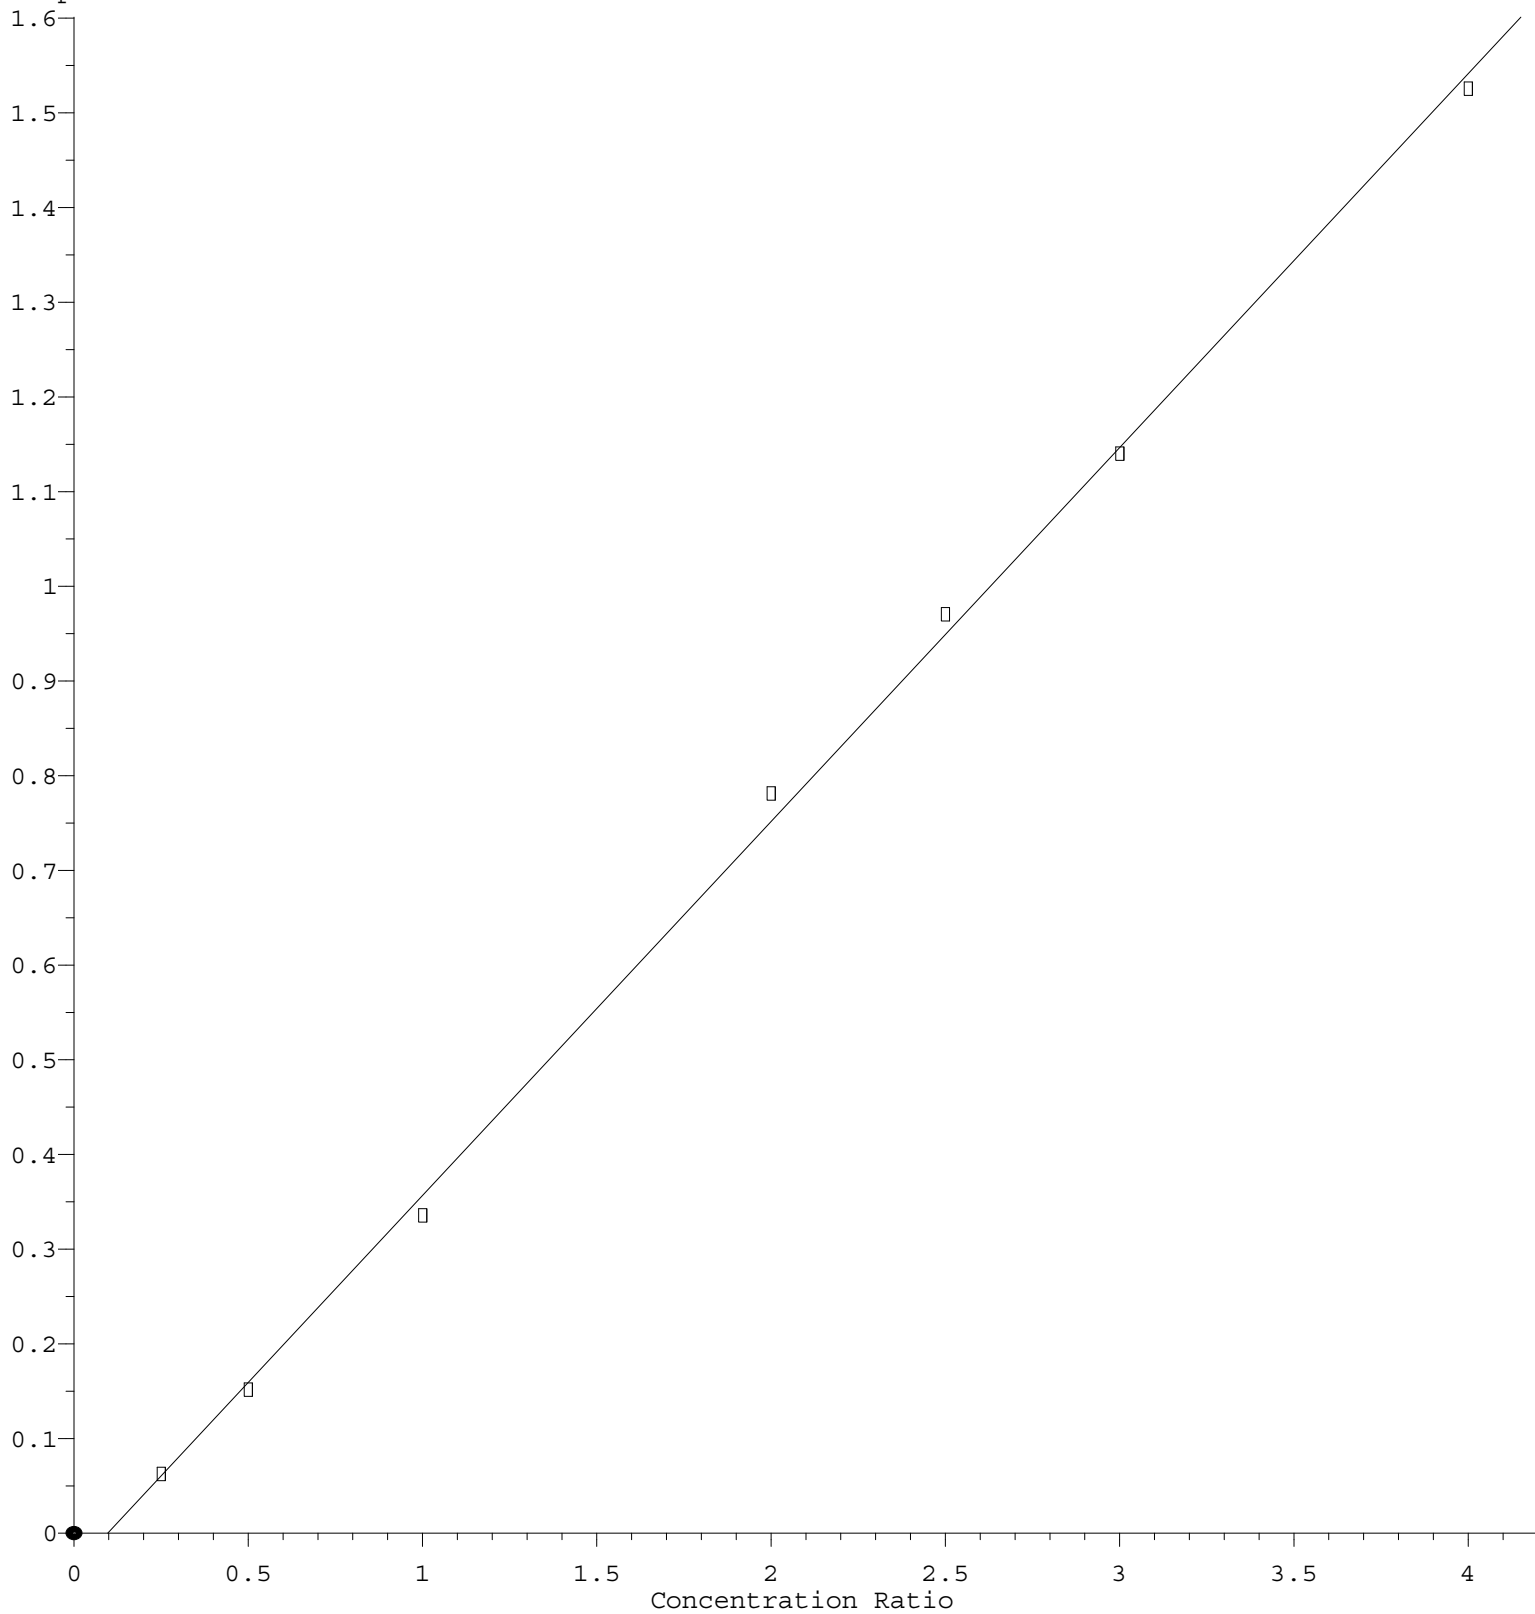

$$\text{Response} = 3.951\text{e-}001 * \text{Amt} - 3.830\text{e-}002$$


Coef of Det (r^2) = 0.998812 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M

Calibration Table Last Updated: Tue Oct 04 03:17:03 2022

2,4-Dinitrotoluene

Response Ratio

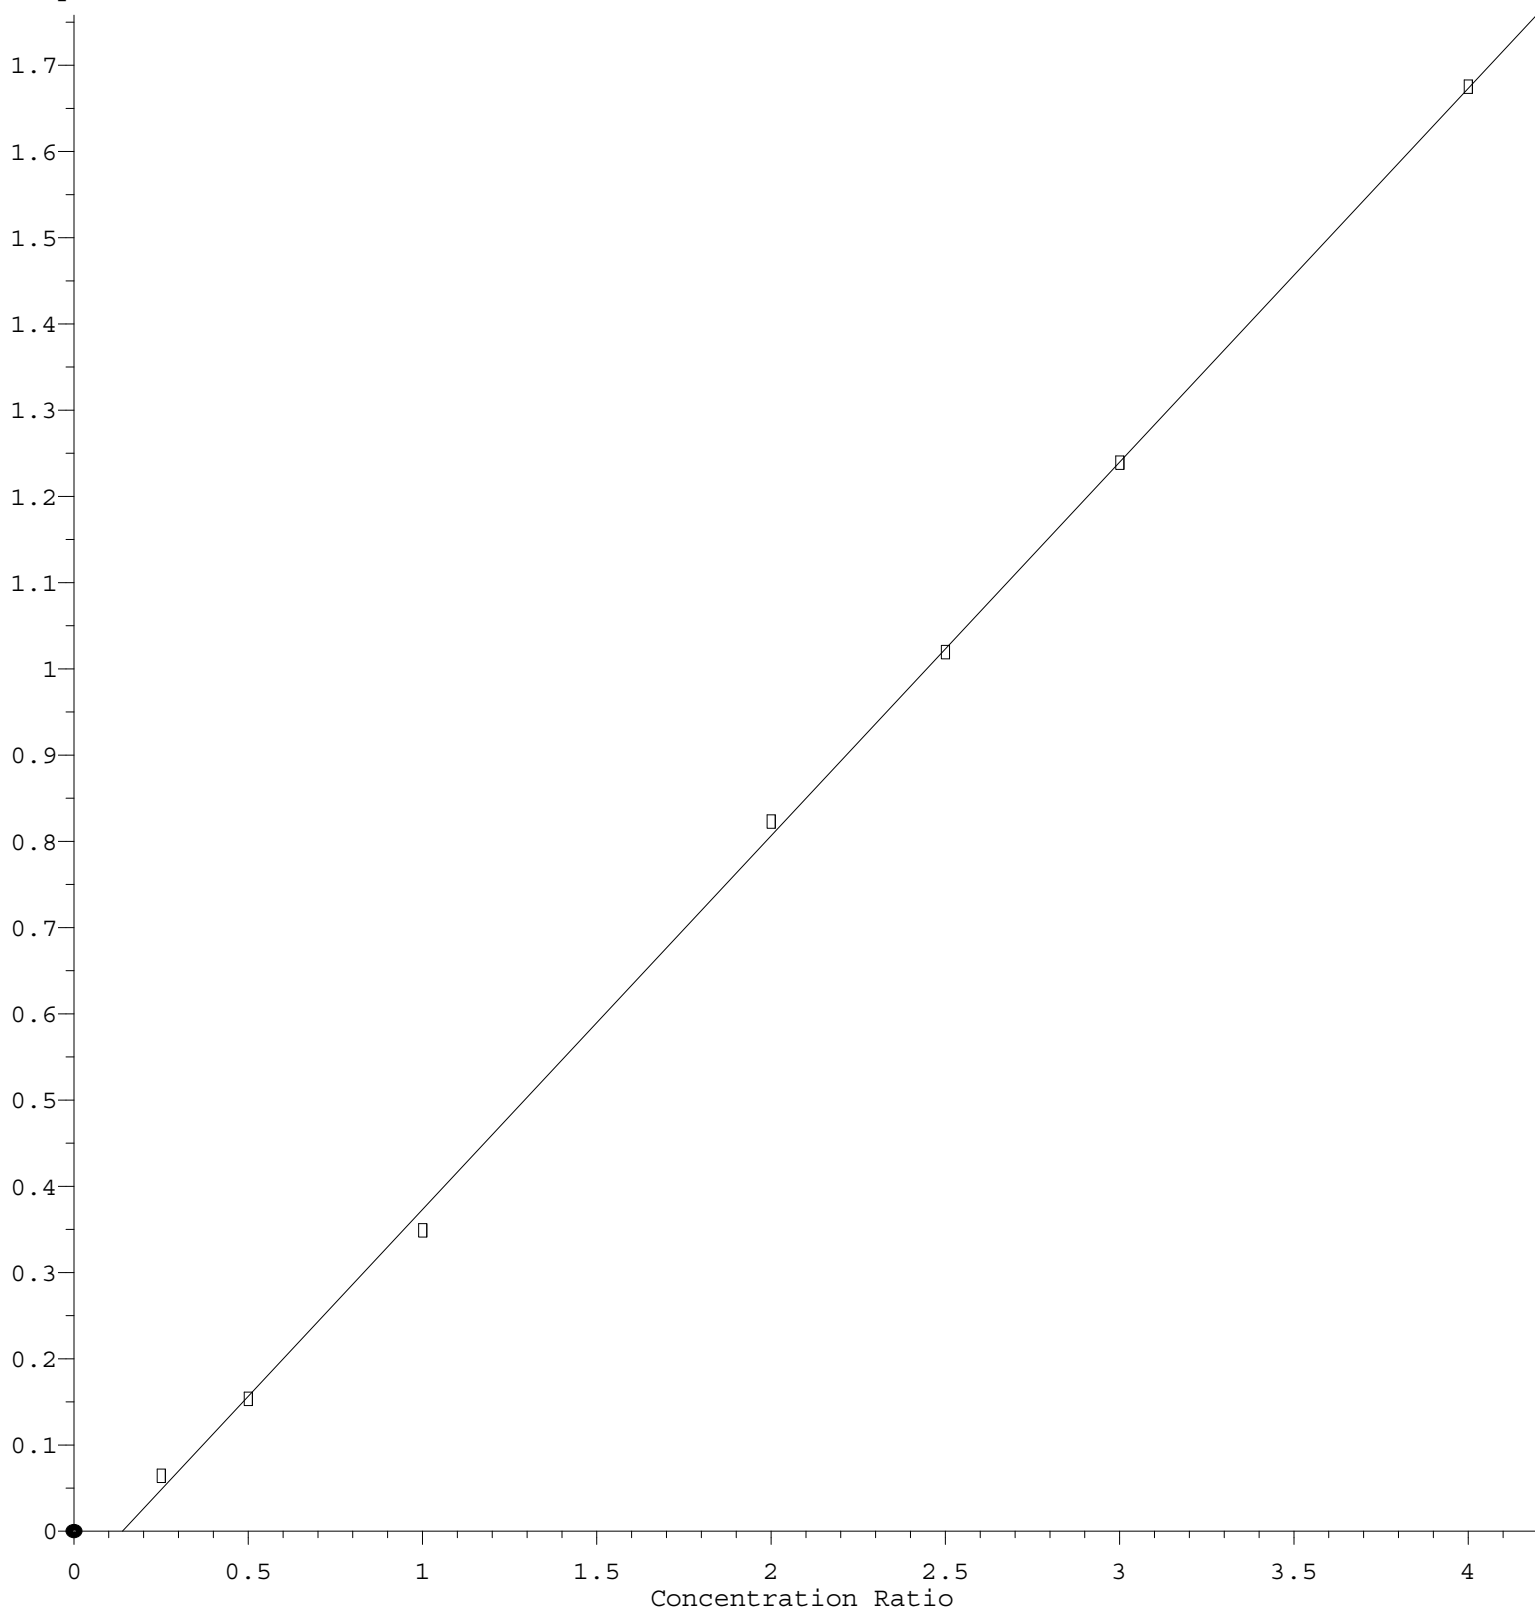


$$\text{Response} = 4.335\text{e-}001 * \text{Amt} - 6.020\text{e-}002$$

Coef of Det (r^2) = 0.999466 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M

Calibration Table Last Updated: Tue Oct 04 03:17:03 2022


2,4-Dinitrophenol

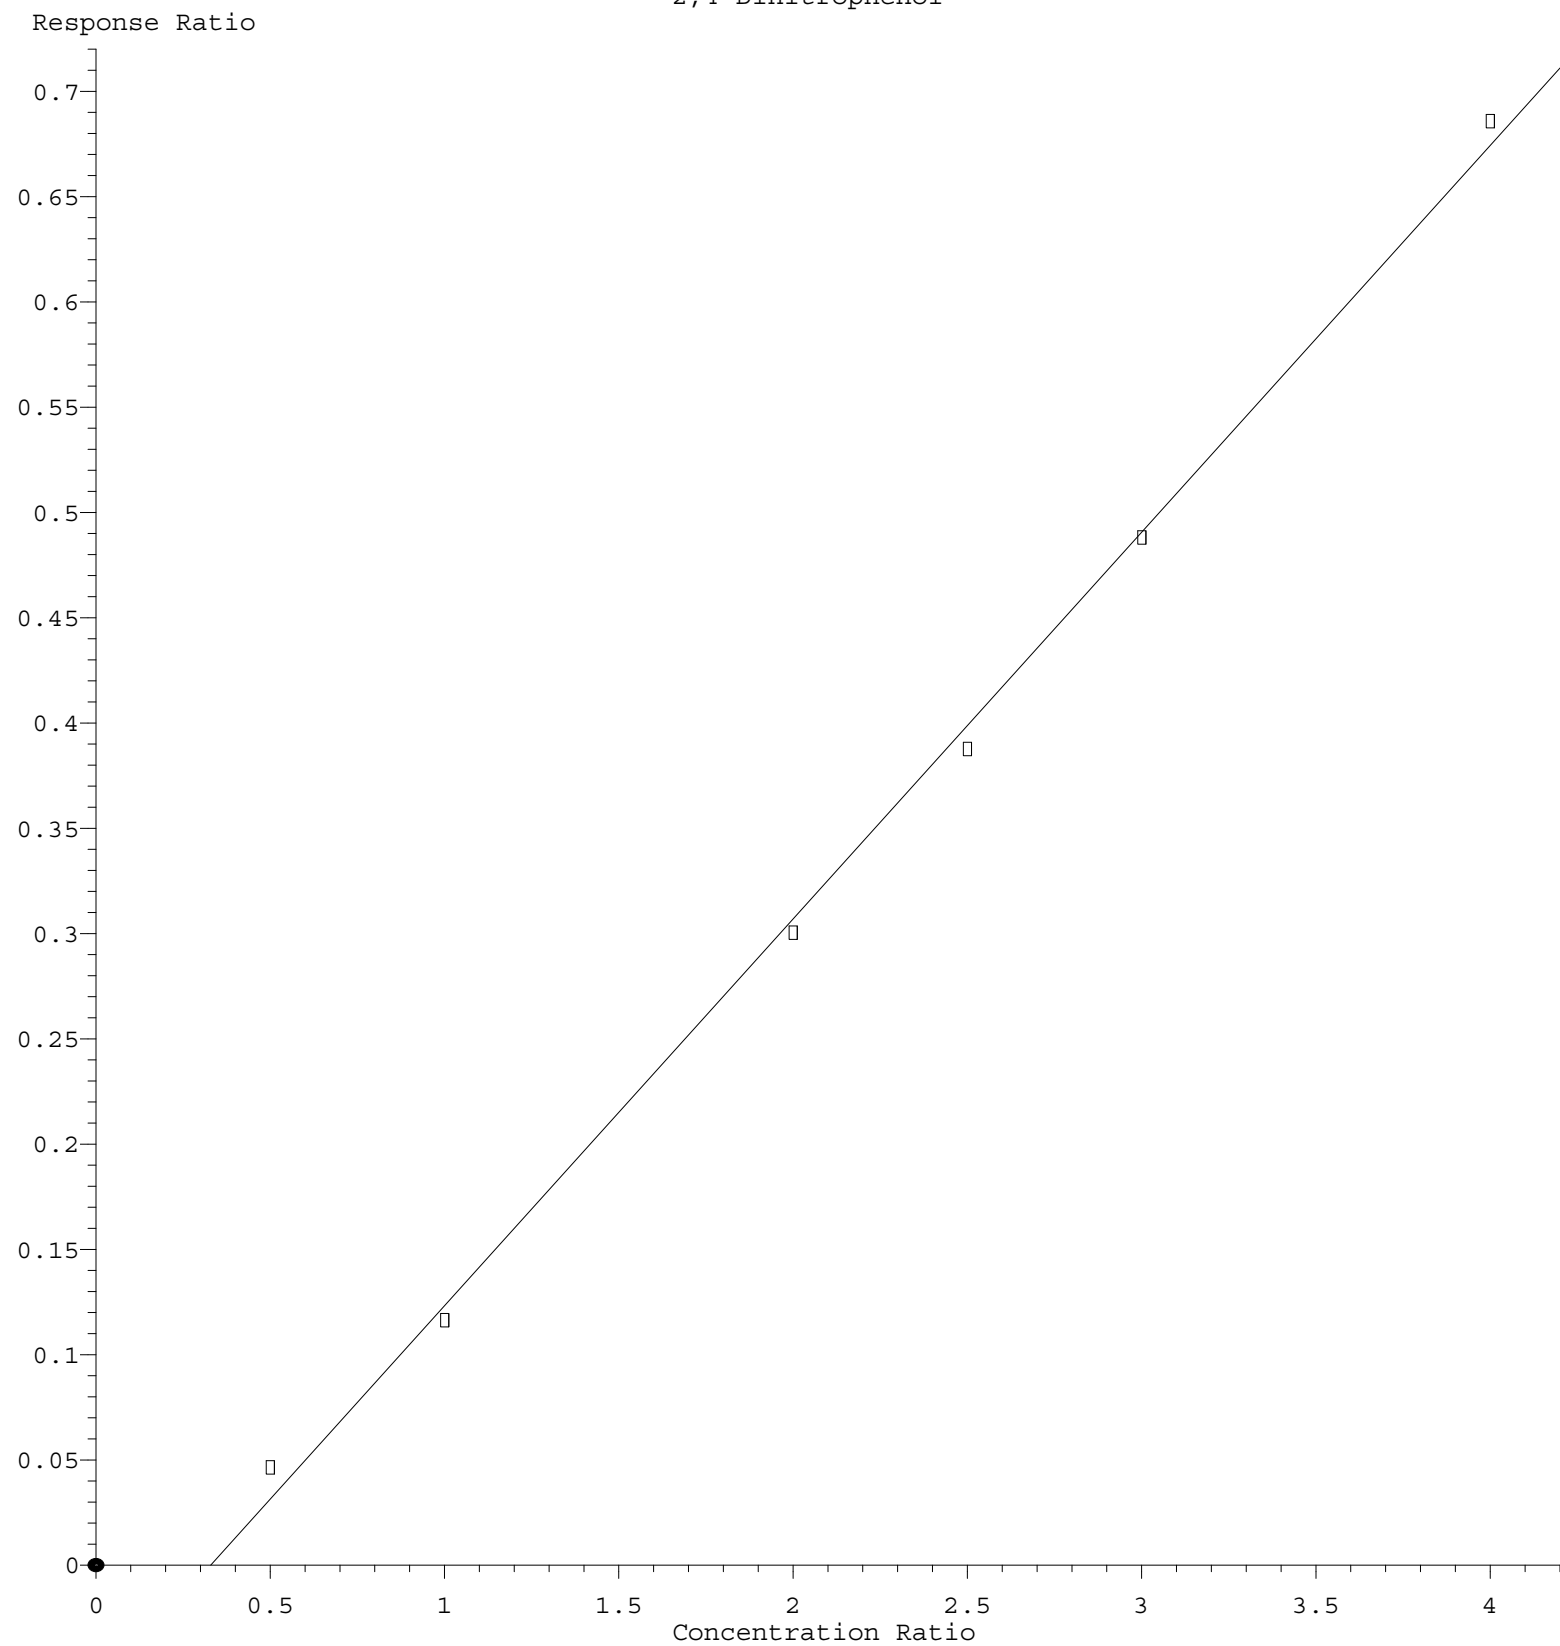

Response = 1.836e-001 * Amt - 6.039e-002
 Coef of Det (r^2) = 0.997941 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M
 Calibration Table Last Updated: Tue Oct 04 03:17:03 2022

2-Nitroaniline

Response Ratio

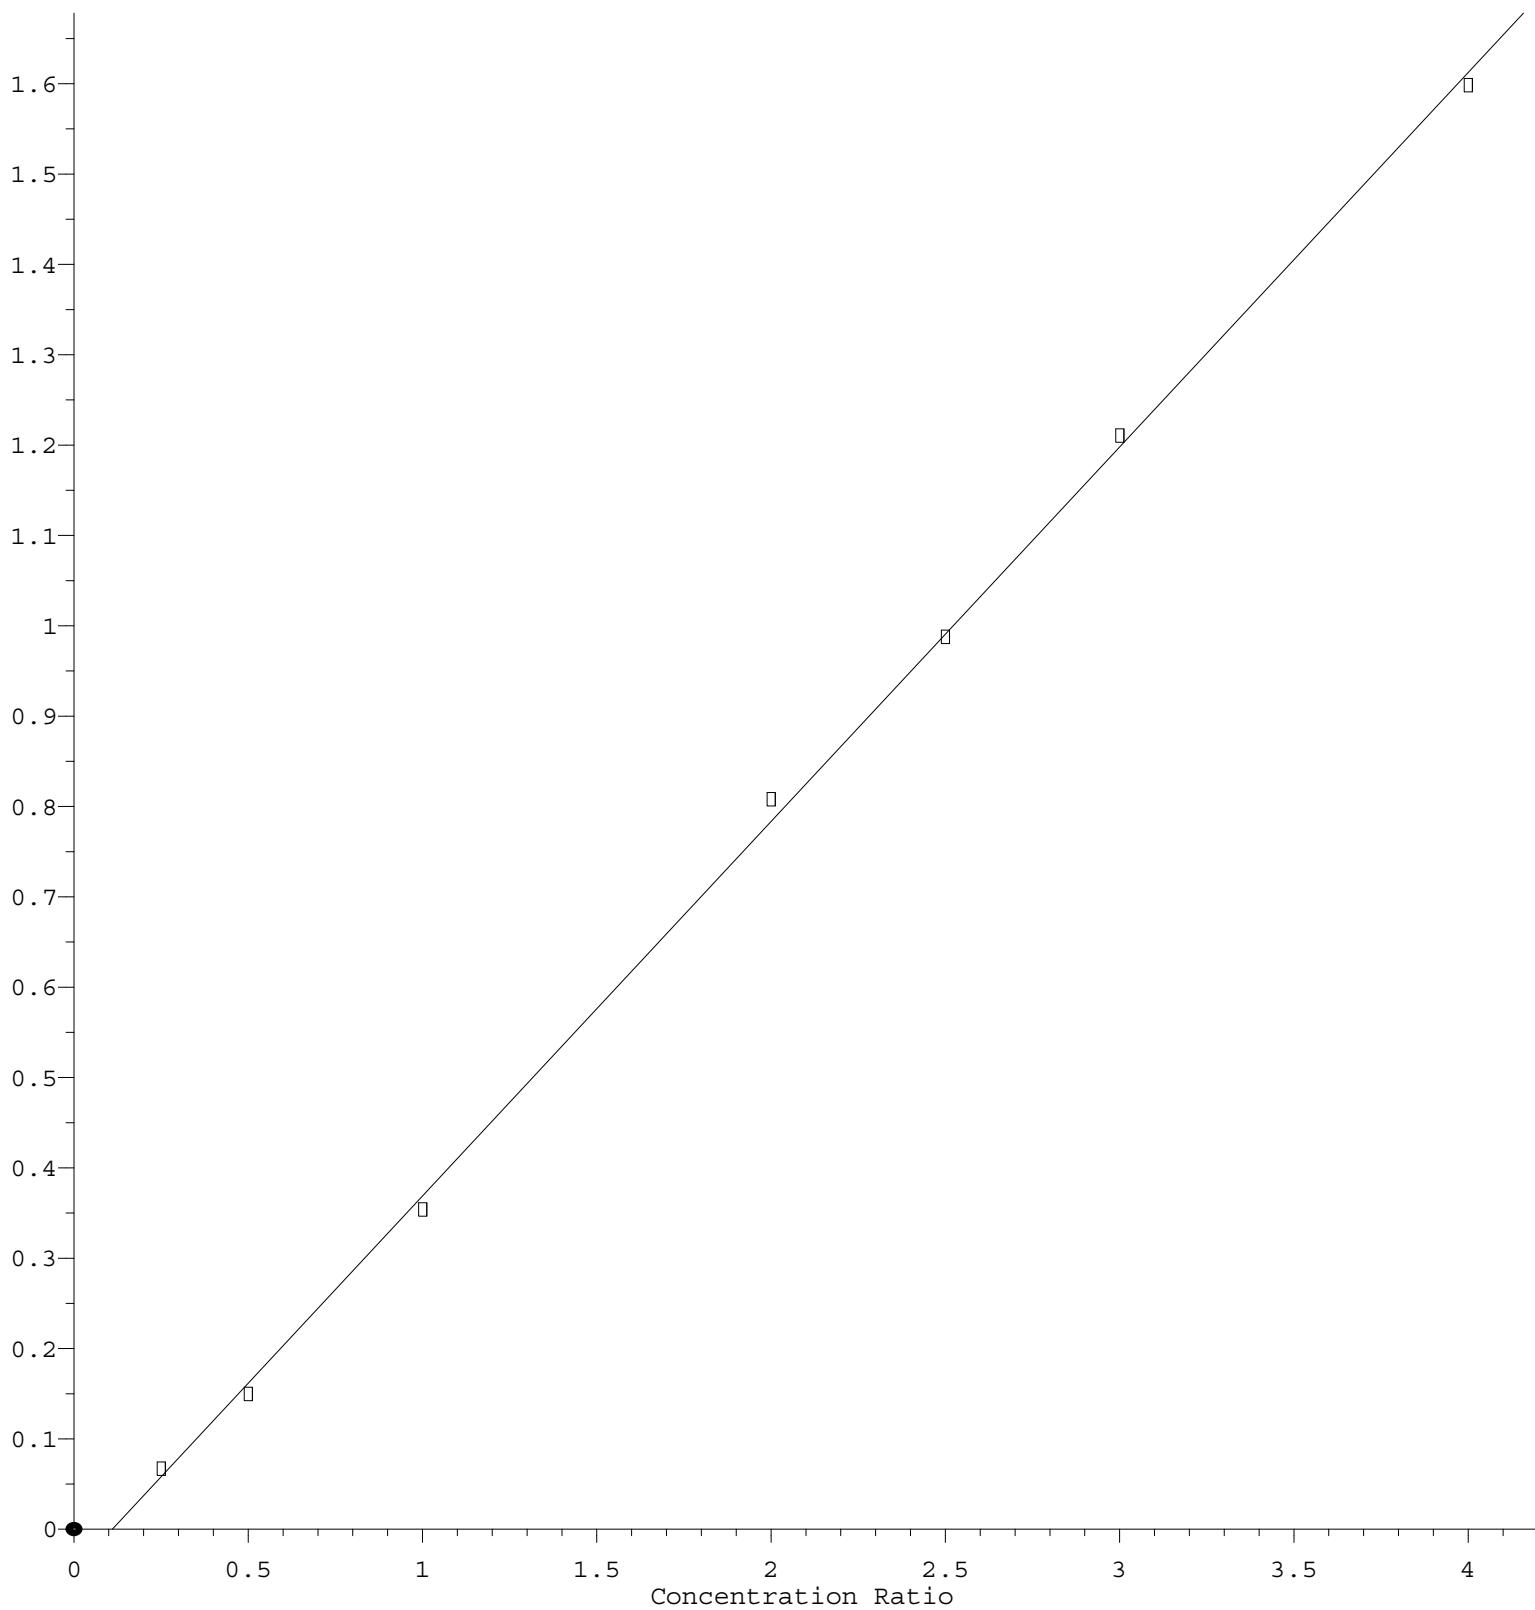

$$\text{Response} = 4.145\text{e-}001 * \text{Amt} - 4.541\text{e-}002$$


Coef of Det (r^2) = 0.999284 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M

Calibration Table Last Updated: Tue Oct 04 03:17:03 2022

Benzoic acid

Response Ratio

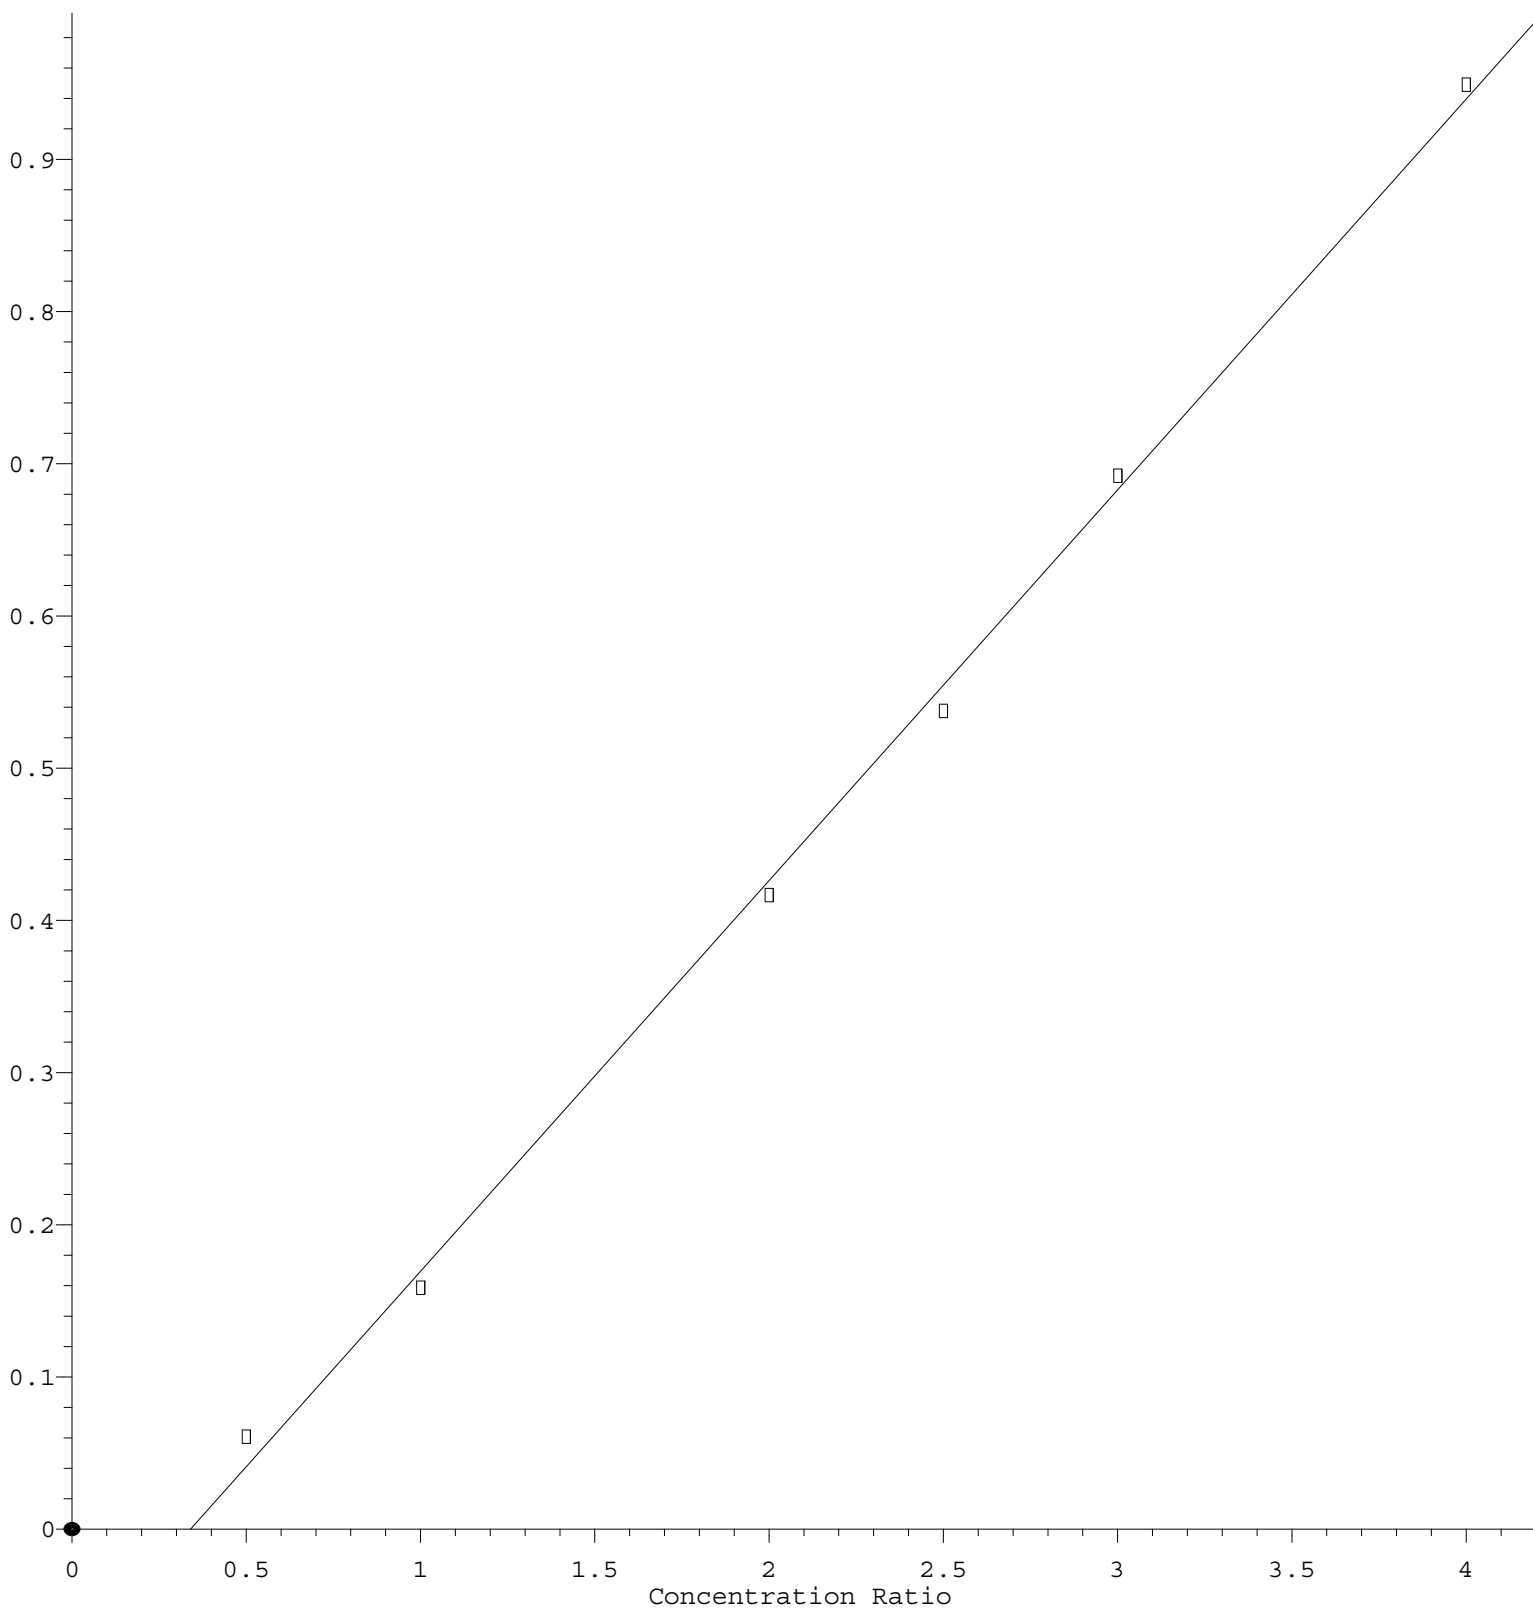

$$\text{Response} = 2.568 \times 10^{-1} \times \text{Amt} - 8.730 \times 10^{-2}$$

Coef of Det (r^2) = 0.998088 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM100322.M

Calibration Table Last Updated: Tue Oct 04 03:17:03 2022