


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100322\
 Data File : BM036814.D
 Acq On : 03 Oct 2022 12:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 03:17:03 2022

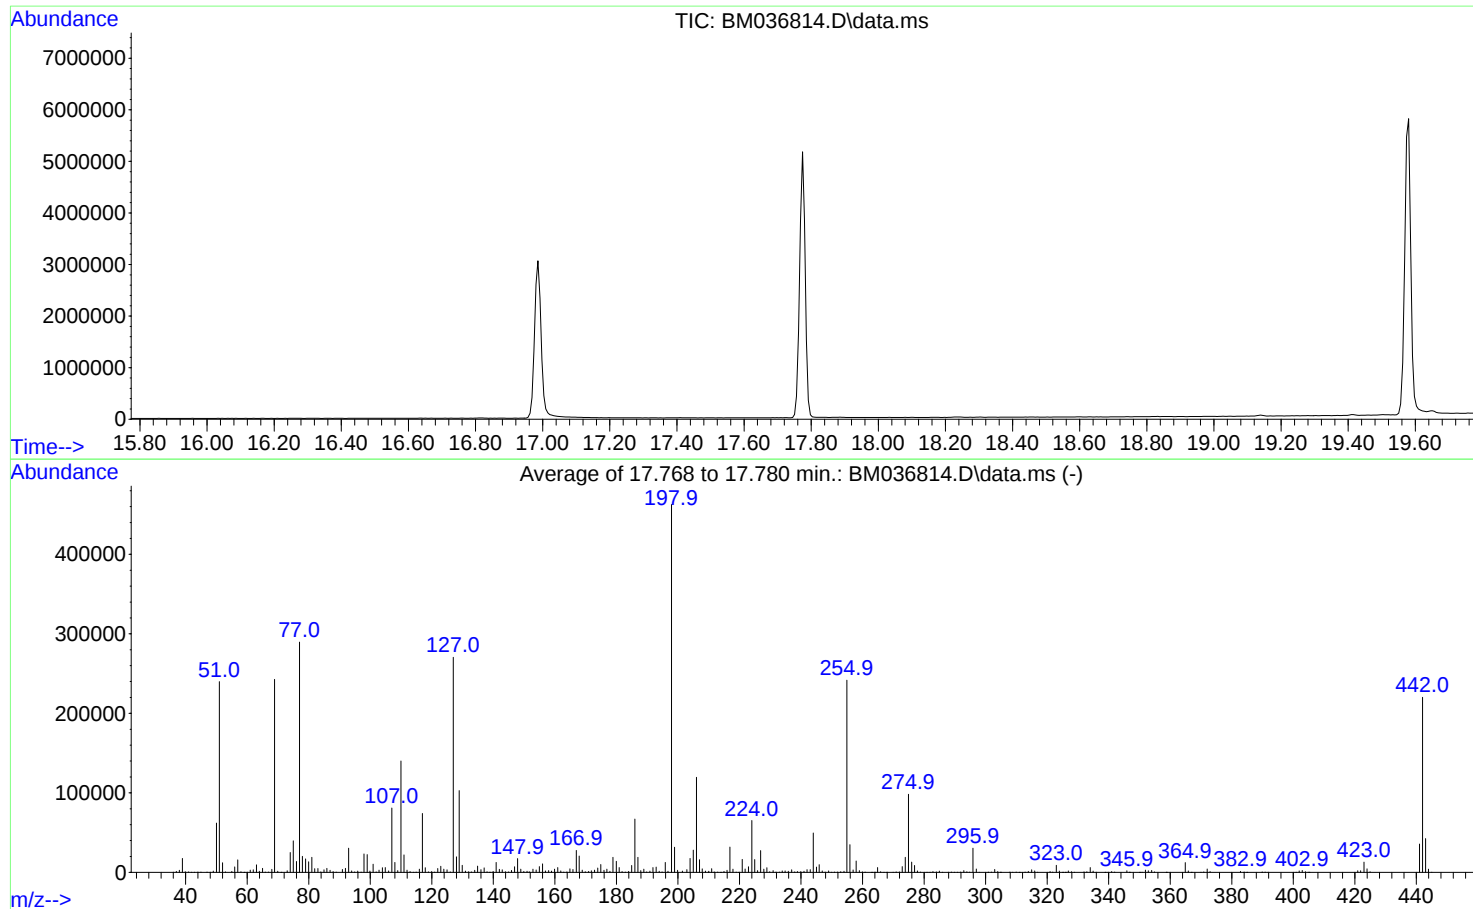


AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.9	239986	PASS
68	69	0.00	2	1.6	3790	PASS
69	198	0.00	100	52.5	242691	PASS
70	69	0.00	2	0.6	1409	PASS
127	198	10	80	58.5	270571	PASS
197	198	0.00	2	0.3	1361	PASS
198	198	100	100	100.0	462677	PASS
199	198	5	9	6.8	31645	PASS
275	198	10	60	21.2	98293	PASS
365	198	1	100	2.7	12375	PASS
441	198	0.01	100	7.7	35624	PASS
442	442	50	100	100.0	220203	PASS
443	442	15	24	19.3	42432	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100322\
Data File : BM036814.D
Acq On : 03 Oct 2022 12:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 04 04:47:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 03:17:03 2022
Response via : Initial Calibration

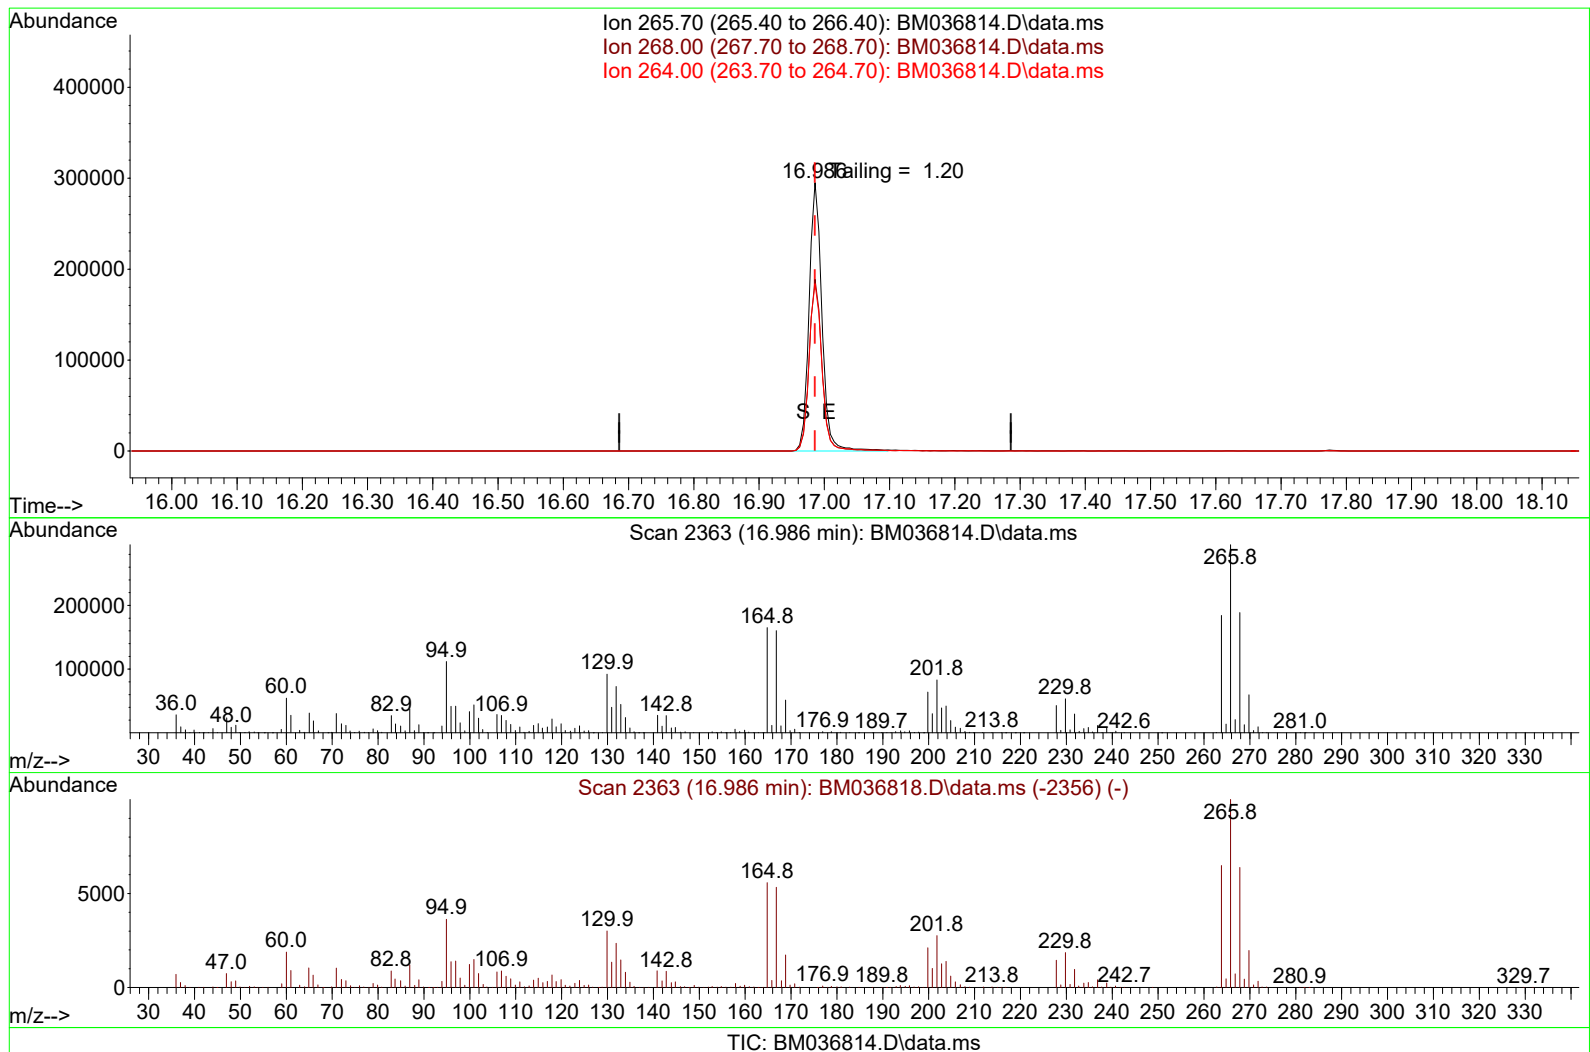

TIC: BM036814.D\data.ms

(70) Pentachlorophenol (C)

16.986min (-0.000) 554545.07 ng




response 406625

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.94
264.00	64.90	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100322\
 Data File : BM036814.D
 Acq On : 03 Oct 2022 12:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Oct 04 04:47:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 04 03:17:03 2022
 Response via : Initial Calibration

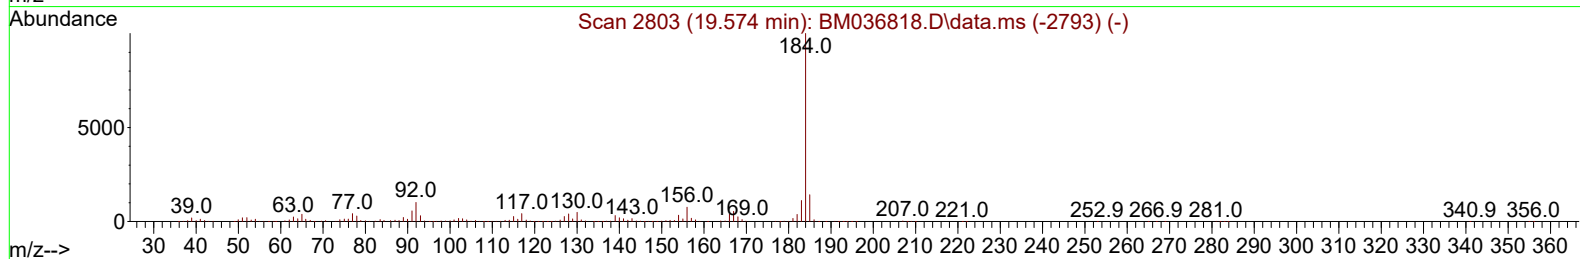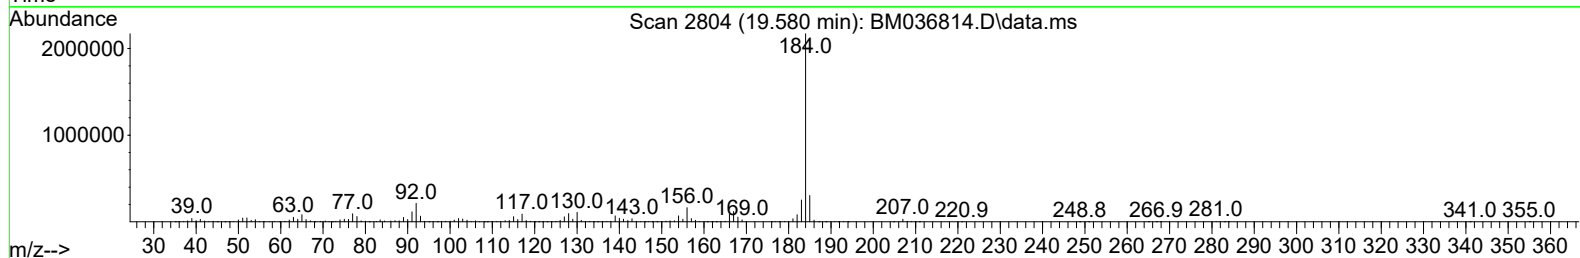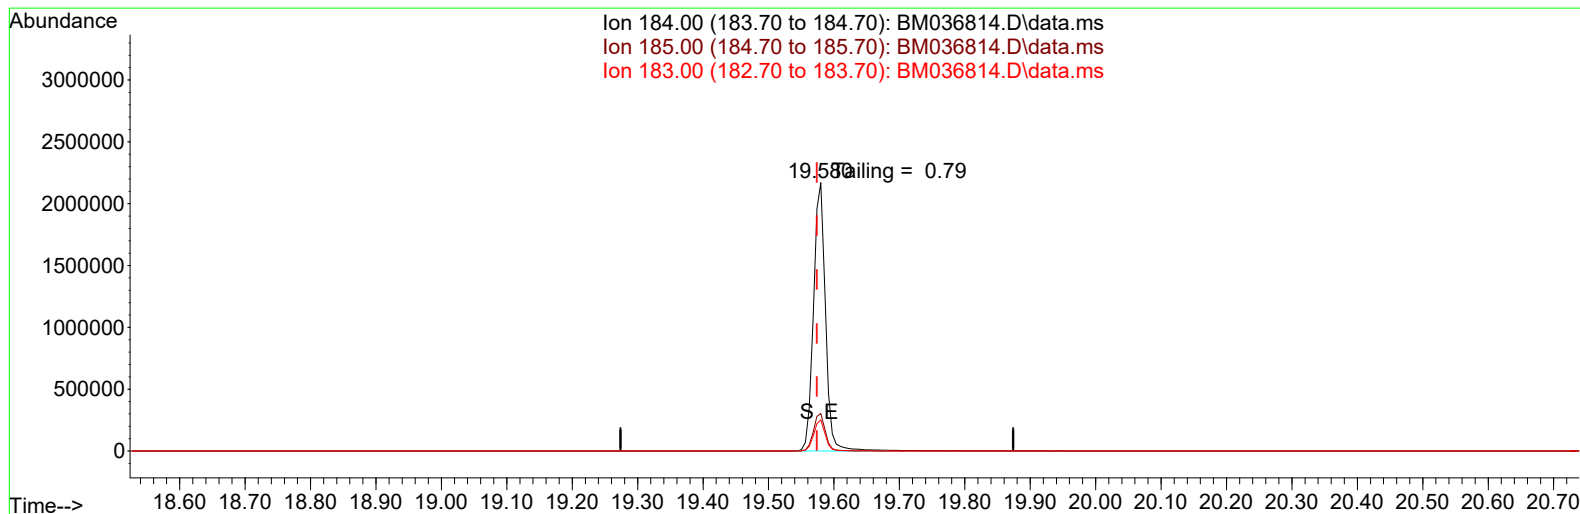

TIC: BM036814.D\data.ms

(77) Benzidine

19.580min (+ 0.006) 0.00 ng

response 2781917

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	11.10	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/3/2022	BNA_M	<u>BM036814.D</u>
Compound Name	Response	Retention Time
DDT	1220323	20.803
DDD	10488	20.362
DDE	556	19.862
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11044	1231367	0.90

Instrument :
BNA_M
ClientSampleId :
DFTPP