

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
 Data File : BM042171.D
 Acq On : 03 Oct 2023 20:46
 Operator : MA/JU
 Sample : PB155904BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK904

Quant Time: Oct 04 03:13:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	4519	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	11687	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.578	164	4972	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.333	188	10003	0.400	ng/ul	0.00
17) Chrysene-d12	21.513	240	4523	0.400	ng/ul	0.00
23) Perylene-d12	23.912	264	5131	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	39330	6.535	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	4771	0.298	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	6257	0.368	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.573	166	2049	0.077	ng/ul#	16
20) Pyrene	19.724	202	1662	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.754	252	3143	0.121	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
Data File : BM042171.D
Acq On : 03 Oct 2023 20:46
Operator : MA/JU
Sample : PB155904BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK904

Quant Time: Oct 04 03:13:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration




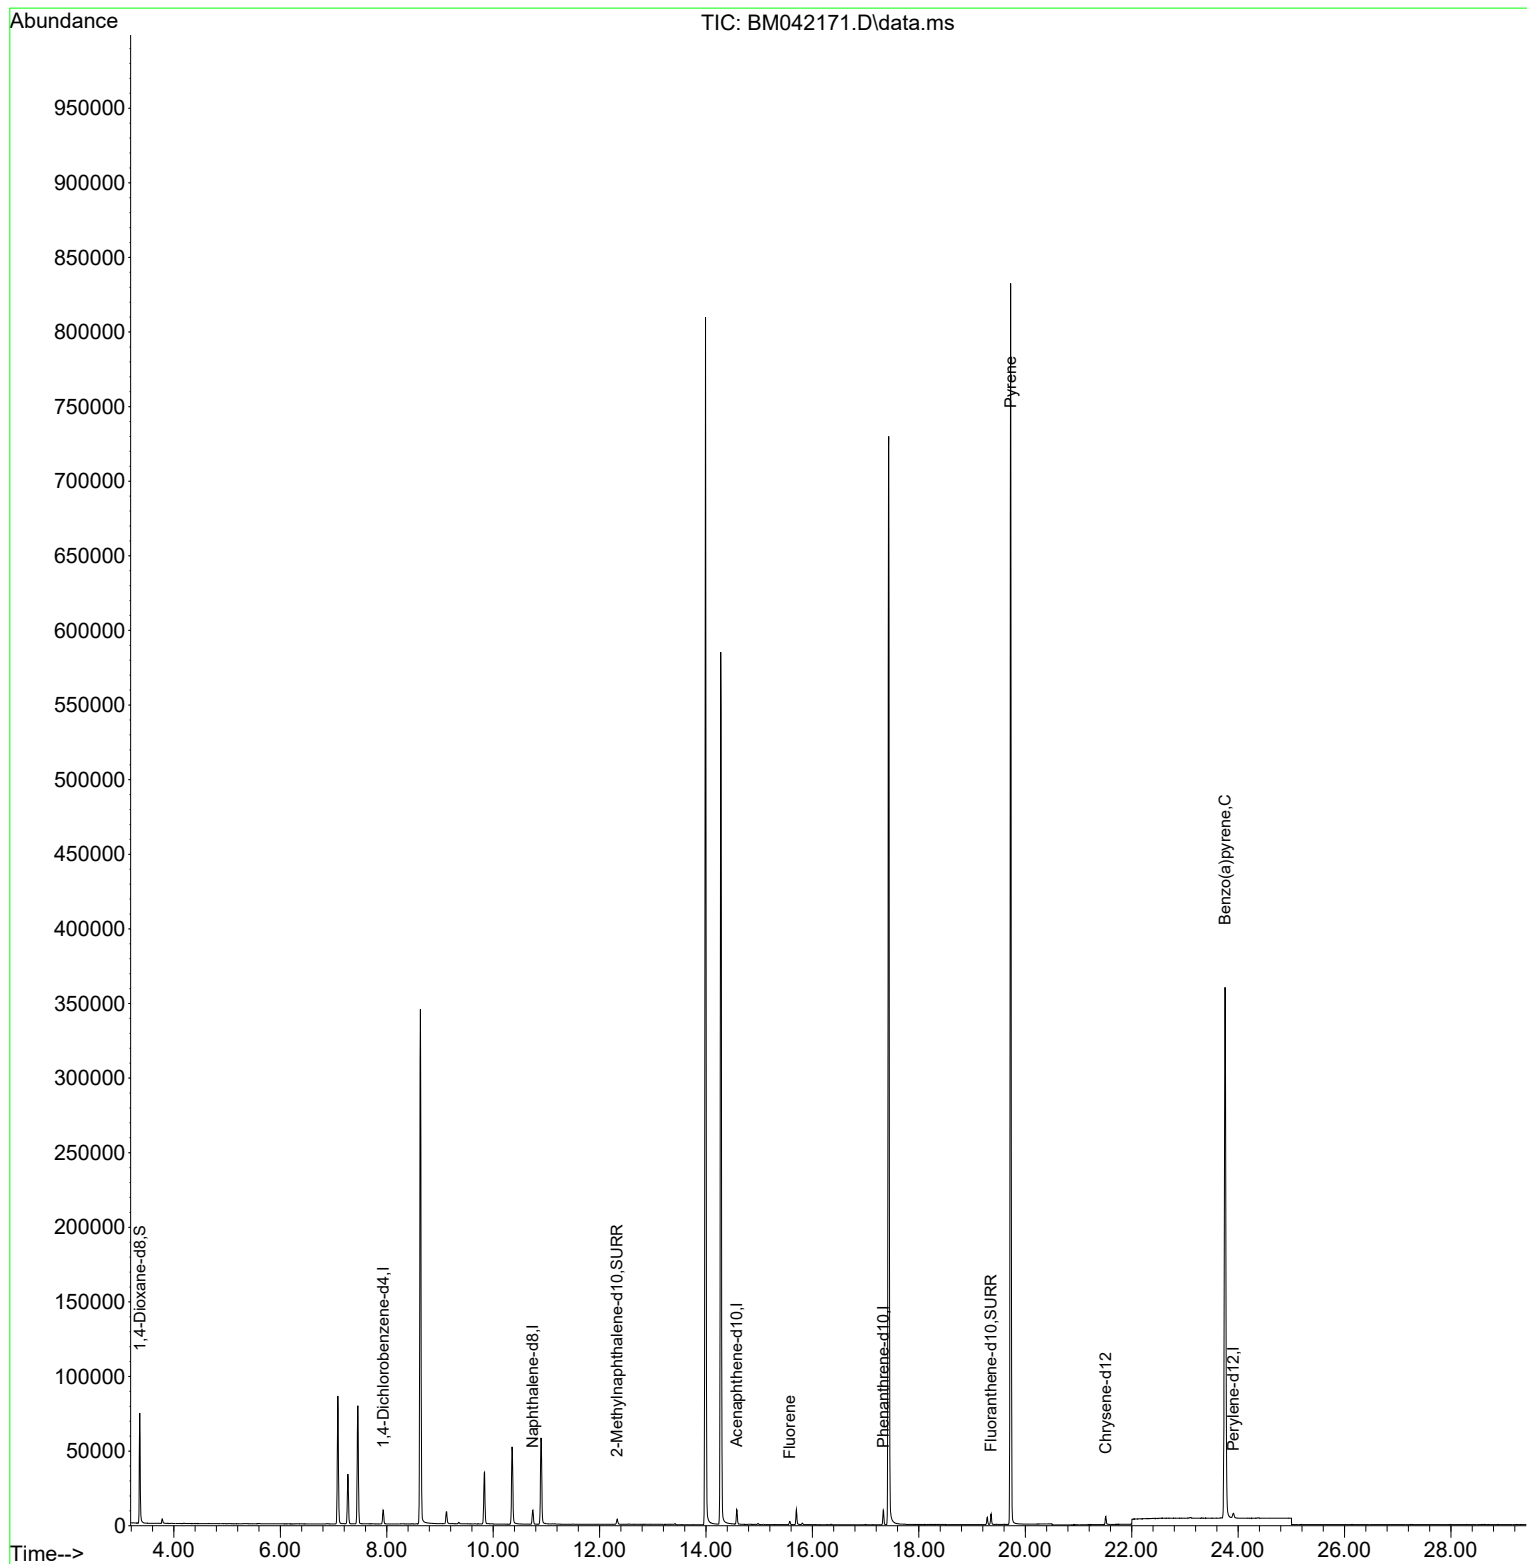


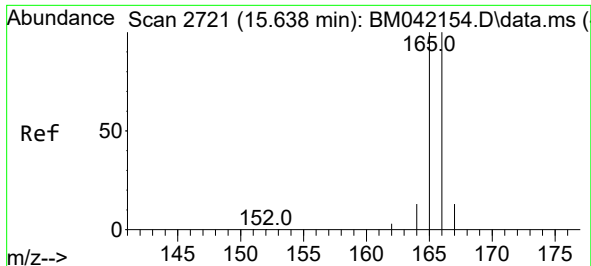

#12
Fluorene
Concen: 0.077 ng/ul
RT: 15.573 min Scan# 21
Delta R.T. -0.065 min
Lab File: BM042171.D
Acq: 03 Oct 2023 20:46




Instrument :
BNA_M
ClientSampleId :
SBLK904


Tgt Ion:166 Resp: 2049
Ion Ratio Lower Upper
166 100
165 9.0 78.4 117.6#
167 32.0 11.5 17.3#

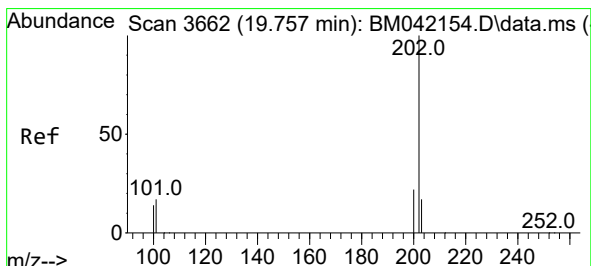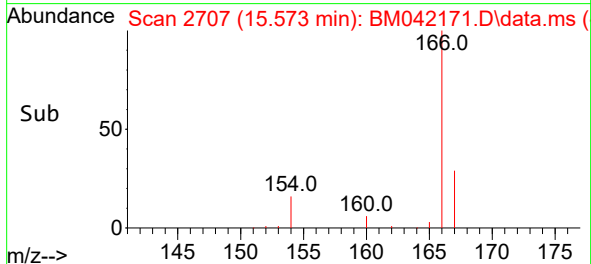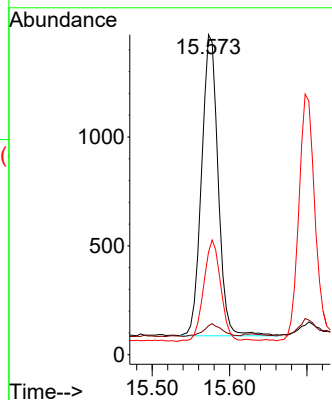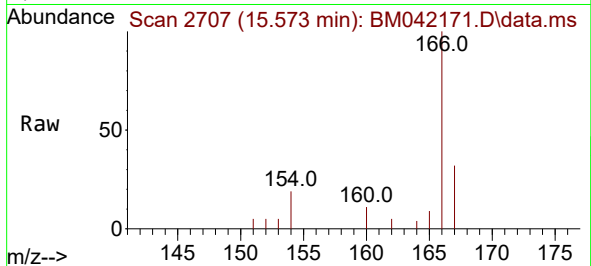

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.724 min Scan# 3655
Delta R.T. -0.037 min
Lab File: BM042171.D
Acq: 03 Oct 2023 20:46


Tgt Ion:202 Resp: 1662
Ion Ratio Lower Upper
202 100
101 175.2 12.7 19.1#
100 1309.6 9.9 14.9#

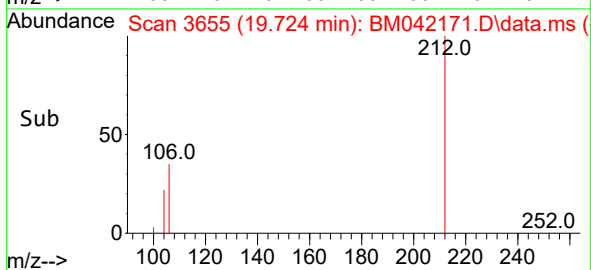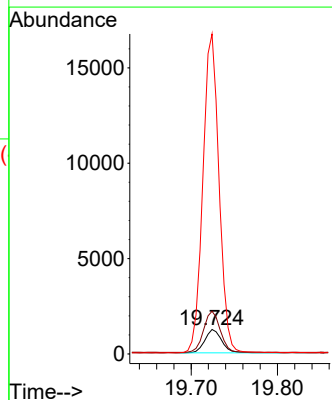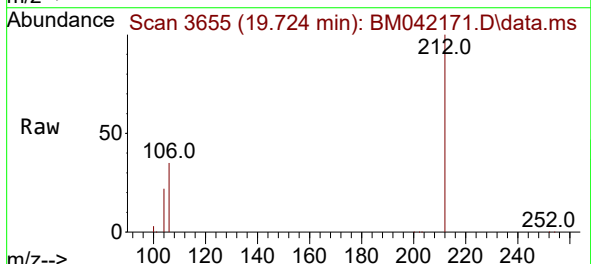

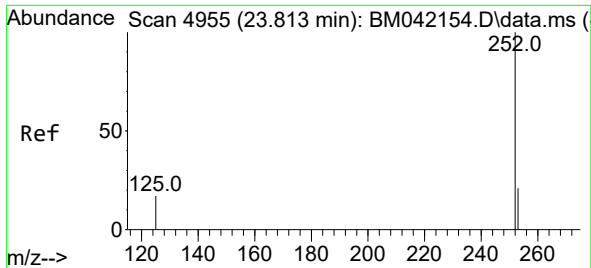

#26
 Benzo(a)pyrene
 Concen: 0.121 ng/ul
 RT: 23.754 min Scan# 4935
 Delta R.T. -0.061 min
 Lab File: BM042171.D
 Acq: 03 Oct 2023 20:46

Instrument :
 BNA_M
 ClientSampleId :
 SBLK904

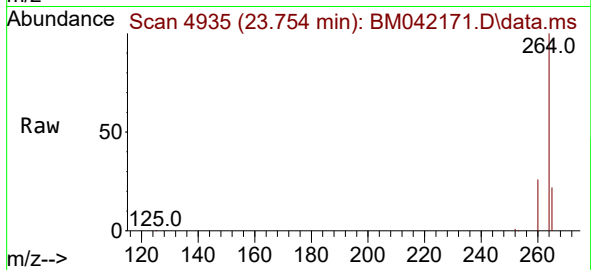

Tgt Ion:	252	Resp:	3143
Ion	Ratio	Lower	Upper
252	100		
253	57.9	25.3	37.9#
125	57.6	23.2	34.8#

