

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
 Data File : BM042172.D
 Acq On : 03 Oct 2023 21:23
 Operator : MA/JU
 Sample : 04571-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ17

Quant Time: Oct 04 03:13:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	4423	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	11739	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.578	164	5044	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.333	188	10625	0.400	ng/ul	0.00
17) Chrysene-d12	21.510	240	4921	0.400	ng/ul	0.00
23) Perylene-d12	23.907	264	5355	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	26238	4.455	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	4939	0.307	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	8523	0.461	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.398	88	1063	0.173	ng/ul	97
20) Pyrene	19.724	202	2640	0.066	ng/ul#	1
26) Benzo(a)pyrene	23.754	252	4113	0.151	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
Data File : BM042172.D
Acq On : 03 Oct 2023 21:23
Operator : MA/JU
Sample : 04571-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJ17

Quant Time: Oct 04 03:13:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration




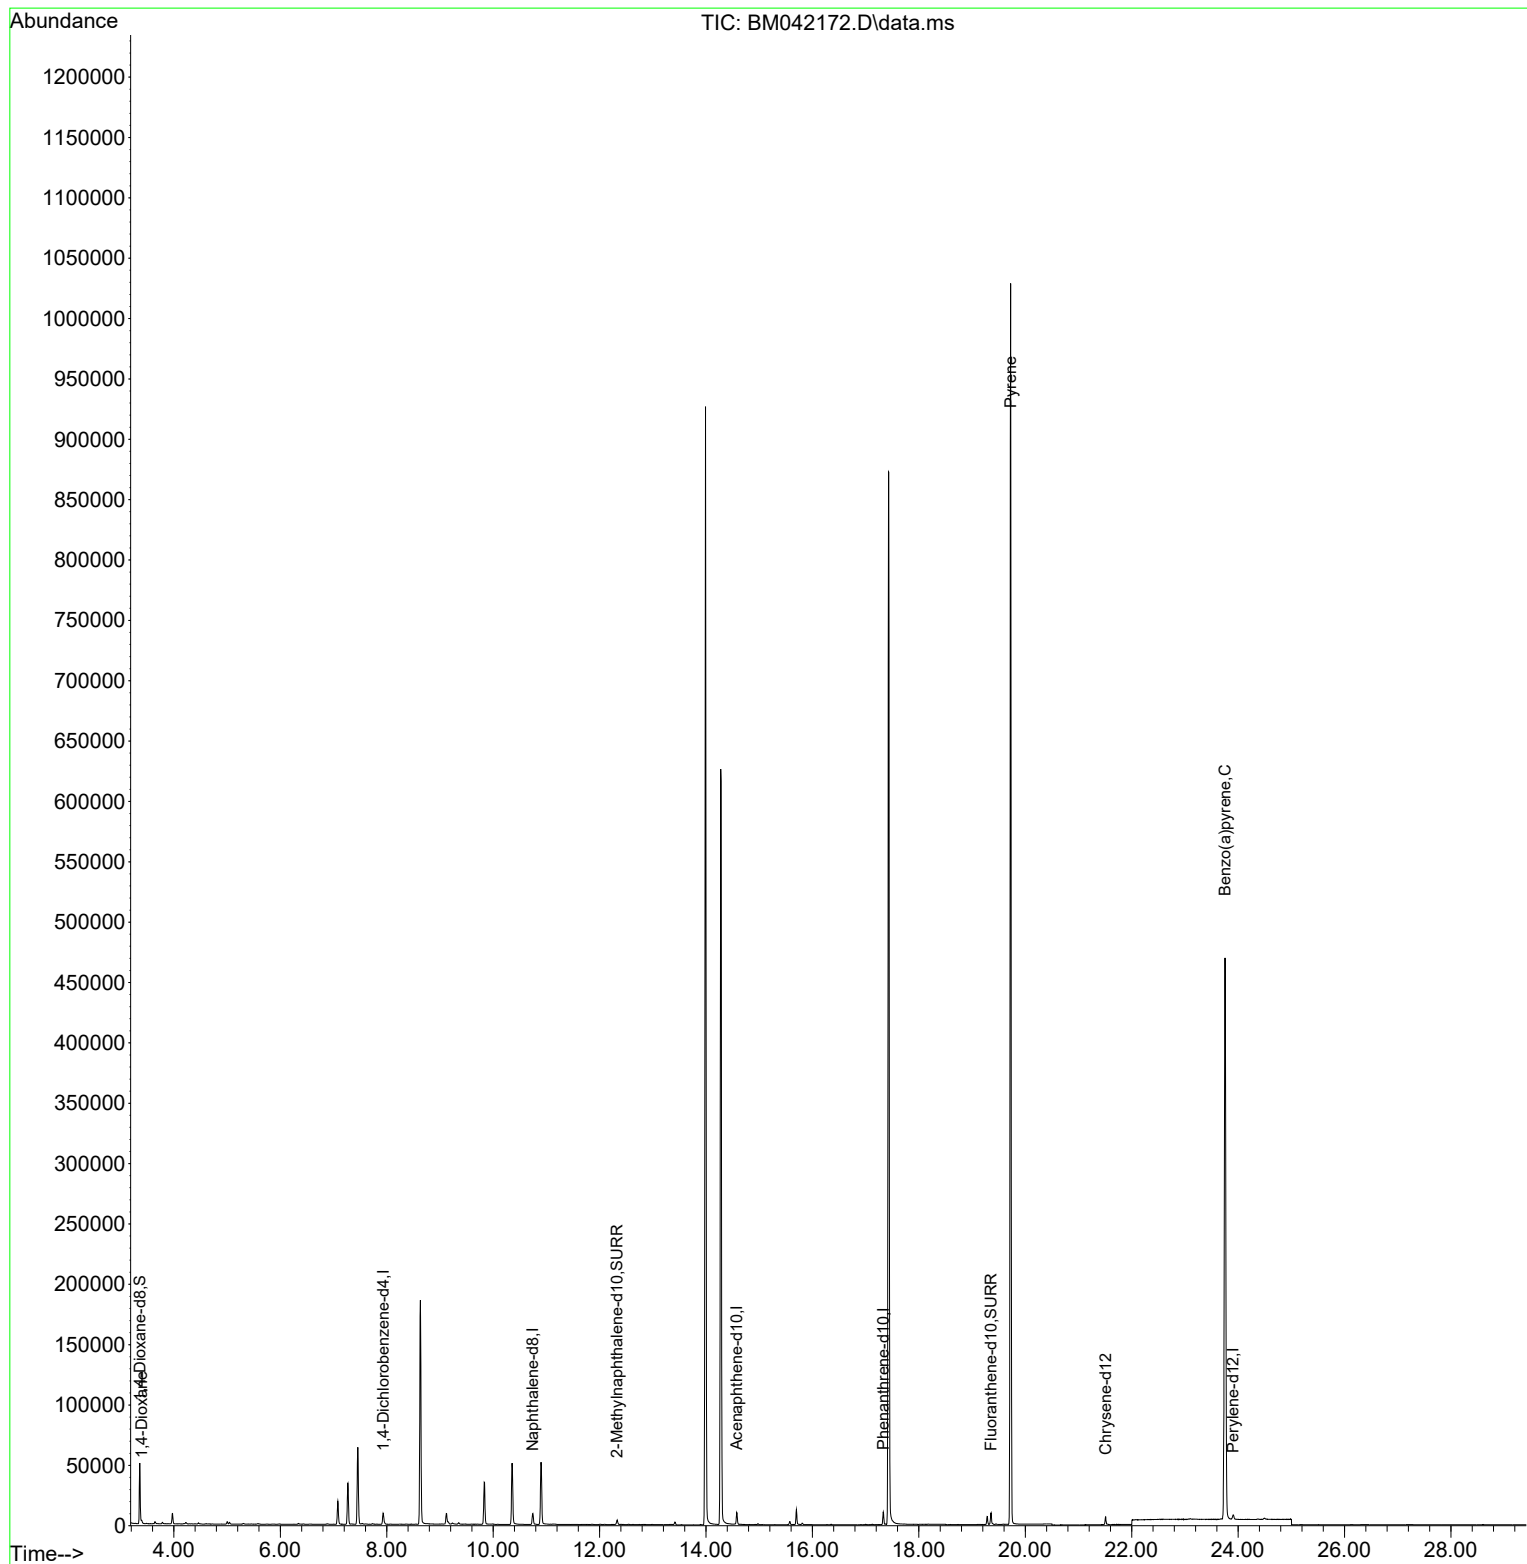


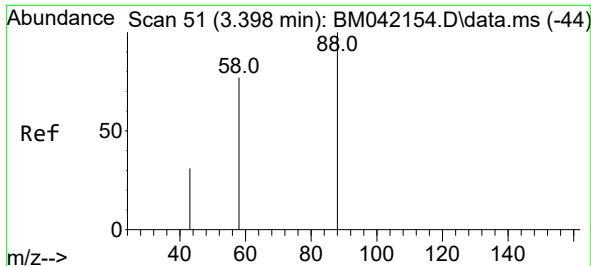

#2
1,4-Dioxane
Concen: 0.173 ng/ul
RT: 3.398 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM042172.D
Acq: 03 Oct 2023 21:23




Instrument :
BNA_M
ClientSampleId :
BBJ17


Tgt Ion: 88 Resp: 1063
Ion Ratio Lower Upper
88 100
43 68.1 52.1 78.1
58 69.4 53.8 80.6

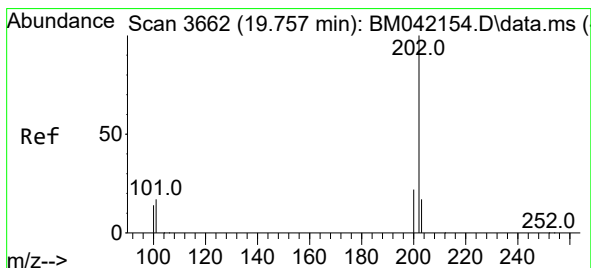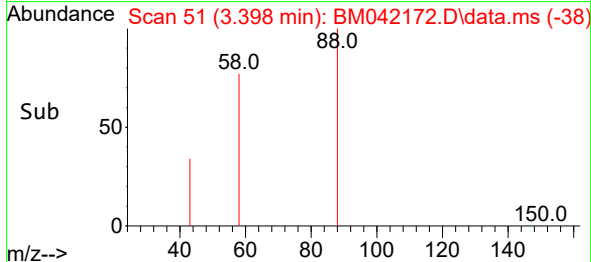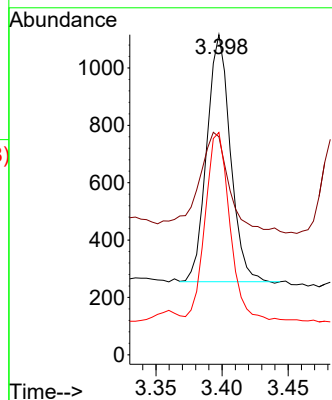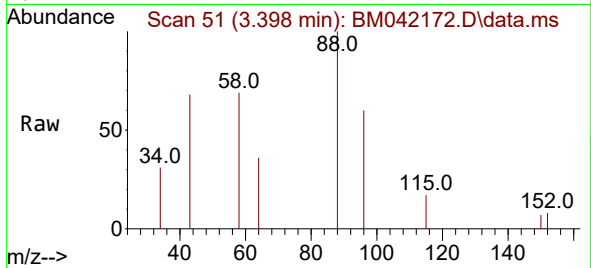

#20
Pyrene
Concen: 0.066 ng/ul
RT: 19.724 min Scan# 3655
Delta R.T. -0.037 min
Lab File: BM042172.D
Acq: 03 Oct 2023 21:23


Tgt Ion: 202 Resp: 2640
Ion Ratio Lower Upper
202 100
101 172.9 12.7 19.1#
100 1281.4 9.9 14.9#

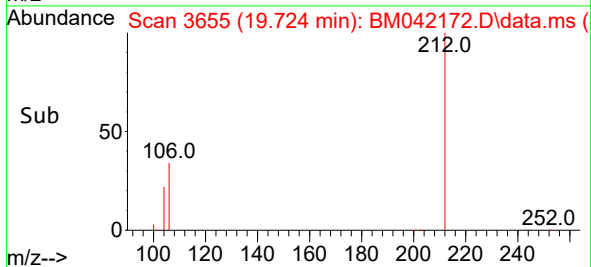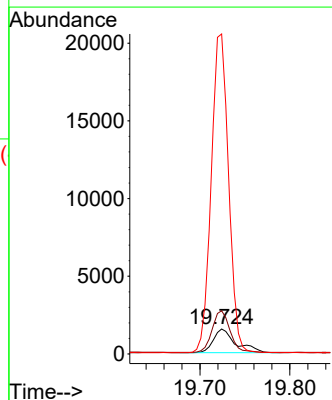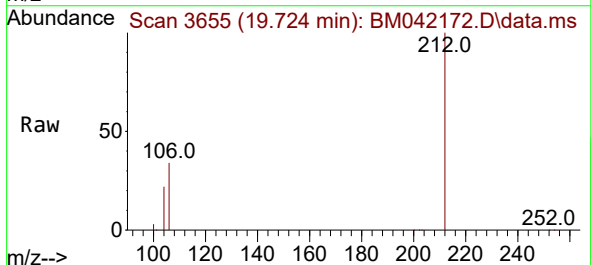

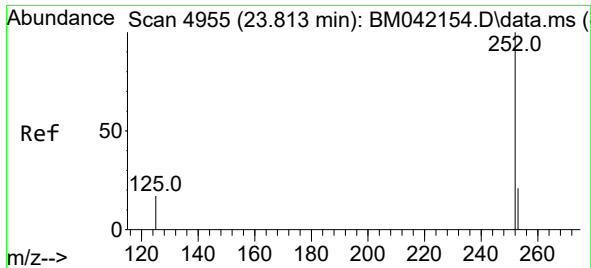

#26
Benzo(a)pyrene
Concen: 0.151 ng/ul
RT: 23.754 min Scan# 4935
Delta R.T. -0.061 min
Lab File: BM042172.D
Acq: 03 Oct 2023 21:23

Instrument :
BNA_M
ClientSampleId :
BBJ17

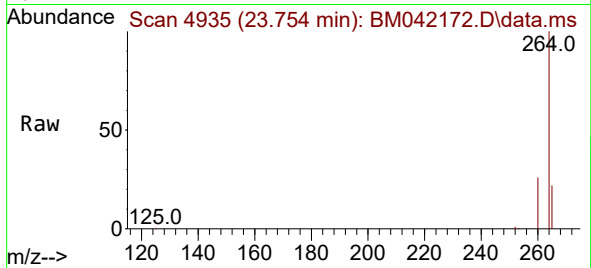

Tgt Ion:252 Resp: 4113
Ion Ratio Lower Upper
252 100
253 52.5 25.3 37.9#
125 55.0 23.2 34.8#

