

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
 Data File : BM042157.D
 Acq On : 03 Oct 2023 10:56
 Operator : MA/JU
 Sample : 04588-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHS6

Quant Time: Oct 03 11:25:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	4506	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	11097	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.583	164	4750	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.333	188	9984	0.400	ng/ul	0.00
17) Chrysene-d12	21.513	240	5310	0.400	ng/ul	0.00
23) Perylene-d12	23.912	264	6073	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	23849	3.974	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	4680	0.307	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	7512	0.377	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.398	88	1124	0.179	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
Data File : BM042157.D
Acq On : 03 Oct 2023 10:56
Operator : MA/JU
Sample : 04588-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHS6


Quant Time: Oct 03 11:25:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration

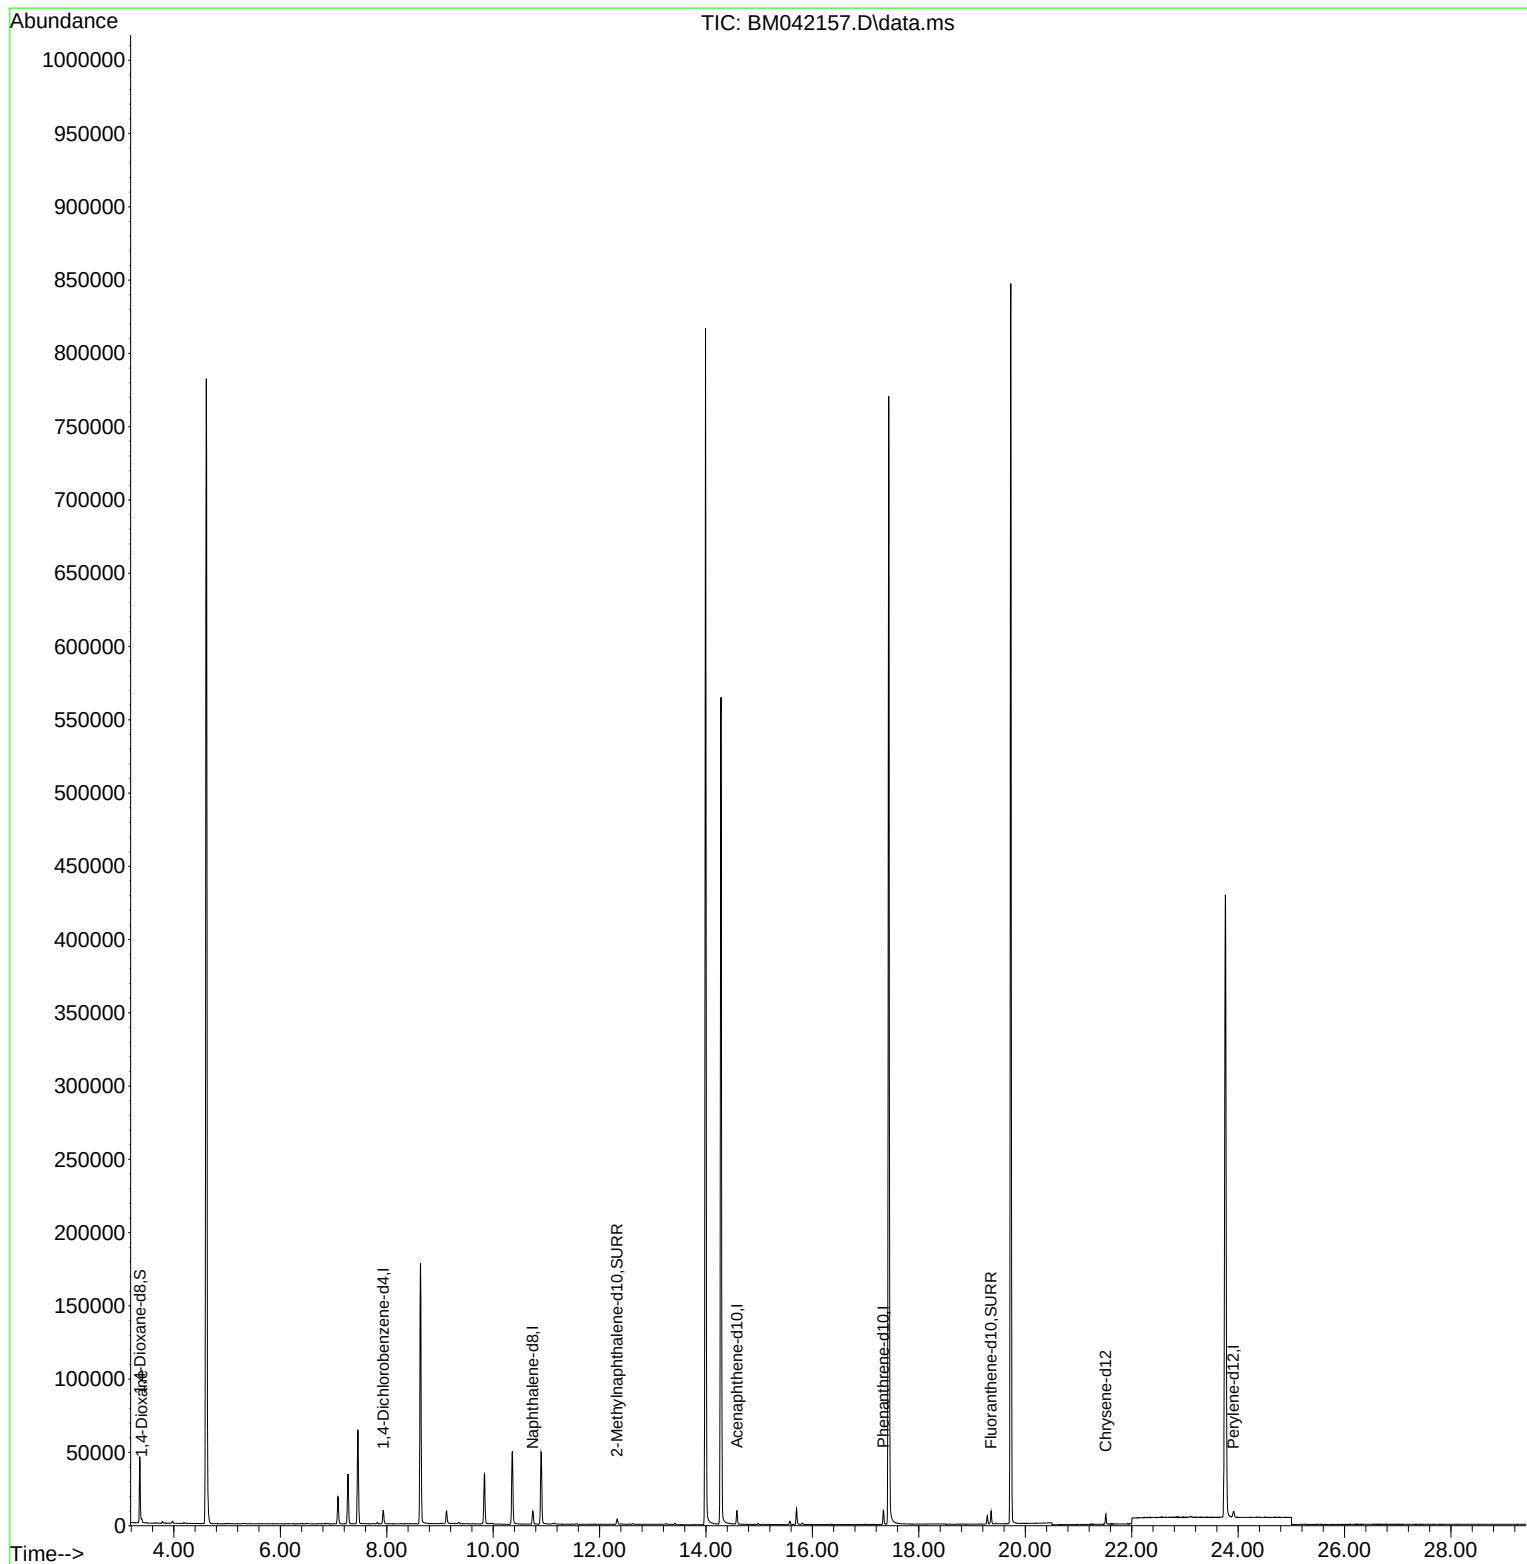

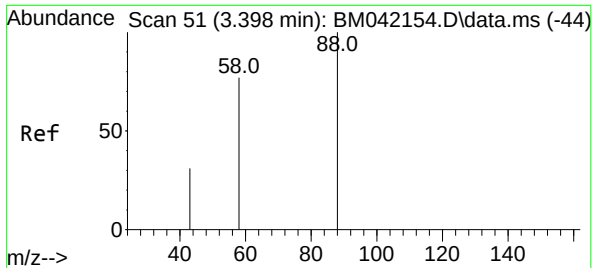

#2
 1,4-Dioxane
 Concen: 0.179 ng/ul
 RT: 3.398 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042157.D
 Acq: 03 Oct 2023 10:56

Instrument :
 BNA_M
 ClientSampleId :
 BBHS6

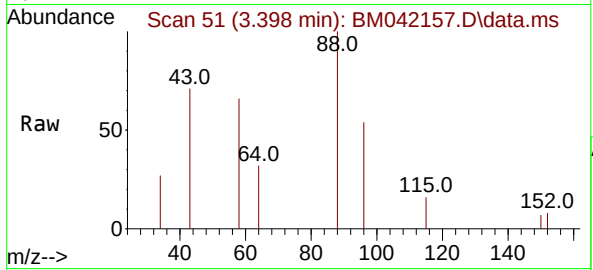

Tgt Ion: 88 Resp: 1124

Ion	Ratio	Lower	Upper
88	100		
43	71.2	52.1	78.1
58	65.9	53.8	80.6

