

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
 Data File : BM042158.D
 Acq On : 03 Oct 2023 11:32
 Operator : MA/JU
 Sample : 04588-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHP4

Quant Time: Oct 03 13:52:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	4008	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	9933	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.583	164	4341	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.333	188	9214	0.400	ng/ul	0.00
17) Chrysene-d12	21.513	240	5157	0.400	ng/ul	0.00
23) Perylene-d12	23.912	264	5787	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	21310	3.993	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	4004	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	6923	0.358	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.398	88	19586	3.514	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
Data File : BM042158.D
Acq On : 03 Oct 2023 11:32
Operator : MA/JU
Sample : 04588-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHP4


Quant Time: Oct 03 13:52:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration

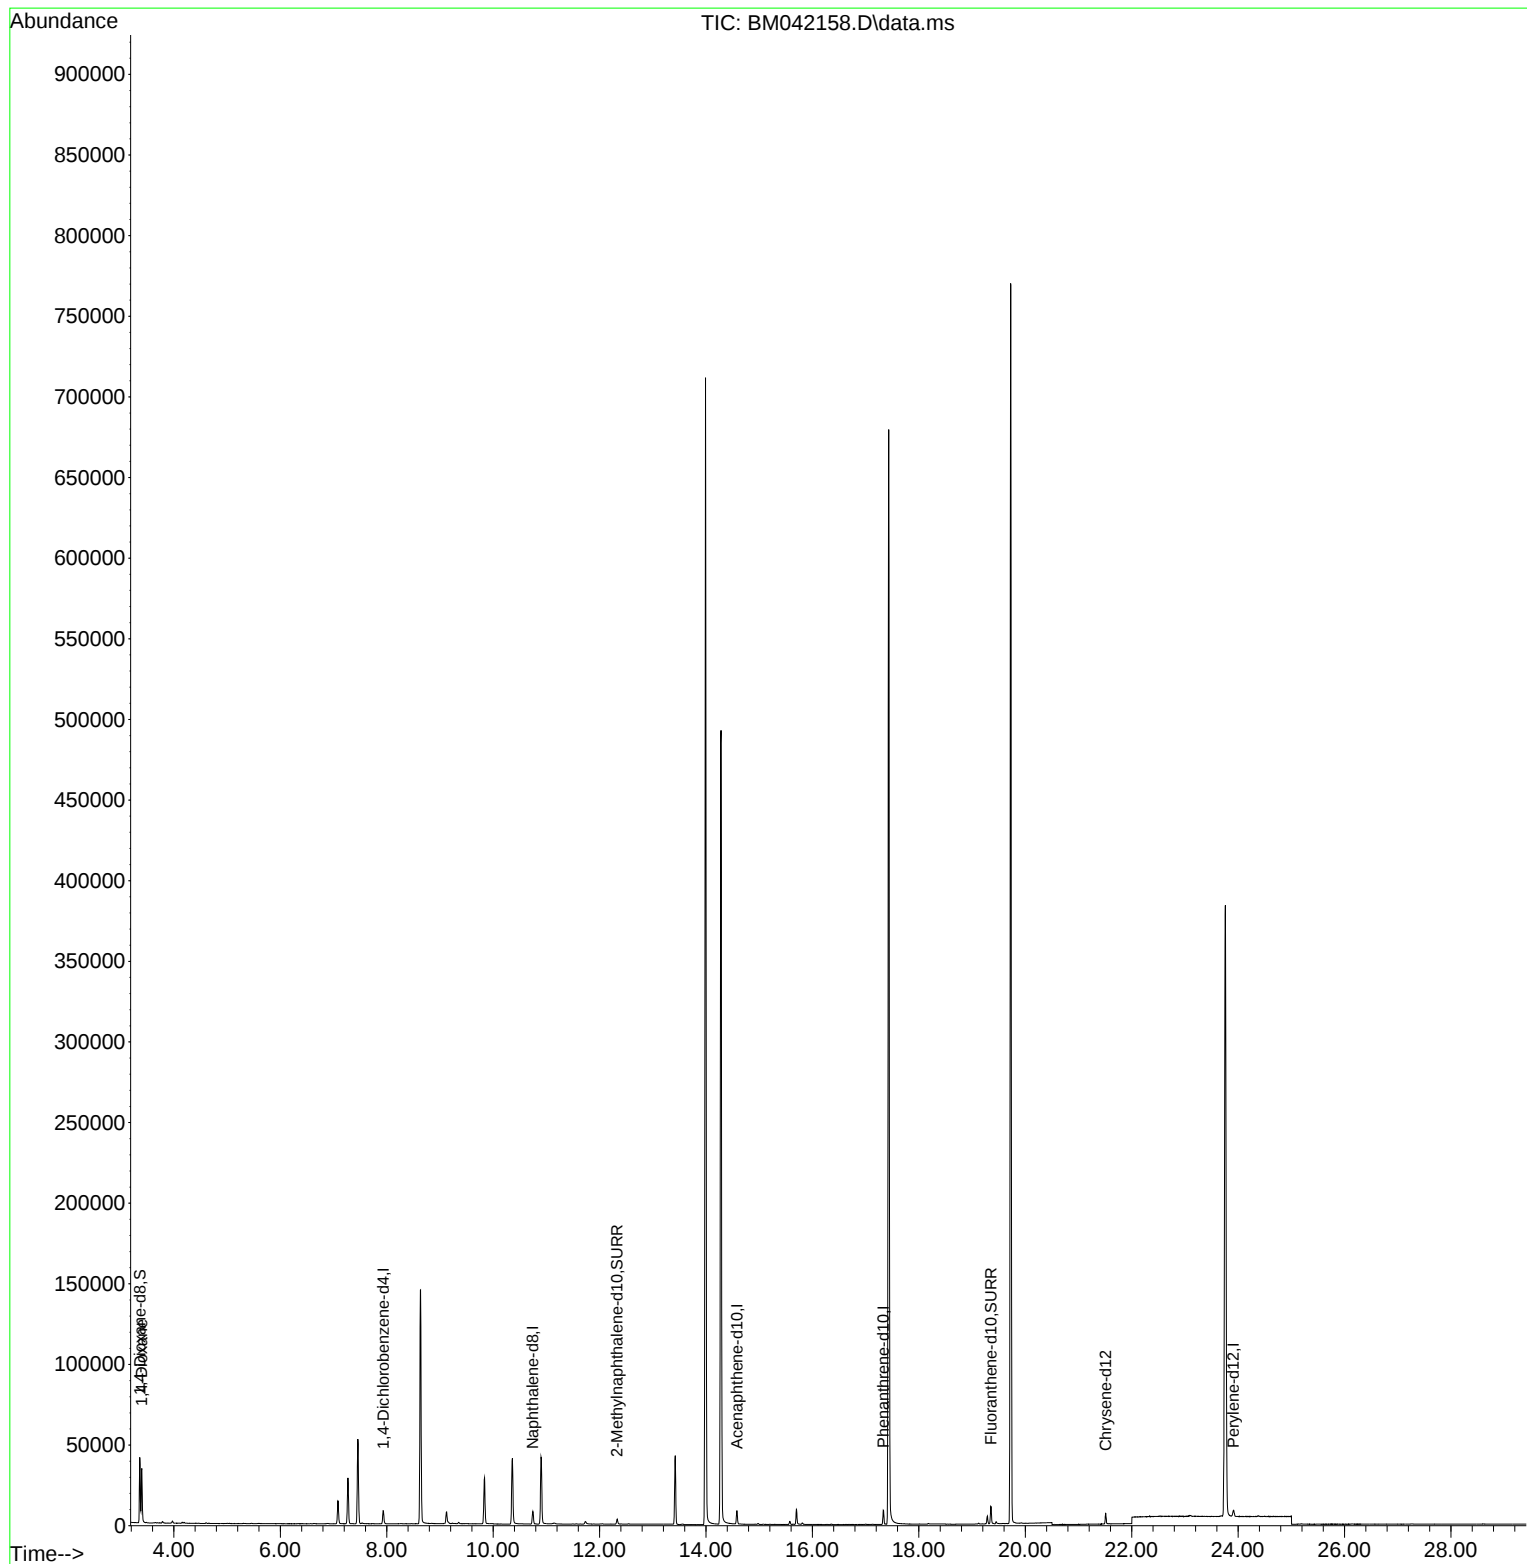

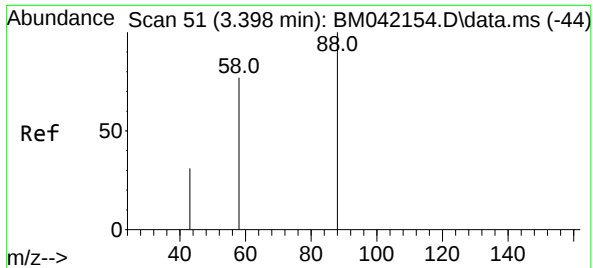

#2
 1,4-Dioxane
 Concen: 3.514 ng/ul
 RT: 3.398 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042158.D
 Acq: 03 Oct 2023 11:32

Instrument :
 BNA_M
 ClientSampleId :
 BBHP4

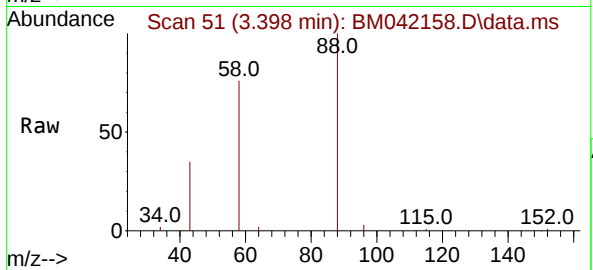

Tgt Ion: 88 Resp: 19586
 Ion Ratio Lower Upper
 88 100
 43 34.7 52.1 78.1#
 58 76.3 53.8 80.6

