

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
 Data File : BM042159.D
 Acq On : 03 Oct 2023 12:09
 Operator : MA/JU
 Sample : 04588-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJE3

Quant Time: Oct 03 13:52:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	4183	0.400	ng/u1	0.00
4) Naphthalene-d8	10.746	136	10064	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.583	164	4449	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.337	188	9199	0.400	ng/u1	0.00
17) Chrysene-d12	21.512	240	4945	0.400	ng/u1	0.00
23) Perylene-d12	23.912	264	5672	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	23956	4.301	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.330	152	4457	0.323	ng/u1	0.00
18) Fluoranthene-d10	19.357	212	7524	0.405	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.397	88	1491	0.256	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
Data File : BM042159.D
Acq On : 03 Oct 2023 12:09
Operator : MA/JU
Sample : 04588-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJE3


Quant Time: Oct 03 13:52:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration

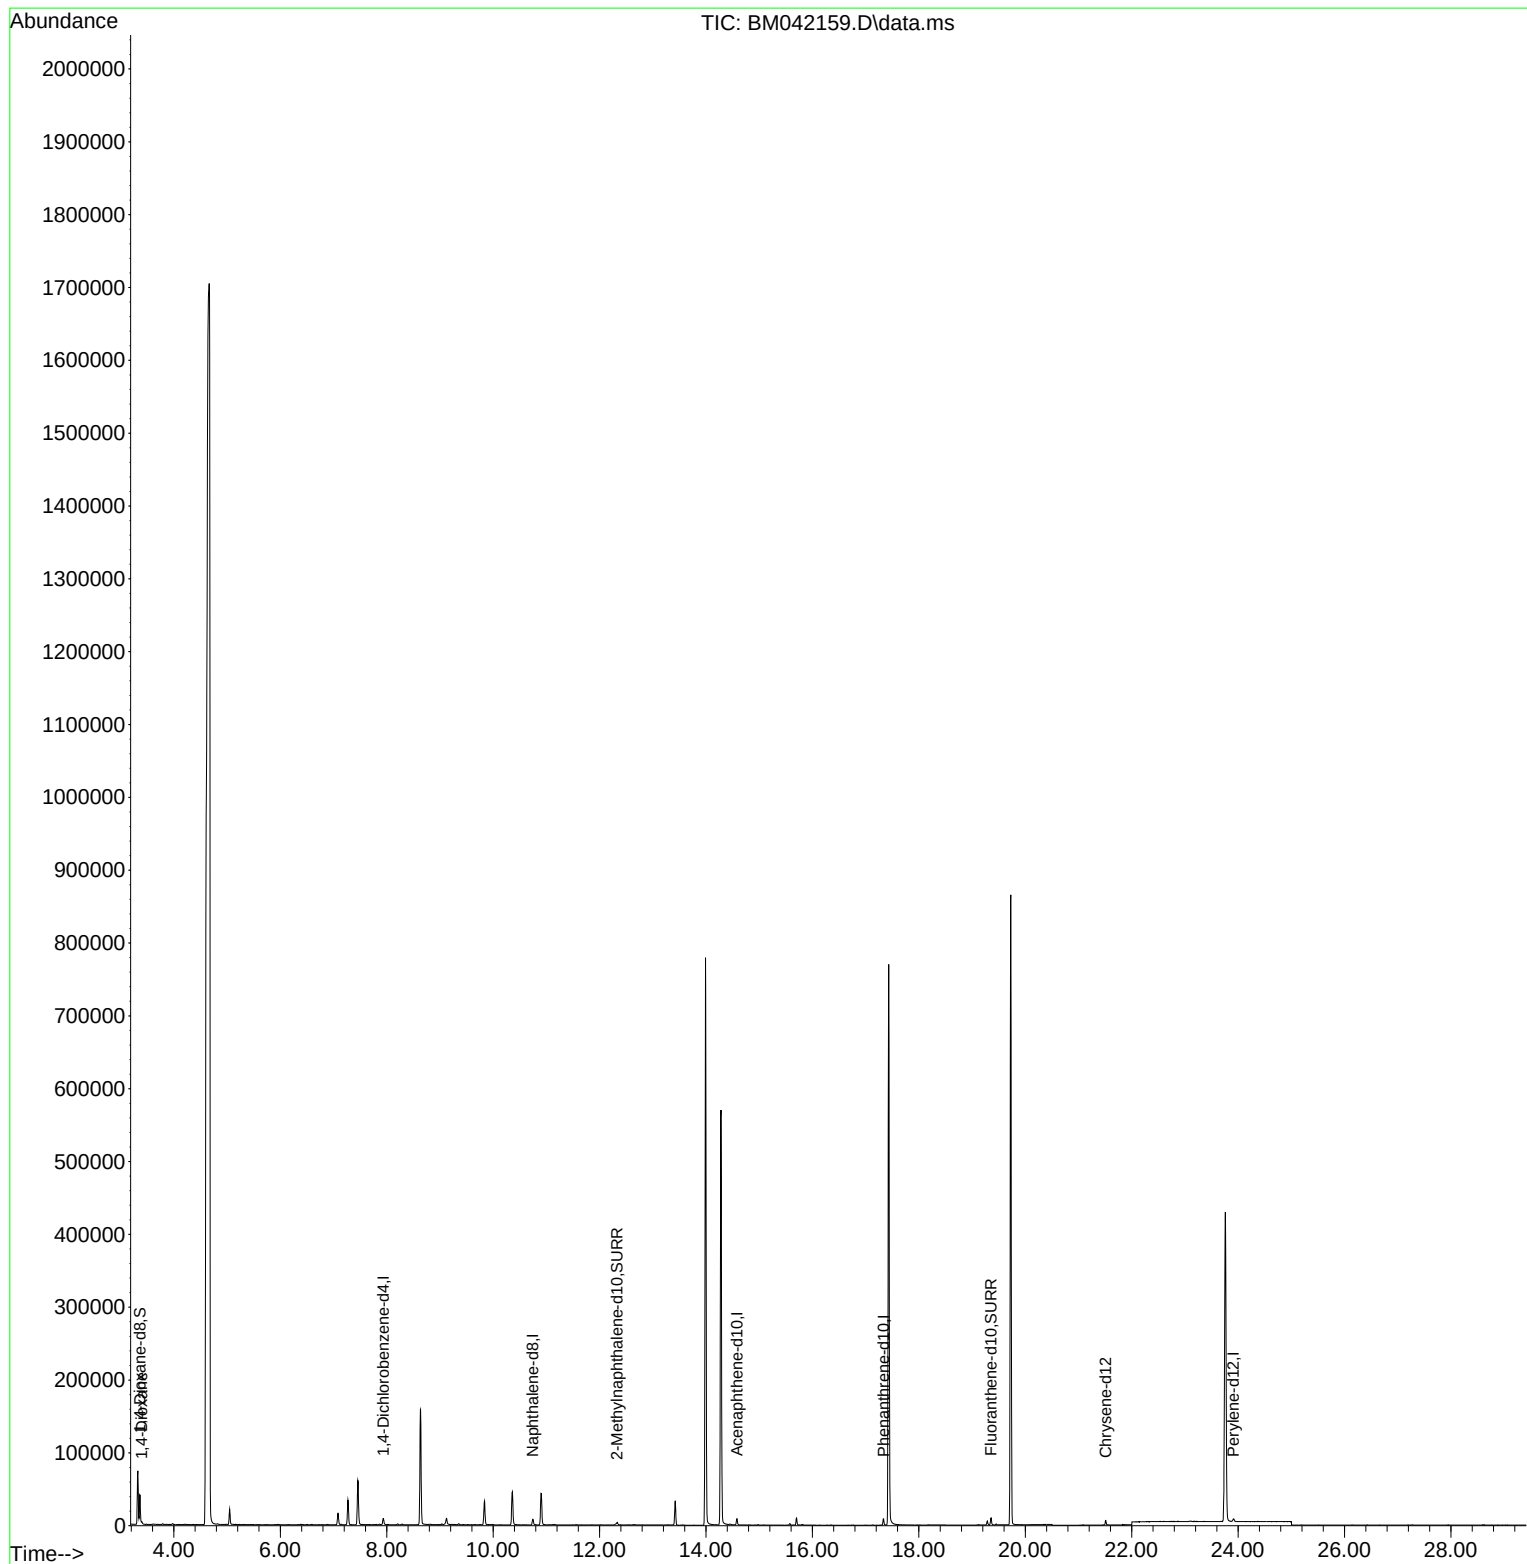

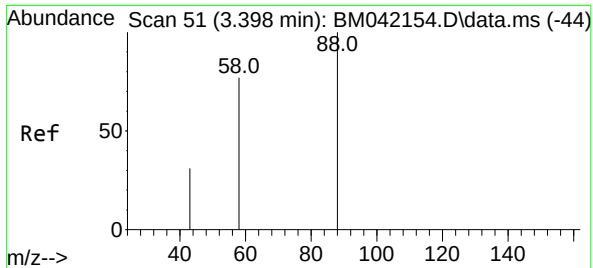

#2
 1,4-Dioxane
 Concen: 0.256 ng/ul
 RT: 3.397 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042159.D
 Acq: 03 Oct 2023 12:09

Instrument :
 BNA_M
 ClientSampleId :
 BBJE3

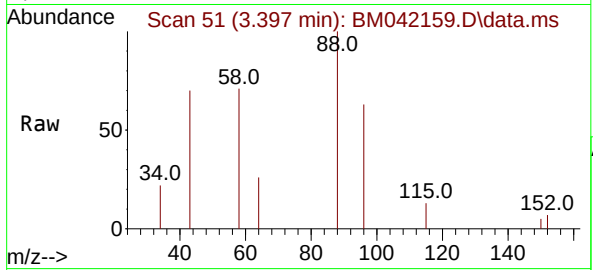

Tgt Ion: 88 Resp: 1491

Ion	Ratio	Lower	Upper
88	100		
43	70.2	52.1	78.1
58	71.2	53.8	80.6

