

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
 Data File : BM042166.D
 Acq On : 03 Oct 2023 16:27
 Operator : MA/JU
 Sample : 04588-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBKH0

Quant Time: Oct 03 17:11:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	4546	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	11769	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.583	164	5047	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.333	188	10550	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.510	240	5269	0.400	ng/ul	0.00
23) Perylene-d12	23.909	264	5933	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	23949	3.956	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	5229	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	8586	0.434	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.398	88	1079	0.171	ng/ul	89
16) Anthracene	17.468	178	1271	0.032	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
Data File : BM042166.D
Acq On : 03 Oct 2023 16:27
Operator : MA/JU
Sample : 04588-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBKH0

Quant Time: Oct 03 17:11:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration




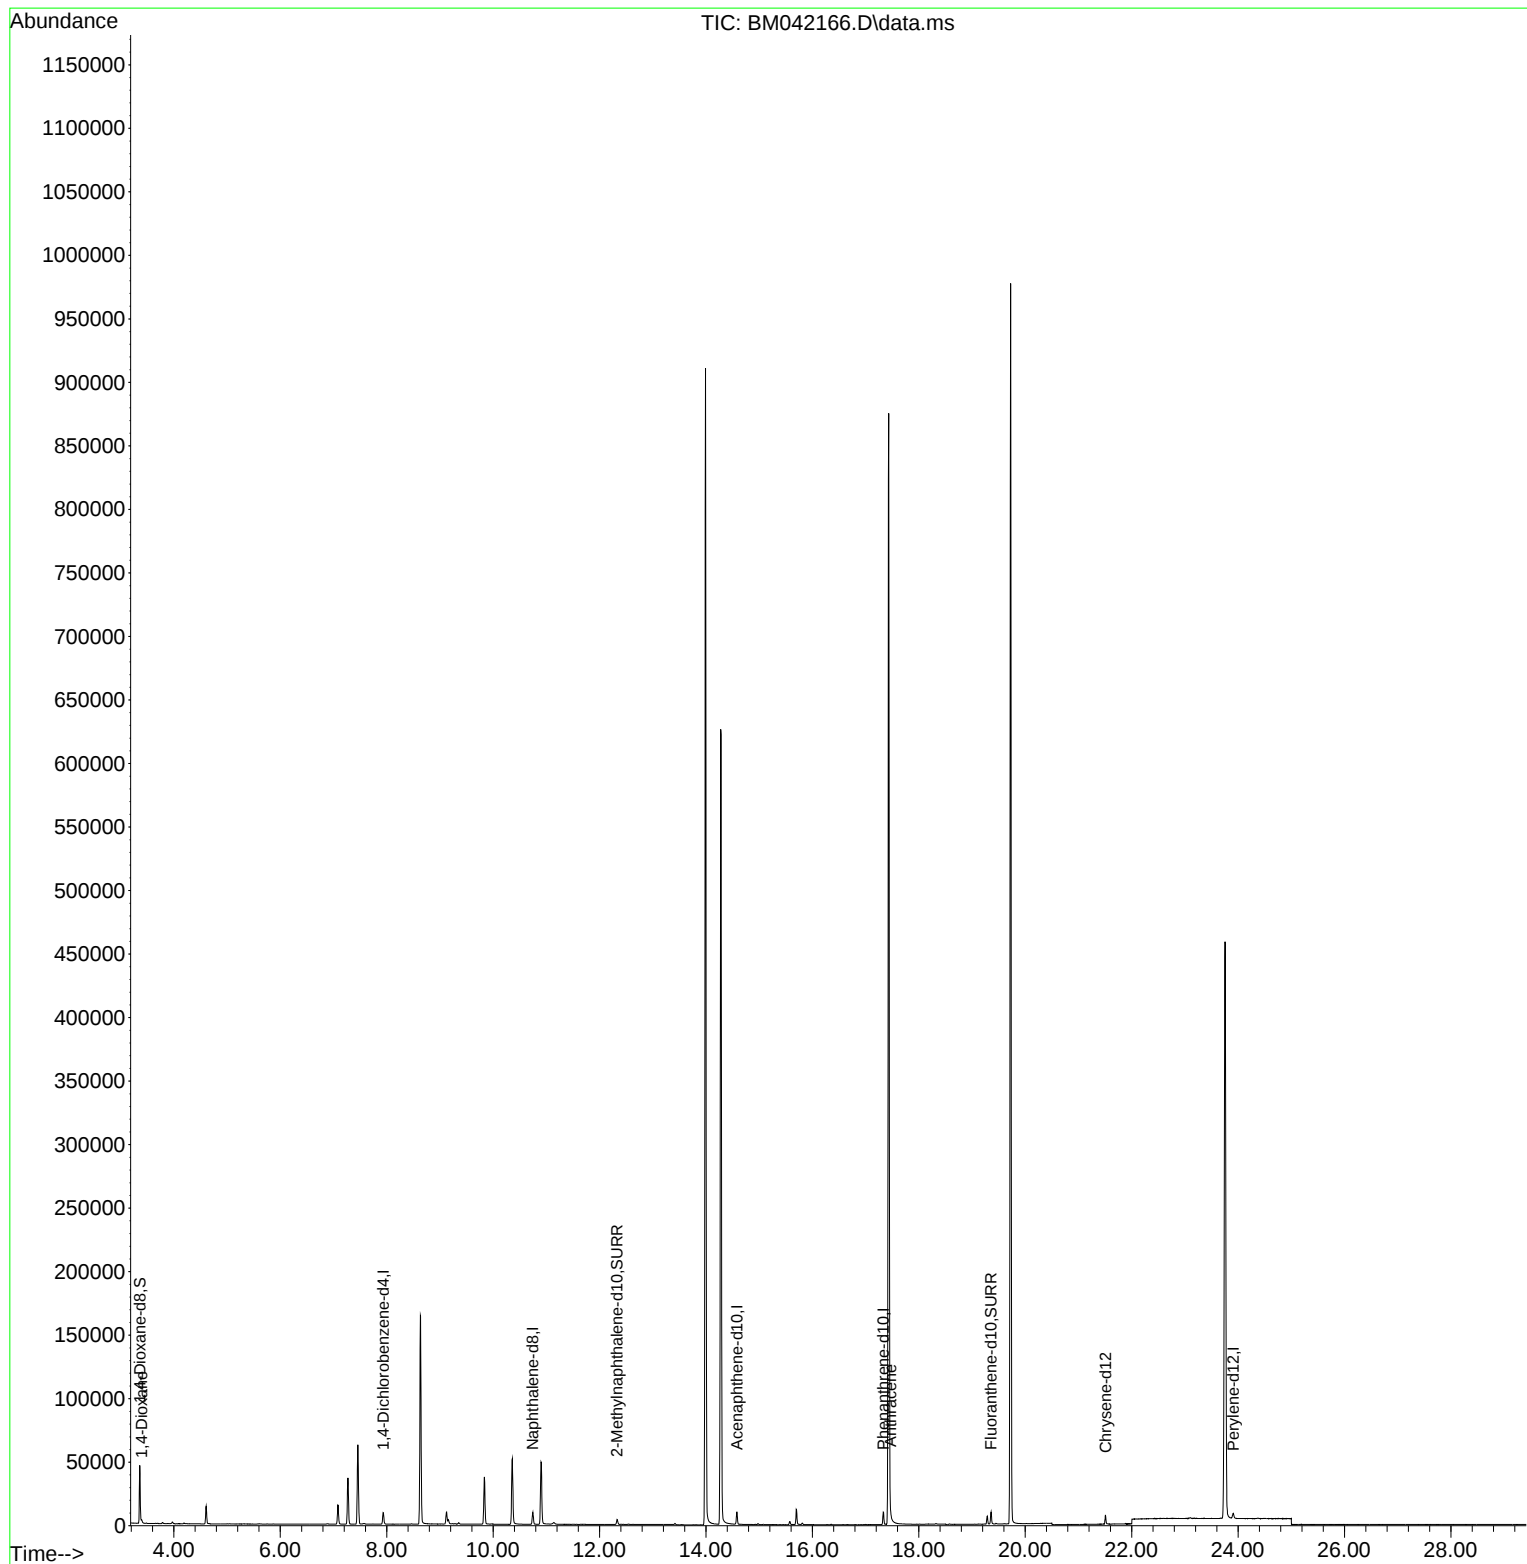


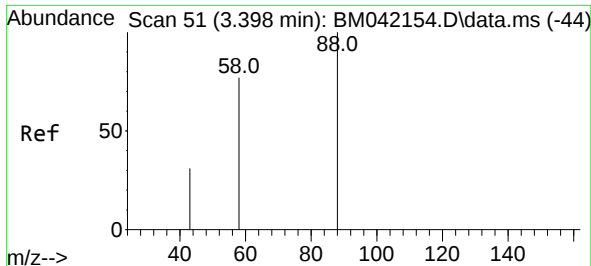

#2
1,4-Dioxane
Concen: 0.171 ng/ul
RT: 3.398 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM042166.D
Acq: 03 Oct 2023 16:27

Instrument :
BNA_M
ClientSampleId :
BBKH0

Tgt Ion: 88 Resp: 1079
Ion Ratio Lower Upper
88 100
43 77.5 52.1 78.1
58 72.2 53.8 80.6

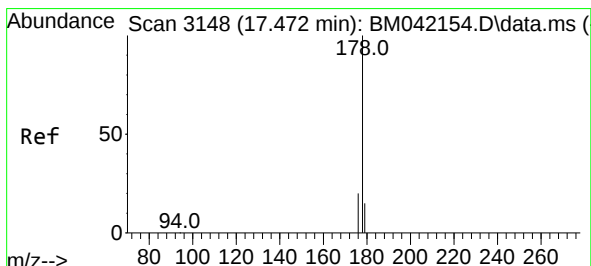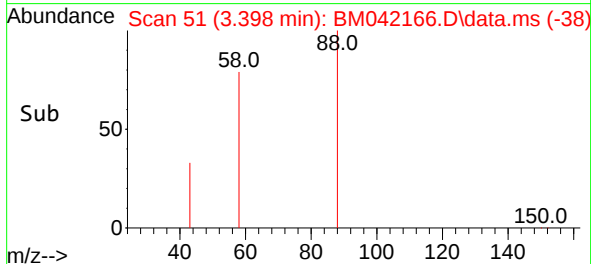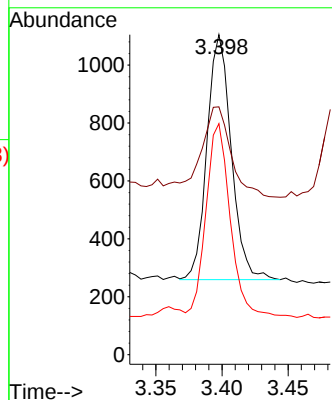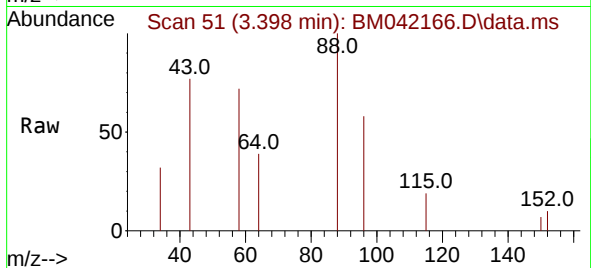

#16
Anthracene
Concen: 0.032 ng/ul
RT: 17.468 min Scan# 3147
Delta R.T. -0.008 min
Lab File: BM042166.D
Acq: 03 Oct 2023 16:27

Tgt Ion: 178 Resp: 1271
Ion Ratio Lower Upper
178 100
179 27.2 12.9 19.3#
176 27.0 16.3 24.5#

