

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
 Data File : BM042167.D
 Acq On : 03 Oct 2023 17:04
 Operator : MA/JU
 Sample : 04571-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHL4

Quant Time: Oct 03 17:48:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	4342	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	11279	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.578	164	4923	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.333	188	10153	0.400	ng/ul	0.00
17) Chrysene-d12	21.507	240	5093	0.400	ng/ul	0.00
23) Perylene-d12	23.909	264	5686	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	24387	4.218	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	4782	0.309	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	7891	0.413	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.398	88	11930	1.976	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100323\
Data File : BM042167.D
Acq On : 03 Oct 2023 17:04
Operator : MA/JU
Sample : 04571-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHL4


Quant Time: Oct 03 17:48:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration

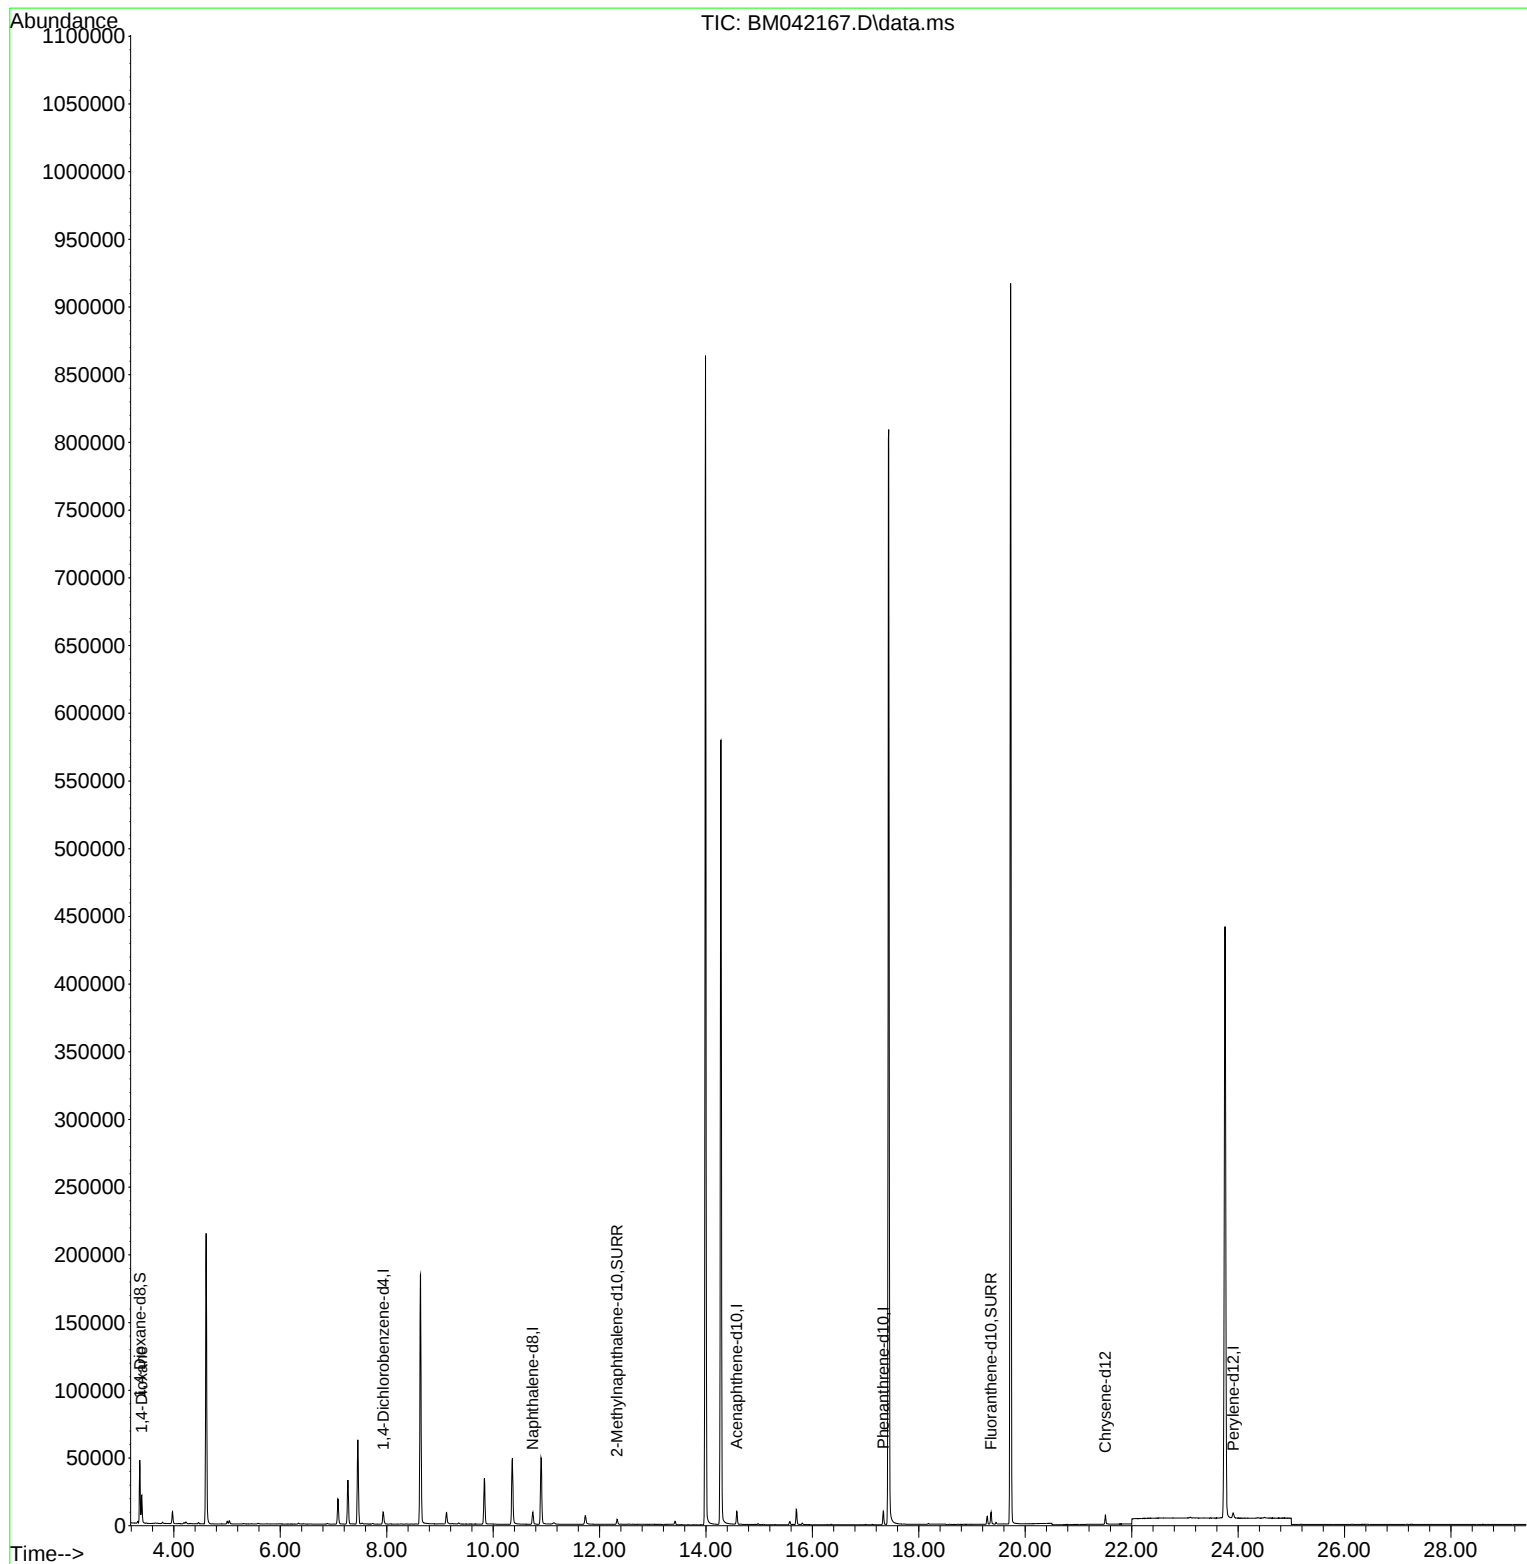

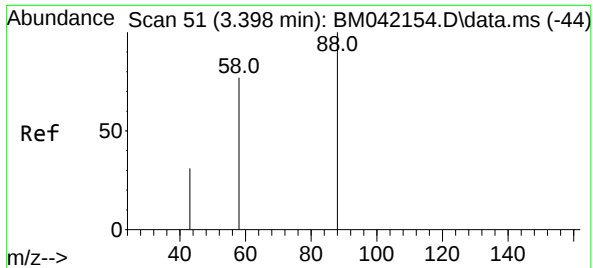

#2
 1,4-Dioxane
 Concen: 1.976 ng/ul
 RT: 3.398 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042167.D
 Acq: 03 Oct 2023 17:04

Instrument :
 BNA_M
 ClientSampleId :
 BBHL4

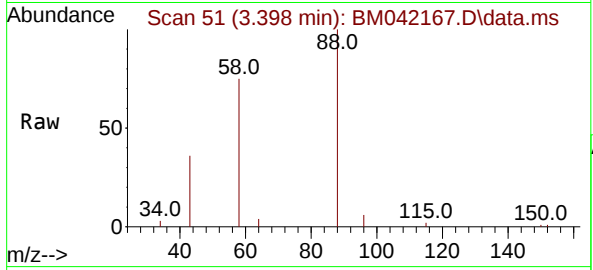

Tgt Ion: 88 Resp: 11930

Ion	Ratio	Lower	Upper
88	100		
43	36.3	52.1	78.1#
58	75.3	53.8	80.6

