


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM100422\  
 Data File : BM036824.D  
 Acq On : 04 Oct 2022 09:58  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM100322.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Oct 04 03:17:03 2022

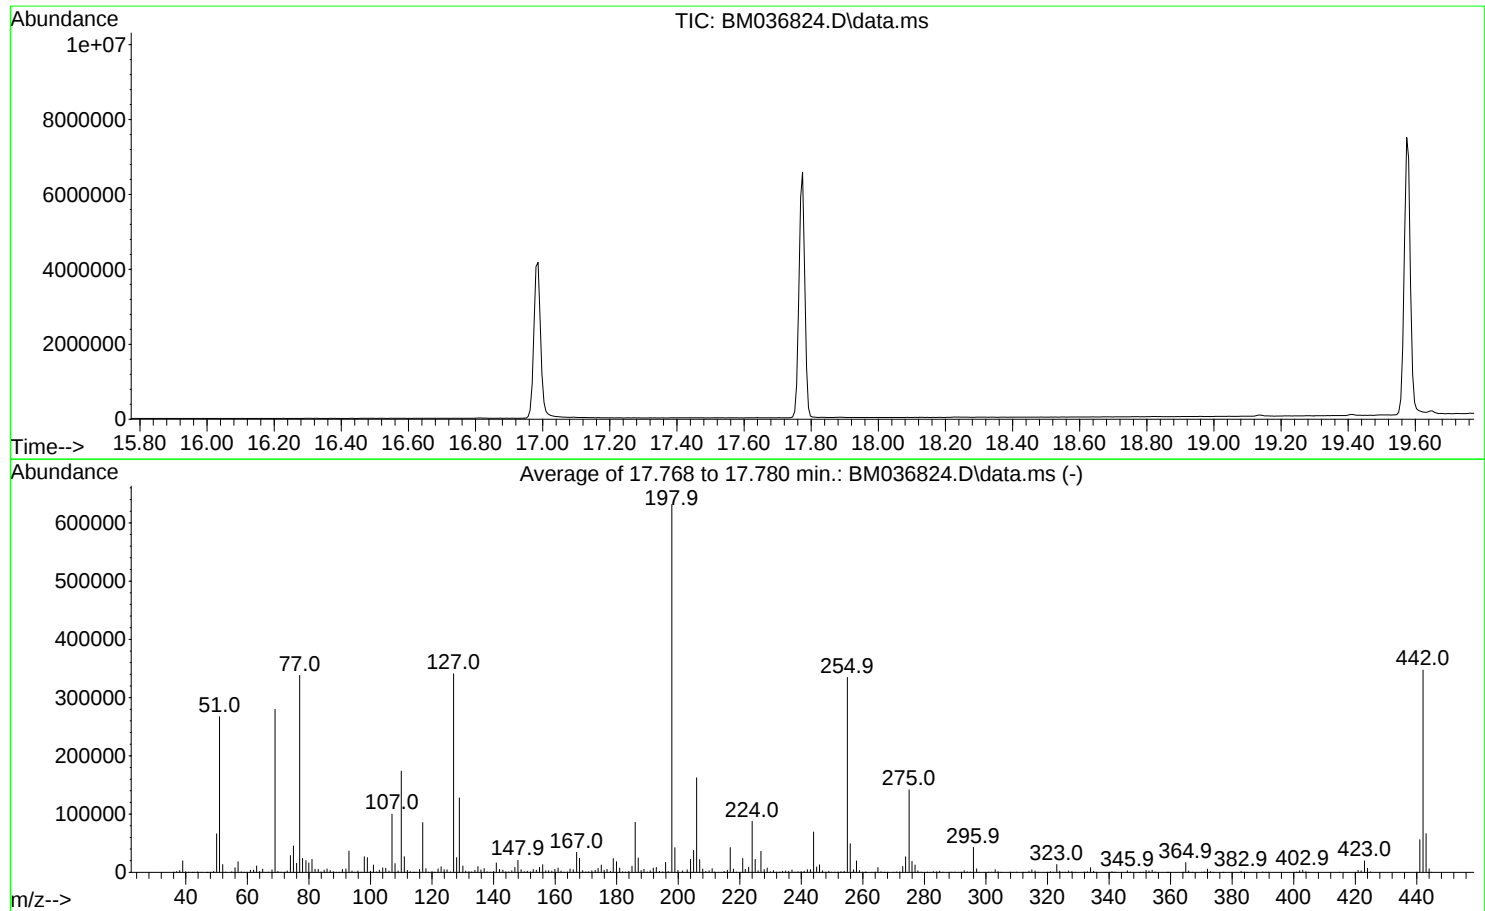




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 42.3         | 267347     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 4305       | PASS                |
| 69             | 198             | 0.00            | 100             | 44.3         | 279788     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 1624       | PASS                |
| 127            | 198             | 10              | 80              | 54.0         | 340779     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 1545       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 631509     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 42181      | PASS                |
| 275            | 198             | 10              | 60              | 22.5         | 141779     | PASS                |
| 365            | 198             | 1               | 100             | 2.7          | 16849      | PASS                |
| 441            | 198             | 0.01            | 100             | 8.9          | 56144      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 347264     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 66451      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM100422\  
Data File : BM036824.D  
Acq On : 04 Oct 2022 09:58  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Oct 04 22:40:16 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM100322.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 04 03:17:03 2022  
Response via : Initial Calibration

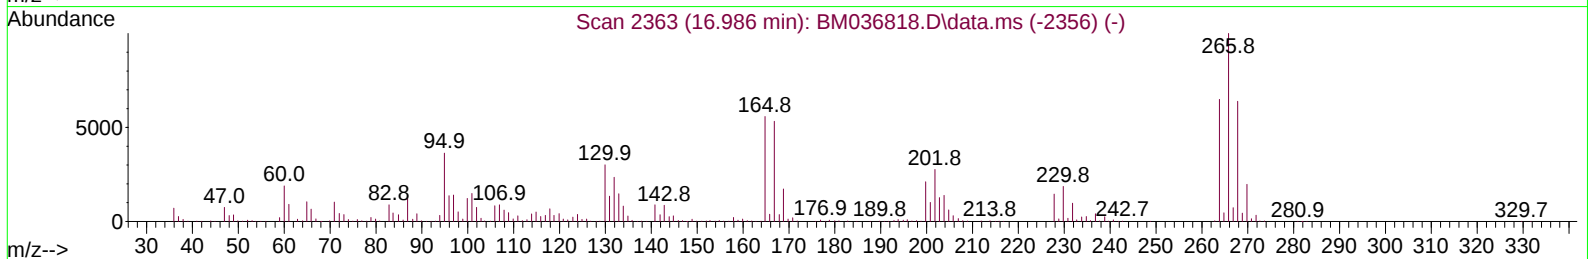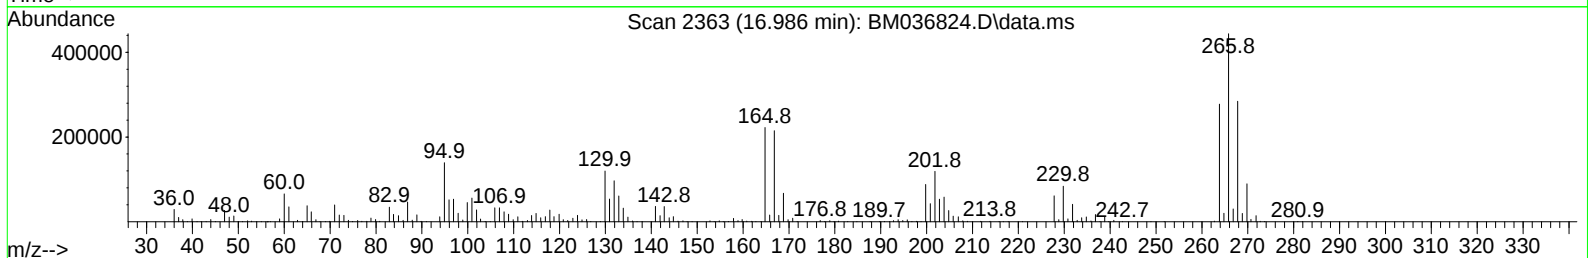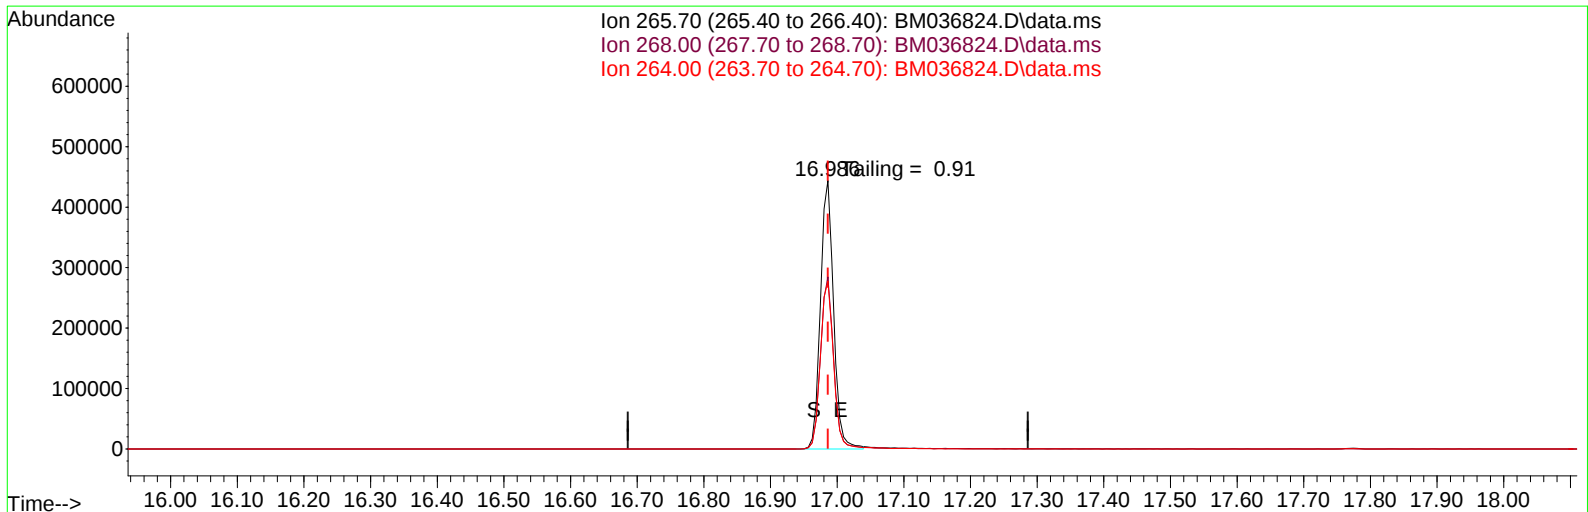

TIC: BM036824.D\data.ms

**(70) Pentachlorophenol (C)**

**16.986min (+ 0.000) 847081.38 ng**




**response 615821**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.90  | 64.08  |
| 264.00 | 64.90  | 62.53  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM100422\  
Data File : BM036824.D  
Acq On : 04 Oct 2022 09:58  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Oct 04 22:40:16 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM100322.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 04 03:17:03 2022  
Response via : Initial Calibration

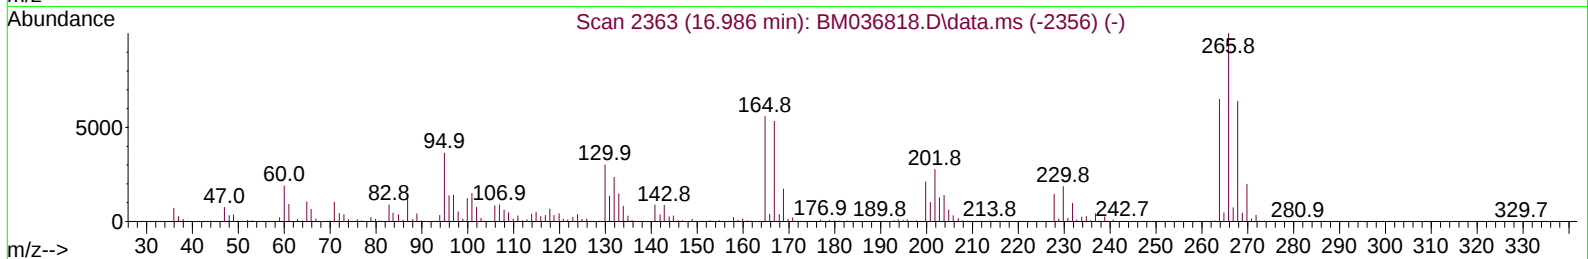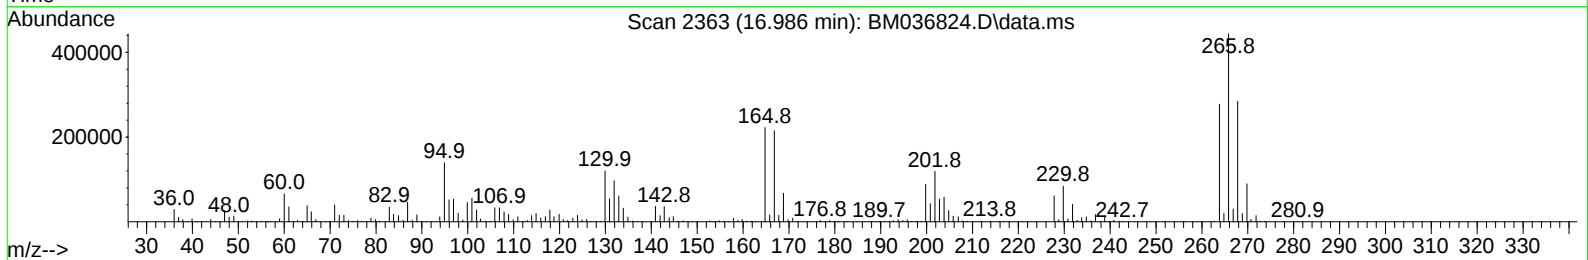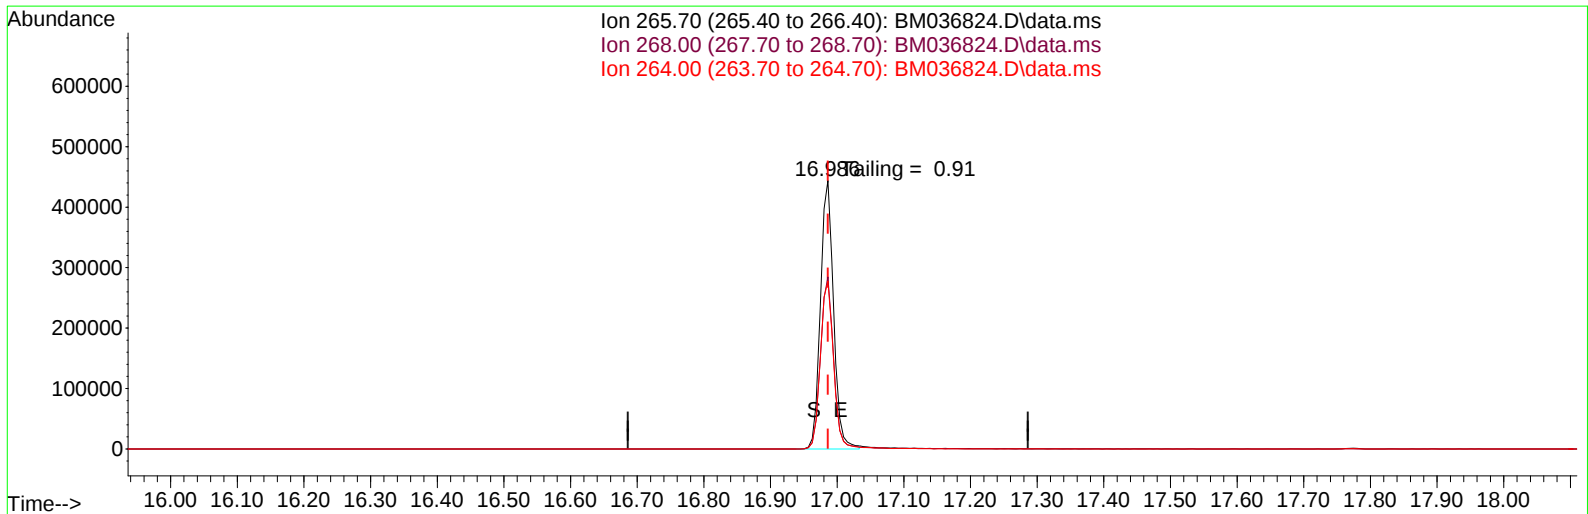

TIC: BM036824.D\data.ms

**(70) Pentachlorophenol (C)**

**16.986min (+ 0.000) 847081.38 ng**

**response 615821**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.90  | 64.08  |
| 264.00 | 64.90  | 62.53  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/4/2022     | BNA_M            | <u>BM036824.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1869730          | 20.803             |
| DDD           | 17057            | 20.362             |
| DDE           | 1457             | 19.862             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 18514         | 1888244          | 0.98               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP