

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
 Data File : BM042195.D
 Acq On : 04 Oct 2023 20:36
 Operator : MA/JU
 Sample : 04469-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EZYP6

Quant Time: Oct 05 01:55:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	3475	0.400	ng/ul	0.00
4) Naphthalene-d8	10.741	136	9989	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.578	164	4398	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.333	188	8975	0.400	ng/ul	0.00
17) Chrysene-d12	21.504	240	4631	0.400	ng/ul	-0.01
23) Perylene-d12	23.903	264	5166	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	20383	4.405	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.324	152	3366	0.246	ng/ul	-0.01
18) Fluoranthene-d10	19.352	212	6413	0.369	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	1023	0.212	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
Data File : BM042195.D
Acq On : 04 Oct 2023 20:36
Operator : MA/JU
Sample : 04469-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EZYP6

Quant Time: Oct 05 01:55:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration

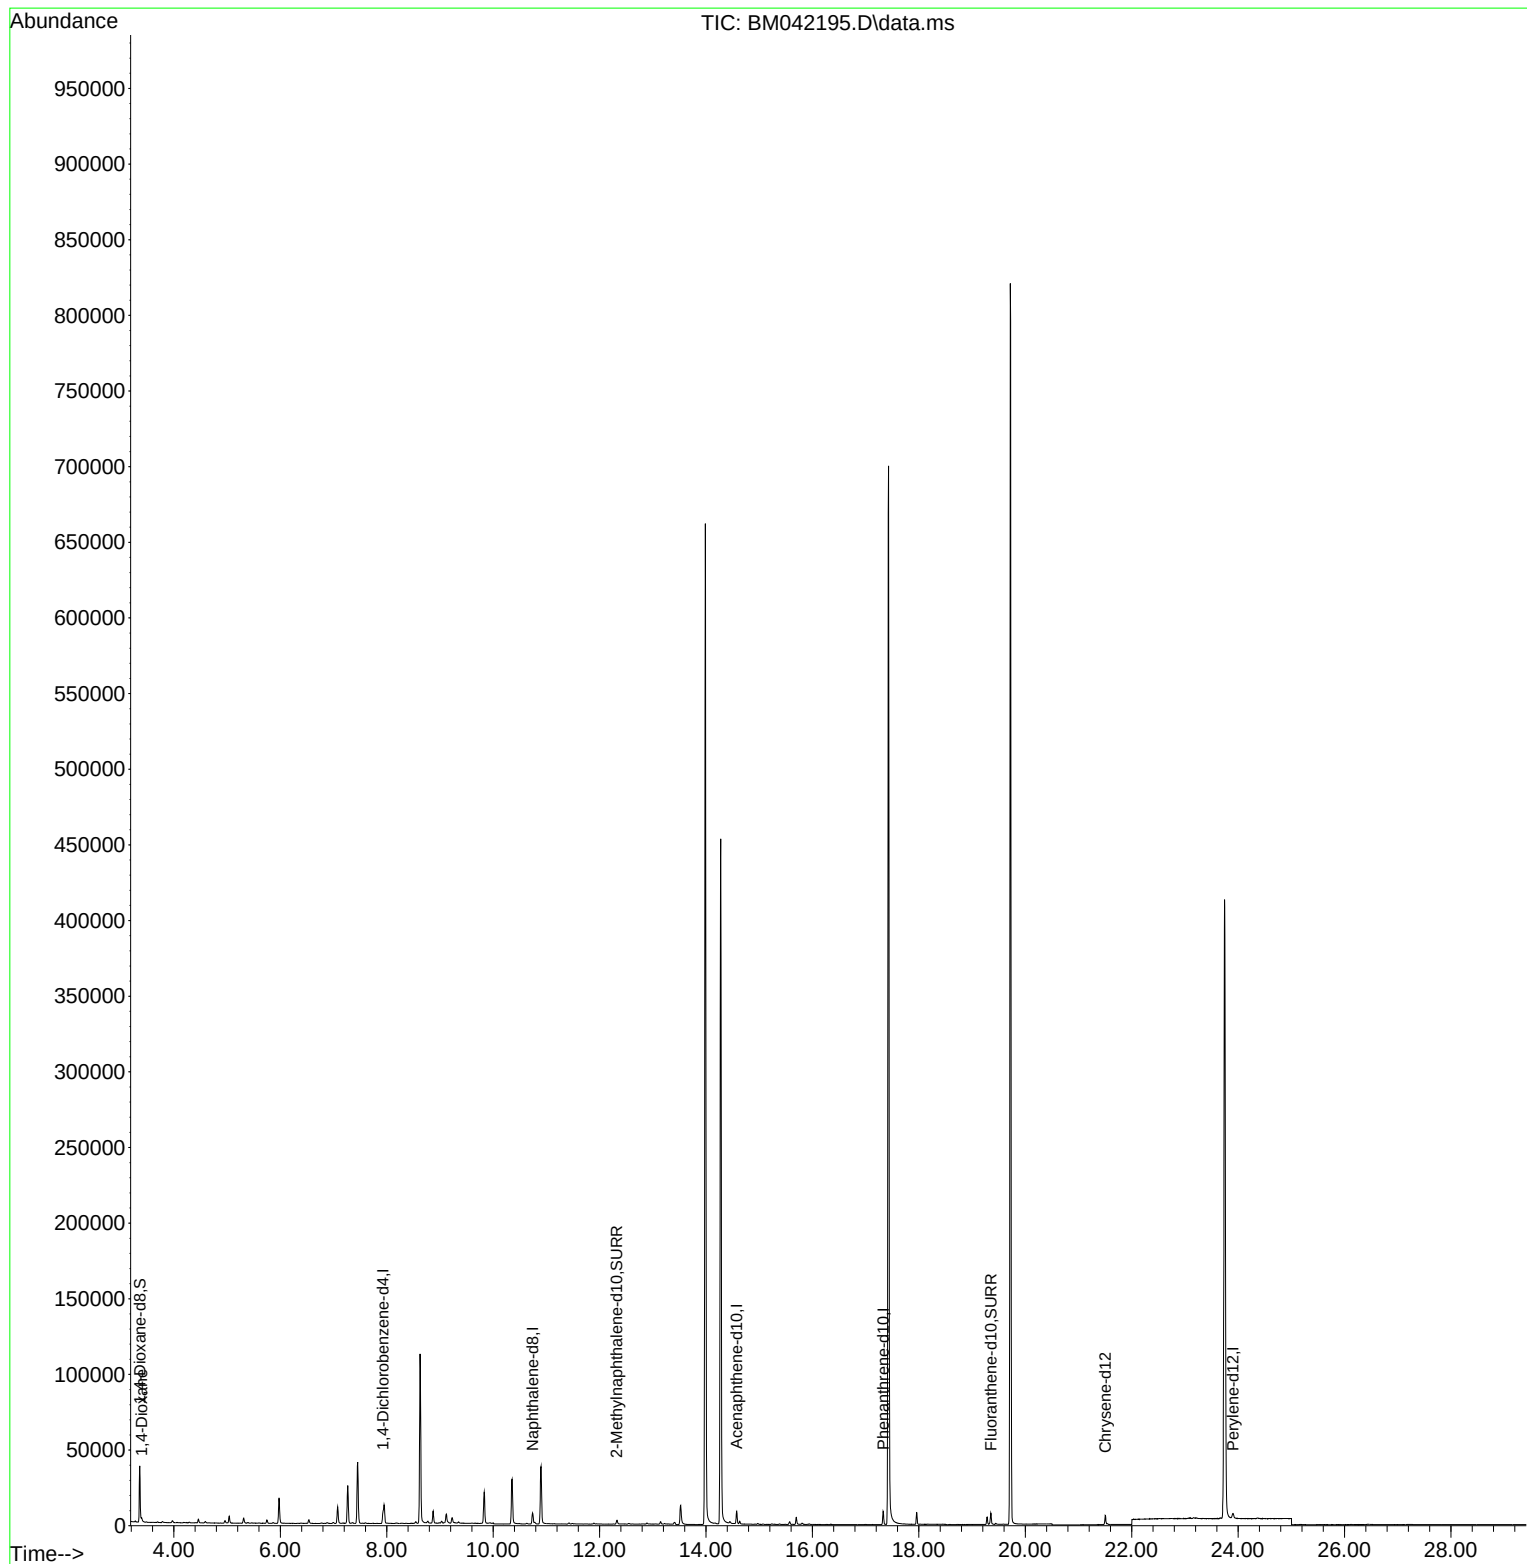

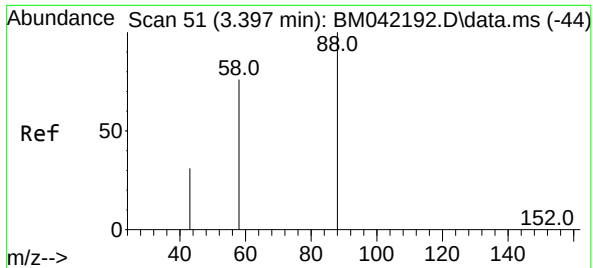

#2
 1,4-Dioxane
 Concen: 0.212 ng/ul
 RT: 3.397 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042195.D
 Acq: 04 Oct 2023 20:36

Instrument :
 BNA_M
 ClientSampleId :
 EZYP6

Tgt Ion: 88 Resp: 1023

Ion	Ratio	Lower	Upper
88	100		
43	66.8	52.1	78.1
58	51.8	53.8	80.6

