

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
 Data File : BM042201.D
 Acq On : 05 Oct 2023 00:19
 Operator : MA/JU
 Sample : 04588-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBK29

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/05/2023
 Supervised By :mohammad ahmed 10/06/2023

Quant Time: Oct 05 01:55:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	3398	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.741	136	9100	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.574	164	4877	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.329	188	10691	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.501	240	6358	0.400	ng/ul	-0.01
23) Perylene-d12	23.901	264	7016	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	20271	4.480	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.324	152	4513	0.362	ng/ul	-0.01
18) Fluoranthene-d10	19.352	212	7961	0.334	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.393	88	8208	1.737	ng/ul	89
5) Naphthalene	10.790	128	175733	5.788	ng/ul	99
7) 2-Methylnaphthalene	12.396	142	131389	7.228	ng/ul	98
8) 1-Methylnaphthalene	12.616	142	130934	7.151	ng/ul	99
10) Acenaphthylene	14.291	152	3072	0.100	ng/ul#	1
11) Acenaphthene	14.638	153	10932	0.469	ng/ul	93
12) Fluorene	15.628	166	14688	0.559	ng/ul#	92
15) Phenanthrene	17.371	178	33085	0.751	ng/ul#	93
16) Anthracene	17.464	178	2882	0.071	ng/ul#	55
19) Fluoranthene	19.380	202	3734	0.077	ng/ul#	75
20) Pyrene	19.747	202	12329m	0.240	ng/ul	
21) Benzo(a)anthracene	21.483	228	3033	0.074	ng/ul#	64
22) Chrysene	21.539	228	4631m	0.116	ng/ul	
24) Benzo(b)fluoranthene	23.161	252	1862	0.045	ng/ul#	4
26) Benzo(a)pyrene	23.793	252	1396	0.039	ng/ul#	18
29) Benzo(g,h,i)perylene	27.159	276	1600	0.038	ng/ul#	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
Data File : BM042201.D
Acq On : 05 Oct 2023 00:19
Operator : MA/JU
Sample : 04588-20
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BBK29

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2023
Supervised By :mohammad ahmed 10/06/2023


Quant Time: Oct 05 01:55:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration

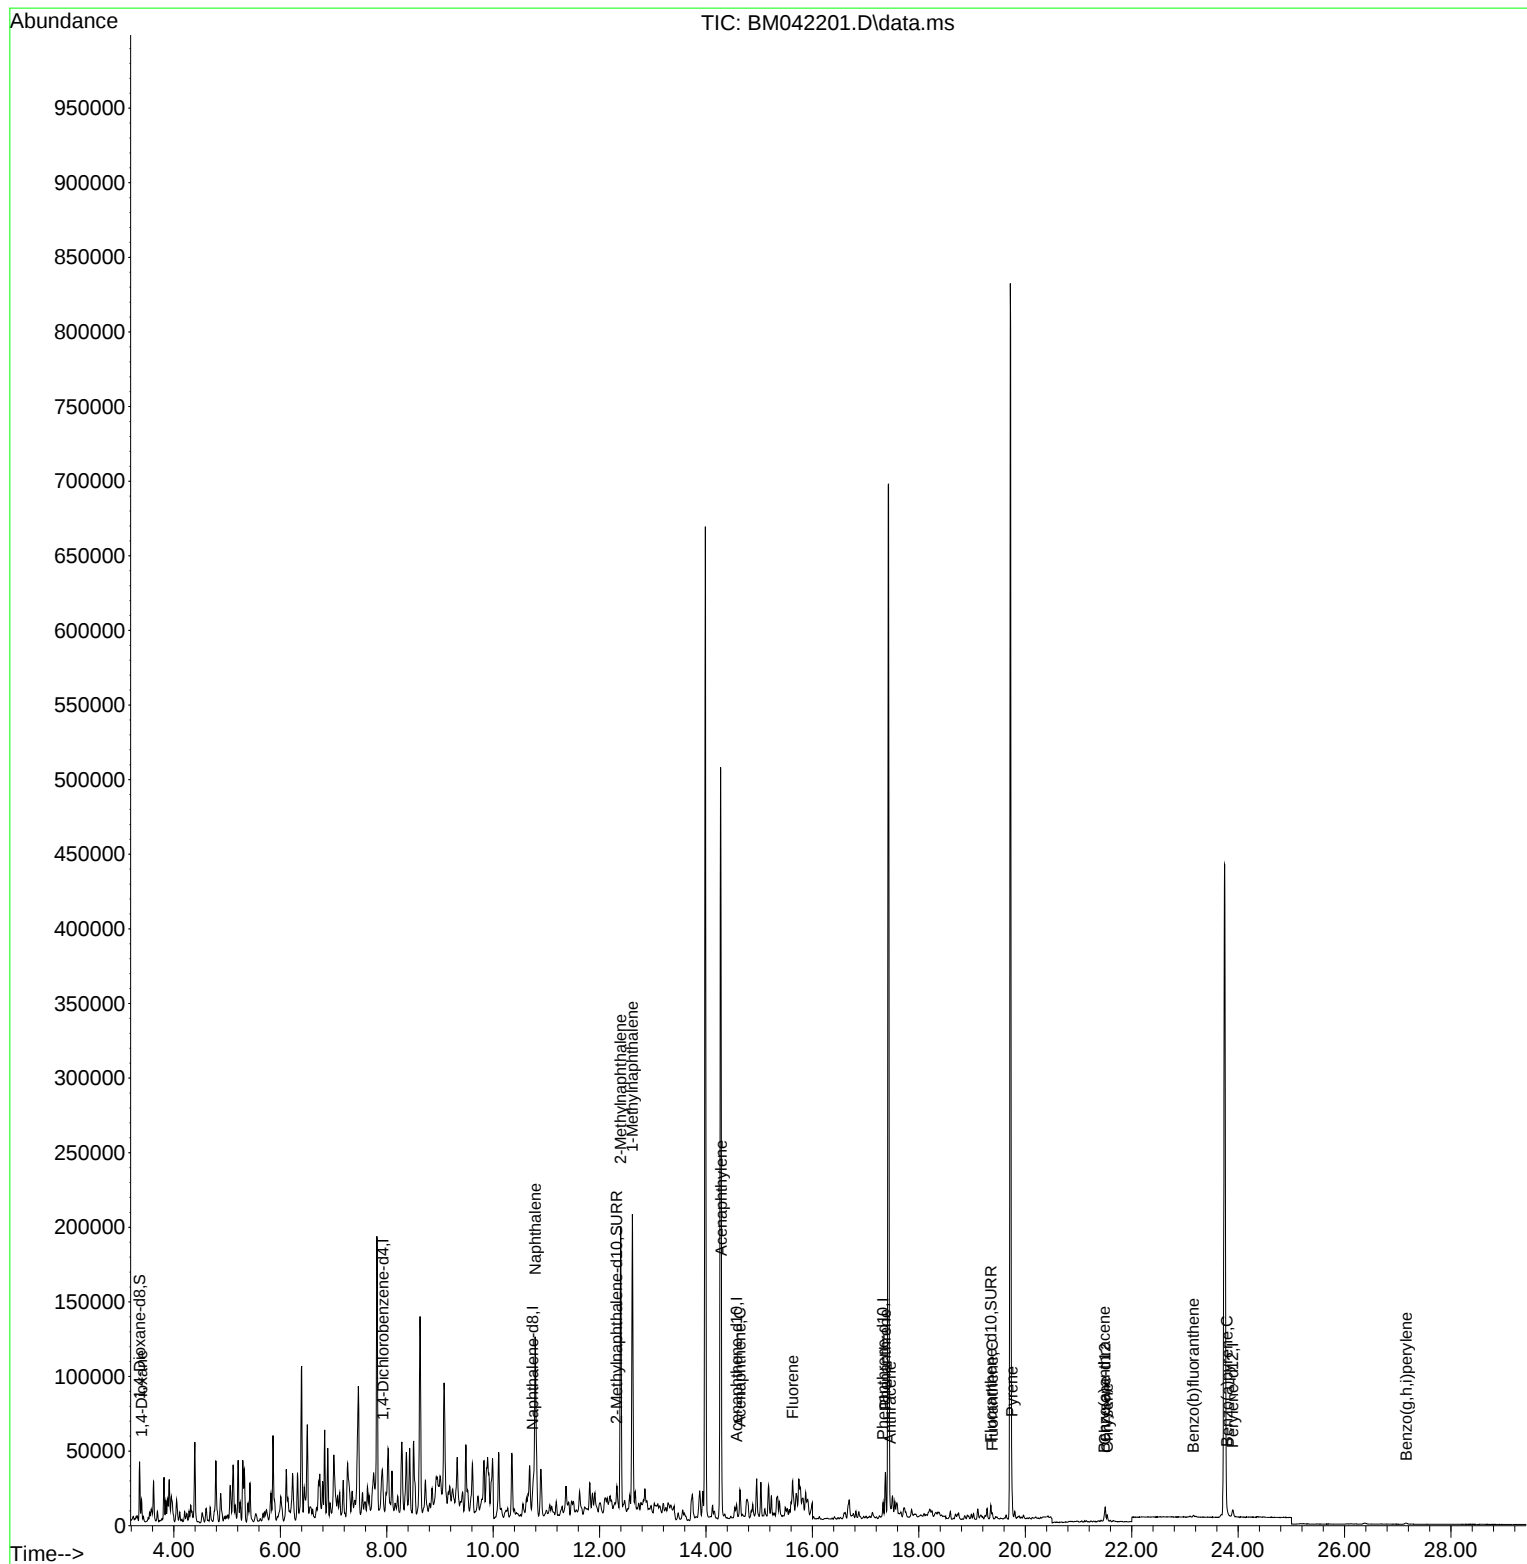



#2
1,4-Dioxane
Concen: 1.737 ng/ul
RT: 3.393 min Scan# 50
Delta R.T. -0.008 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19




Instrument :
BNA_M
ClientSampleId :
BBK29




Tgt Ion: 88 Resp: 8208
Ion Ratio Lower Upper
88 100
43 57.2 52.1 78.1
58 76.3 53.8 80.6

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 10/05/2023
Supervised By :mohammad ahmed 10/06/2023

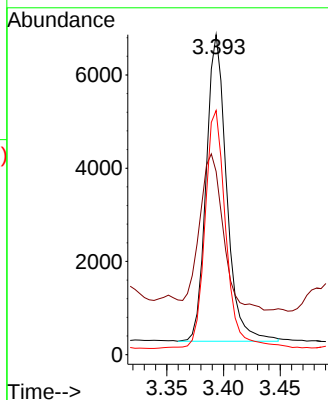


#5
Naphthalene
Concen: 5.788 ng/ul
RT: 10.790 min Scan# 1763
Delta R.T. -0.011 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19




Tgt Ion:128 Resp: 175733
Ion Ratio Lower Upper
128 100
129 11.4 9.4 14.2
127 13.2 11.0 16.4

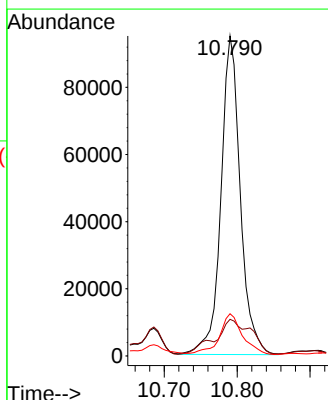



#7
2-Methylnaphthalene
Concen: 7.228 ng/ul
RT: 12.396 min Scan# 2055
Delta R.T. -0.011 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19




Instrument :
BNA_M
ClientSampleId :
BBK29




Tgt Ion:142 Resp: 131389
Ion Ratio Lower Upper
142 100
141 89.5 70.2 105.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 10/05/2023
Supervised By :mohammad ahmed 10/06/2023

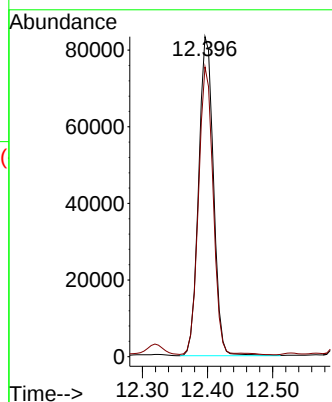


#8
1-Methylnaphthalene
Concen: 7.151 ng/ul
RT: 12.616 min Scan# 2095
Delta R.T. -0.011 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19




Tgt Ion:142 Resp: 130934
Ion Ratio Lower Upper
142 100
141 91.4 73.5 110.3

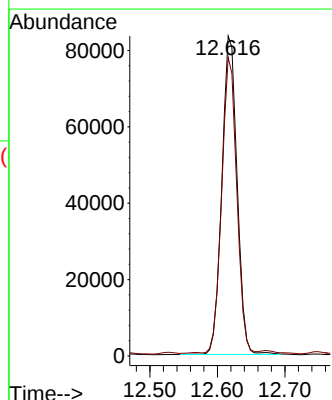



#10
Acenaphthylene
Concen: 0.100 ng/u1
RT: 14.291 min Scan# 2435
Delta R.T. -0.023 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19




Instrument :
BNA_M
ClientSampleId :
BBK29



Tgt Ion:152 Resp: 3072
Ion Ratio Lower Upper
152 100
151 78.3 16.4 24.6
153 108.2 10.9 16.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/05/2023
Supervised By :mohammad ahmed 10/06/2023

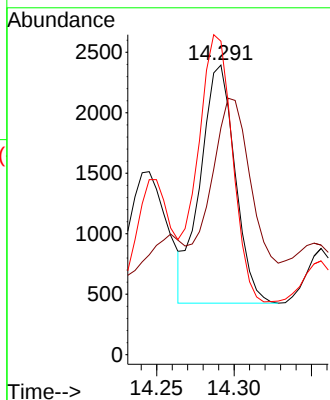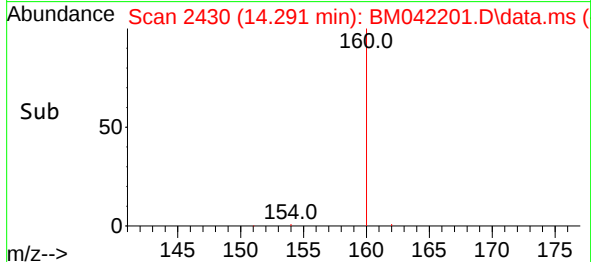

#11
Acenaphthene
Concen: 0.469 ng/u1
RT: 14.638 min Scan# 2505
Delta R.T. -0.009 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19


Tgt Ion:153 Resp: 10932
Ion Ratio Lower Upper
153 100
152 57.7 41.1 61.7
154 82.2 69.5 104.3

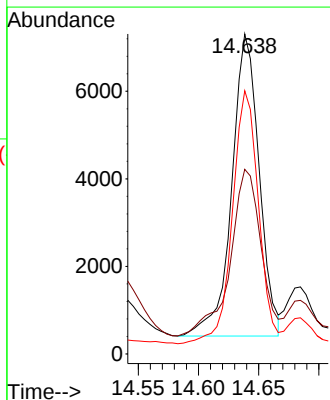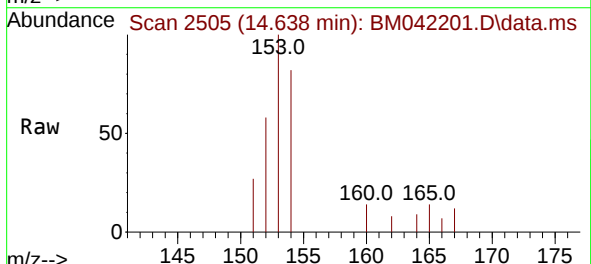



#12
Fluorene
Concen: 0.559 ng/ul
RT: 15.628 min Scan# 2719
Delta R.T. -0.009 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19




Instrument :
BNA_M
ClientSampleId :
BBK29



Tgt Ion:166 Resp: 1468
Ion Ratio Lower Upper
166 100
165 104.8 78.4 117.6
167 20.0 11.5 17.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/05/2023
Supervised By :mohammad ahmed 10/06/2023

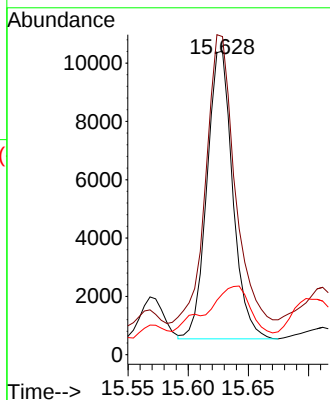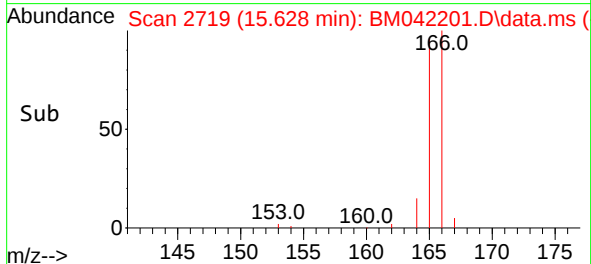

#15
Phenanthrene
Concen: 0.751 ng/ul
RT: 17.371 min Scan# 3124
Delta R.T. -0.013 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19

Tgt Ion:178 Resp: 33085
Ion Ratio Lower Upper
178 100
179 21.9 13.0 19.4#
176 22.1 16.8 25.2

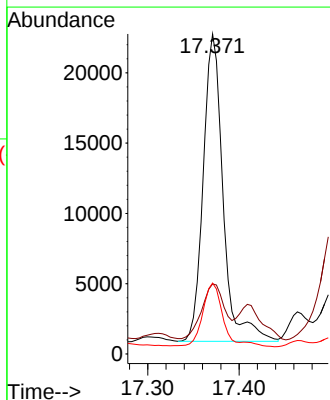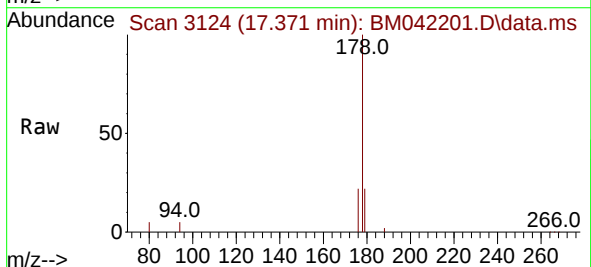



#16

Anthracene

Concen: 0.071 ng/ul

RT: 17.464 min Scan# 3146

Delta R.T. -0.013 min

Lab File: BM042201.D

Acq: 05 Oct 2023 00:19

Instrument :

BNA_M

ClientSampleId :

BBK29





Tgt Ion:178	Resp:	288
Ion Ratio	Lower	Upper
178	100	
179	46.3	12.9 19.3
176	31.9	16.3 24.5

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 10/05/2023

Supervised By :mohammad ahmed 10/06/2023

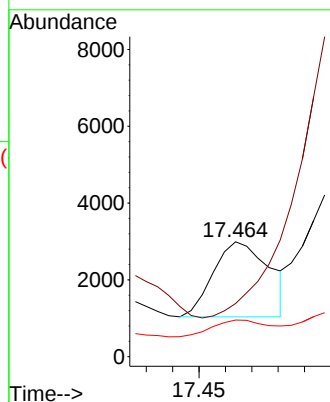

#19

Fluoranthene

Concen: 0.077 ng/ul




RT: 19.380 min Scan# 3581


Delta R.T. -0.014 min

Lab File: BM042201.D

Acq: 05 Oct 2023 00:19

Tgt Ion:202	Resp:	3734
Ion Ratio	Lower	Upper
202	100	
101	26.9	11.1 16.7
100	16.3	8.2 12.2

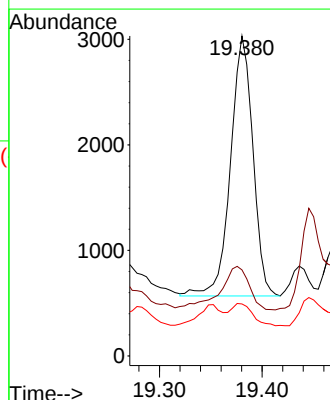



#20

Pyrene

Concen: 0.240 ng/ul m

RT: 19.747 min Scan# 3

Delta R.T. -0.014 min

Lab File: BM042201.D

Acq: 05 Oct 2023 00:19

Instrument :

BNA_M

ClientSampleId :

BBK29





Tgt Ion:	202	Resp:	12329
Ion Ratio	Lower	Upper	
202	100		
101	23.7	12.7	19.1
100	15.9	9.9	14.9

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 10/05/2023

Supervised By :mohammad ahmed 10/06/2023

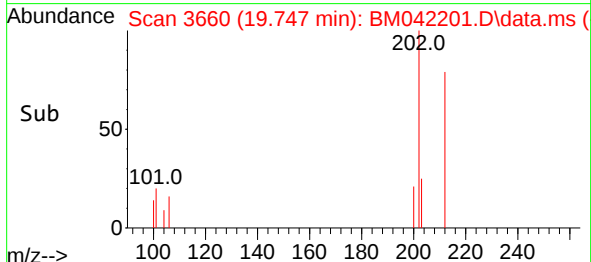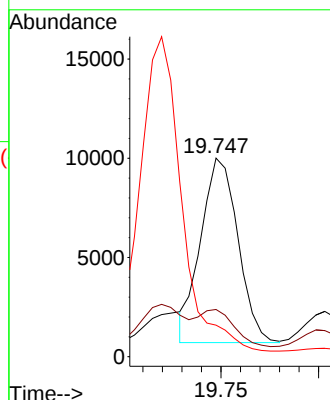

#21

Benzo(a)anthracene

Concen: 0.074 ng/ul




RT: 21.483 min Scan# 4158


Delta R.T. -0.015 min

Lab File: BM042201.D

Acq: 05 Oct 2023 00:19


Tgt Ion:	228	Resp:	3033
Ion Ratio	Lower	Upper	
228	100		
229	49.5	15.8	23.8#
226	40.6	24.6	37.0#

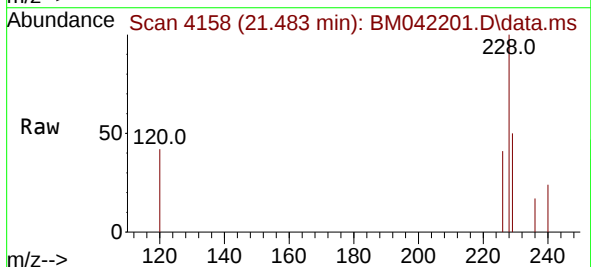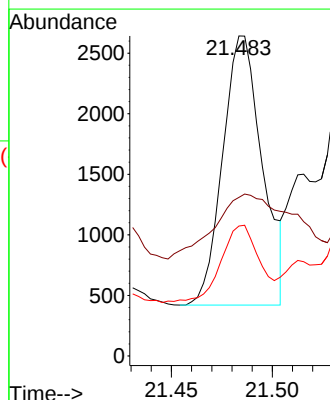



#22
Chrysene
Concen: 0.116 ng/ul m
RT: 21.539 min Scan# 4180
Delta R.T. -0.014 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19




Instrument :
BNA_M
ClientSampleId :
BBK29



Tgt Ion:228 Resp: 463
Ion Ratio Lower Upper
228 100
226 42.5 26.7 40.1
229 49.7 15.8 23.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/05/2023
Supervised By :mohammad ahmed 10/06/2023

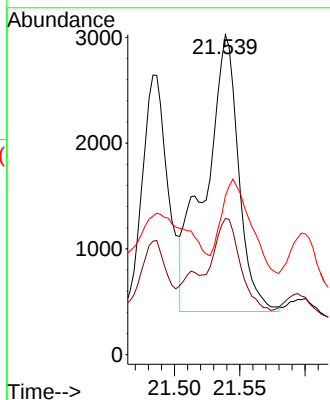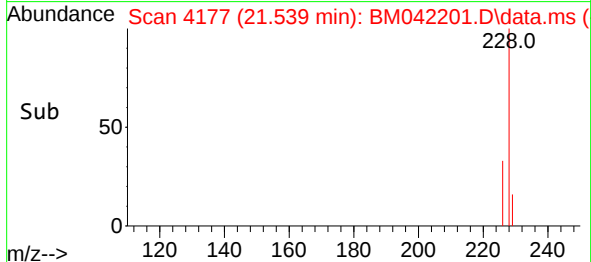

#24
Benzo(b)fluoranthene
Concen: 0.045 ng/ul
RT: 23.161 min Scan# 4732
Delta R.T. -0.017 min
Lab File: BM042201.D
Acq: 05 Oct 2023 00:19

Tgt Ion:252 Resp: 1862
Ion Ratio Lower Upper
252 100
253 76.1 0.0 59.0#
125 78.7 0.0 49.6#

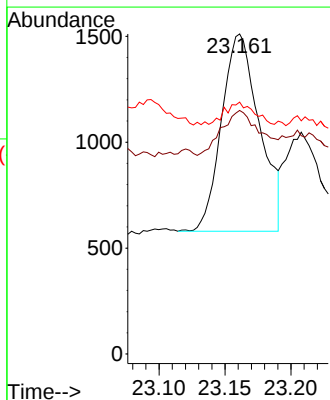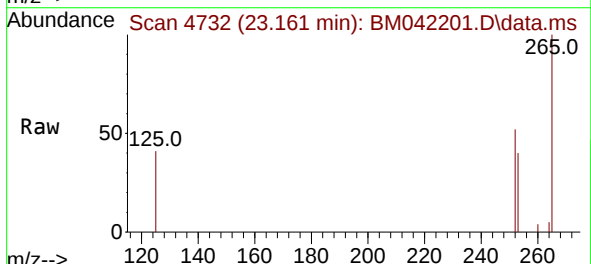



#26

Benzo(a)pyrene

Concen: 0.039 ng/ul

RT: 23.793 min Scan# 4954

Delta R.T. -0.023 min

Lab File: BM042201.D

Acq: 05 Oct 2023 00:19

Instrument :

BNA_M

ClientSampleId :

BBK29





Tgt Ion:	252	Resp:	1390
Ion Ratio	Lower	Upper	
252	100		
253	75.4	25.3	37.9
125	74.7	23.2	34.8

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 10/05/2023

Supervised By :mohammad ahmed 10/06/2023

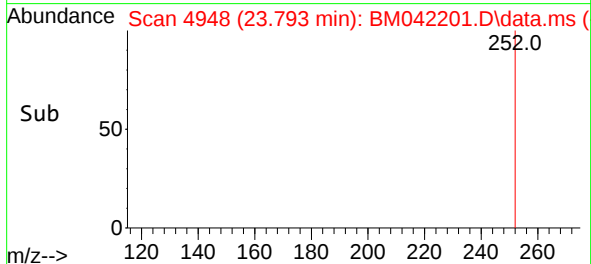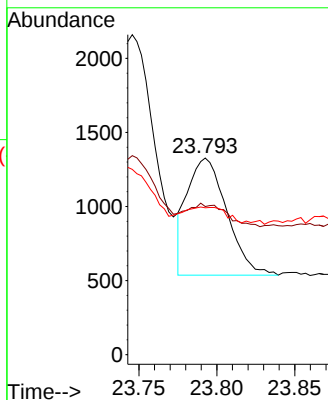

#29

Benzo(g,h,i)perylene

Concen: 0.038 ng/ul

RT: 27.159 min Scan# 6005

Delta R.T. -0.037 min

Lab File: BM042201.D

Acq: 05 Oct 2023 00:19

Tgt Ion:	276	Resp:	1600
Ion Ratio	Lower	Upper	
276	100		
138	55.0	26.8	40.2
277	43.0	20.1	30.1

