

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
 Data File : BM042207.D
 Acq On : 05 Oct 2023 03:59
 Operator : MA/JU
 Sample : 04607-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJE1

Quant Time: Oct 05 04:30:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 02 19:28:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	3611	0.400	ng/u1	0.00
4) Naphthalene-d8	10.741	136	9756	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.574	164	4333	0.400	ng/u1	#-0.01
13) Phenanthrene-d10	17.329	188	9686	0.400	ng/u1	#-0.01
17) Chrysene-d12	21.507	240	4876	0.400	ng/u1	# 0.00
23) Perylene-d12	23.901	264	5574	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	23752	4.939	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.324	152	5239	0.392	ng/u1	-0.01
18) Fluoranthene-d10	19.352	212	9075	0.496	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.393	88	1145	0.228	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
Data File : BM042207.D
Acq On : 05 Oct 2023 03:59
Operator : MA/JU
Sample : 04607-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJE1

Quant Time: Oct 05 04:30:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 02 19:28:41 2023
Response via : Initial Calibration

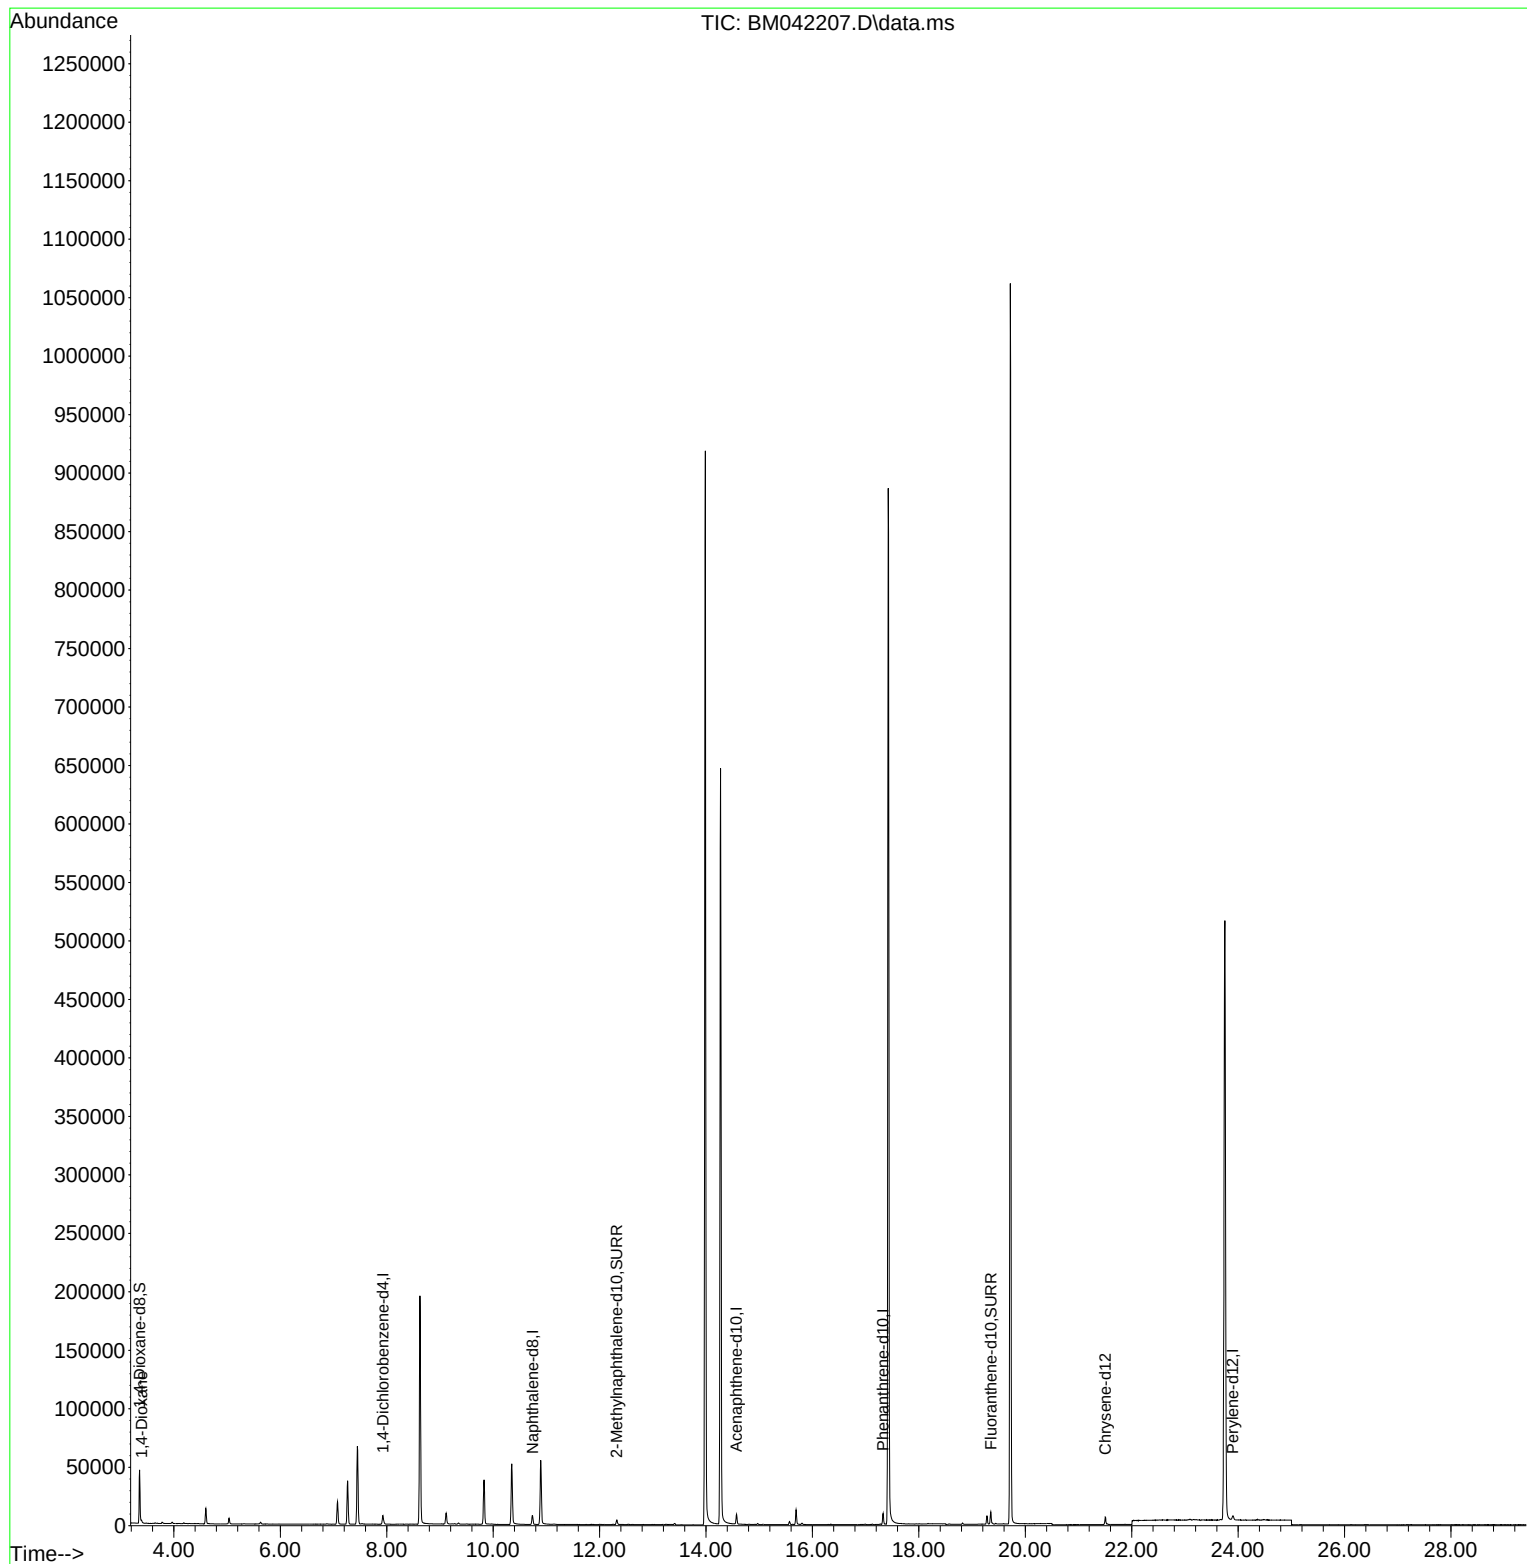

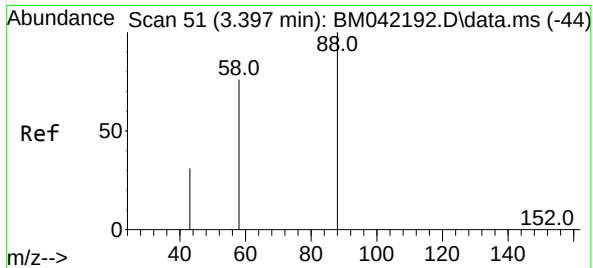

#2
 1,4-Dioxane
 Concen: 0.228 ng/ul
 RT: 3.393 min Scan# 50
 Delta R.T. -0.008 min
 Lab File: BM042207.D
 Acq: 05 Oct 2023 03:59

Instrument :
 BNA_M
 ClientSampleId :
 BBJE1

Tgt Ion: 88 Resp: 1145

Ion	Ratio	Lower	Upper
88	100		
43	66.5	52.1	78.1
58	61.1	53.8	80.6

