

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
 Data File : BM042214.D
 Acq On : 05 Oct 2023 12:49
 Operator : MA/JU
 Sample : 04607-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJF9

Quant Time: Oct 06 05:27:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:25:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	4972	0.400	ng/ul	0.00
4) Naphthalene-d8	10.735	136	14262	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.574	164	5883	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.329	188	12567	0.400	ng/ul	-0.01
17) Chrysene-d12	21.507	240	5989	0.400	ng/ul	0.00
23) Perylene-d12	23.901	264	6525	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	59457	8.980	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.324	152	4590	0.235	ng/ul	0.00
18) Fluoranthene-d10	19.352	212	8858	0.394	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.393	88	4537	0.656	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
Data File : BM042214.D
Acq On : 05 Oct 2023 12:49
Operator : MA/JU
Sample : 04607-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJF9

Quant Time: Oct 06 05:27:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:25:26 2023
Response via : Initial Calibration

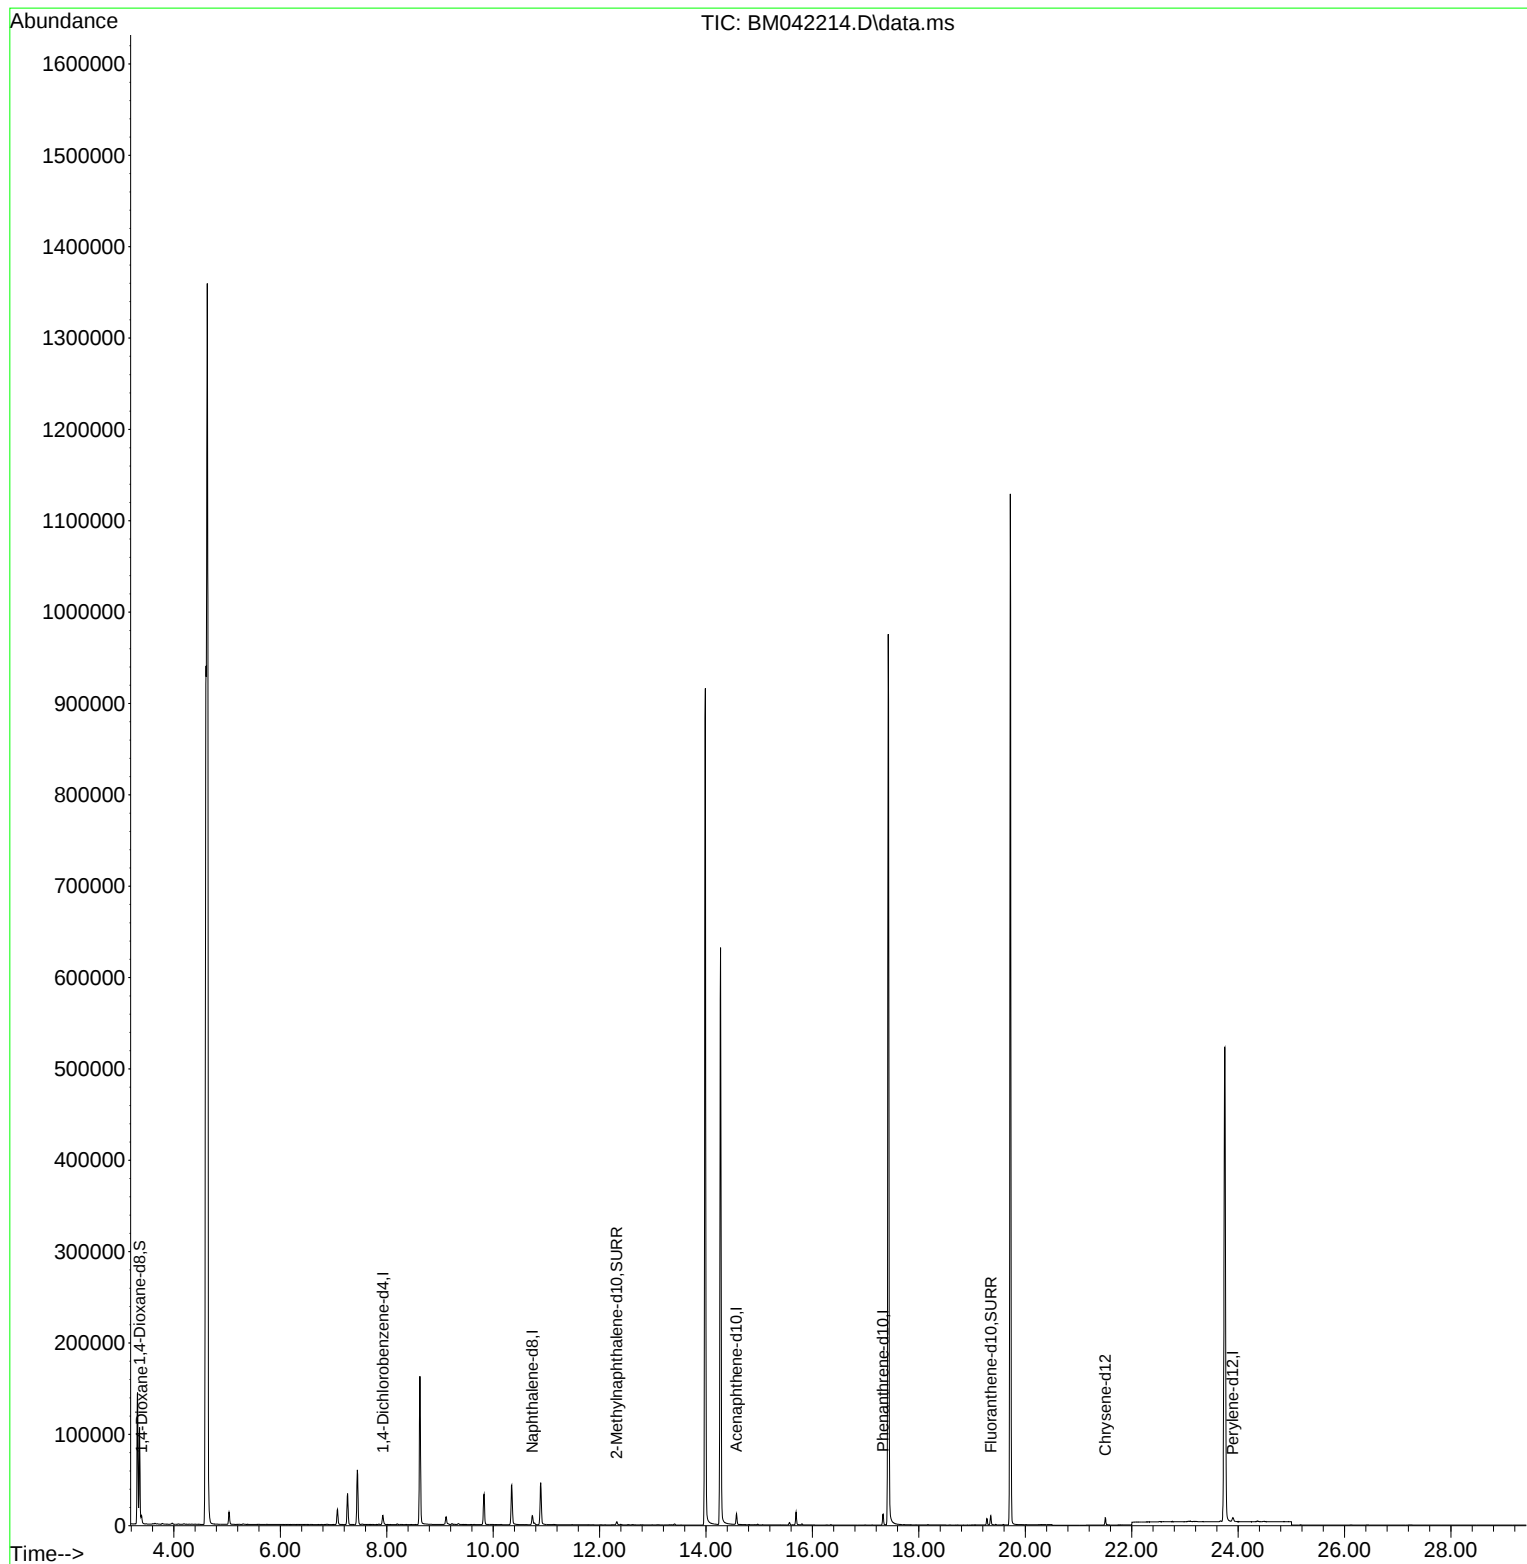

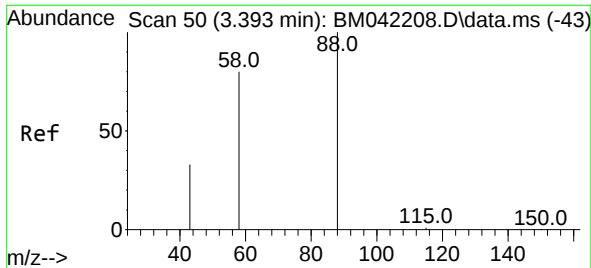

#2
 1,4-Dioxane
 Concen: 0.656 ng/ul
 RT: 3.393 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: BM042214.D
 Acq: 05 Oct 2023 12:49

Instrument :
 BNA_M
 ClientSampleId :
 BBJF9

Tgt Ion:	88	Resp:	4537
Ion	Ratio	Lower	Upper
88	100		
43	42.4	52.1	78.1#
58	75.1	53.8	80.6

