

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
 Data File : BM042216.D
 Acq On : 05 Oct 2023 14:40
 Operator : MA/JU
 Sample : 04469-09
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EZYP6

Quant Time: Oct 06 05:27:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:25:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	3909	0.400	ng/u1	0.00
4) Naphthalene-d8	10.735	136	11136	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.574	164	4886	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.329	188	9914	0.400	ng/u1	-0.01
17) Chrysene-d12	21.507	240	4757	0.400	ng/u1	0.00
23) Perylene-d12	23.904	264	5140	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.355	96	16219	3.116	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.324	152	2597	0.170	ng/u1	0.00
18) Fluoranthene-d10	19.352	212	4638	0.260	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.393	88	832	0.153	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100423\
Data File : BM042216.D
Acq On : 05 Oct 2023 14:40
Operator : MA/JU
Sample : 04469-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EZYP6

Quant Time: Oct 06 05:27:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:25:26 2023
Response via : Initial Calibration

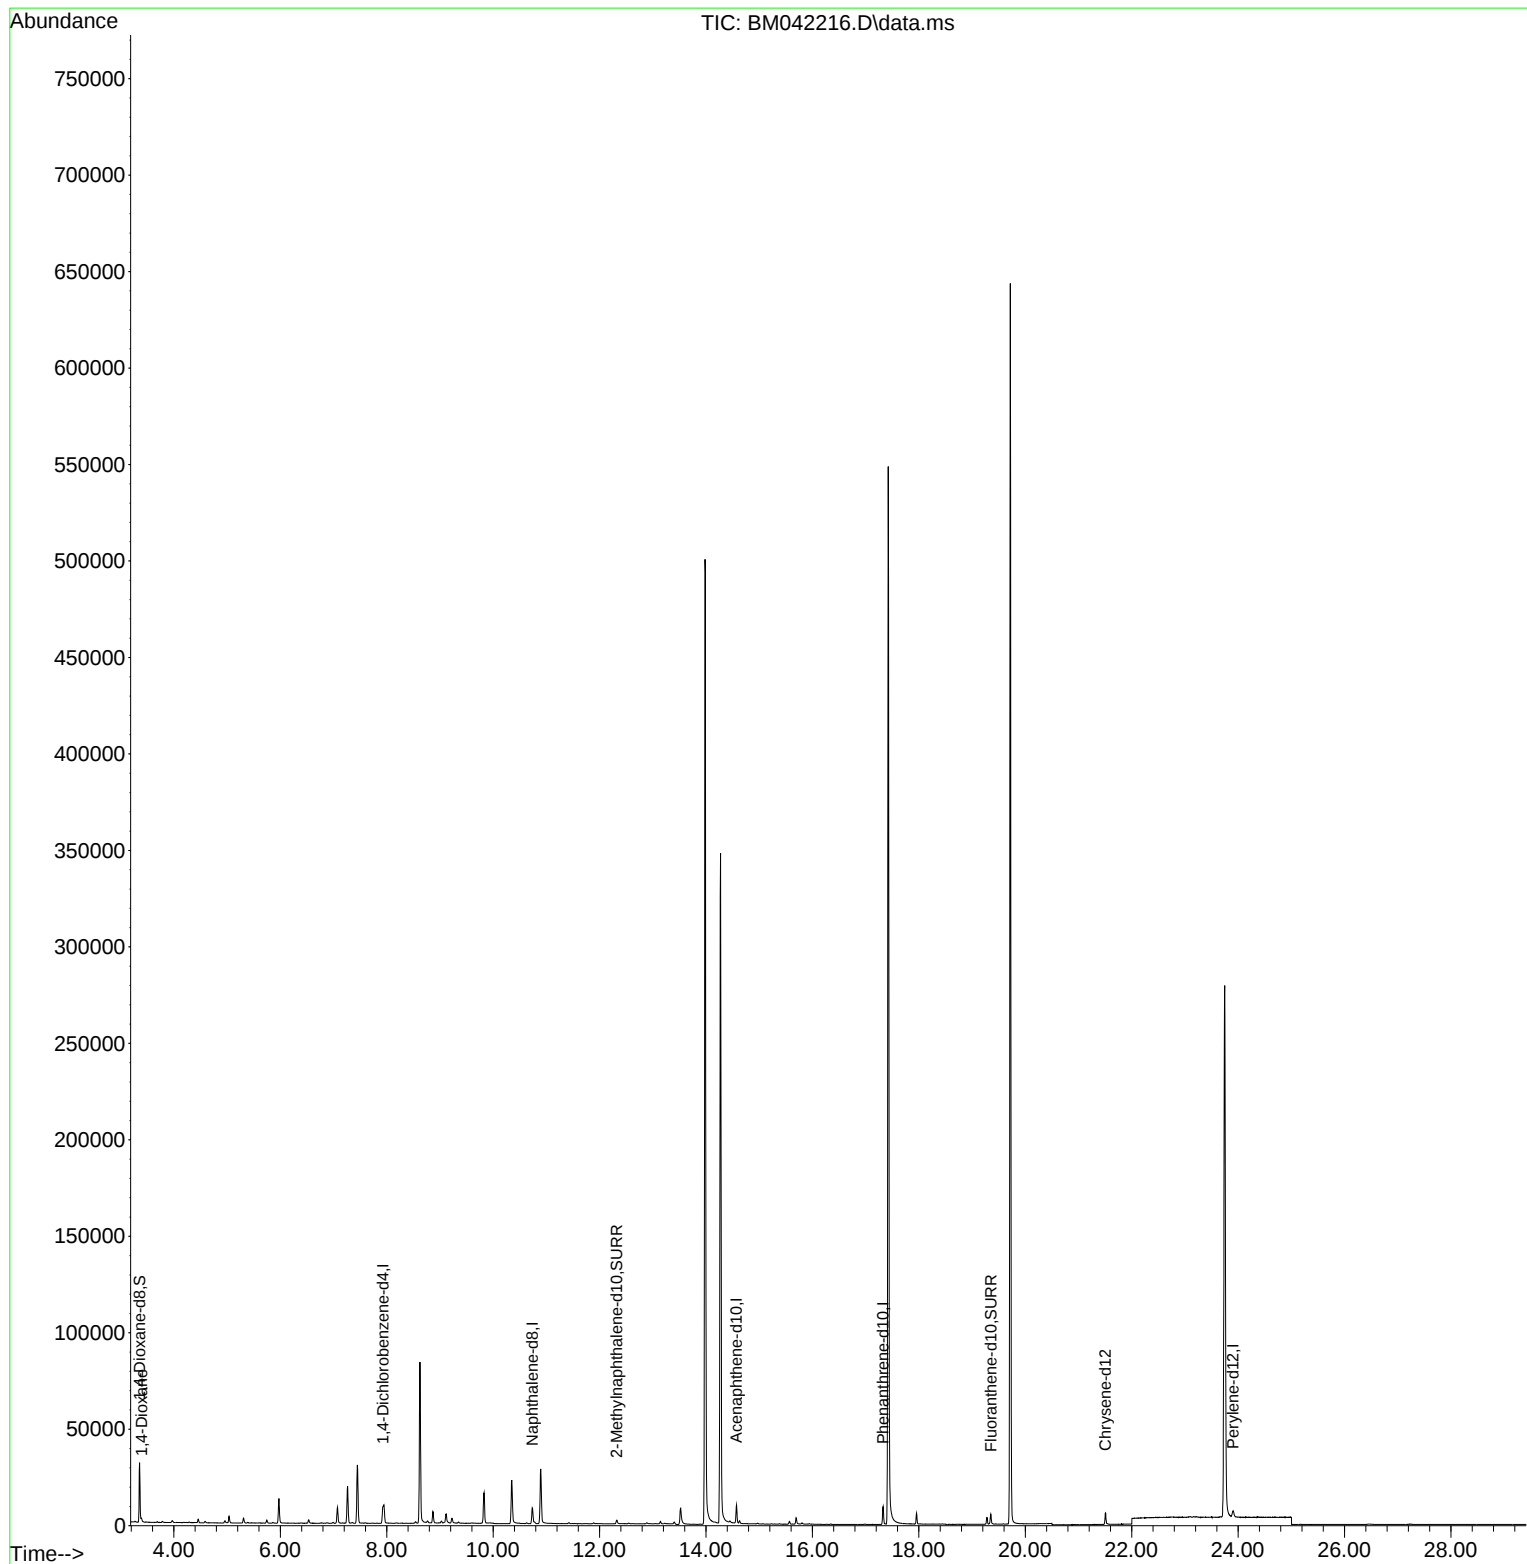

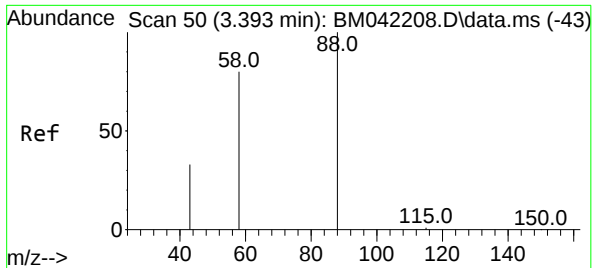

#2
 1,4-Dioxane
 Concen: 0.153 ng/ul
 RT: 3.393 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: BM042216.D
 Acq: 05 Oct 2023 14:40

Instrument :
 BNA_M
 ClientSampleId :
 EZYP6

Tgt Ion: 88 Resp: 832

Ion	Ratio	Lower	Upper
88	100		
43	72.8	52.1	78.1
58	68.5	53.8	80.6

