

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100518\
 Data File : BM017054.D
 Acq On : 06 Oct 2018 02:29
 Operator : MJ/SJ
 Sample : J5298-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 06 06:44:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 06 06:43:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	215624	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	946327	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.33	164	547759	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.08	188	1219259	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1323551	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	1328985	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	20809	4.80	ng/uL	0.00
5) Phenol-d5	6.87	99	120832	6.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	330500	30.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	379535	25.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	230162	16.30	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	225329	32.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	233744	33.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	434343	30.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	19139	1.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.75	166	1404046	32.31	ng/ul	0.00
47) Acenaphthylene-d8	14.03	160	1838936	33.10	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	37686	4.59	ng/ul	0.00
58) Fluorene-d10	15.33	176	1273371	32.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	174136	24.22	ng/ul	0.00
71) Anthracene-d10	17.18	188	1924895	33.05	ng/ul	0.00
79) Pyrene-d10	19.48	212	2111044	35.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.35	264	2335067	34.32	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.80	163	47526	1.104	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100518\
Data File : BM017054.D
Acq On : 06 Oct 2018 02:29
Operator : MJ/SJ
Sample : J5298-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 06 06:44:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 06:43:32 2018
Response via : Initial Calibration

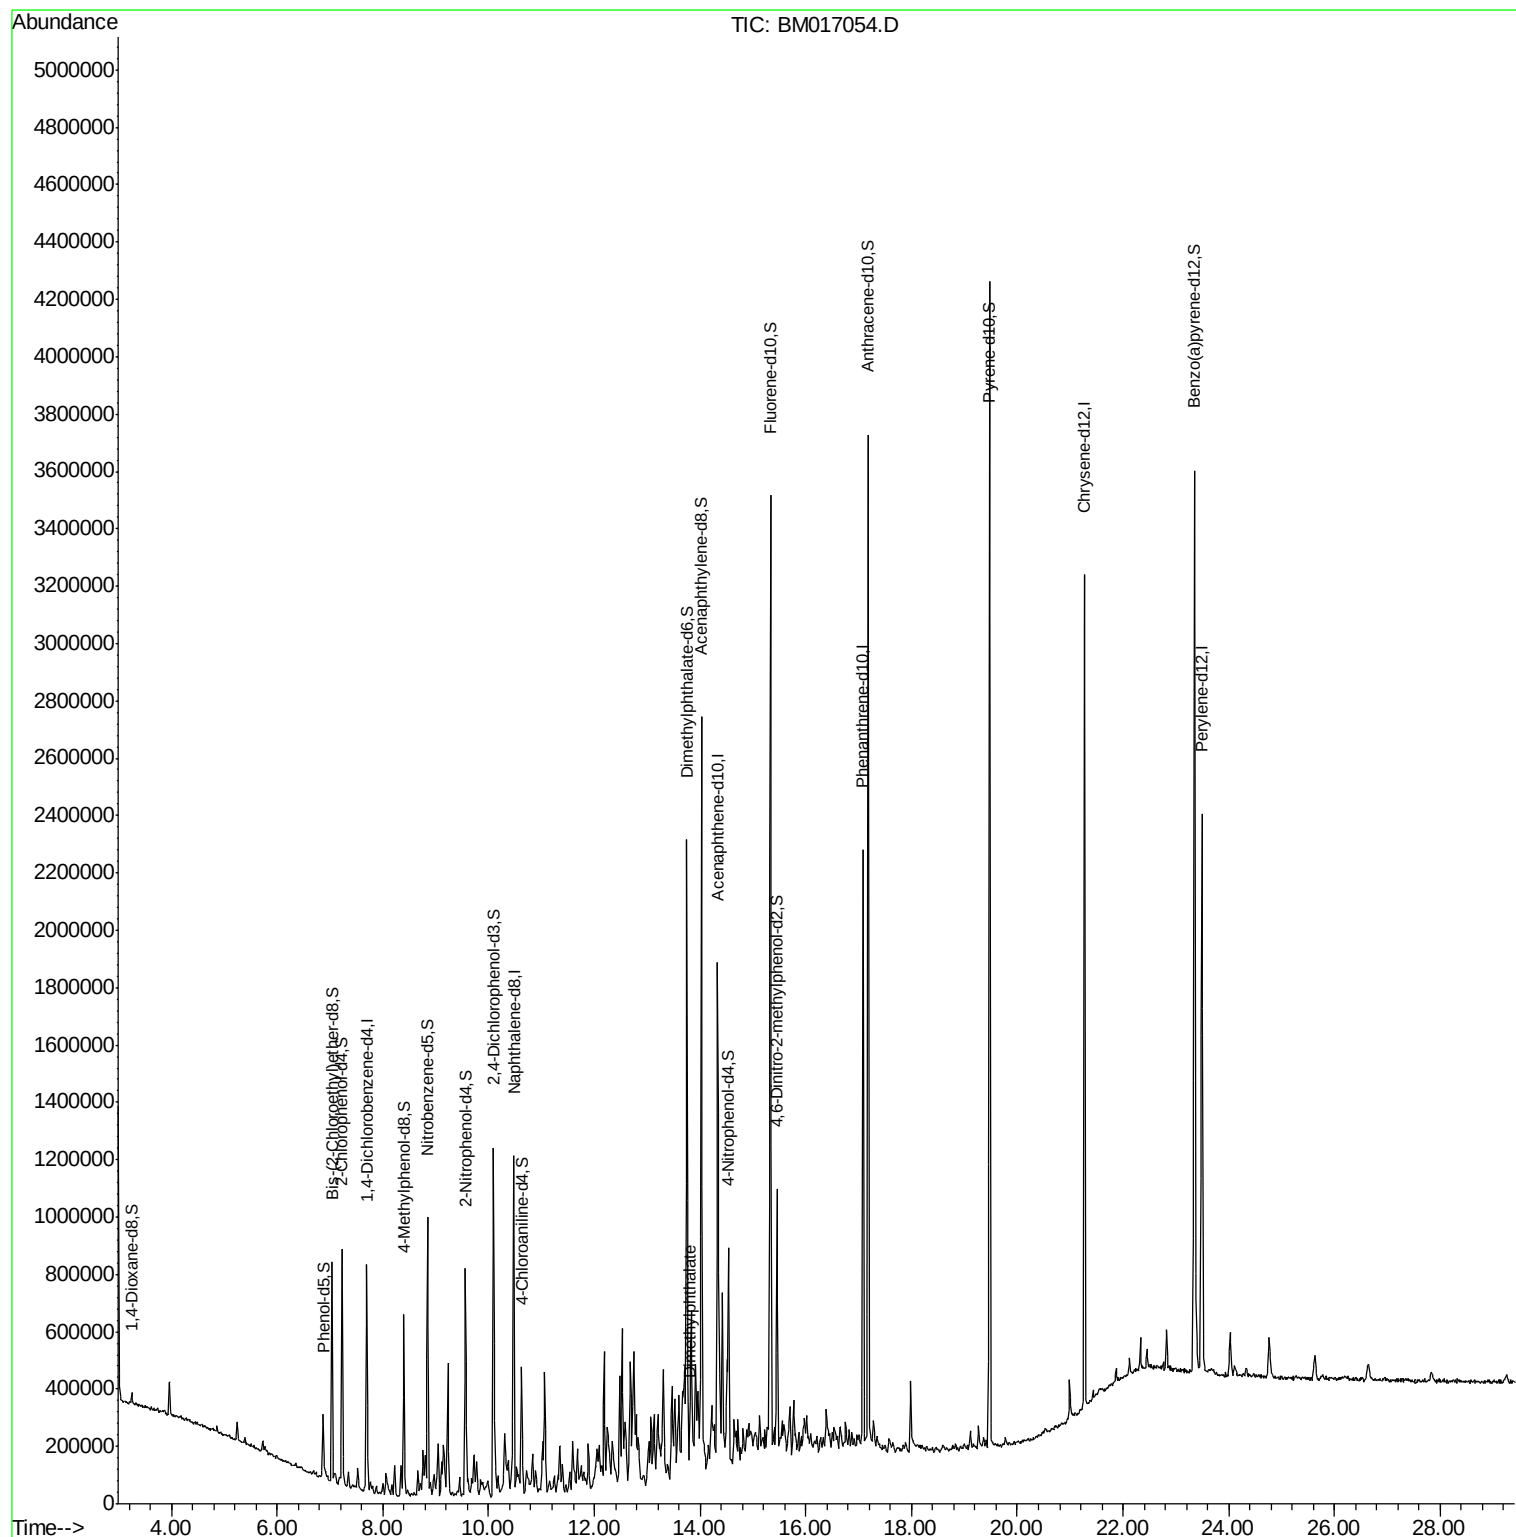

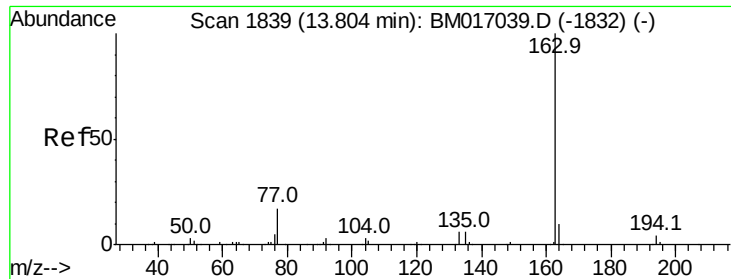

#45

Dimethylphthalate

Concen: 1.104 ng/ul

RT: 13.80 min Scan# 1838

Delta R.T. -0.01 min

Lab File: BM017054.D

Acq: 06 Oct 2018 02:29

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 47526

Ion Ratio Lower Upper

163 100

194 3.7 3.3 4.9

164 9.8 8.0 12.0

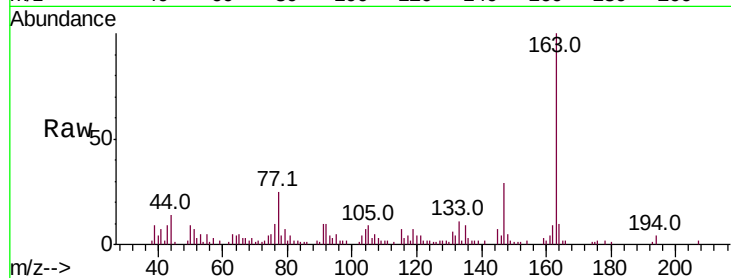

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

